




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122716\
Data File : BM008678.D
Acq On : 27 Dec 2016 18:00
Operator : UM/SJ
Sample : H6040-17DL 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA8X0DL

Manual Integrations
APPROVED

sohil
12/28/2016 6:01:46 PM

Quant Time: Dec 28 04:34:36 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 28 03:24:04 2016
Response via : Initial Calibration

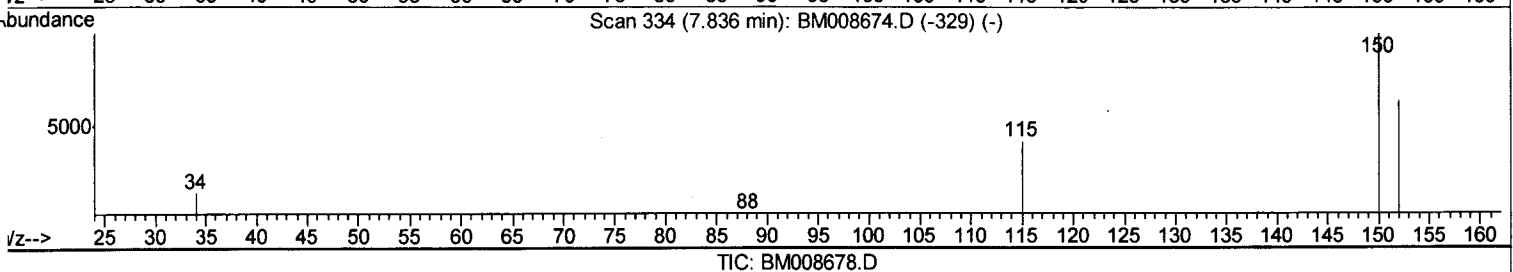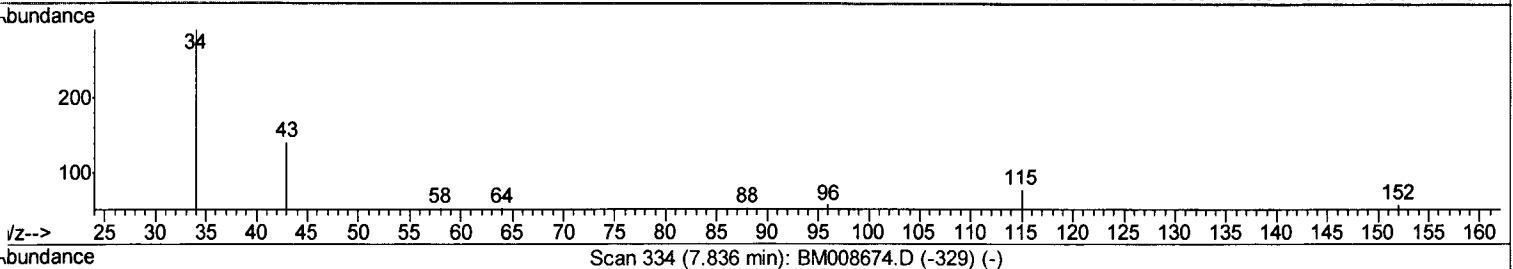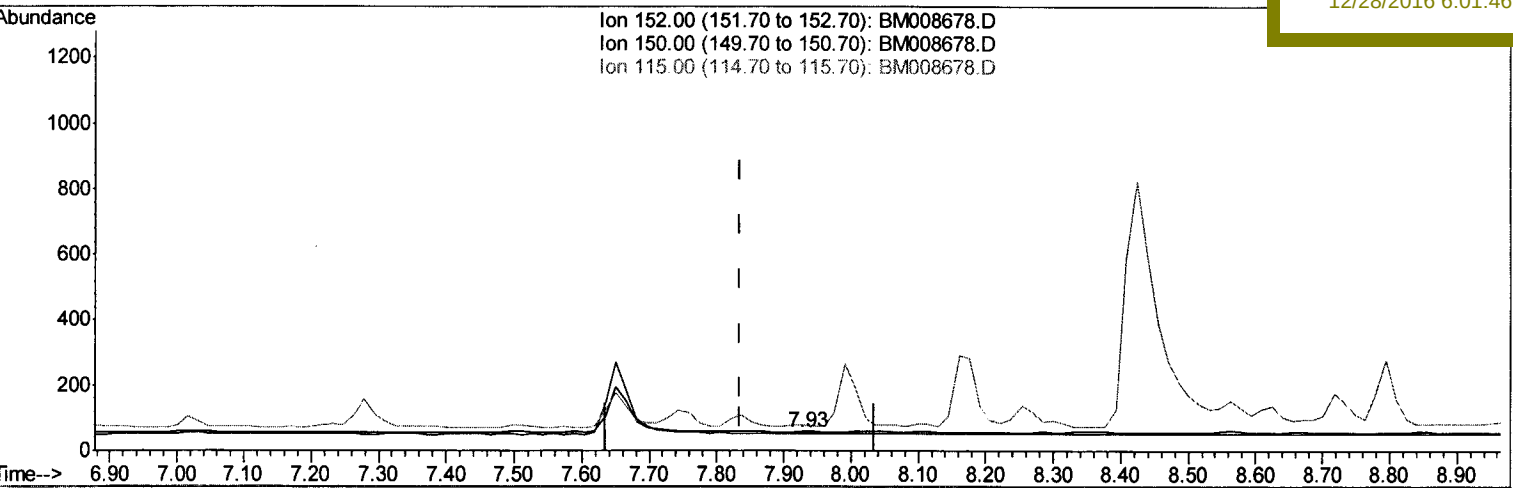

(1) 1,4-Dichlorobenzene-d4 (I)

7.929min (+0.093) 0.40ng/ul

response 6

Ion	Exp%	Act%
152.00	100	100
150.00	143.40	88.14#
115.00	64.90	132.20#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122716\
 Data File : BM008678.D
 Acq On : 27 Dec 2016 18:00
 Operator : UM/SJ
 Sample : H6040-17DL 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA8X0DL

Manual Integrations
 APPROVED

sohil
 12/28/2016 6:01:46 PM

Quant Time: Dec 28 04:34:36 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 28 03:24:04 2016
 Response via : Initial Calibration

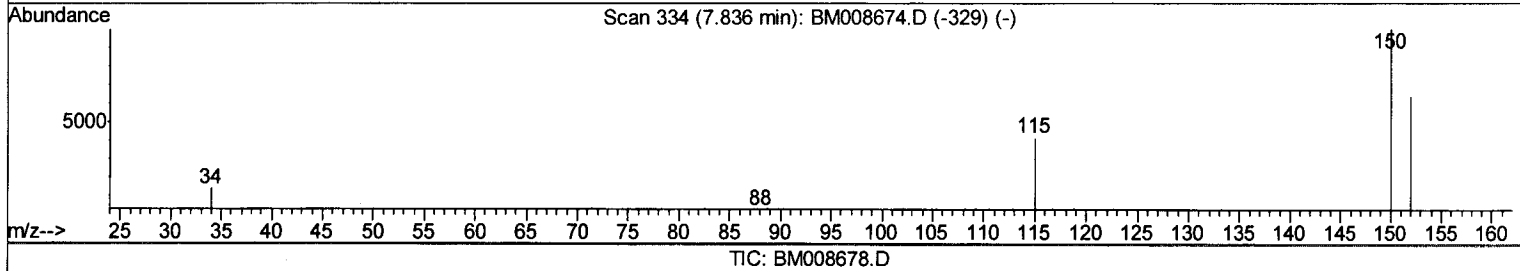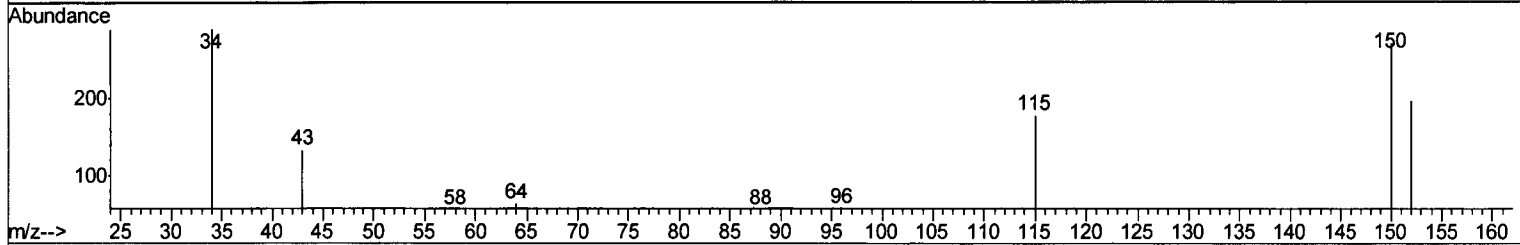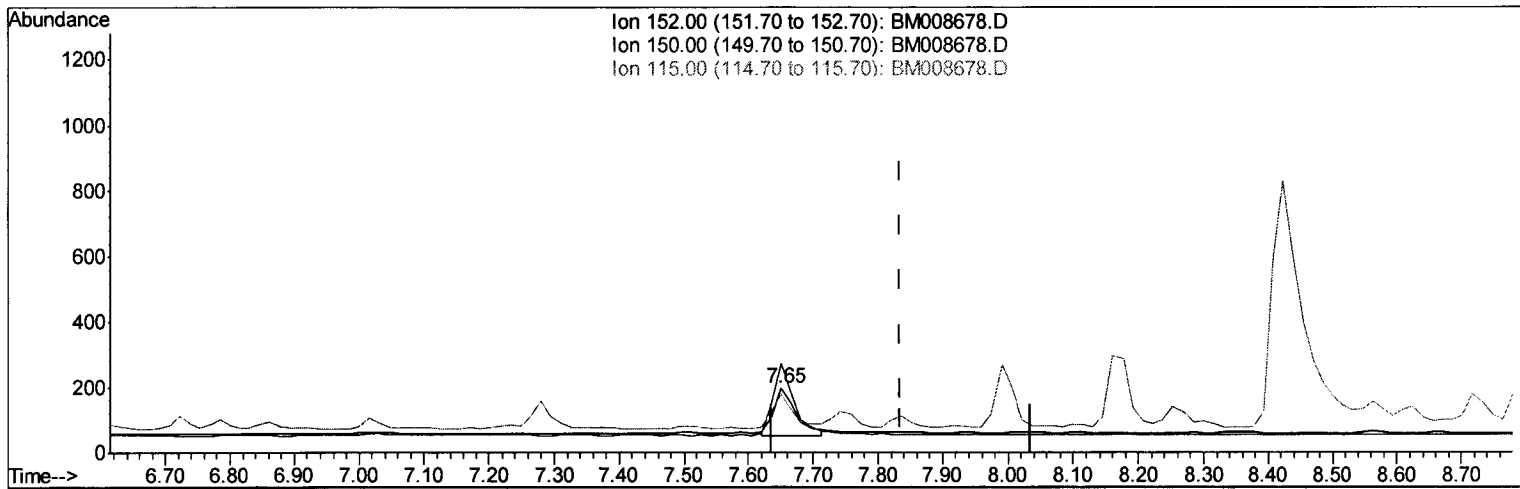

(1) 1,4-Dichlorobenzene-d4 (I)

7.650min (-0.186) 0.40ng/ul m

response 366

Ion	Exp%	Act%
152.00	100	100
150.00	143.40	137.56
115.00	64.90	90.36#
0.00	0.00	0.00

S. J
 12/29/16




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122716\
Data File : BM008678.D
Acq On : 27 Dec 2016 18:00
Operator : UM/SJ
Sample : H6040-17DL 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA8X0DL

Manual Integrations
APPROVED

sohil
12/28/2016 6:01:46 PM

Quant Time: Dec 28 04:34:36 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 28 03:24:04 2016
Response via : Initial Calibration

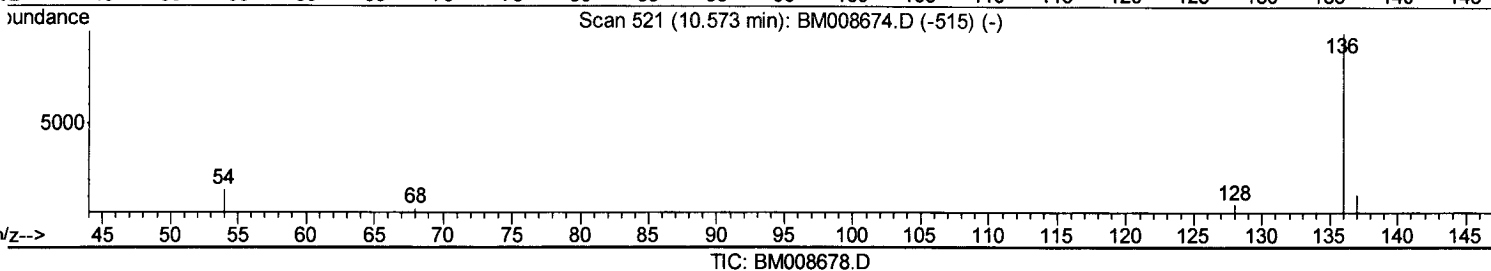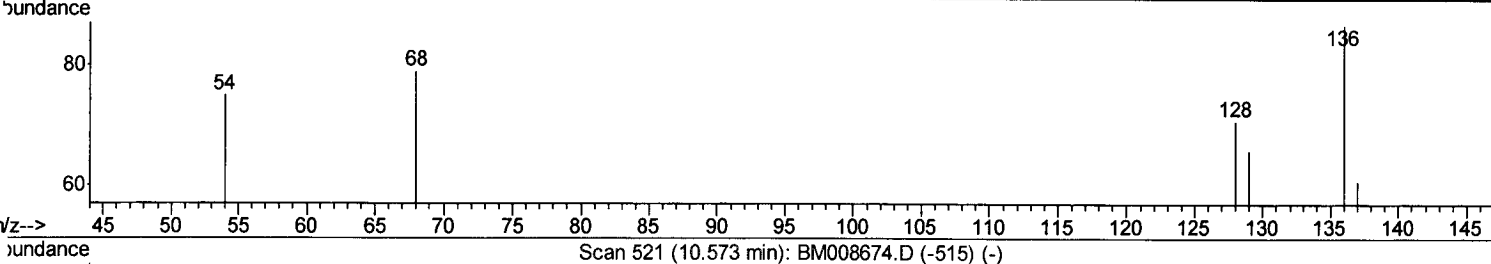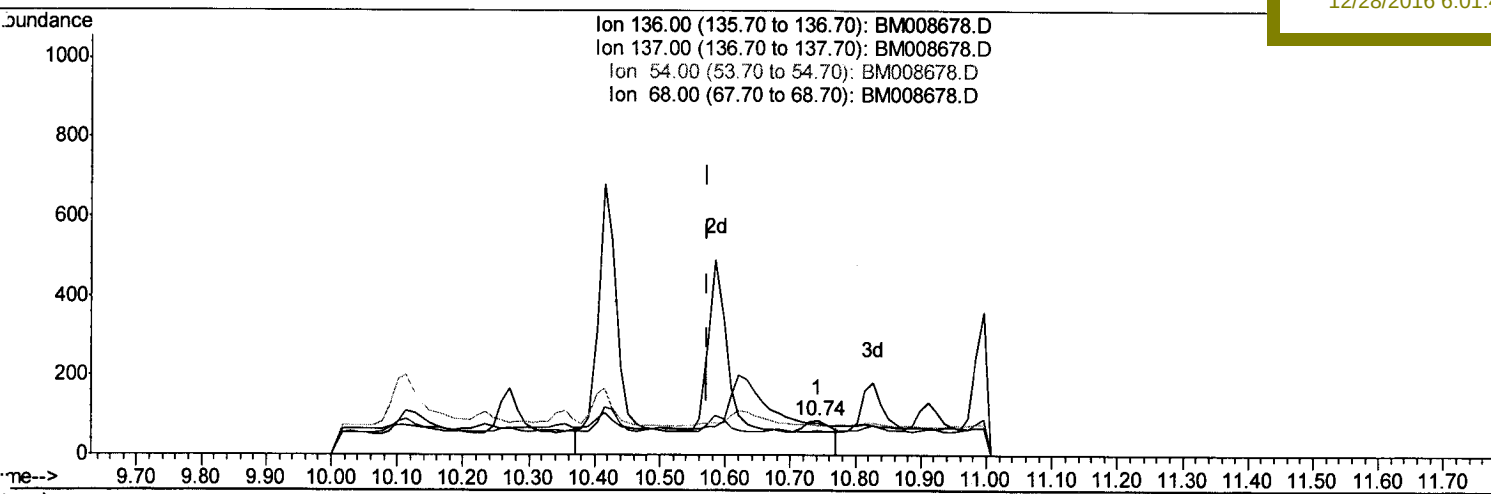

(2) Naphthalene-d8 (I)

10.742min (+0.169) 0.40ng/ul

response 57

Ion	Exp%	Act%
136.00	100	100
137.00	13.90	70.11#
54.00	15.50	86.21#
68.00	9.90	90.80#

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122716\
 Data File : BM008678.D
 Acq On : 27 Dec 2016 18:00
 Operator : UM/SJ
 Sample : H6040-17DL 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA8X0DL

Manual Integrations
 APPROVED

sohil
 12/28/2016 6:01:46 PM

Quant Time: Dec 28 04:34:36 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 28 03:24:04 2016
 Response via : Initial Calibration

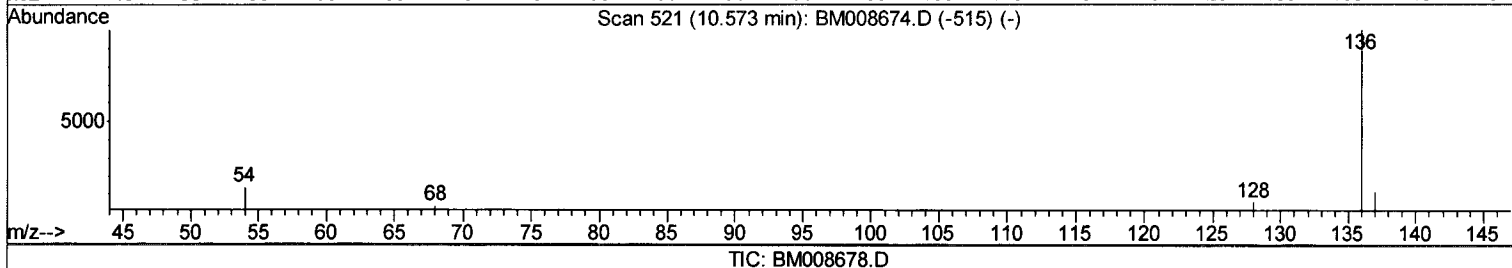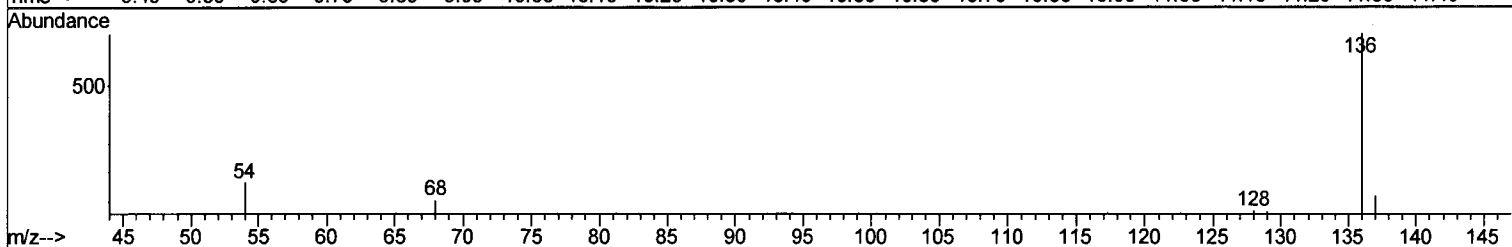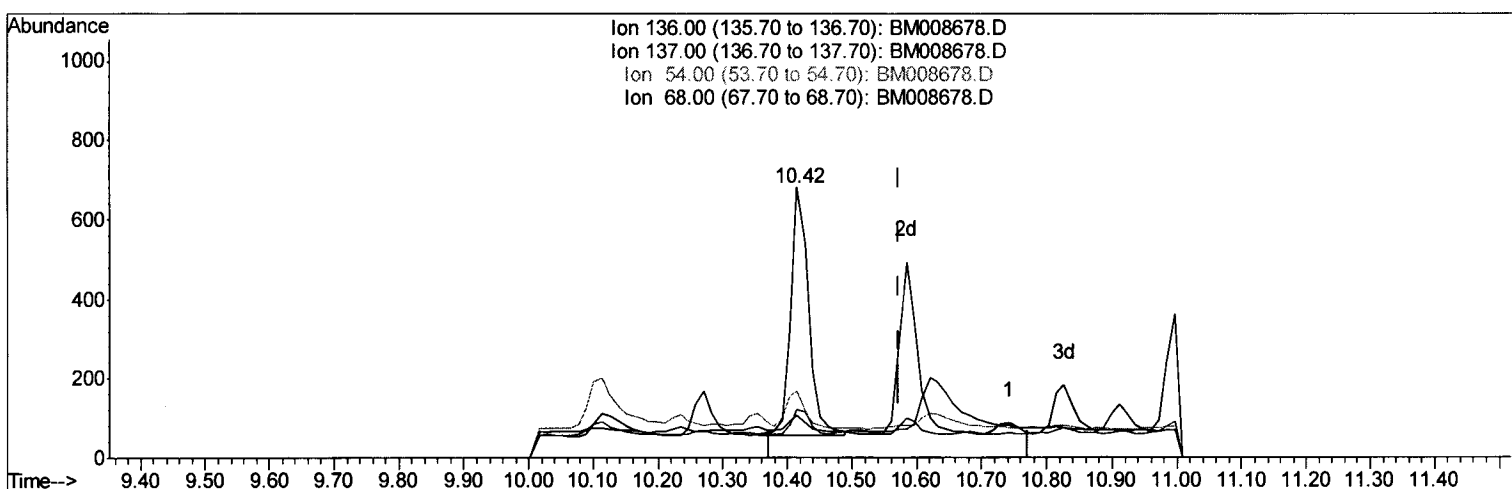

(2) Naphthalene-d8 (I)

10.415min (-0.157) 0.40ng/ul m

response 1219

Ion	Exp%	Act%
136.00	100	100
137.00	13.90	17.79#
54.00	15.50	24.41#
68.00	9.90	15.29#

S. J
 12/29/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122716\
 Data File : BM008678.D
 Acq On : 27 Dec 2016 18:00
 Operator : UM/SJ
 Sample : H6040-17DL 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA8X0DL

Quant Time: Dec 28 04:34:36 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 28 03:24:04 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

sohil
 12/28/2016 6:01:46 PM

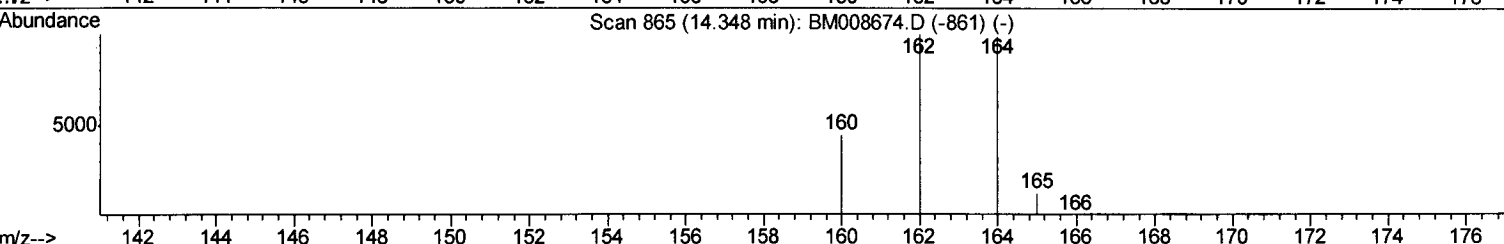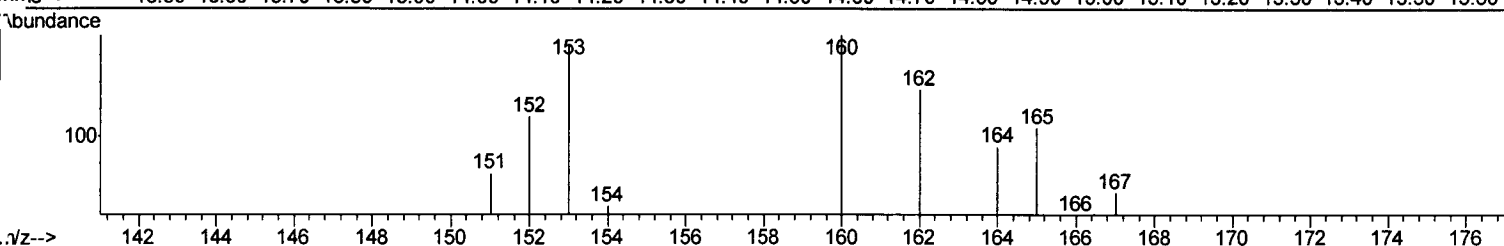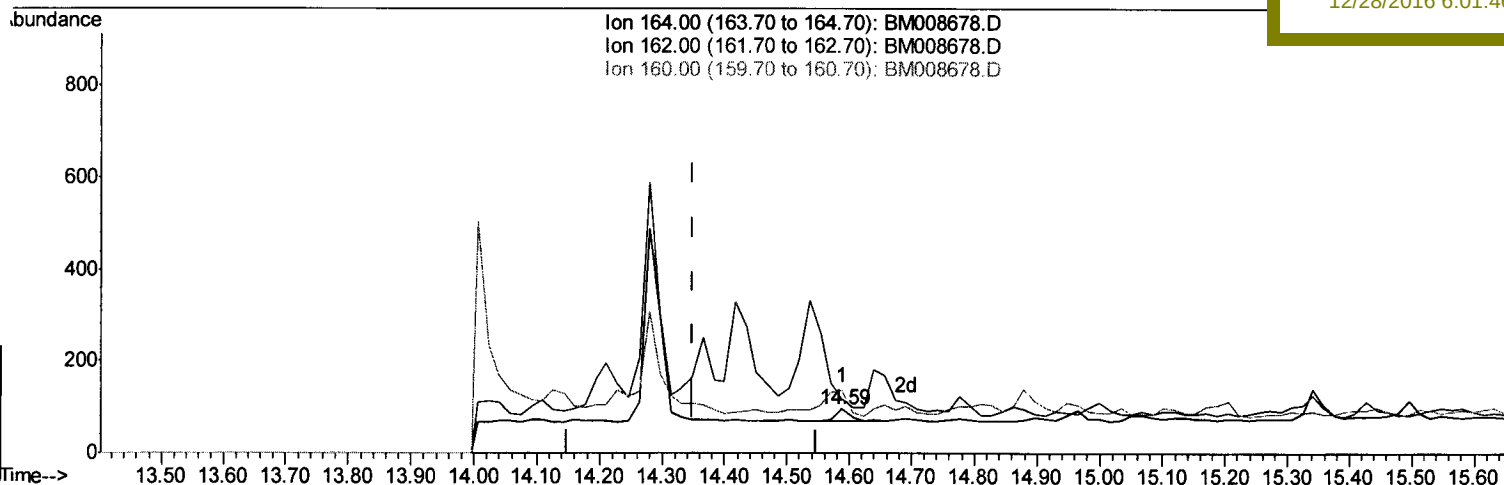

TIC: BM008678.D

(6) Acenaphthene-d10 (I)

14.588min (+0.240) 0.40ng/ul

response 48

Ion	Exp%	Act%
164.00	100	100
162.00	98.60	121.88#
160.00	48.80	142.71#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122716\
 Data File : BM008678.D
 Acq On : 27 Dec 2016 18:00
 Operator : UM/SJ
 Sample : H6040-17DL 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA8X0DL

Manual Integrations
 APPROVED

sohil
 12/28/2016 6:01:46 PM

Quant Time: Dec 28 04:34:36 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 28 03:24:04 2016
 Response via : Initial Calibration

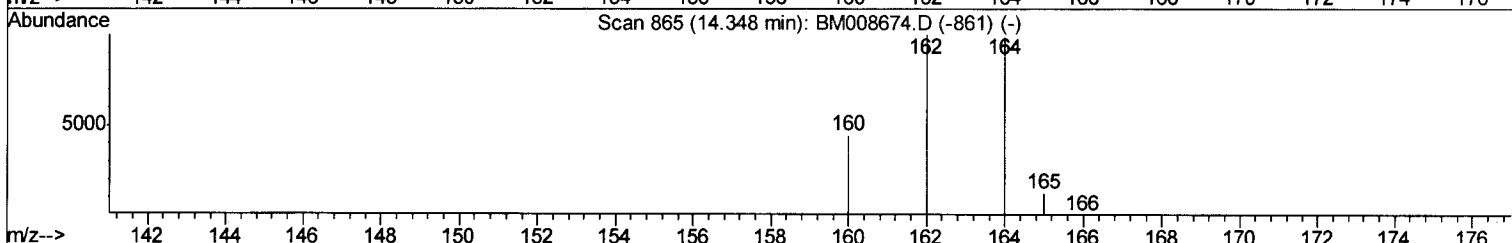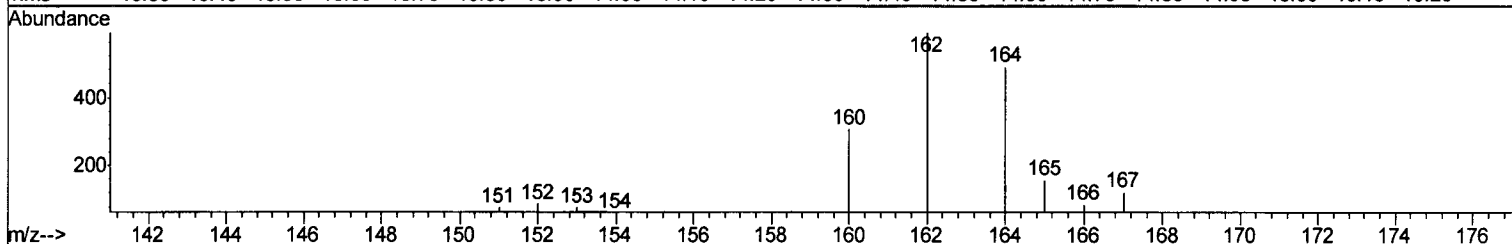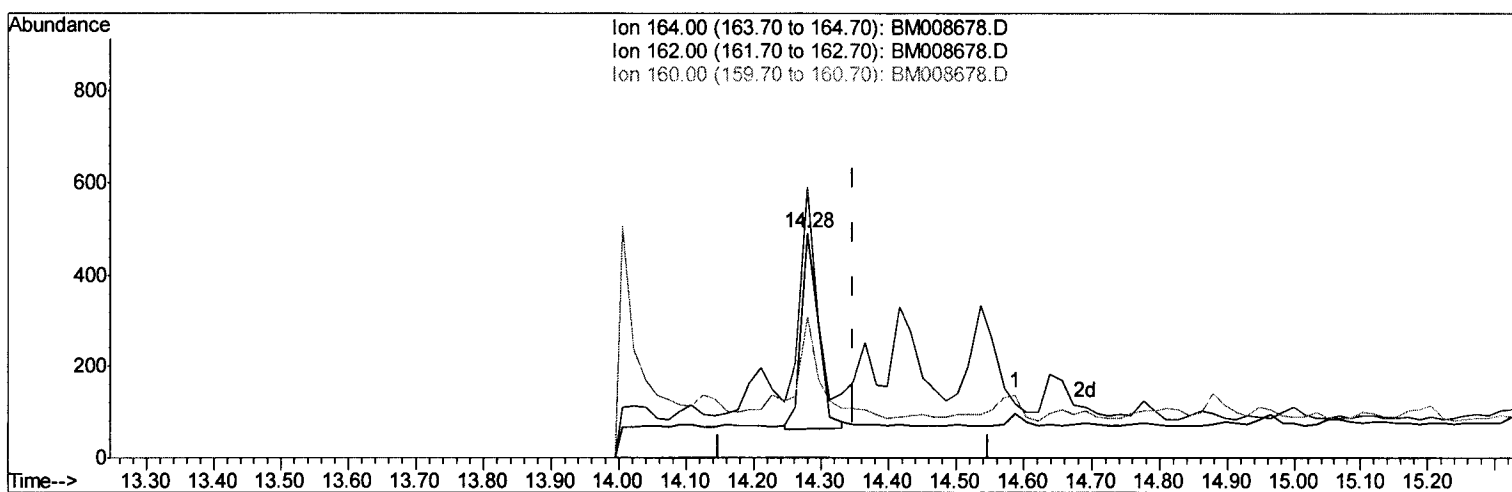

TIC: BM008678.D

(6) Acenaphthene-d10 (I)

14.280min (-0.068) 0.40ng/ul m

response 764

Ion	Exp%	Act%
164.00	100	100
162.00	98.60	120.20#
160.00	48.80	62.65#
0.00	0.00	0.00

S.J
 12/29/16




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122716\
Data File : BM008678.D
Acq On : 27 Dec 2016 18:00
Operator : UM/SJ
Sample : H6040-17DL 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Dec 28 04:34:36 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 28 03:24:04 2016
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
DA8X0DL

Manual Integrations
APPROVED

sohil
12/28/2016 6:01:46 PM

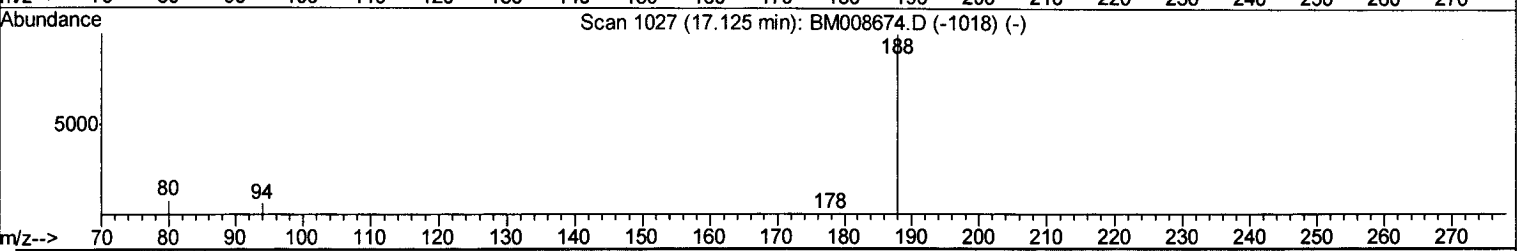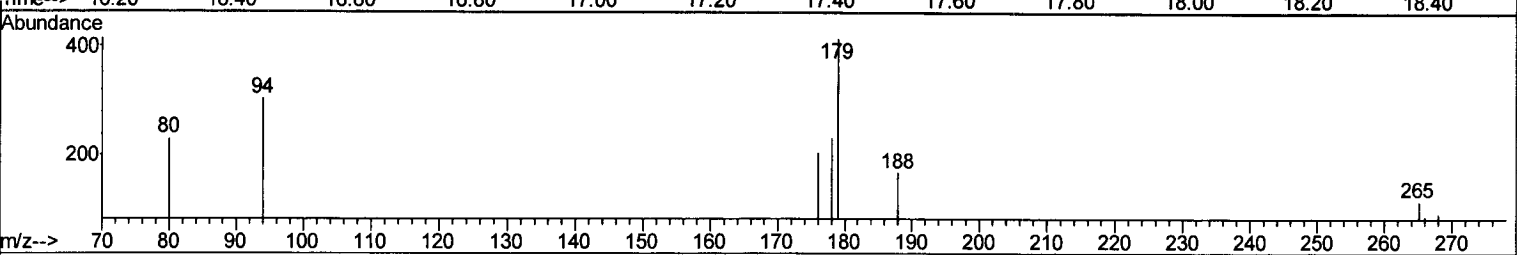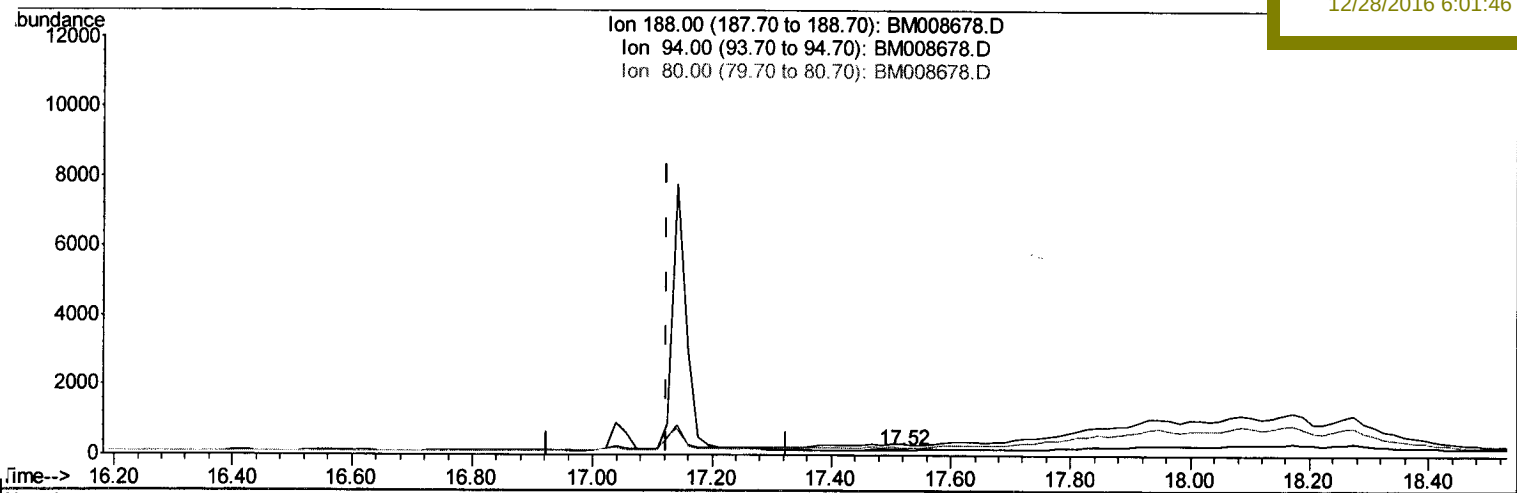

TIC: BM008678.D

(10) Phenanthrene-d10 (I)

17.519min (+0.395) 0.40ng/ul

response 65

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	180.95#
80.00	11.80	136.90#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122716\
 Data File : BM008678.D
 Acq On : 27 Dec 2016 18:00
 Operator : UM/SJ
 Sample : H6040-17DL 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA8X0DL

Manual Integrations
 APPROVED

sohil
 12/28/2016 6:01:46 PM

Quant Time: Dec 28 04:34:36 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 28 03:24:04 2016
 Response via : Initial Calibration

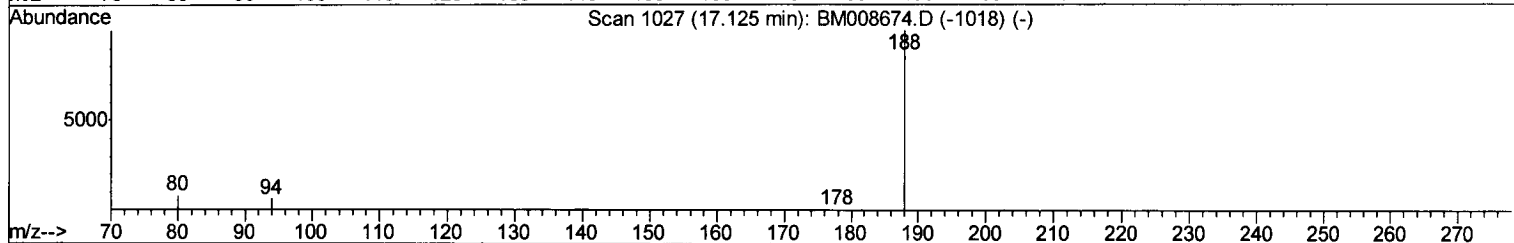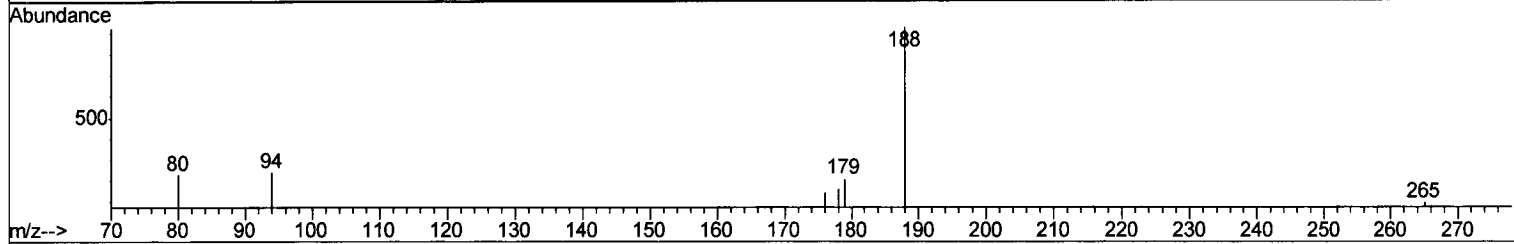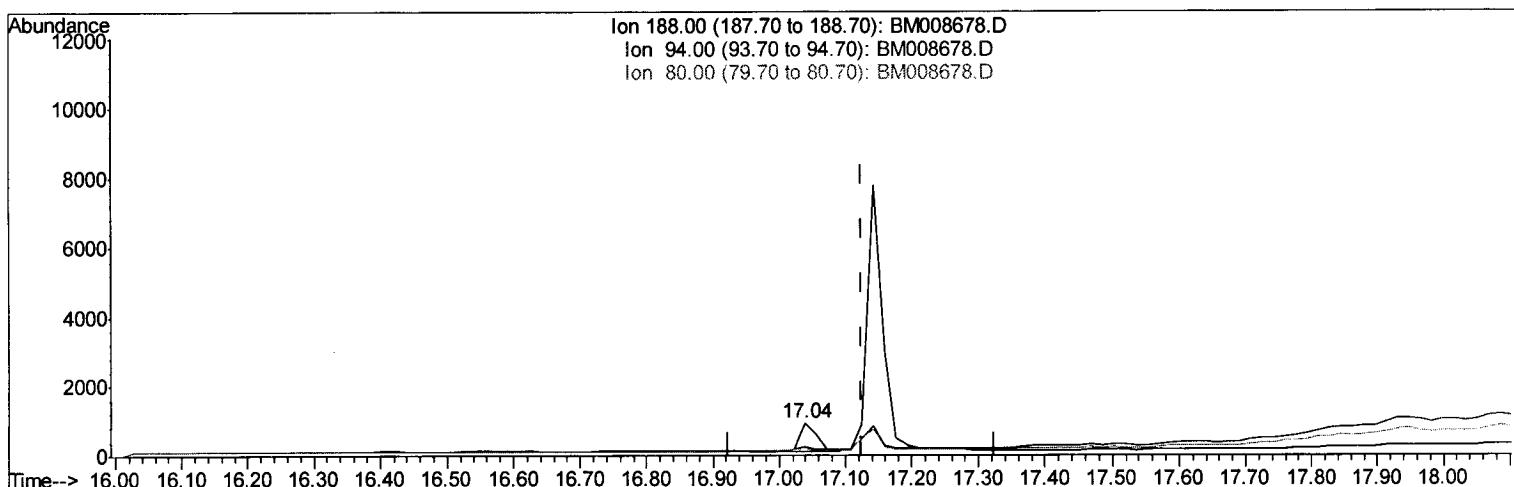

TIC: BM008678.D

(10) Phenanthrene-d10 (I)

17.039min (-0.086) 0.40ng/ul m

response 1605

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	26.00#
80.00	11.80	24.70#
0.00	0.00	0.00

S.J
 12/29/16




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122716\
Data File : BM008678.D
Acq On : 27 Dec 2016 18:00
Operator : UM/SJ
Sample : H6040-17DL 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA8X0DL

Manual Integrations
APPROVED

sohil
12/28/2016 6:01:46 PM

Quant Time: Dec 28 04:34:36 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 28 03:24:04 2016
Response via : Initial Calibration

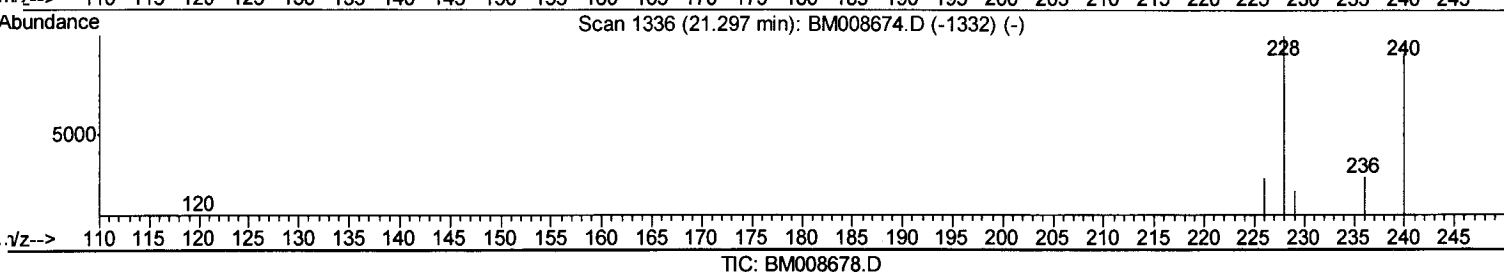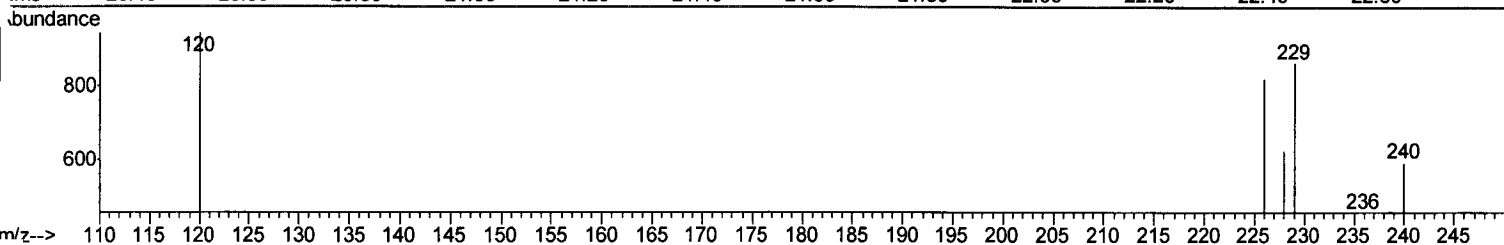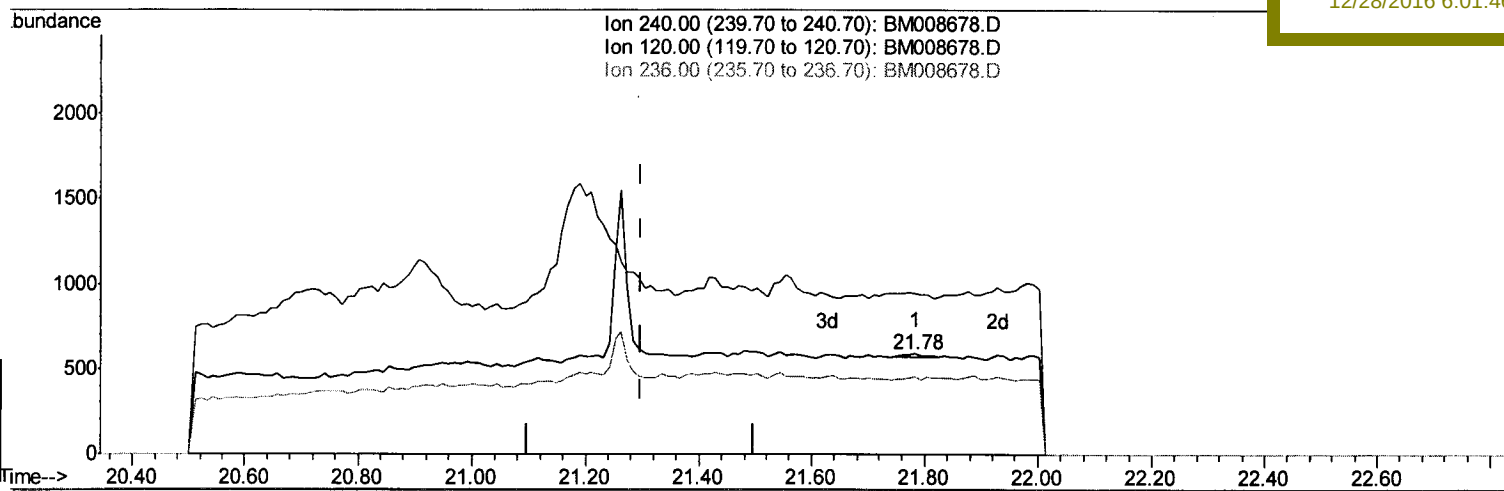

(16) Chrysene-d12 (I)

21.783min (+0.486) 0.40ng/ul

response 54

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	160.17#
236.00	34.90	76.95#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122716\
 Data File : BM008678.D
 Acq On : 27 Dec 2016 18:00
 Operator : UM/SJ
 Sample : H6040-17DL 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA8X0DL

Manual Integrations
 APPROVED

sohil
 12/28/2016 6:01:46 PM

Quant Time: Dec 28 04:34:36 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 28 03:24:04 2016
 Response via : Initial Calibration

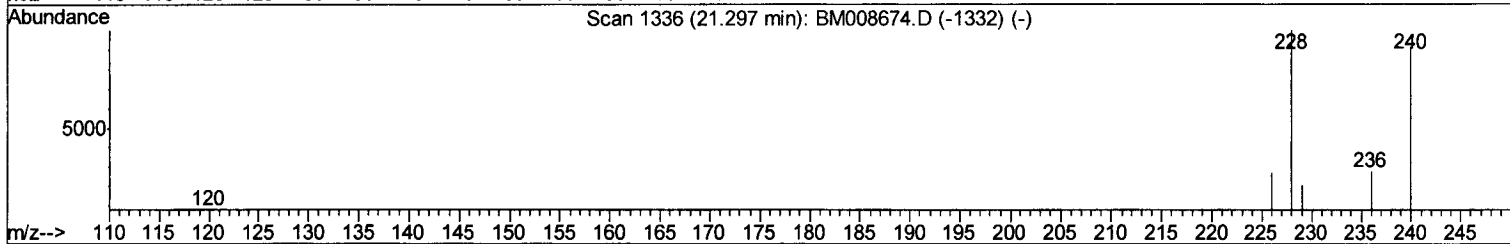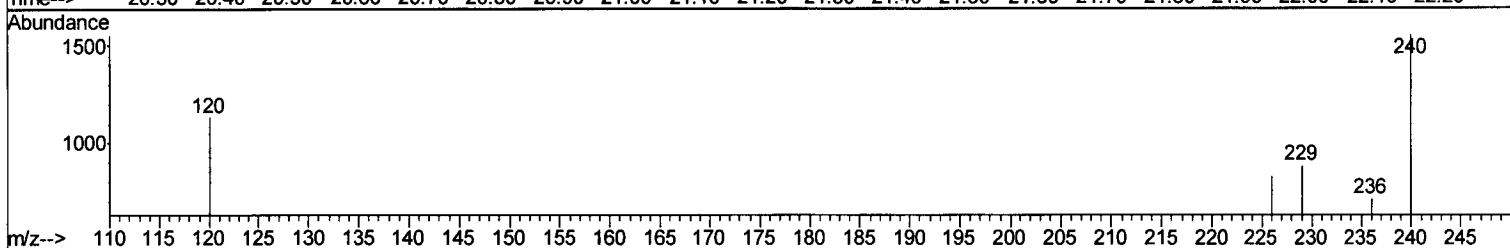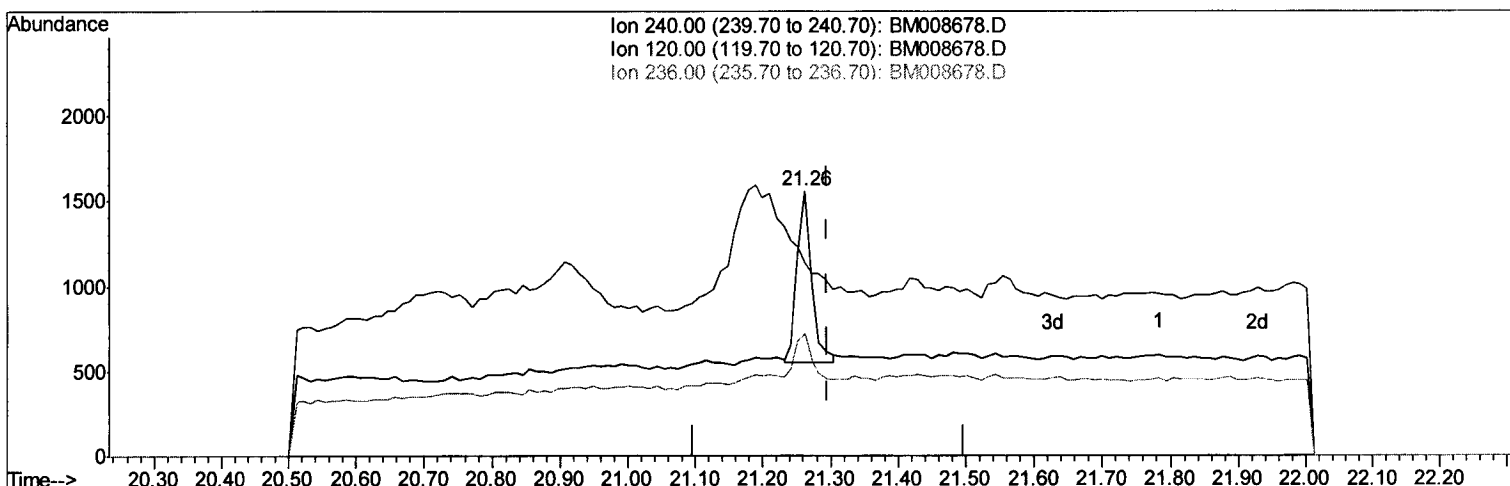

TIC: BM008678.D

(16) Chrysene-d12 (I)

21.262min (-0.035) 0.40ng/ul m

response 1506

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	73.02#
236.00	34.90	45.91#
0.00	0.00	0.00

S. J
 12/29/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122716\
Data File : BM008678.D
Acq On : 27 Dec 2016 18:00
Operator : UM/SJ
Sample : H6040-17DL 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Dec 28 04:34:36 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 28 03:24:04 2016
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampled :
DA8X0DL

Manual Integrations
APPROVED

sohil
12/28/2016 6:01:46 PM

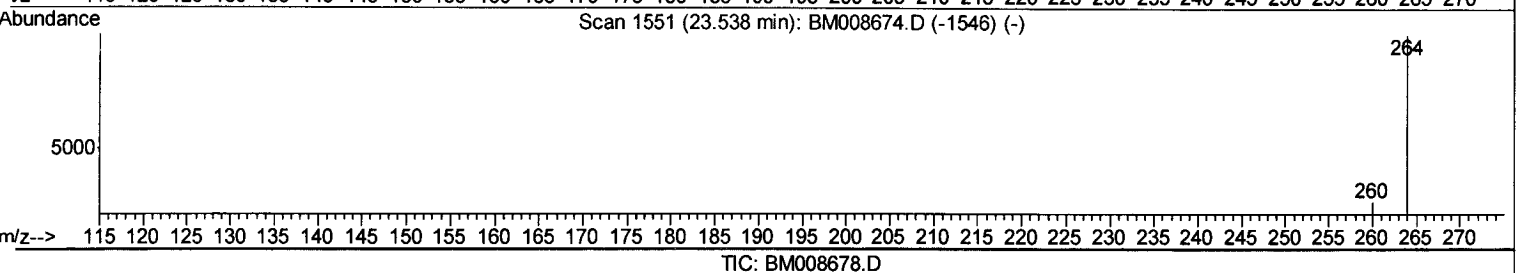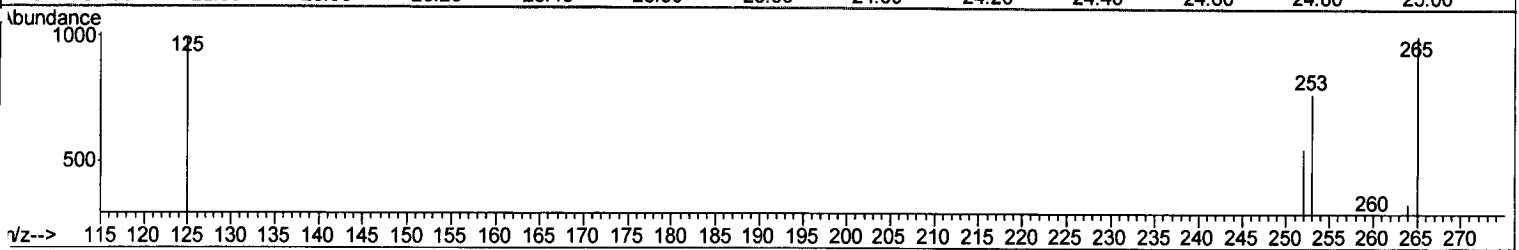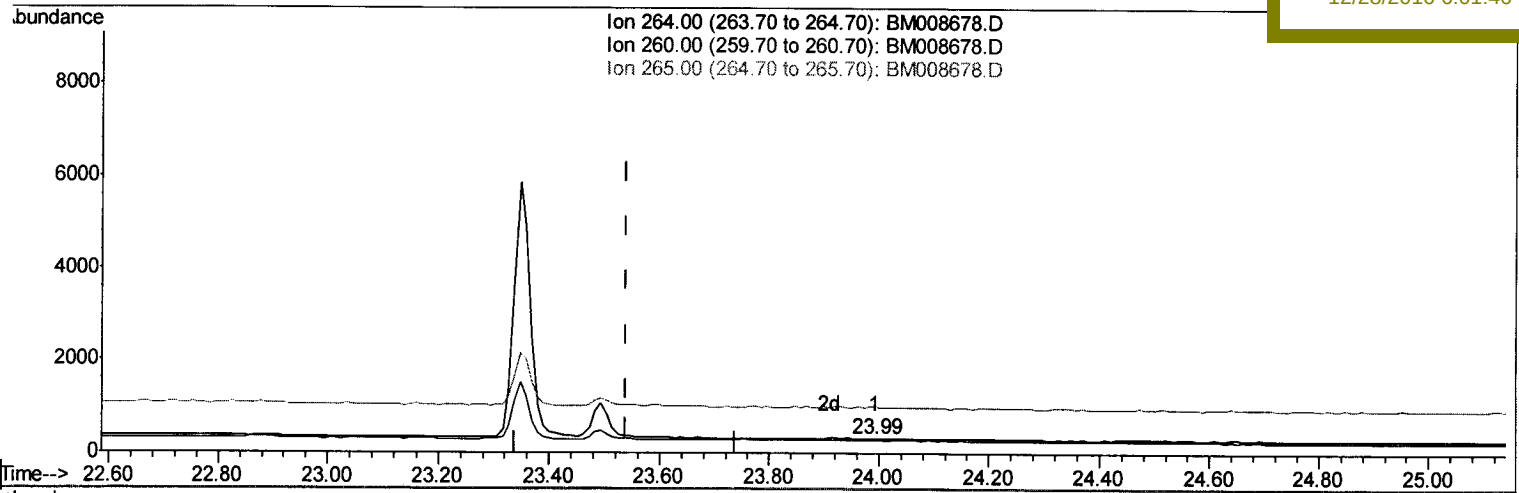

(20) Perylene-d12 (I)

23.993min (+0.455) 0.40ng/ul

response 78

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	88.22#
265.00	103.50	305.74#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122716\
 Data File : BM008678.D
 Acq On : 27 Dec 2016 18:00
 Operator : UM/SJ
 Sample : H6040-17DL 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA8X0DL

Manual Integrations
 APPROVED

sohil
 12/28/2016 6:01:46 PM

Quant Time: Dec 28 04:34:36 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 28 03:24:04 2016
 Response via : Initial Calibration

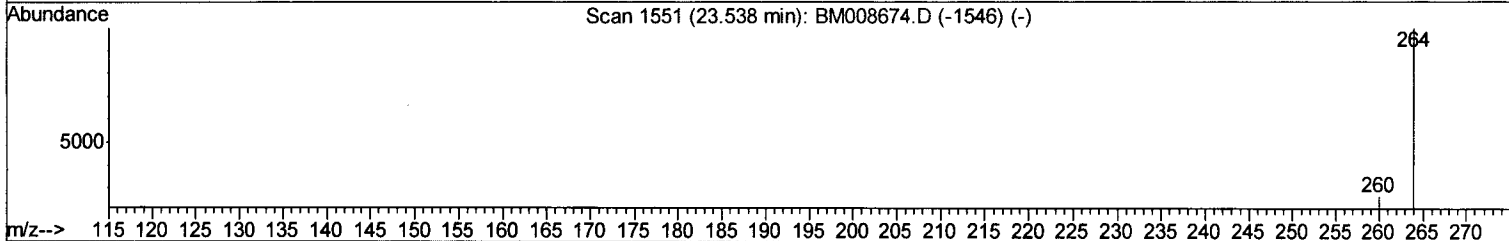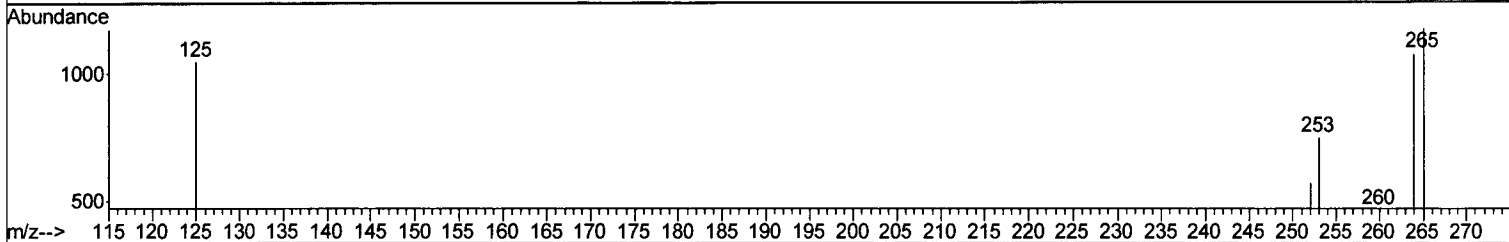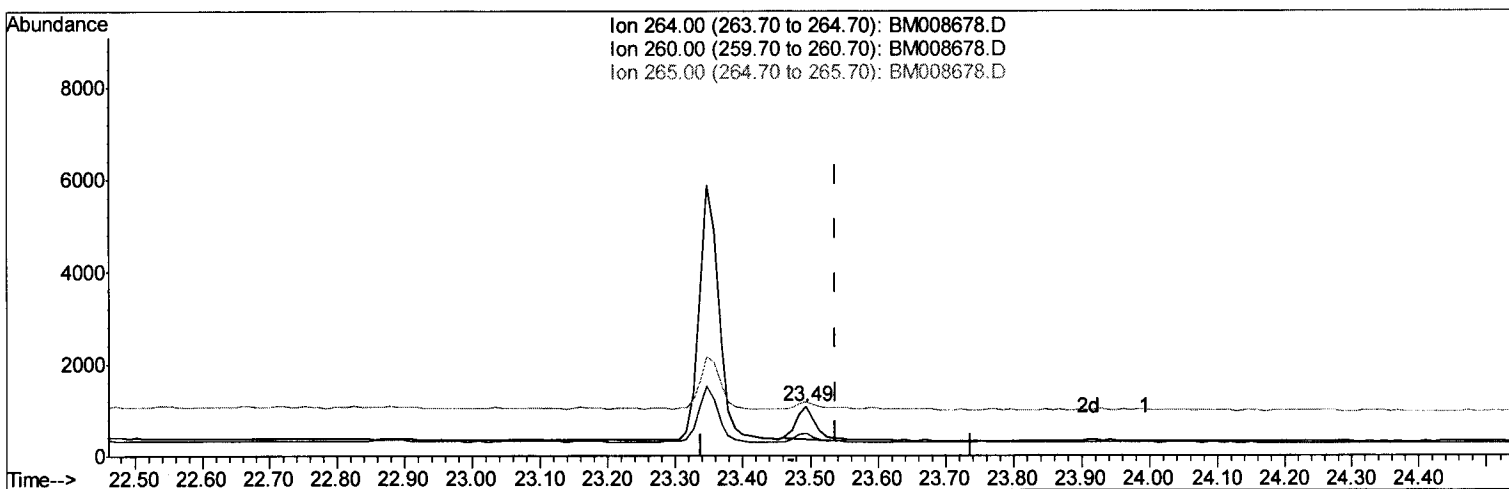

TIC: BM008678.D

(20) Perylene-d12 (I)

23.493min (-0.045) 0.40ng/ul m)

response 1384

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	43.96#
265.00	103.50	109.20
0.00	0.00	0.00

S.J
 12/29/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122716\
 Data File : BM008678.D
 Acq On : 27 Dec 2016 18:00
 Operator : UM/SJ
 Sample : H6040-17DL 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA8X0DL

Quant Time: Dec 28 04:36:16 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 28 03:24:04 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

sohil
 12/28/2016 6:01:46 PM

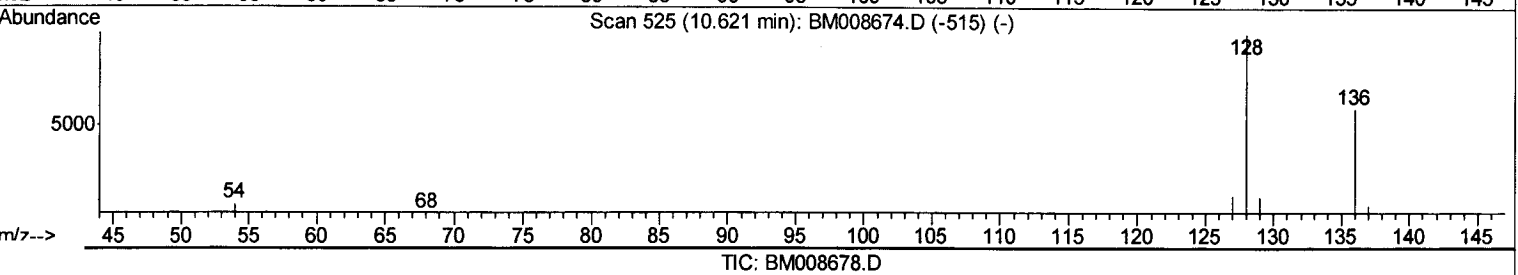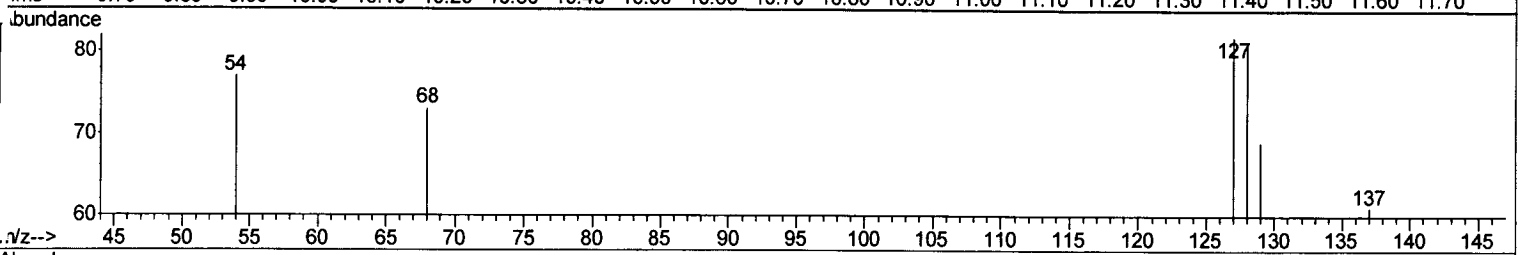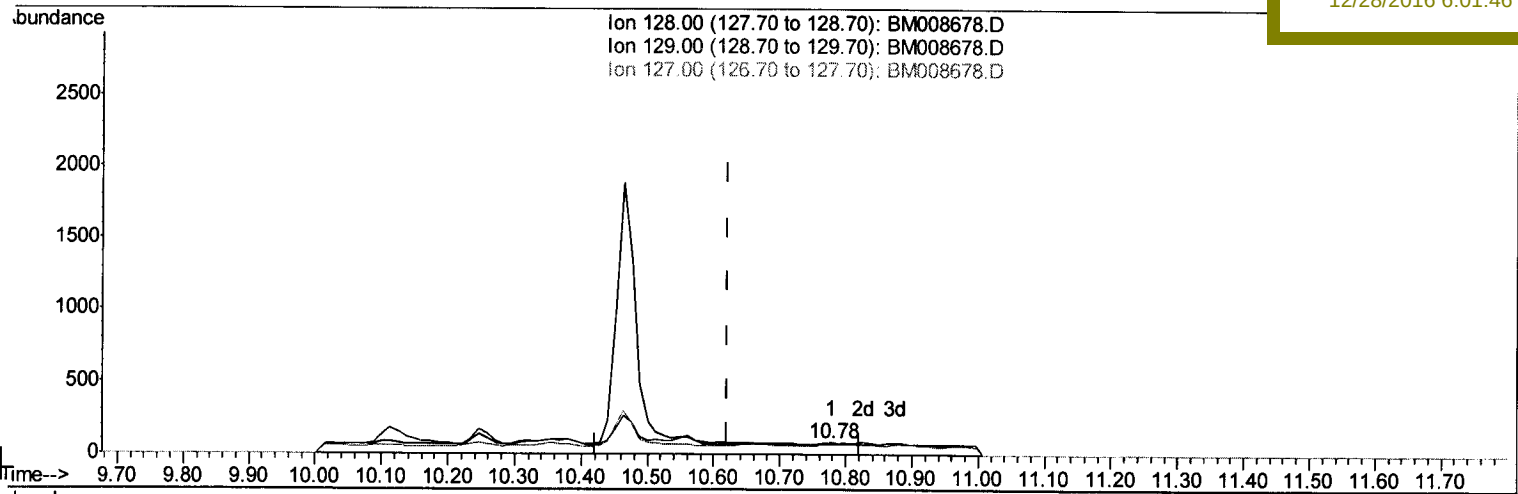

(3) Naphthalene

10.778min (+0.157) 0.01ng/ul

response 23

Ion	Exp%	Act%
128.00	100	100
129.00	14.10	85.19#
127.00	16.00	101.23#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122716\
 Data File : BM008678.D
 Acq On : 27 Dec 2016 18:00
 Operator : UM/SJ
 Sample : H6040-17DL 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA8X0DL

Manual Integrations
 APPROVED

sohil
 12/28/2016 6:01:46 PM

Quant Time: Dec 28 04:36:16 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 28 03:24:04 2016
 Response via : Initial Calibration

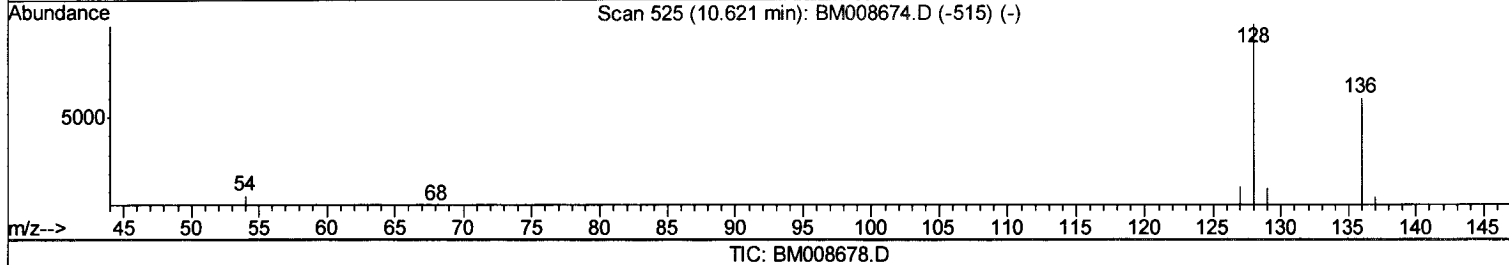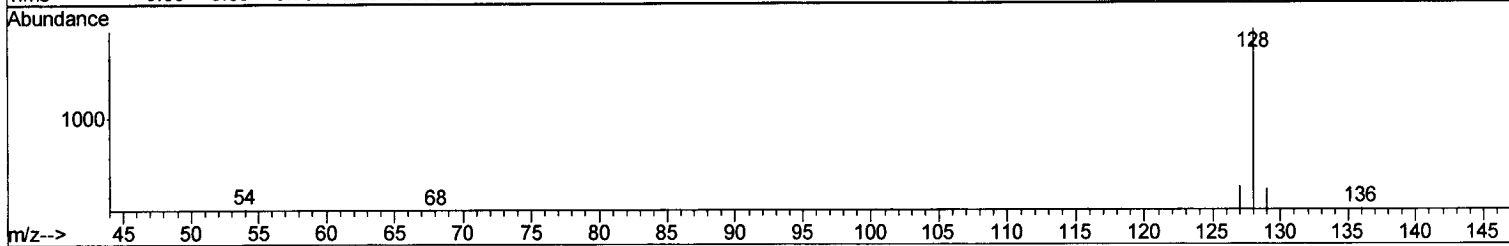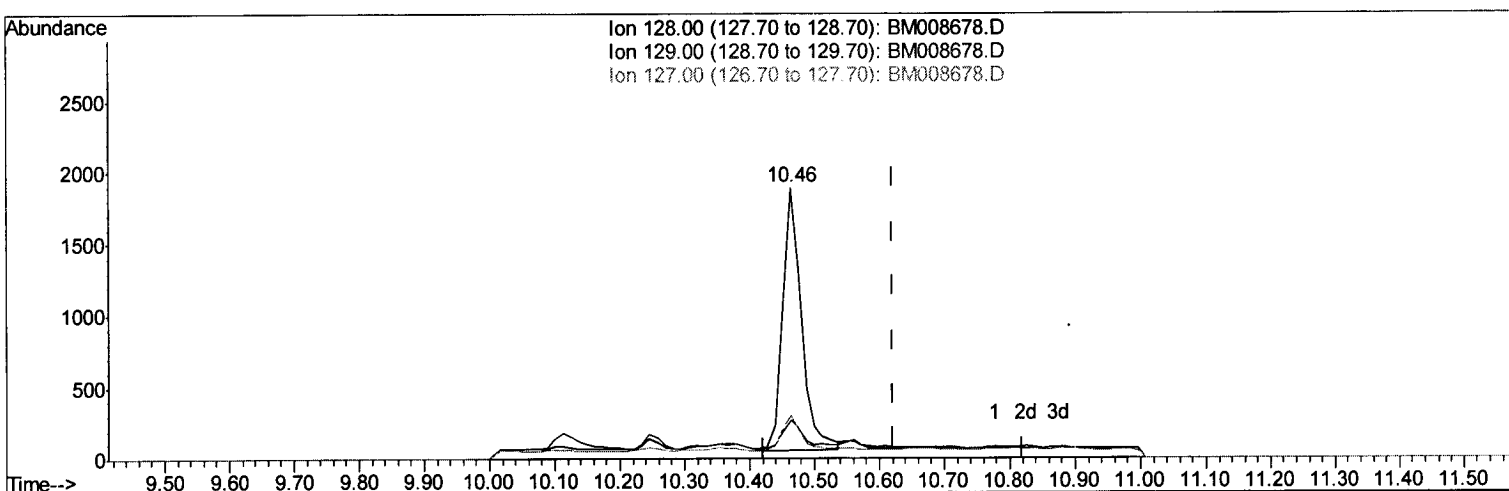

(3) Naphthalene

10.464min (-0.157) 1.08ng/ul m

response 3699

S. J
 12/29/16

Ion	Exp%	Act%
128.00	100	100
129.00	14.10	14.30
127.00	16.00	16.00
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122716\
Data File : BM008678.D
Acq On : 27 Dec 2016 18:00
Operator : UM/SJ
Sample : H6040-17DL 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
Client Sample ID :
DA8X0DL

Quant Time: Dec 28 04:36:16 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 28 03:24:04 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

sohil
12/28/2016 6:01:46 PM

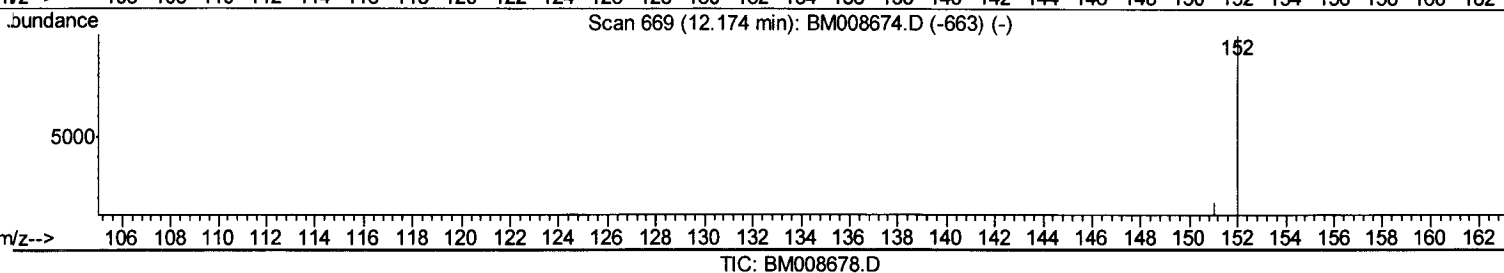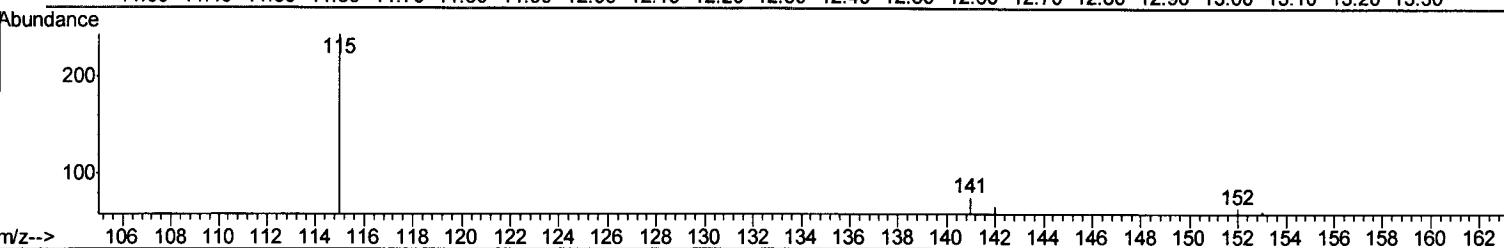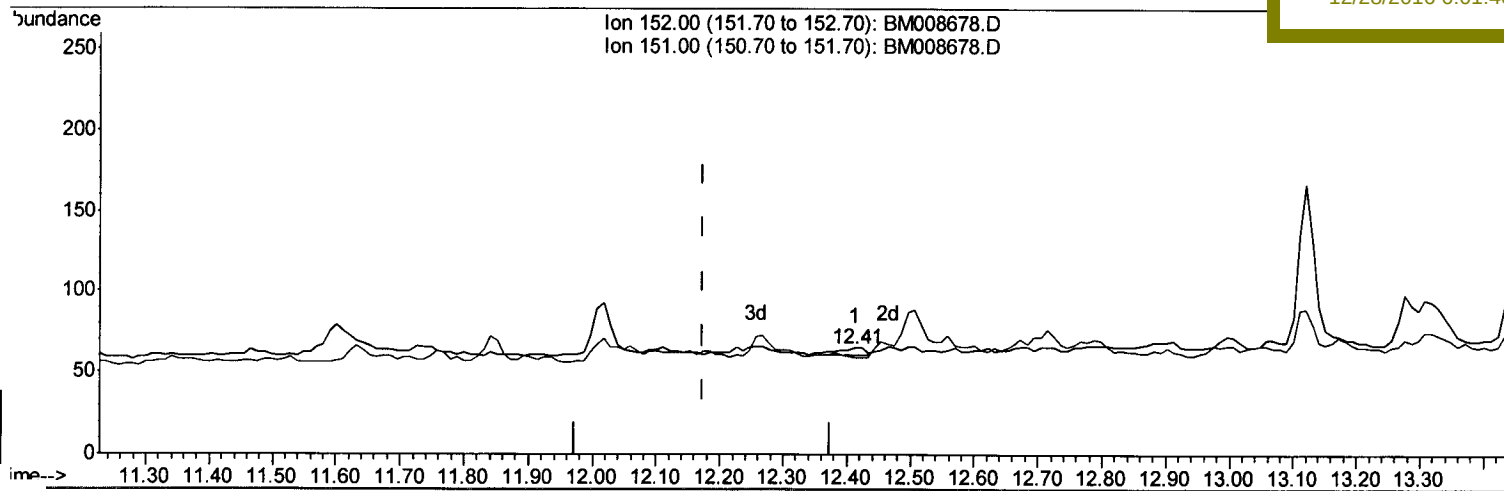

(4) 2-Methylnaphthalene-d10 (SURR)

12.413min (+0.239) 0.01ng/ul

response 13

Ion	Exp%	Act%
152.00	100	100
151.00	19.30	0.00#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122716\
 Data File : BM008678.D
 Acq On : 27 Dec 2016 18:00
 Operator : UM/SJ
 Sample : H6040-17DL 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleID :
 DA8X0DL

Manual Integrations
 APPROVED

sohil
 12/28/2016 6:01:46 PM

Quant Time: Dec 28 04:36:16 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 28 03:24:04 2016
 Response via : Initial Calibration

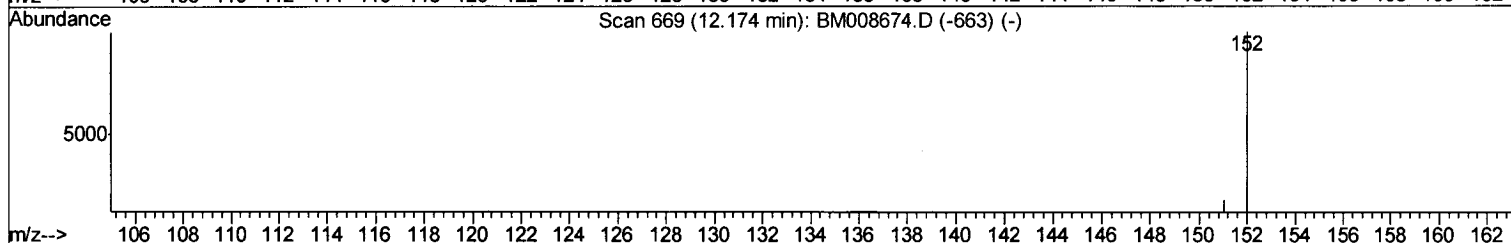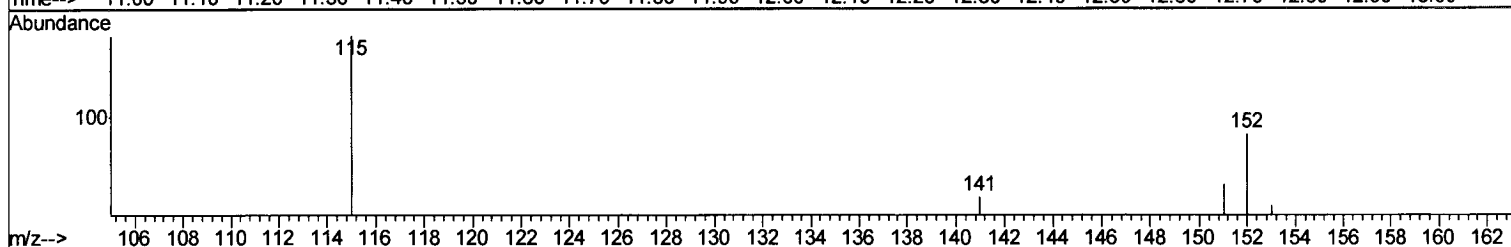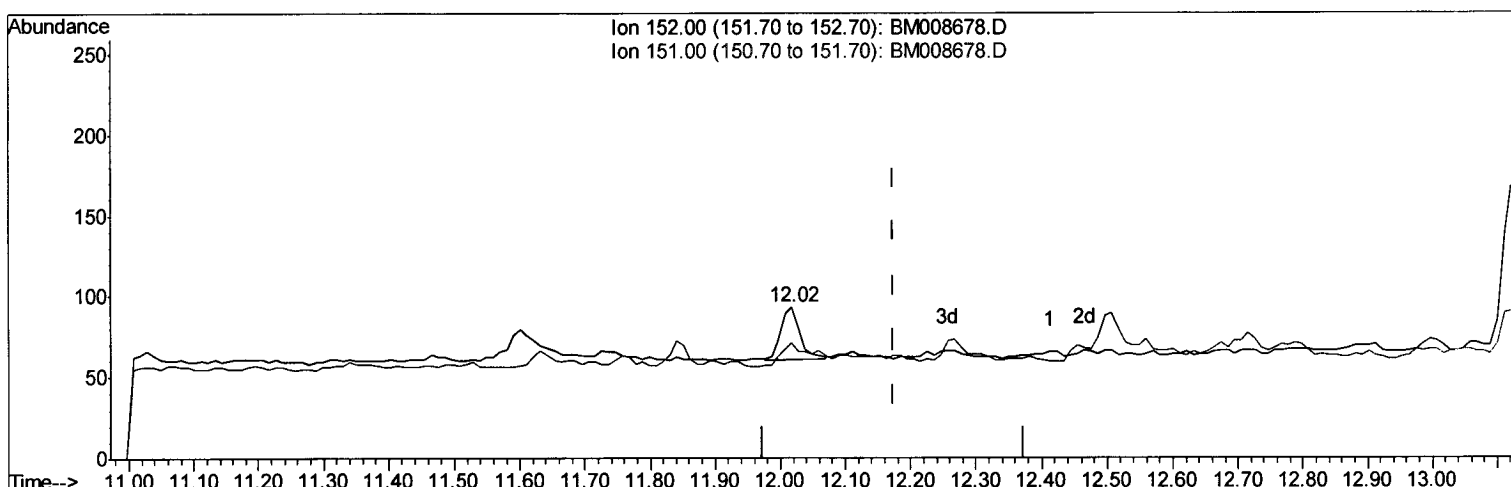

(4) 2-Methylnaphthalene-d10 (SURR)

12.018min (-0.156) 0.04ng/ul m

response 69

Ion	Exp%	Act%
152.00	100	100
151.00	19.30	0.00#
0.00	0.00	0.00
0.00	0.00	0.00

S. J
 12/29/16




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122716\
Data File : BM008678.D
Acq On : 27 Dec 2016 18:00
Operator : UM/SJ
Sample : H6040-17DL 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Dec 28 04:36:16 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 28 03:24:04 2016
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
DA8X0DL

Manual Integrations
APPROVED

sohil
12/28/2016 6:01:46 PM

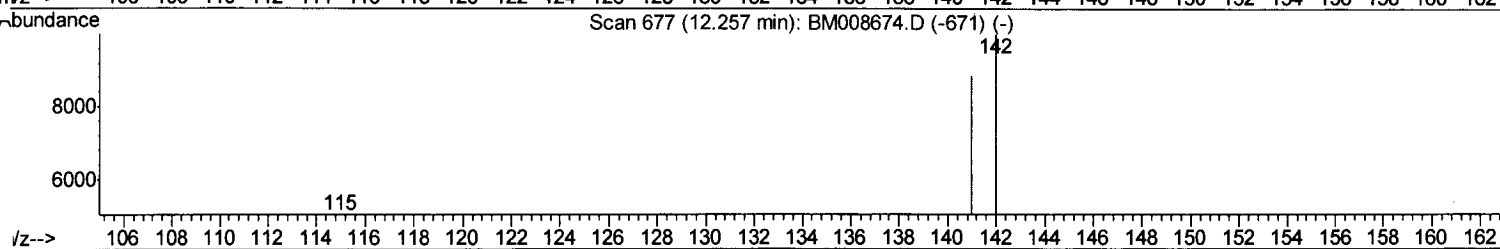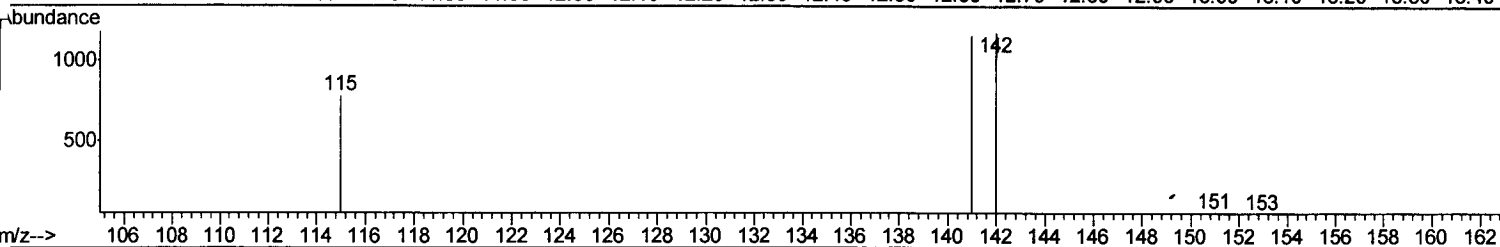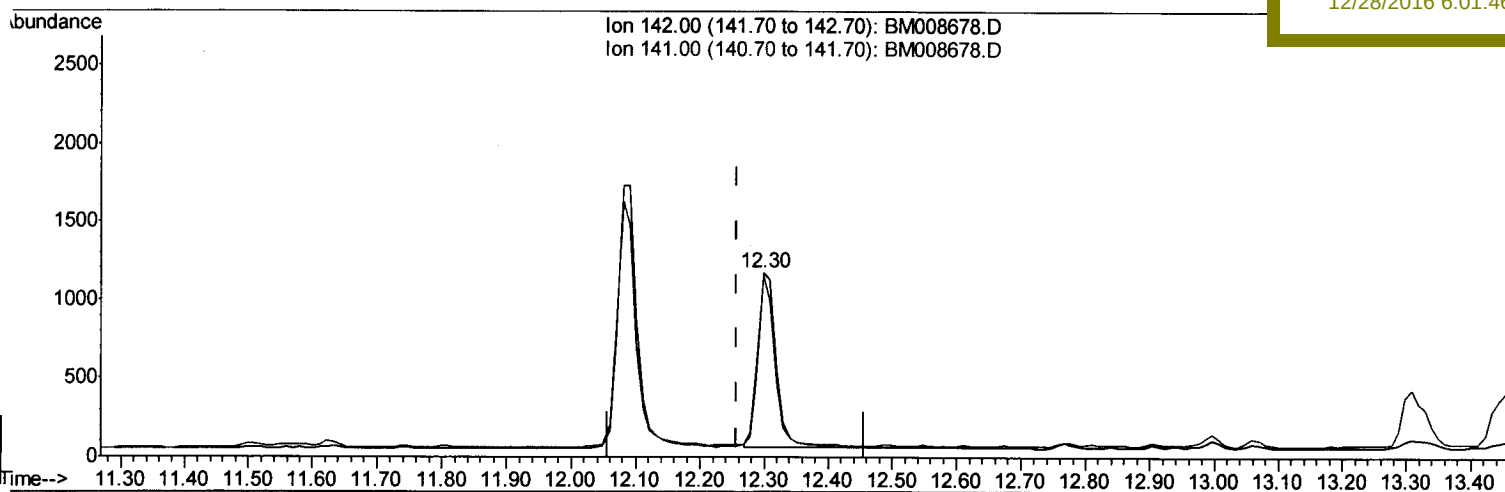

TIC: BM008678.D

(5) 2-Methylnaphthalene

12.299min (+0.042) 0.95ng/ul

response 2185

Ion	Exp%	Act%
142.00	100	100
141.00	90.70	93.64
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122716\
 Data File : BM008678.D
 Acq On : 27 Dec 2016 18:00
 Operator : UM/SJ
 Sample : H6040-17DL 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleID :
 DA8X0DL

Manual Integrations
 APPROVED

sohil
 12/28/2016 6:01:46 PM

Quant Time: Dec 28 04:36:16 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 28 03:24:04 2016
 Response via : Initial Calibration

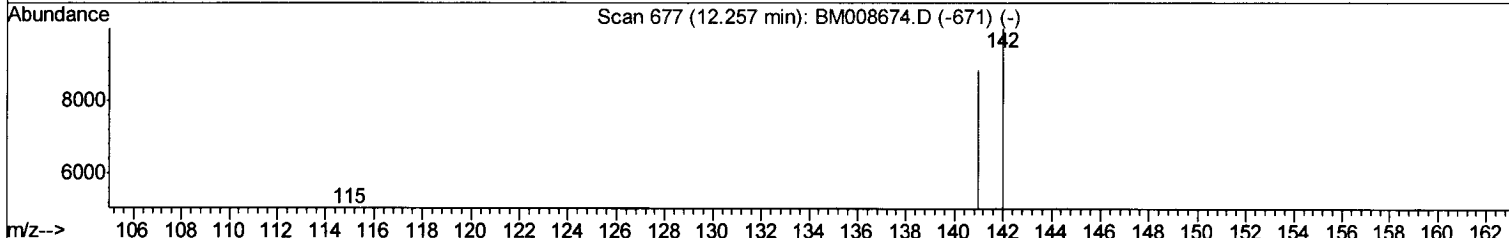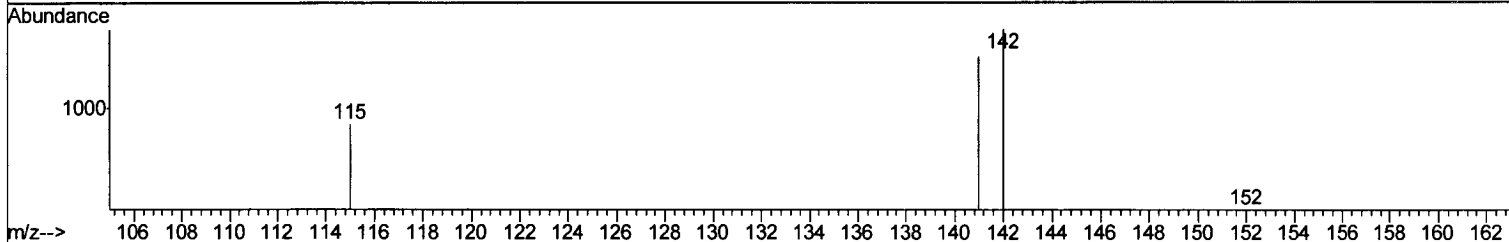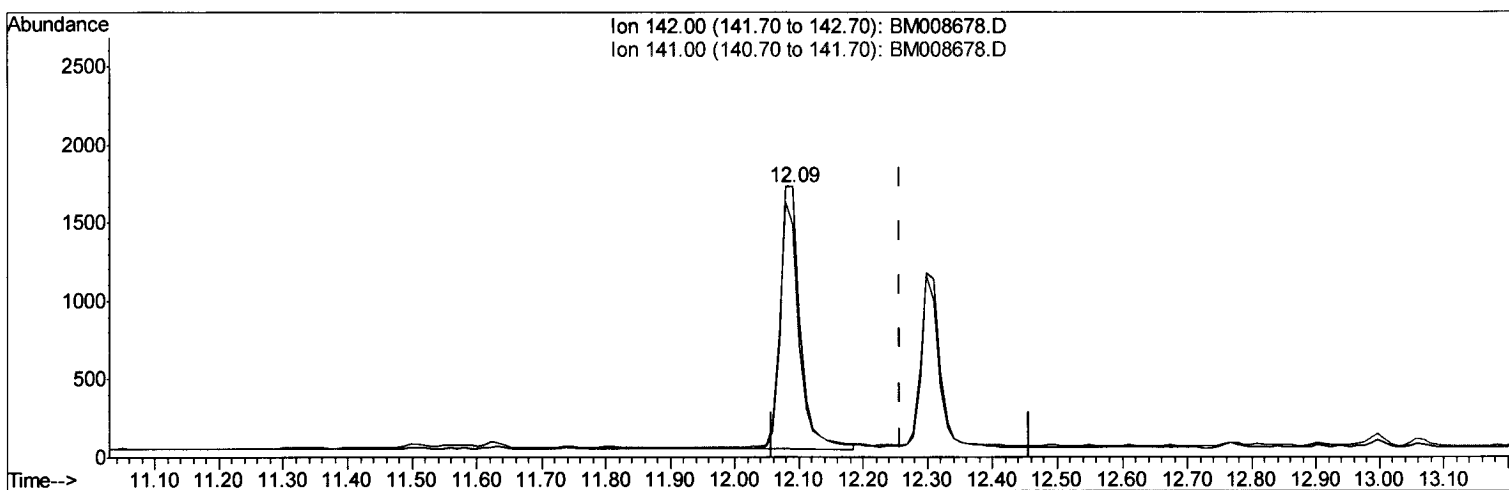

(5) 2-Methylnaphthalene

12.091min (-0.166) 1.54ng/ul m

response 3553

Ion	Exp%	Act%
142.00	100	100
141.00	90.70	57.59#
0.00	0.00	0.00
0.00	0.00	0.00

S. J
 12/29/16




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122716\
Data File : BM008678.D
Acq On : 27 Dec 2016 18:00
Operator : UM/SJ
Sample : H6040-17DL 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA8X0DL

Quant Time: Dec 28 04:36:16 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 28 03:24:04 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

sohil
12/28/2016 6:01:46 PM

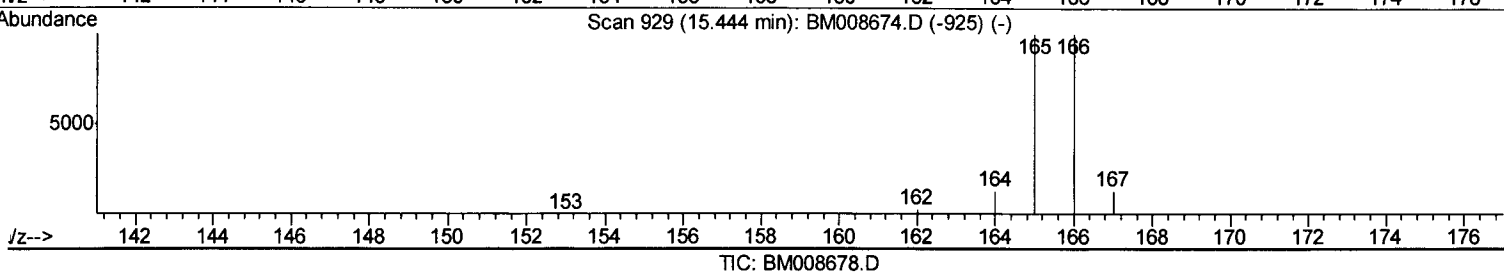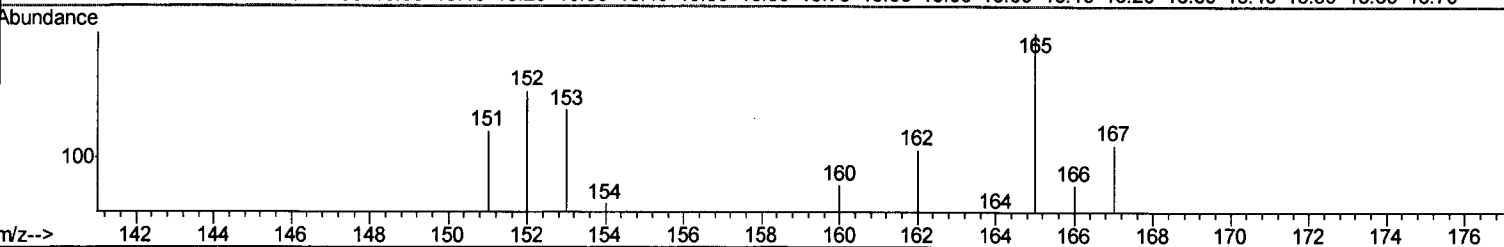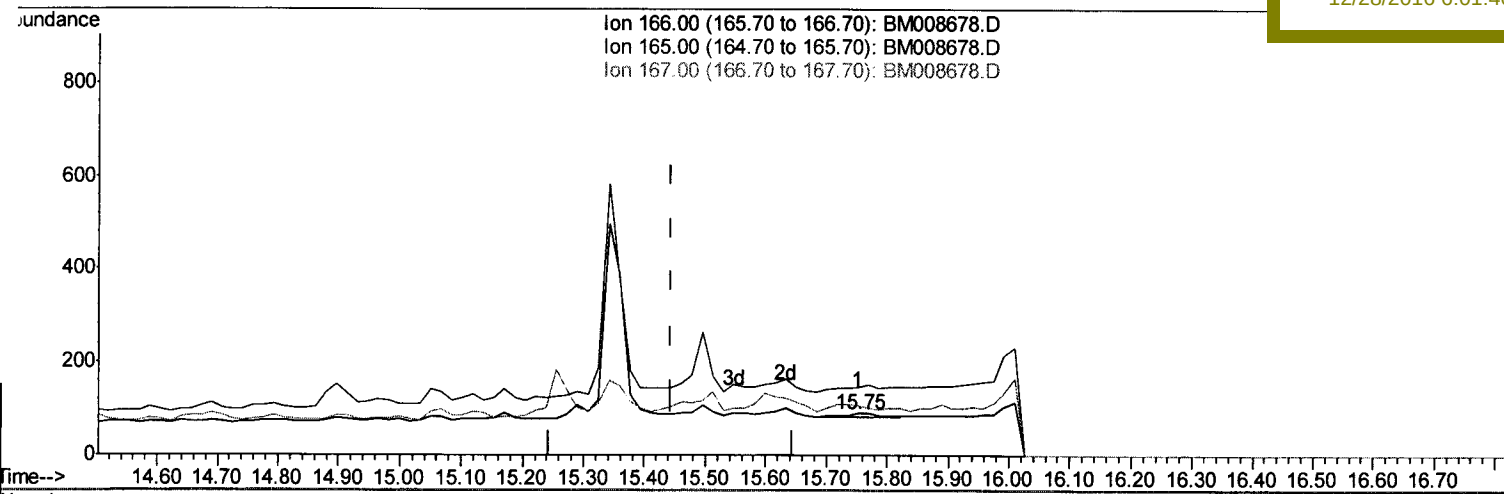

(9) Fluorene

15.753min (+0.308) 0.01ng/ul

response 27

Ion	Exp%	Act%
166.00	100	100
165.00	91.80	163.33#
167.00	18.30	116.67#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122716\
 Data File : BM008678.D
 Acq On : 27 Dec 2016 18:00
 Operator : UM/SJ
 Sample : H6040-17DL 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA8X0DL

Manual Integrations
 APPROVED

sohil
 12/28/2016 6:01:46 PM

Quant Time: Dec 28 04:36:16 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 28 03:24:04 2016
 Response via : Initial Calibration

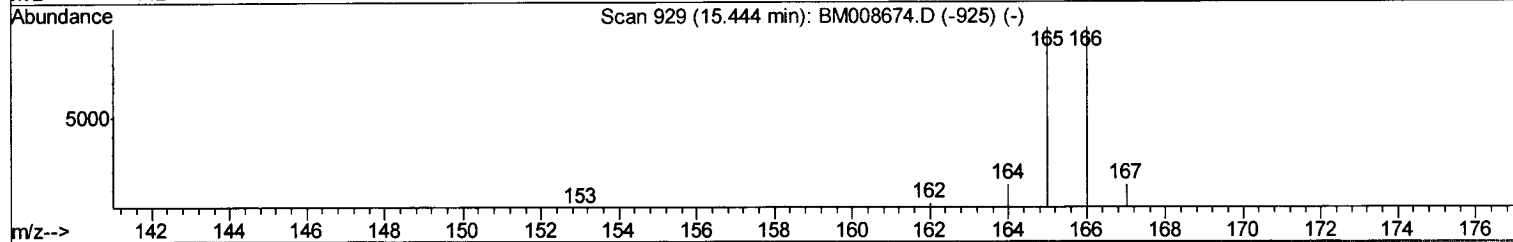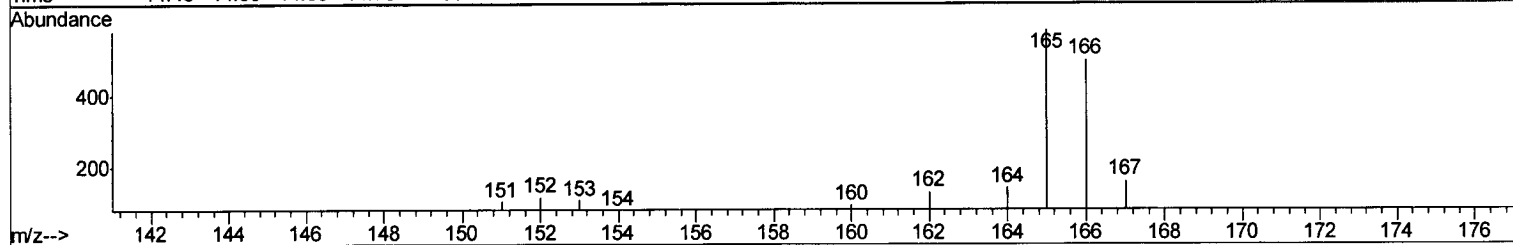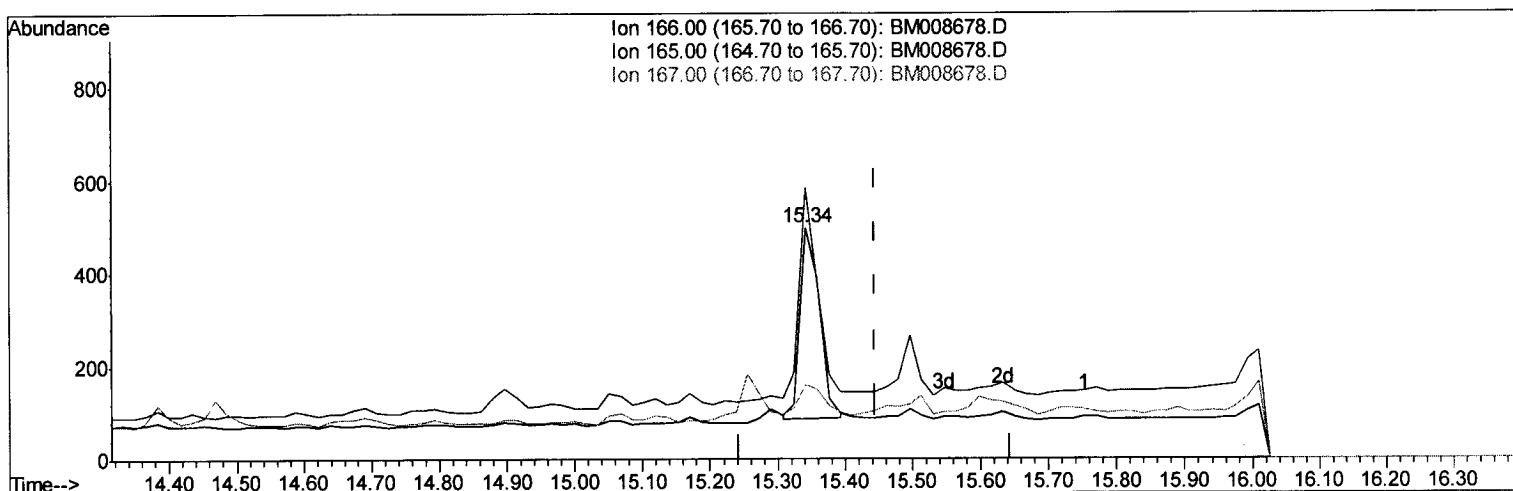

TIC: BM008678.D

(9) Fluorene

15.342min (-0.103) 0.28ng/ul m)

response 822

Ion	Exp%	Act%
166.00	100	100
165.00	91.80	117.30#
167.00	18.30	31.79#
0.00	0.00	0.00

S. J
 12/29/16




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122716\
Data File : BM008678.D
Acq On : 27 Dec 2016 18:00
Operator : UM/SJ
Sample : H6040-17DL 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA8X0DL

Manual Integrations
APPROVED

sohil
12/28/2016 6:01:46 PM

Quant Time: Dec 28 04:36:16 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 28 03:24:04 2016
Response via : Initial Calibration

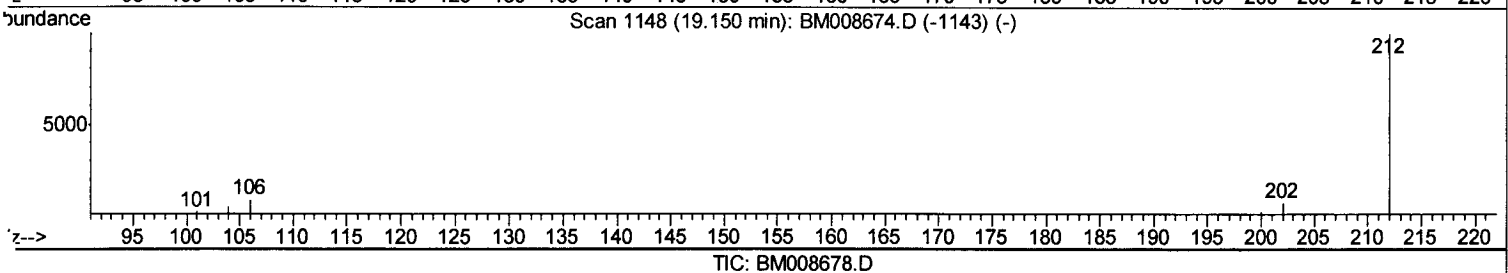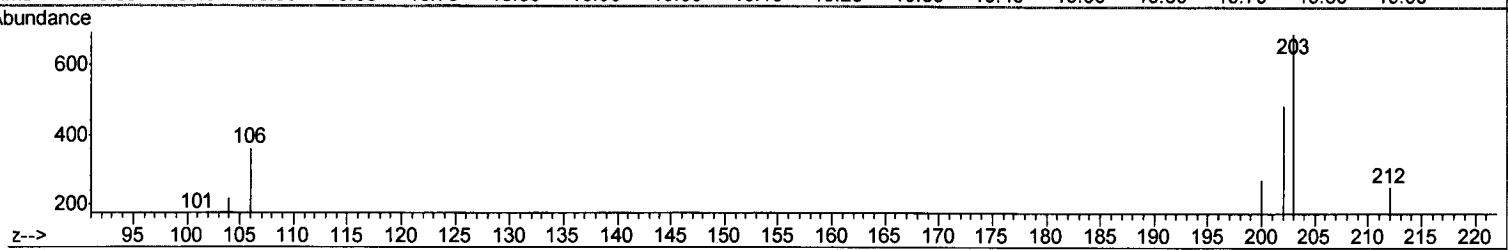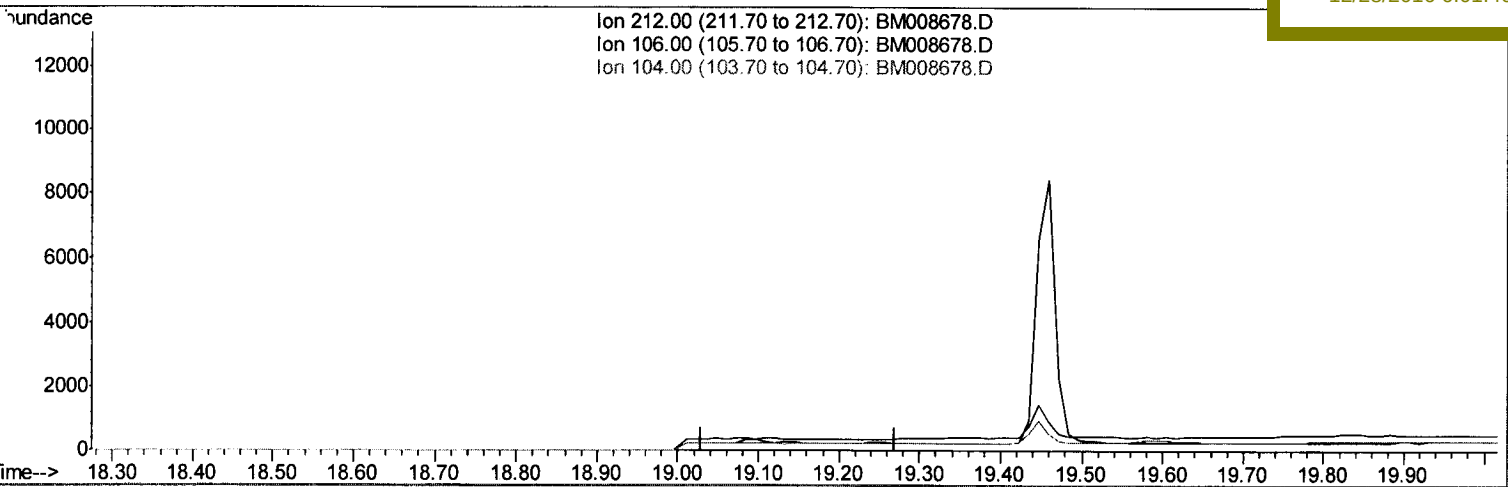

(14) Fluoranthene-d10 (SURR)

19.150min (-19.150) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122716\
 Data File : BM008678.D
 Acq On : 27 Dec 2016 18:00
 Operator : UM/SJ
 Sample : H6040-17DL 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA8X0DL

Manual Integrations
 APPROVED

sohil
 12/28/2016 6:01:46 PM

Quant Time: Dec 28 04:36:16 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 28 03:24:04 2016
 Response via : Initial Calibration

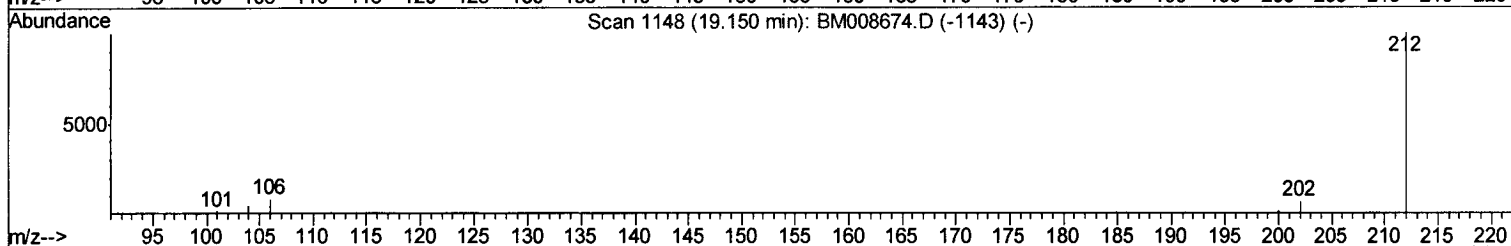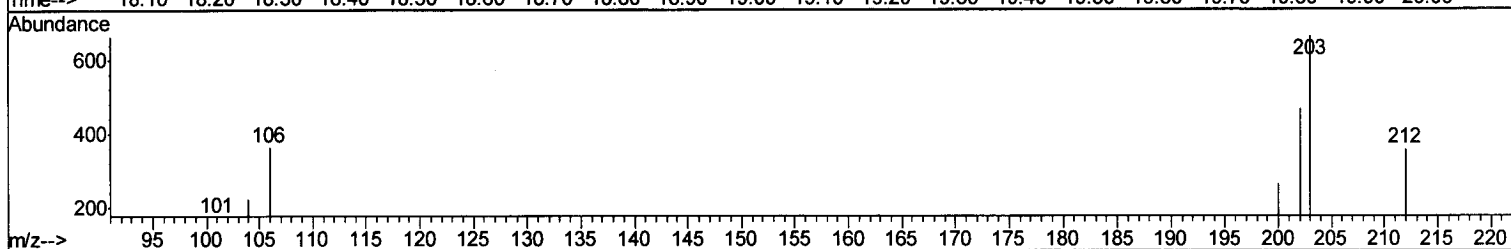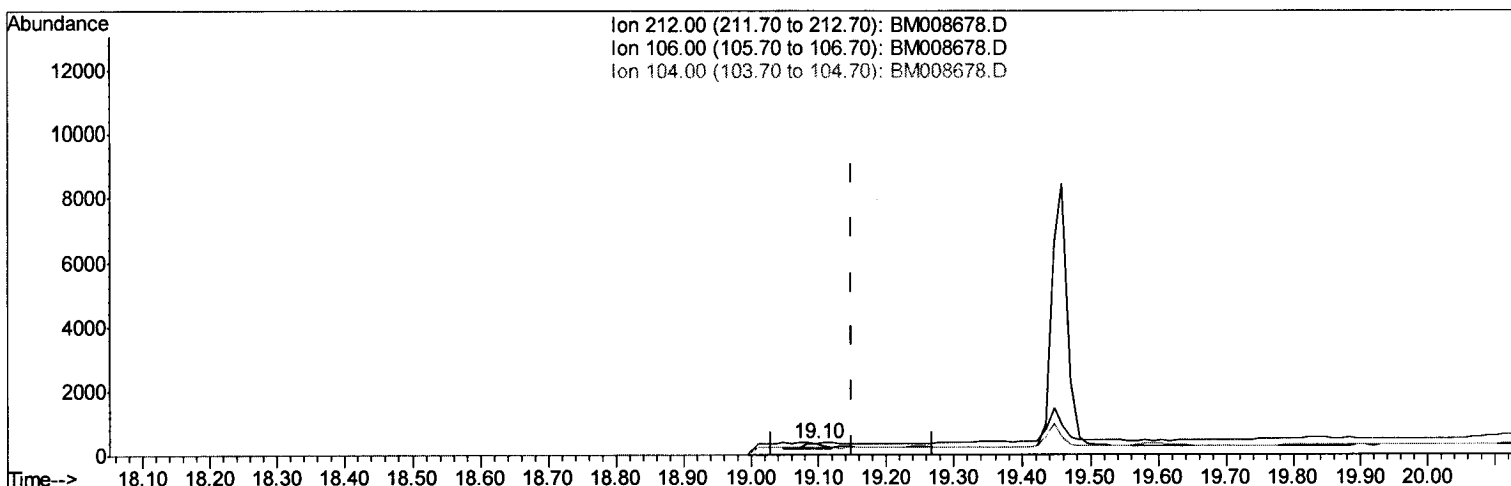

TIC: BM008678.D

(14) Fluoranthene-d10 (SURR)

19.096min (-0.053) 0.07ng/ul m

response 310

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

S.J
 12/29/16

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122716\
 Data File : BM008678.D
 Acq On : 27 Dec 2016 18:00
 Operator : UM/SJ
 Sample : H6040-17DL 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA8X0DL

Manual Integrations
 APPROVED

sohil
 12/28/2016 6:01:46 PM

Quant Time: Dec 28 04:37:58 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 28 03:24:04 2016
 Response via : Initial Calibration

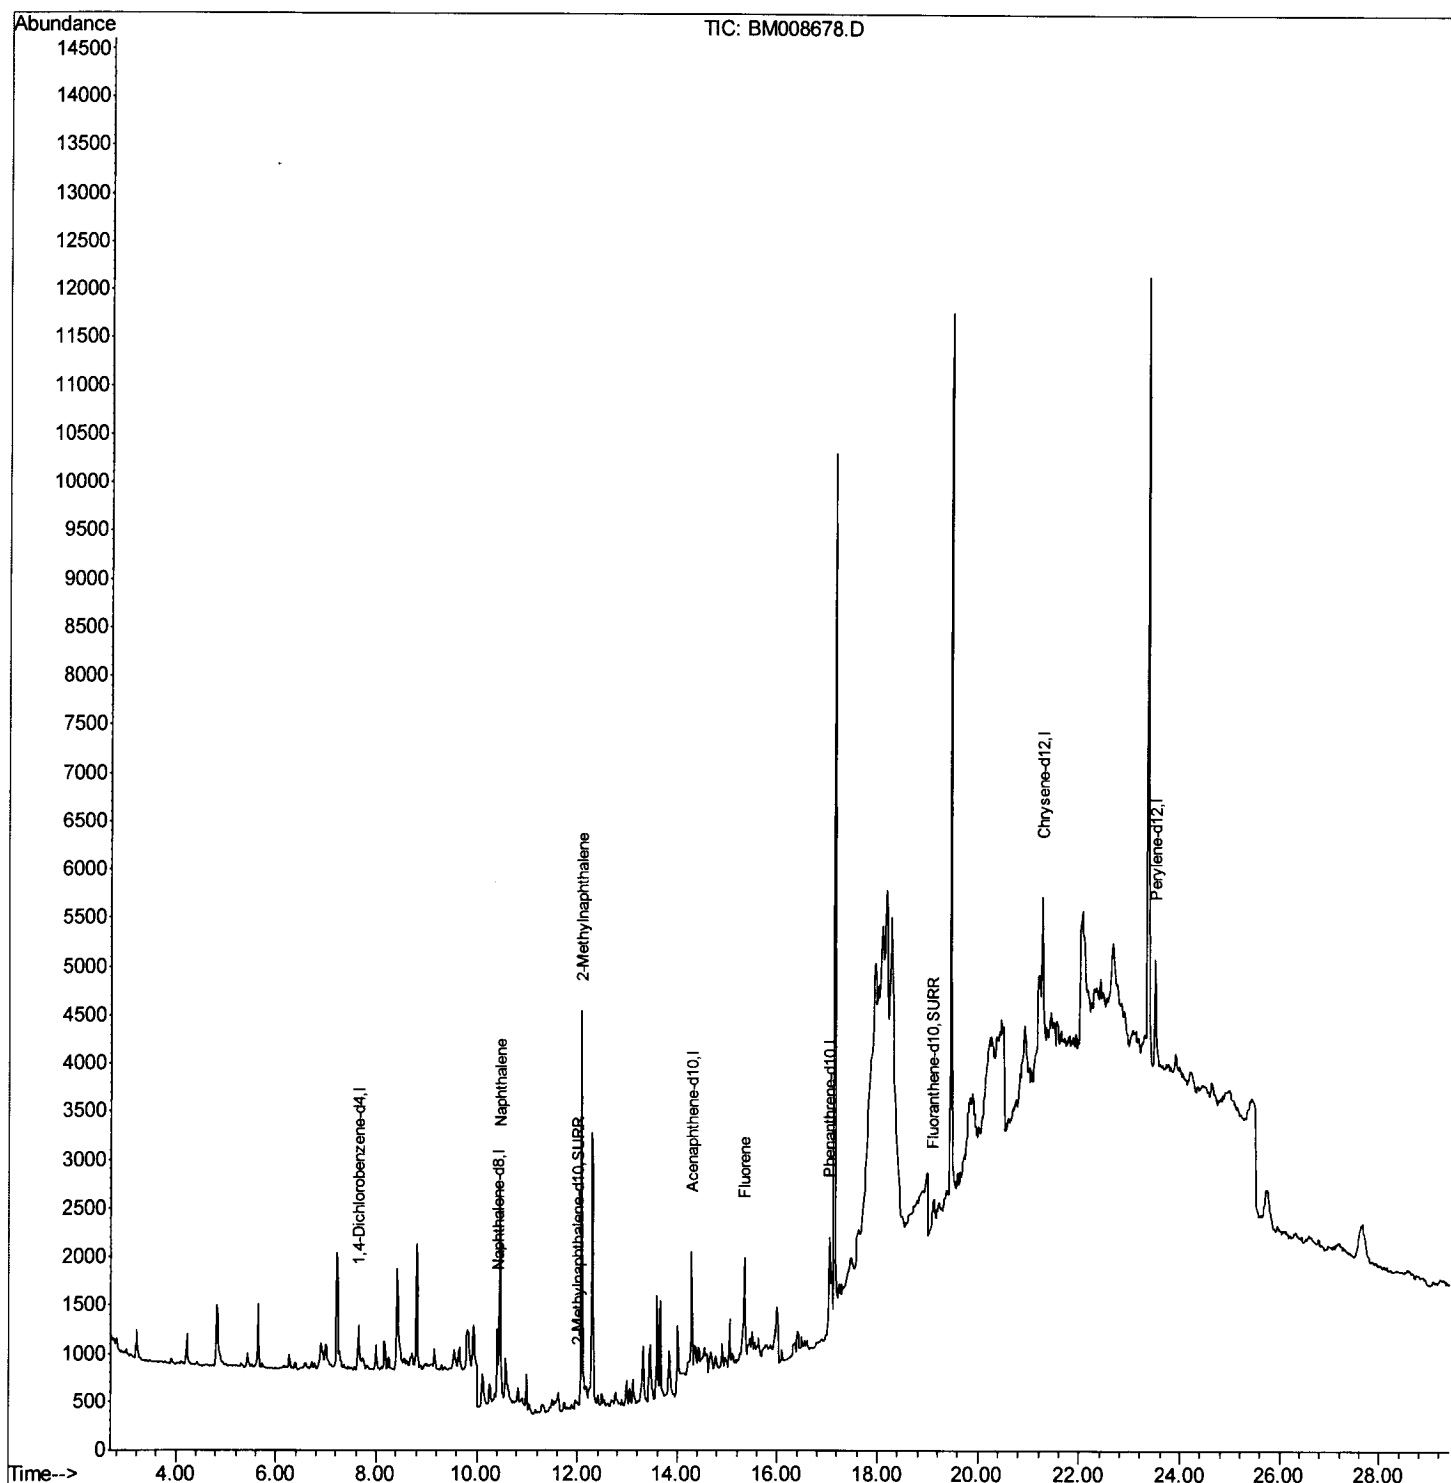

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122716\
 Data File : BM008678.D
 Acq On : 27 Dec 2016 18:00
 Operator : UM/SJ
 Sample : H6040-17DL 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA8X0DL

Manual Integrations
 APPROVED

sohil
 12/28/2016 6:01:46 PM

Quant Time: Dec 28 04:37:58 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 28 03:24:04 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	366m	0.40	ng/ul	-0.19
2) Naphthalene-d8	10.42	136	1219m	0.40	ng/ul	-0.16
6) Acenaphthene-d10	14.28	164	764m	0.40	ng/ul	-0.07
10) Phenanthrene-d10	17.04	188	1605m	0.40	ng/ul	-0.09
16) Chrysene-d12	21.26	240	1506m	0.40	ng/ul	-0.03
20) Perylene-d12	23.49	264	1384m	0.40	ng/ul	-0.05
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	69m	0.04	ng/ul	-0.16
14) Fluoranthene-d10	19.10	212	310m	0.07	ng/ul	-0.05
Target Compounds						
3) Naphthalene	10.46	128	3699m	1.08	ng/ul	Qvalue
5) 2-Methylnaphthalene	12.09	142	3553m	1.54	ng/ul	
9) Fluorene	15.34	166	822m	0.28	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed