

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122717\
 Data File : BM013550.D
 Acq On : 27 Dec 2017 10:27
 Operator : SJ/JU
 Sample : PB105321BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK21

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.216	20	22	27	rVB2	36063	43053	1.09%	0.098%
2	6.845	634	639	654	rVB	767499	1266546	31.96%	2.870%
3	7.010	661	667	676	rBV	604902	923448	23.30%	2.092%
4	7.204	693	700	709	rVB	797636	1293330	32.64%	2.931%
5	7.669	773	779	786	rVB	585443	955701	24.12%	2.166%
6	8.375	892	899	908	rBV	1031680	1671996	42.19%	3.789%
7	8.822	967	975	983	rBV	874281	1425714	35.98%	3.231%
8	9.539	1088	1097	1107	rBV	692466	1200307	30.29%	2.720%
9	10.075	1180	1188	1199	rBV	1047184	1807532	45.61%	4.096%
10	10.445	1243	1251	1258	rVB	859735	1446672	36.51%	3.278%
11	10.592	1268	1276	1290	rBV	939889	1719758	43.40%	3.897%
12	13.727	1802	1809	1819	rBV	1950579	2687760	67.83%	6.090%
13	13.998	1848	1855	1864	rBV	2151508	3252351	82.07%	7.370%
14	14.310	1901	1908	1916	rBV2	1275882	1947707	49.15%	4.413%
15	14.533	1940	1946	1963	rBV2	497511	1003581	25.33%	2.274%
16	15.309	2071	2078	2090	rBV	2741771	3848189	97.11%	8.720%
17	15.439	2094	2100	2111	rVV	493603	790154	19.94%	1.790%
18	15.545	2113	2118	2123	rVB3	27360	41020	1.04%	0.093%
19	17.062	2369	2376	2384	rBV2	1517229	2233398	56.36%	5.061%
20	17.156	2384	2392	2400	rBV2	2702657	3884138	98.02%	8.801%
21	19.456	2777	2783	2792	rBV	2938773	3962774	100.00%	8.979%
22	21.174	3072	3075	3078	rVB2	49908	47806	1.21%	0.108%
23	21.250	3083	3088	3097	rBV	1501004	1967245	49.64%	4.458%
24	23.333	3435	3442	3451	rBV2	1609117	3104609	78.34%	7.035%
25	23.474	3459	3466	3476	rVB	823303	1606882	40.55%	3.641%


Sum of corrected areas: 44131671

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122717\
Data File : BM013550.D
Acq On : 27 Dec 2017 10:27
Operator : SJ/JU
Sample : PB105321BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
SBLK21

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

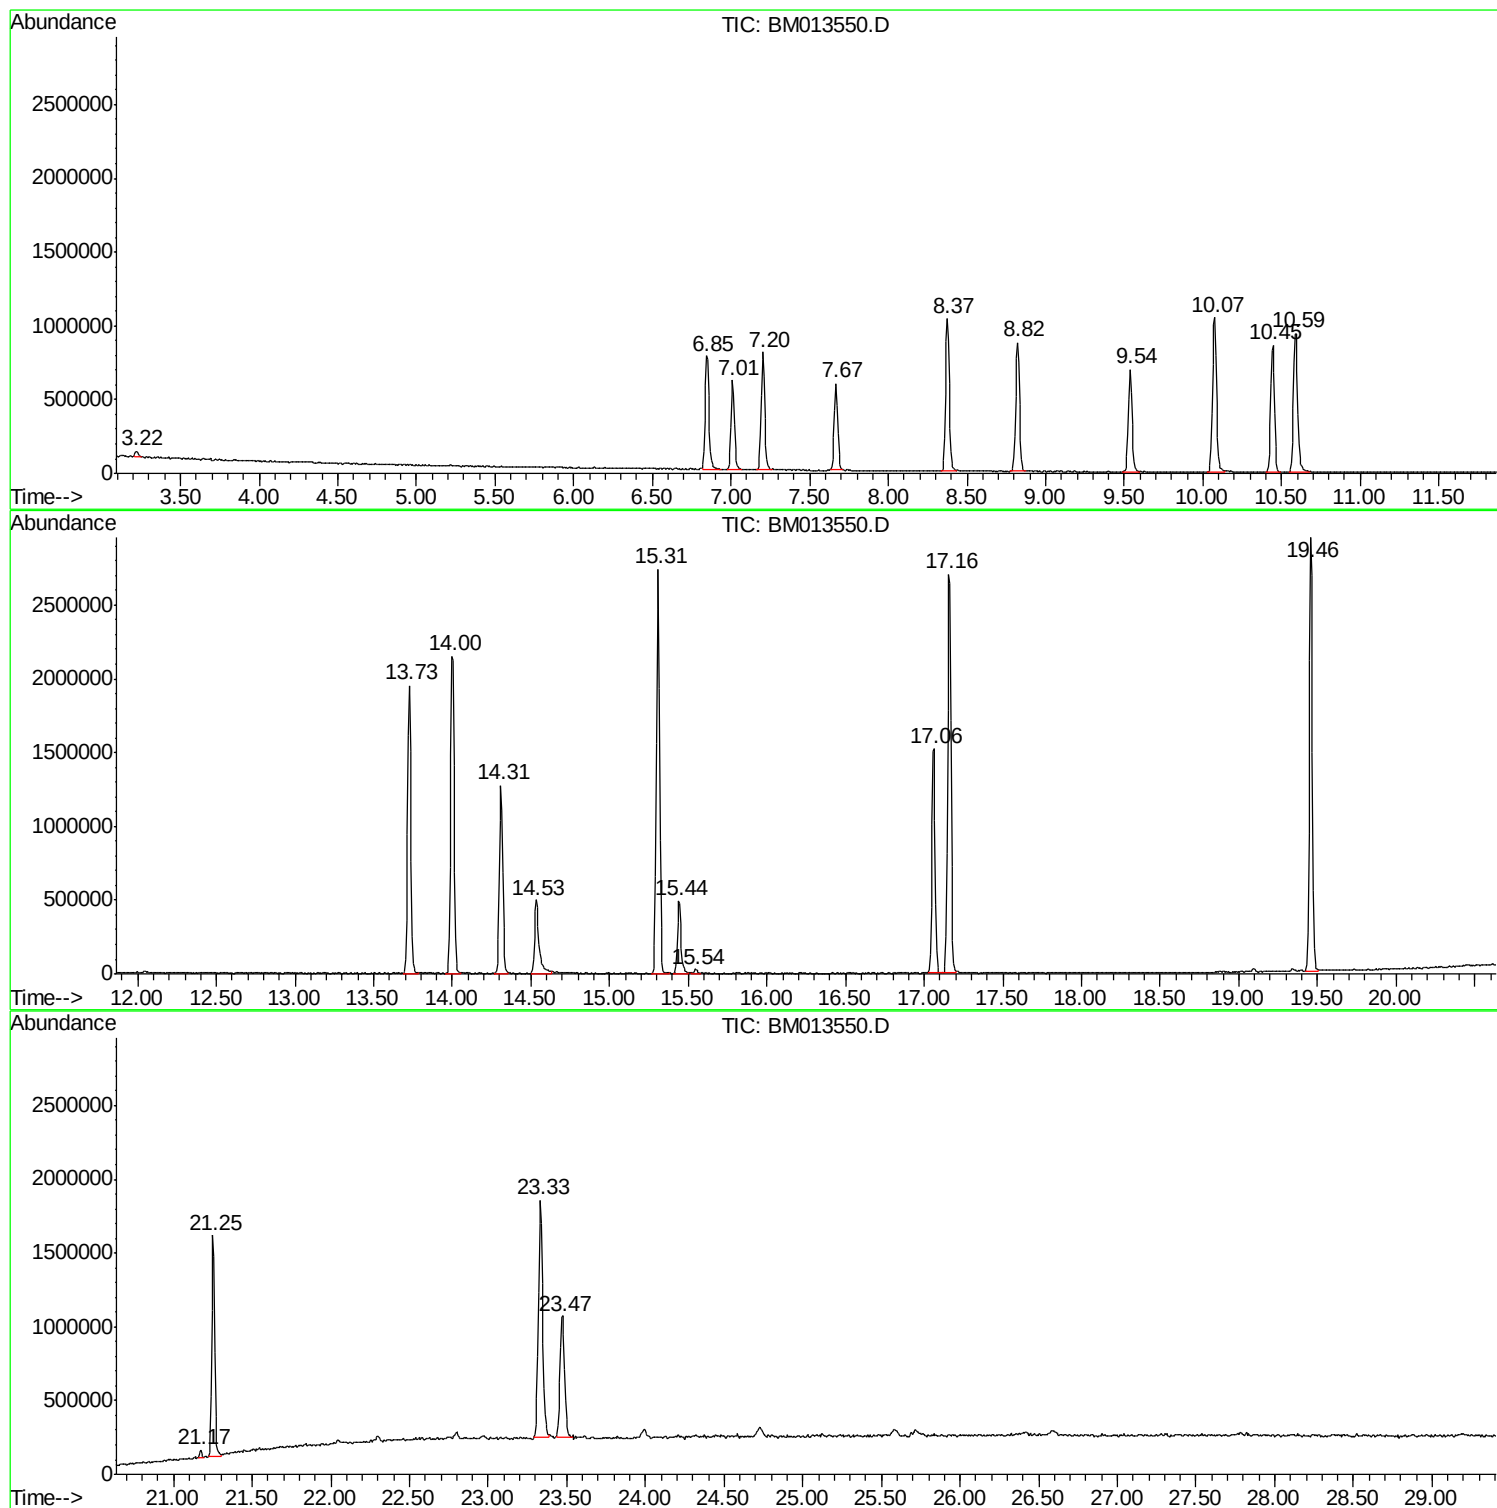

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122717\
Data File : BM013550.D
Acq On : 27 Dec 2017 10:27
Operator : SJ/JU
Sample : PB105321BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK21

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122717\
Data File : BM013550.D
Acq On : 27 Dec 2017 10:27
Operator : SJ/JU
Sample : PB105321BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK21

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc