

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM122719\
 Data File : BM024339.D
 Acq On : 27 Dec 2019 22:44
 Operator : JU
 Sample : K6281-06
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFQX4

Quant Time: Dec 27 23:55:18 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 27 23:52:10 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.42	152	223408	20.00	ng/ul	0.00
18) Naphthalene-d8	10.18	136	941225	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.08	164	545683	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.84	188	1102354	20.00	ng/ul	0.00
78) Chrysene-d12	21.05	240	1042711	20.00	ng/ul	0.00
86) Perylene-d12	23.17	264	1255214	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.99	96	33747	6.67	ng/uL	0.00
5) Phenol-d5	6.62	99	137928	6.52	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.77	67	379656	29.93	ng/ul	0.00
9) 2-Chlorophenol-d4	6.96	132	380219	25.20	ng/ul	0.00
13) 4-Methylphenol-d8	8.15	113	257754	14.91	ng/ul	0.00
19) Nitrobenzene-d5	8.57	128	211248	31.23	ng/ul	0.00
22) 2-Nitrophenol-d4	9.29	143	240921	32.40	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.83	165	411220	28.45	ng/ul	0.00
29) 4-Chloroaniline-d4	10.36	131	25542	1.45	ng/ul	0.02
44) Dimethylphthalate-d6	13.50	166	1344681	33.32	ng/ul	0.00
47) Acenaphthylene-d8	13.77	160	1597250	33.03	ng/ul	0.00
52) 4-Nitrophenol-d4	14.36	143	41690	5.75	ng/ul	0.02
58) Fluorene-d10	15.08	176	1139359	32.21	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.24	200	180447	26.83	ng/ul	0.00
71) Anthracene-d10	16.94	188	1720920	34.31	ng/ul	0.00
79) Pyrene-d10	19.24	212	1855528	37.36	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.04	264	2201298	35.31	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.55	163	48499	1.156	ng/ul	99
65) N-Nitrosodiphenylamine	15.36	169	98099	3.061	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM122719\
Data File : BM024339.D
Acq On : 27 Dec 2019 22:44
Operator : JU
Sample : K6281-06
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFQX4

Quant Time: Dec 27 23:55:18 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 27 23:52:10 2019
Response via : Initial Calibration

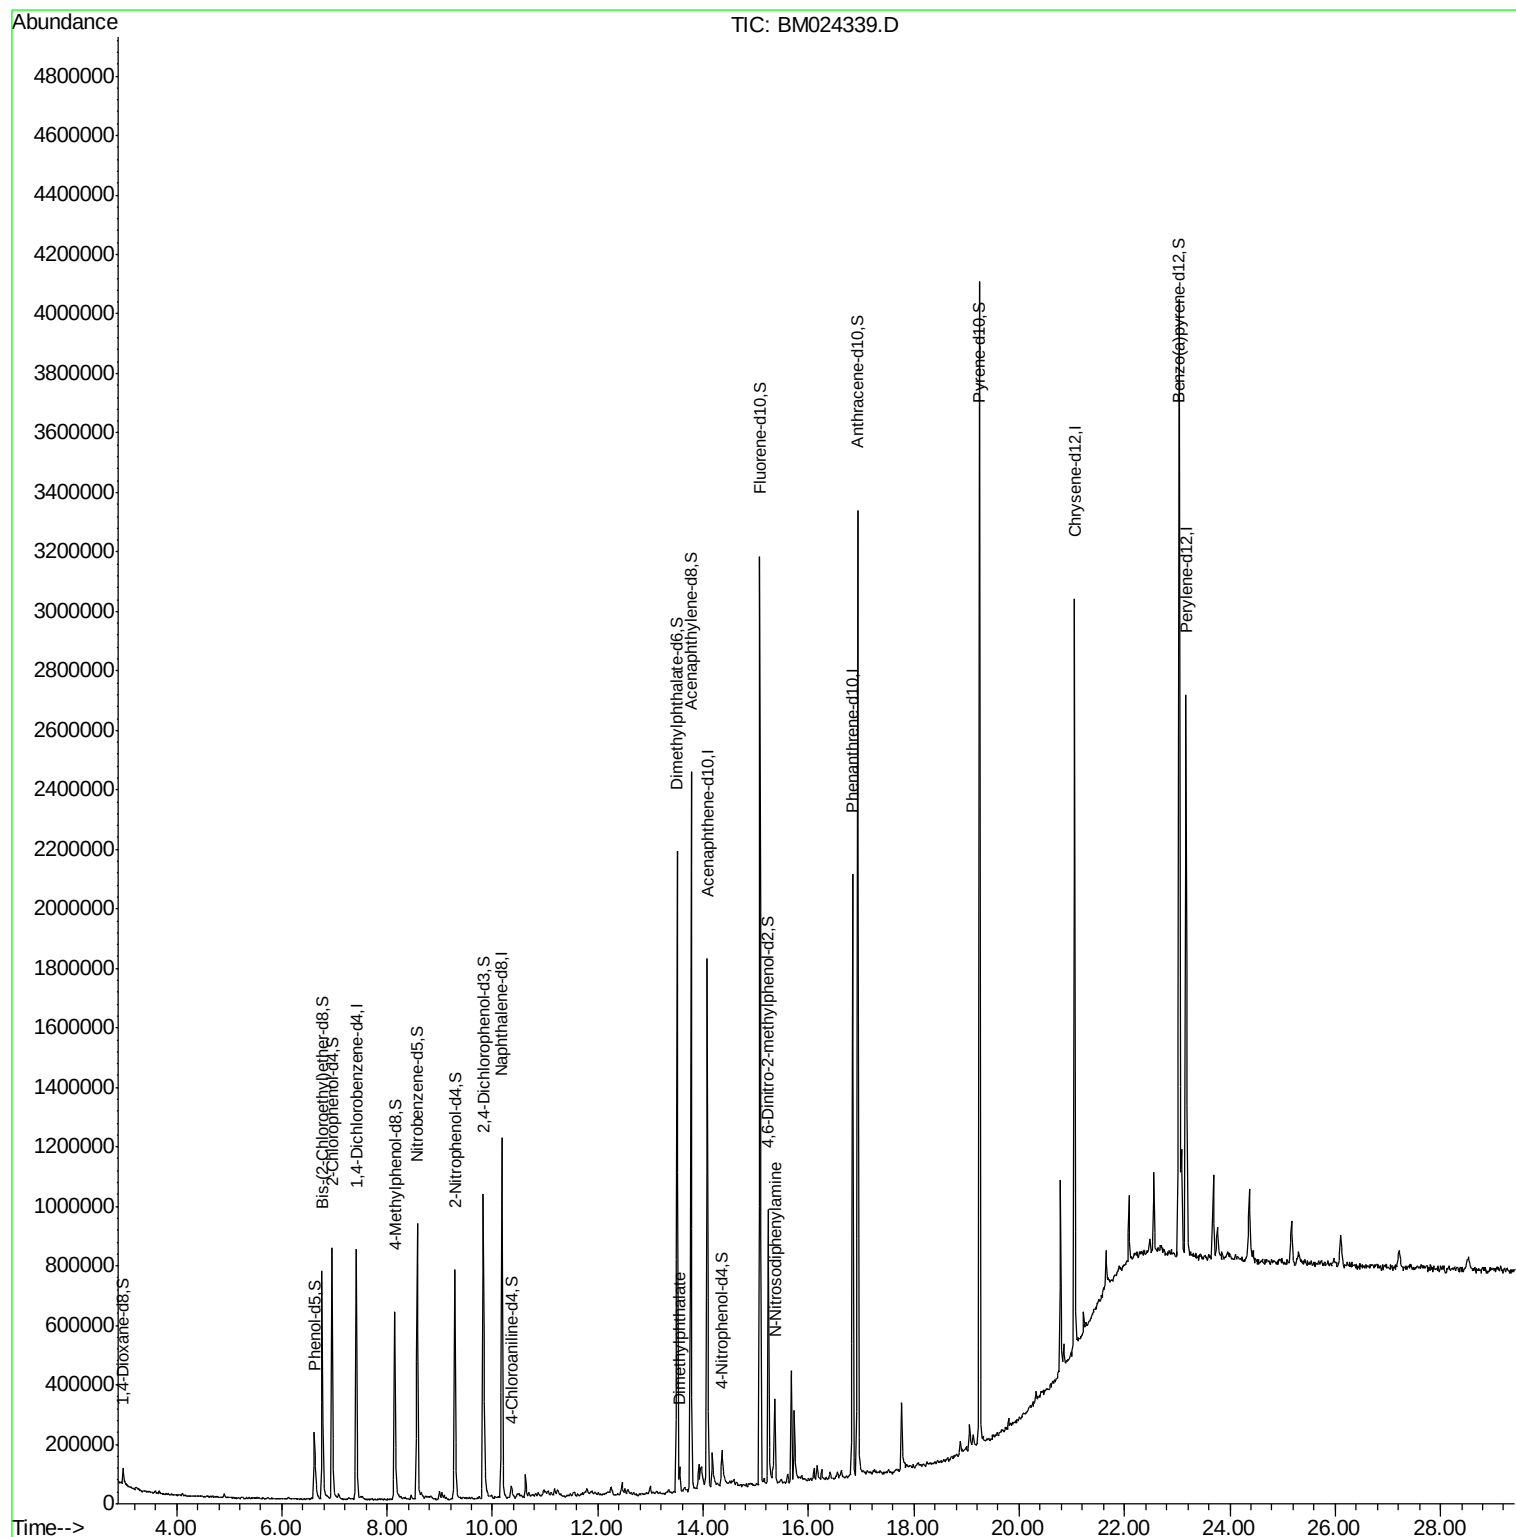

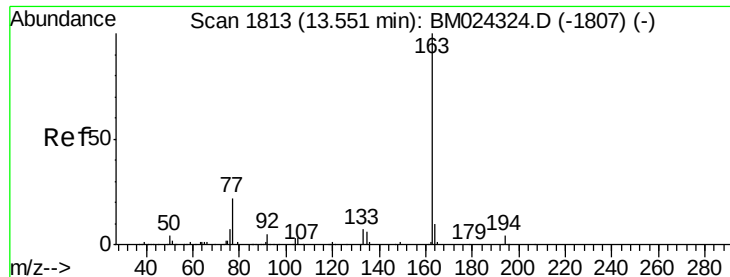

#45

Dimethylphthalate

Concen: 1.156 ng/ul

RT: 13.55 min Scan# 1813

Delta R.T. -0.00 min

Lab File: BM024339.D

Acq: 27 Dec 2019 22:44

Instrument :

BNA_M

ClientSampleId :

BFQX4


Tot Ion:163 Resp: 48499

Ion Ratio Lower Upper




163 100

194 3.4 3.2 4.8

164 10.2 7.8 11.6

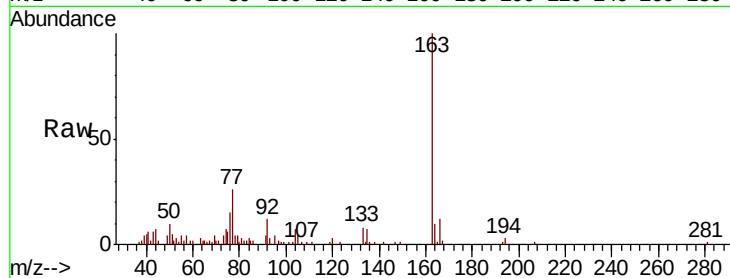

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

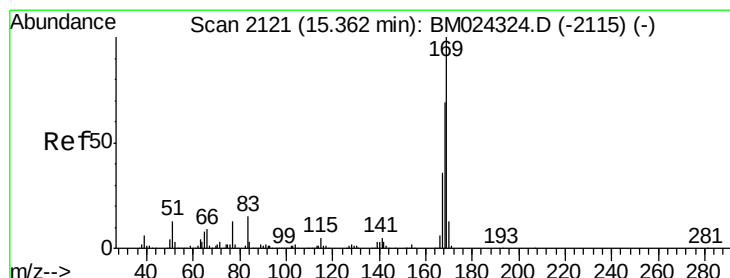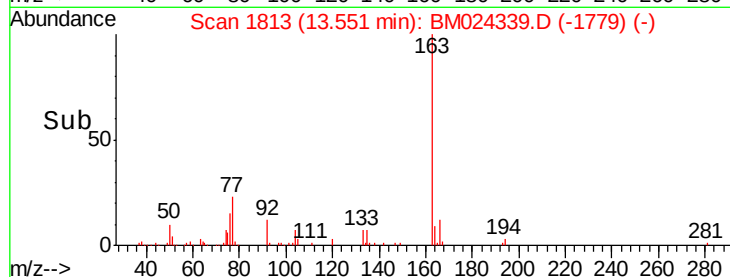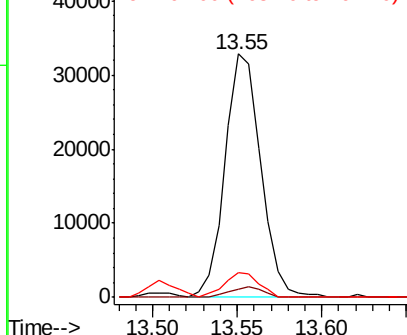

#65

N-Nitrosodiphenylamine

Concen: 3.061 ng/ul

RT: 15.36 min Scan# 2121

Delta R.T. -0.00 min

Lab File: BM024339.D

Acq: 27 Dec 2019 22:44


Tgt Ion:169 Resp: 98099

Ion Ratio Lower Upper

169 100

168 69.4 54.4 81.6

167 37.8 28.7 43.1

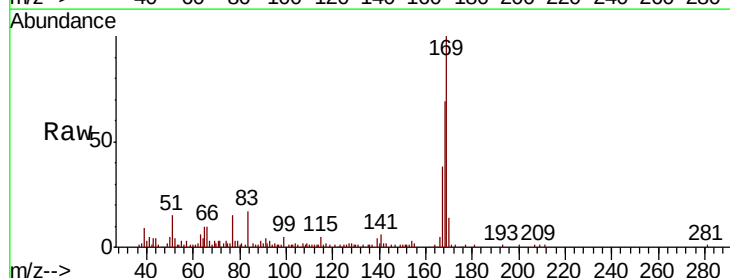

Abundance Ion 169.00 (168.70 to 169.70): E
Ion 168.00 (167.70 to 168.70): E
Ion 167.00 (166.70 to 167.70): E

