
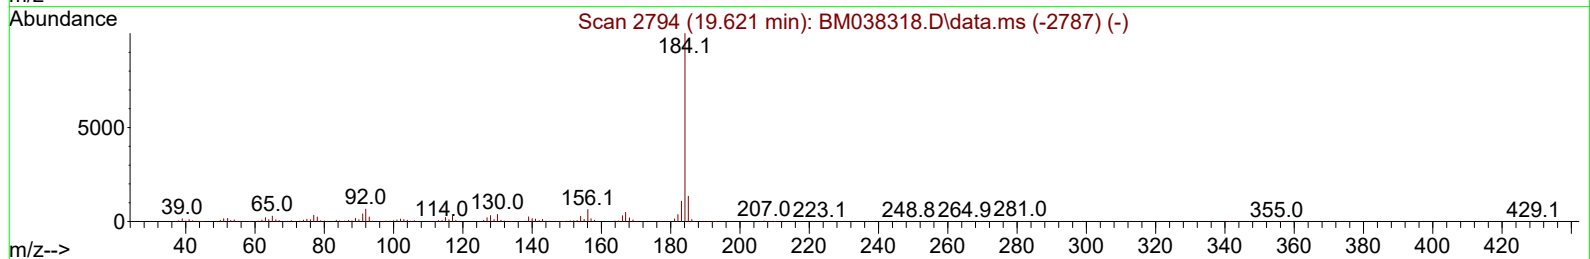
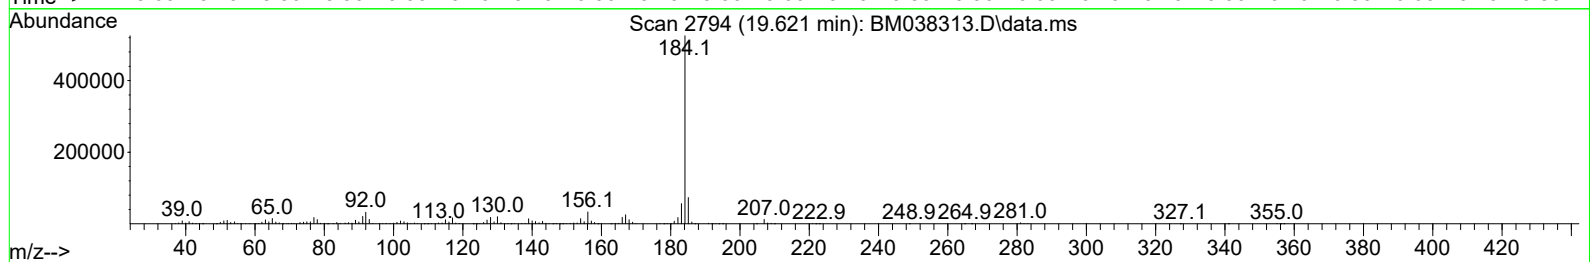


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122722\
Data File : BM038313.D
Acq On : 27 Dec 2022 13:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 28 06:15:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 28 01:33:07 2022
Response via : Initial Calibration

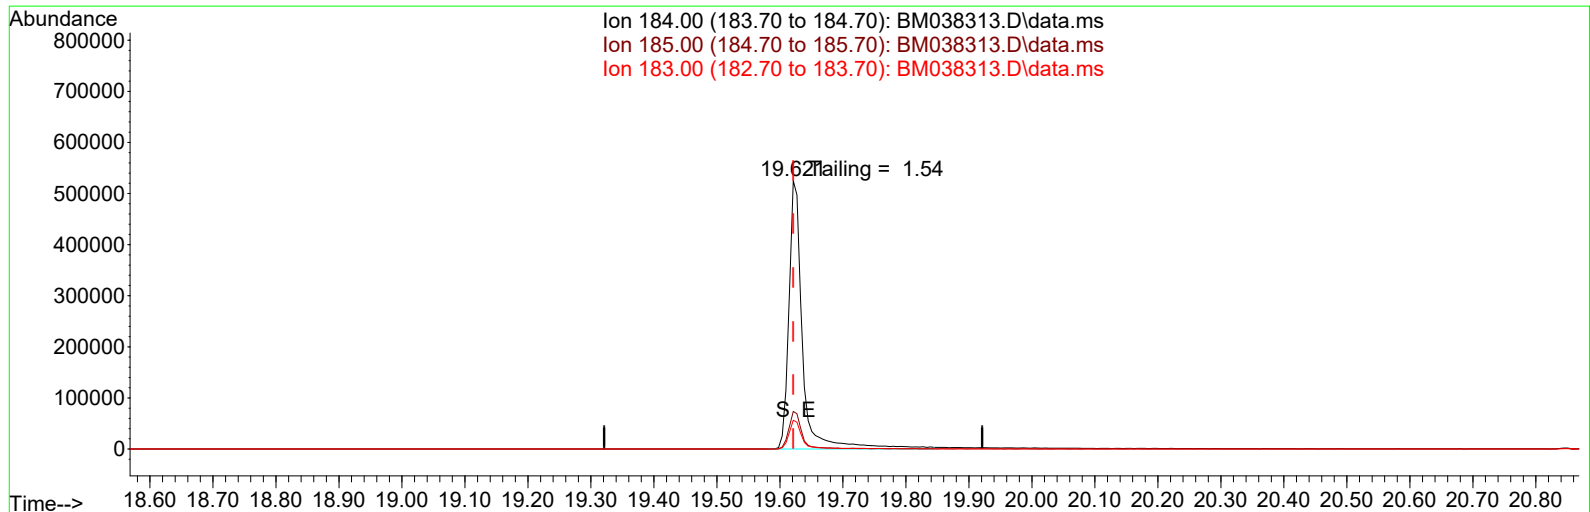

TIC: BM038313.D\data.ms

(77) Benzidine

19.621min (+ 0.000) 0.00 ng

response 803250

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.00
183.00	10.80	10.72
0.00	0.00	0.00