

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122722\
 Data File : BM038324.D
 Acq On : 27 Dec 2022 20:34
 Operator : CG/JU
 Sample : PB149775BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB149775BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM122722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM038324.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.087	318	323	335	rBV	546131	746028	20.16%	4.058%
2	5.557	397	403	416	rBV	1271247	1822271	49.24%	9.912%
3	7.175	671	678	693	rBV	1183937	1798096	48.59%	9.781%
4	8.010	812	820	827	rBV	324499	495481	13.39%	2.695%
5	9.187	1012	1020	1035	rBV	1000266	1618515	43.73%	8.804%
6	10.822	1291	1298	1308	rBV	358126	613641	16.58%	3.338%
7	13.269	1706	1714	1731	rBV	2461366	3287135	88.82%	17.880%
8	14.639	1941	1947	1955	rBV	502795	724403	19.57%	3.940%
9	16.127	2194	2200	2213	rBV	1011421	1372705	37.09%	7.467%
10	17.386	2406	2414	2426	rBV	525174	762947	20.62%	4.150%
11	19.992	2852	2857	2868	rBV	3364476	3700808	100.00%	20.131%
12	21.550	3118	3122	3132	rBV	543201	719768	19.45%	3.915%
13	23.986	3531	3536	3546	rVB2	355060	722171	19.51%	3.928%




Sum of corrected areas: 18383969

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122722\
Data File : BM038324.D
Acq On : 27 Dec 2022 20:34
Operator : CG/JU
Sample : PB149775BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB149775BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

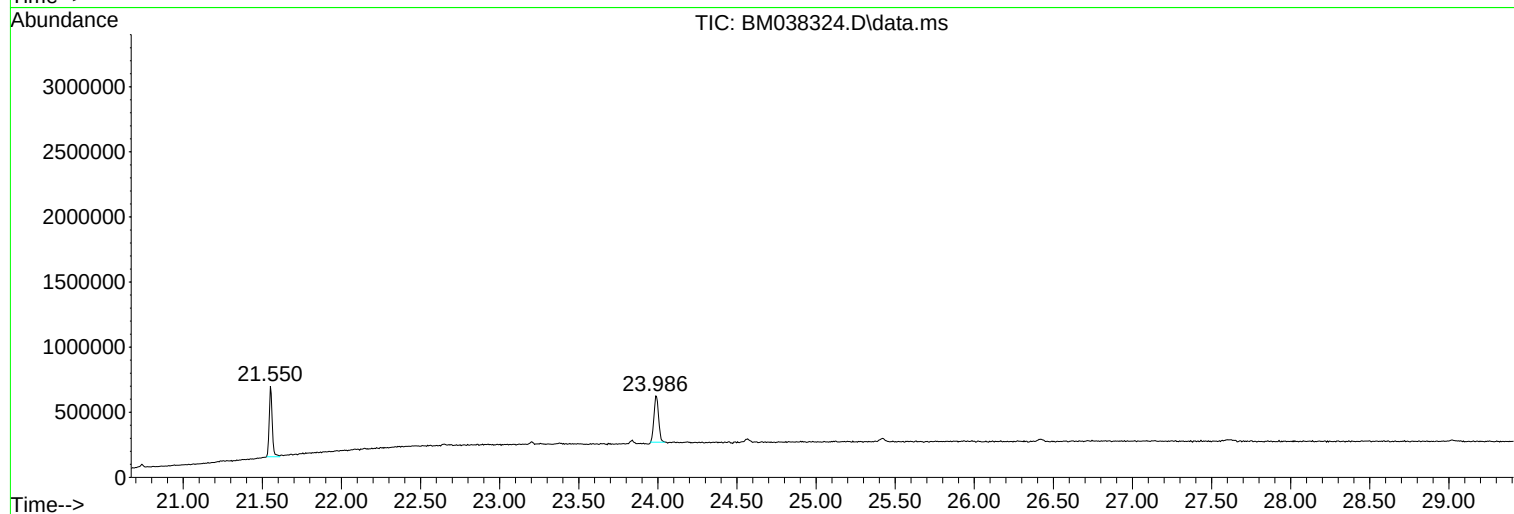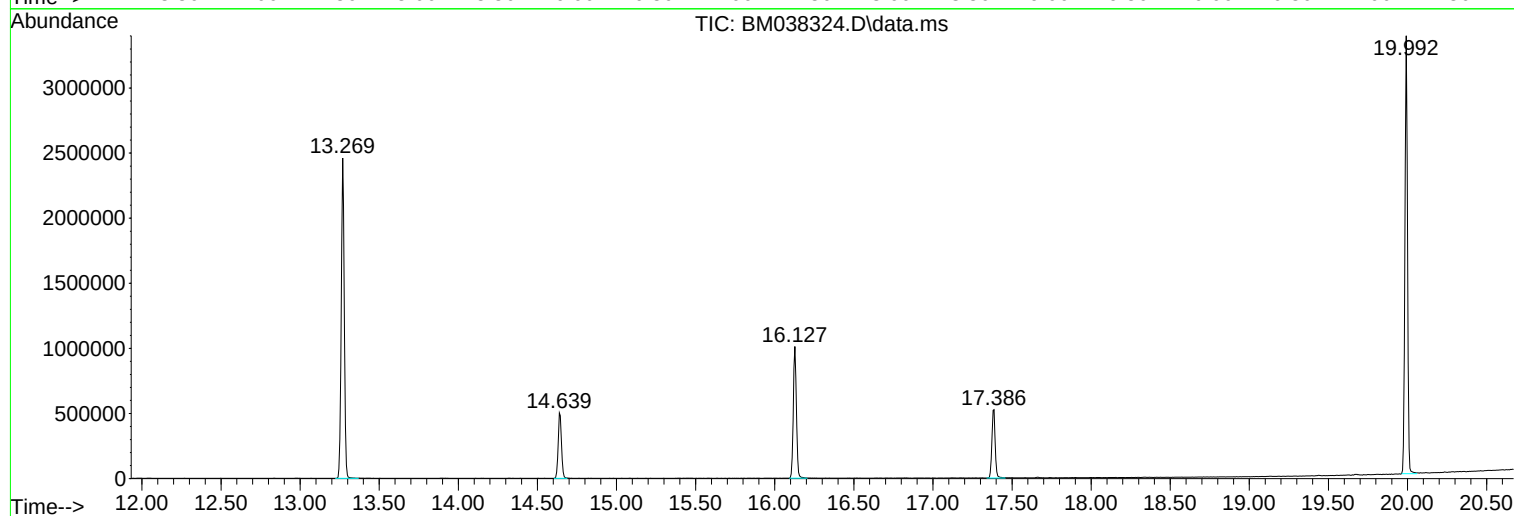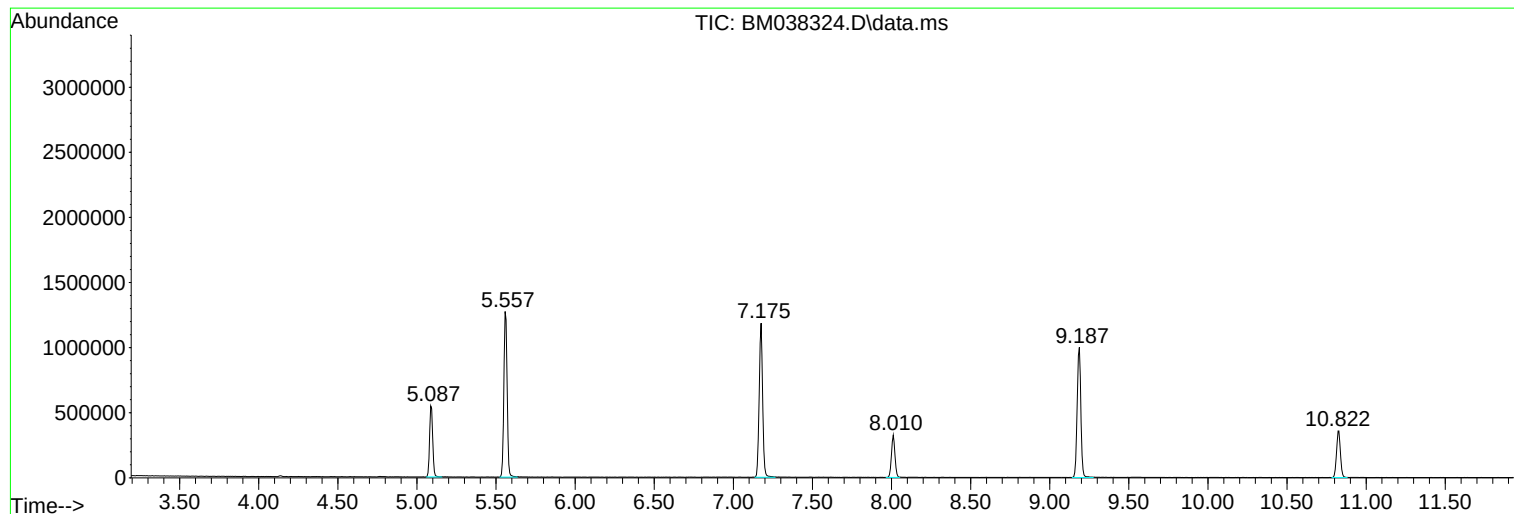

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122722\
Data File : BM038324.D
Acq On : 27 Dec 2022 20:34
Operator : CG/JU
Sample : PB149775BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB149775BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.087	30.11 ng	746028	1,4-Dichlorobenzene-d4	8.010

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56
2			Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23
3			1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10
4			2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	9
5			Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9

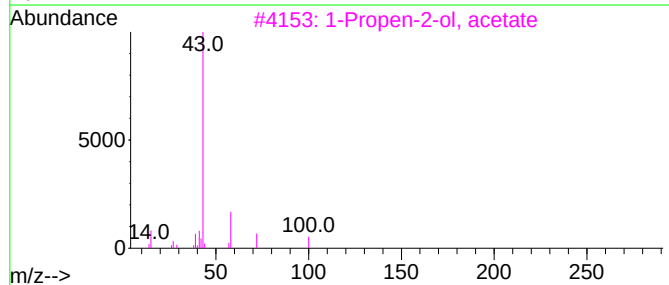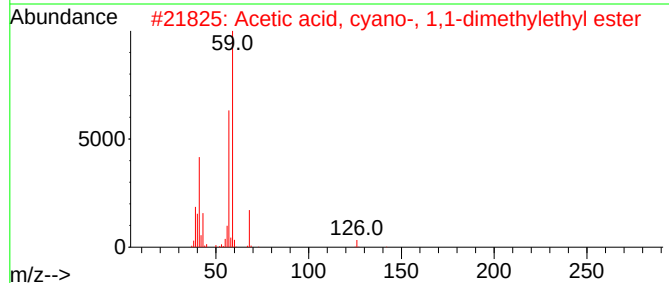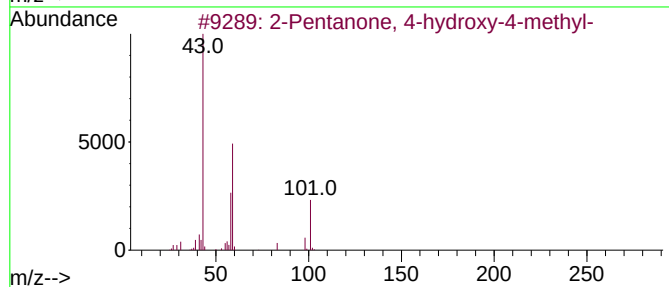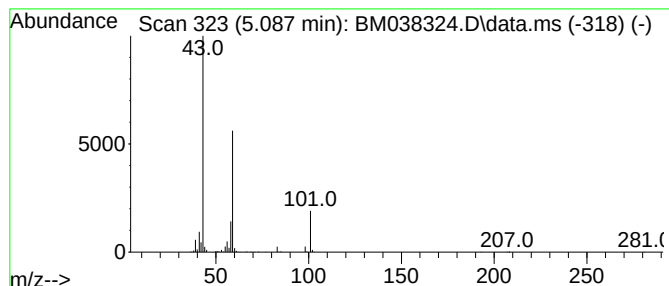

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122722\
Data File : BM038324.D
Acq On : 27 Dec 2022 20:34
Operator : CG/JU
Sample : PB149775BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB149775BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.087	30.1	ng	746028	1	8.010	495481	20.0