
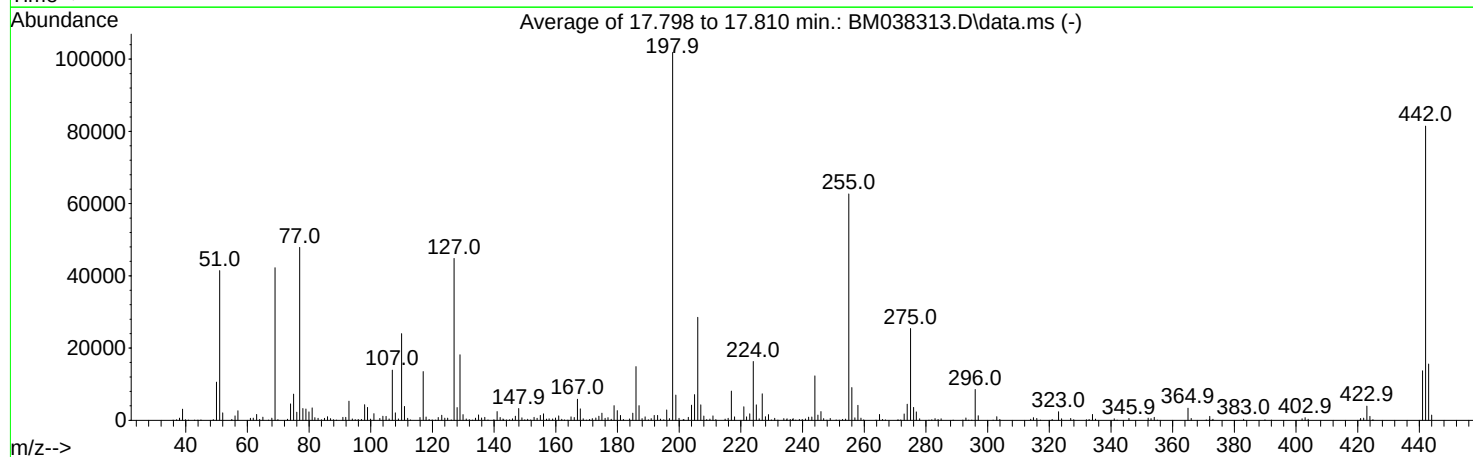


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122722\
 Data File : BM038313.D
 Acq On : 27 Dec 2022 13:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM122722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 28 01:33:07 2022

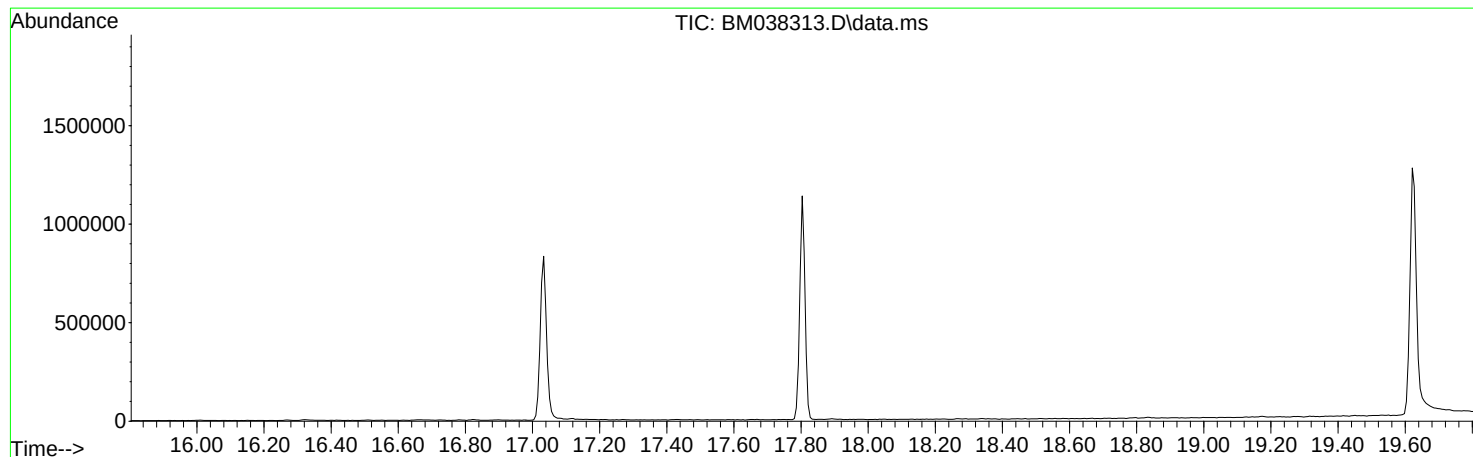

AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.7	41429	PASS
68	69	0.00	2	1.4	603	PASS
69	198	0.00	100	41.5	42230	PASS
70	69	0.00	2	0.5	207	PASS
127	198	10	80	44.0	44816	PASS
197	198	0.00	2	0.5	475	PASS
198	198	100	100	100.0	101859	PASS
199	198	5	9	6.9	6986	PASS
275	198	10	60	25.0	25435	PASS
365	198	1	100	3.3	3346	PASS
441	198	0.01	100	13.5	13725	PASS
442	442	50	100	100.0	81451	PASS
443	442	15	24	19.1	15557	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/27/2022	BNA_M	<u>BM038313.D</u>
Compound Name	Response	Retention Time
DDT	407024	20.845
DDD	3974	20.456
DDE	0	19.9
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3974	410998	0.97

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122722\
Data File : BM038313.D
Acq On : 27 Dec 2022 13:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Dec 28 06:15:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 28 01:33:07 2022
Response via : Initial Calibration

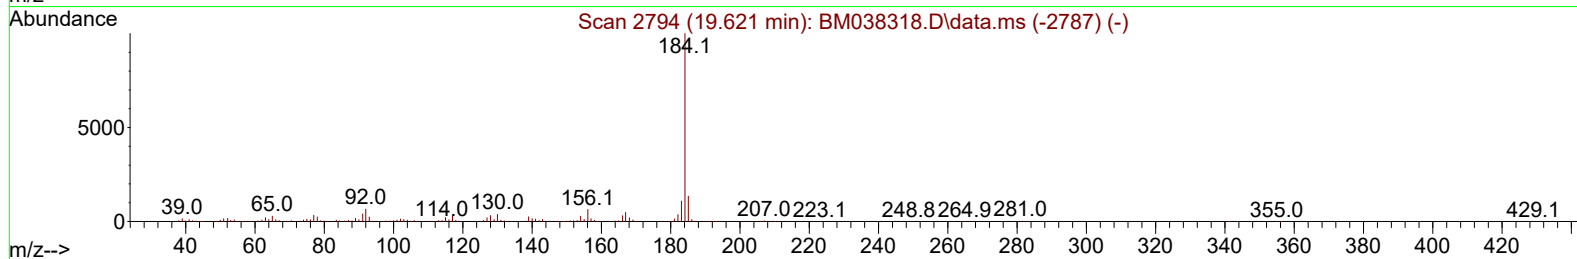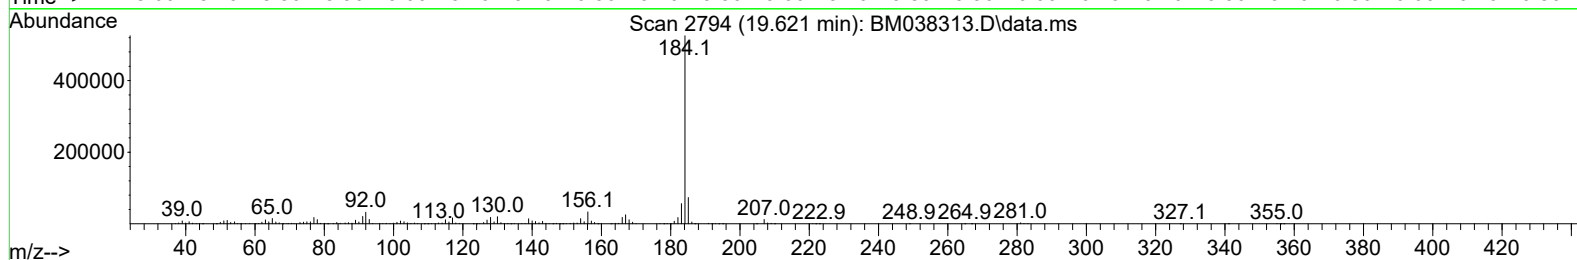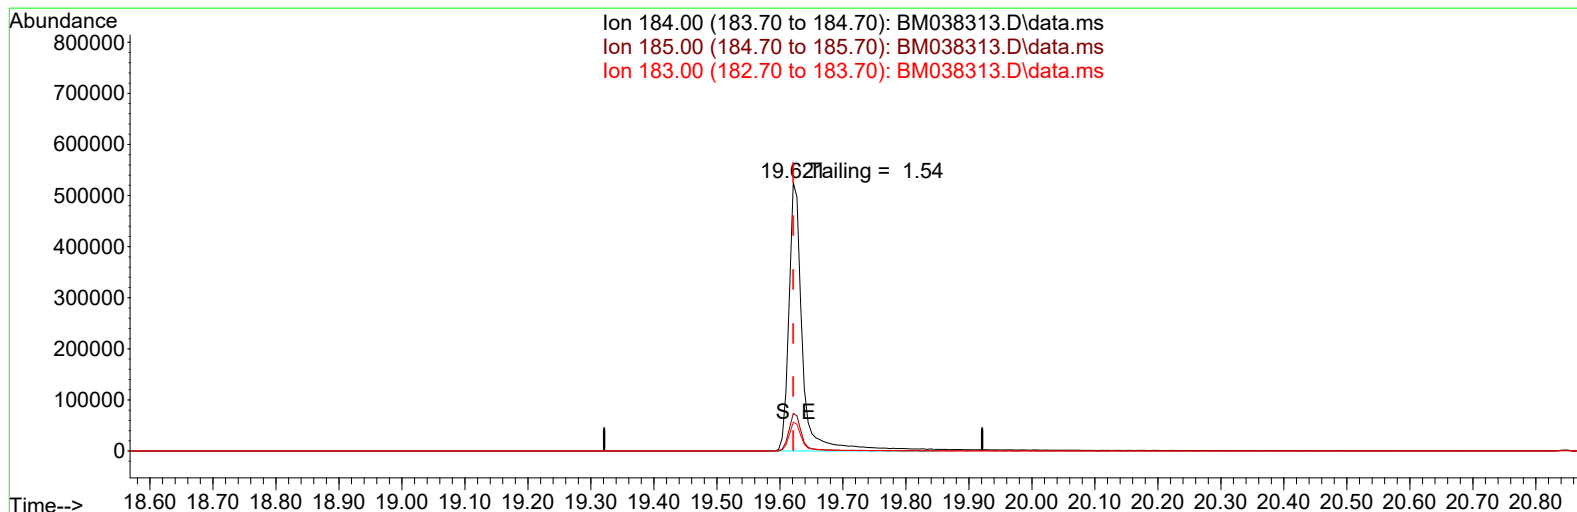

TIC: BM038313.D\data.ms

(77) Benzidine

19.621min (+ 0.000) 0.00 ng

response 803250

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.00
183.00	10.80	10.72
0.00	0.00	0.00