

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122724\
 Data File : BM049244.D
 Acq On : 27 Dec 2024 08:07
 Operator : RC/JU
 Sample : PB165797BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK797

Quant Time: Dec 27 22:11:03 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 26 11:35:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.544	152	2628	0.400	ng/ul	0.00
4) Naphthalene-d8	10.303	136	7613	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.182	164	4389	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.026	188	700553	0.400	ng/ul	0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.13
23) Perylene-d12	23.288	264	13634	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.134	96	18267	6.027	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.925	152	3042	0.297	ng/ul	0.02
18) Fluoranthene-d10	18.968	212	7718	0.000	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.181	166	1133	0.076	ng/ul#	18
26) Benzo(a)pyrene	23.148	252	3146	0.075	ng/ul#	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122724\
Data File : BM049244.D
Acq On : 27 Dec 2024 08:07
Operator : RC/JU
Sample : PB165797BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK797

Quant Time: Dec 27 22:11:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 26 11:35:38 2024
Response via : Initial Calibration




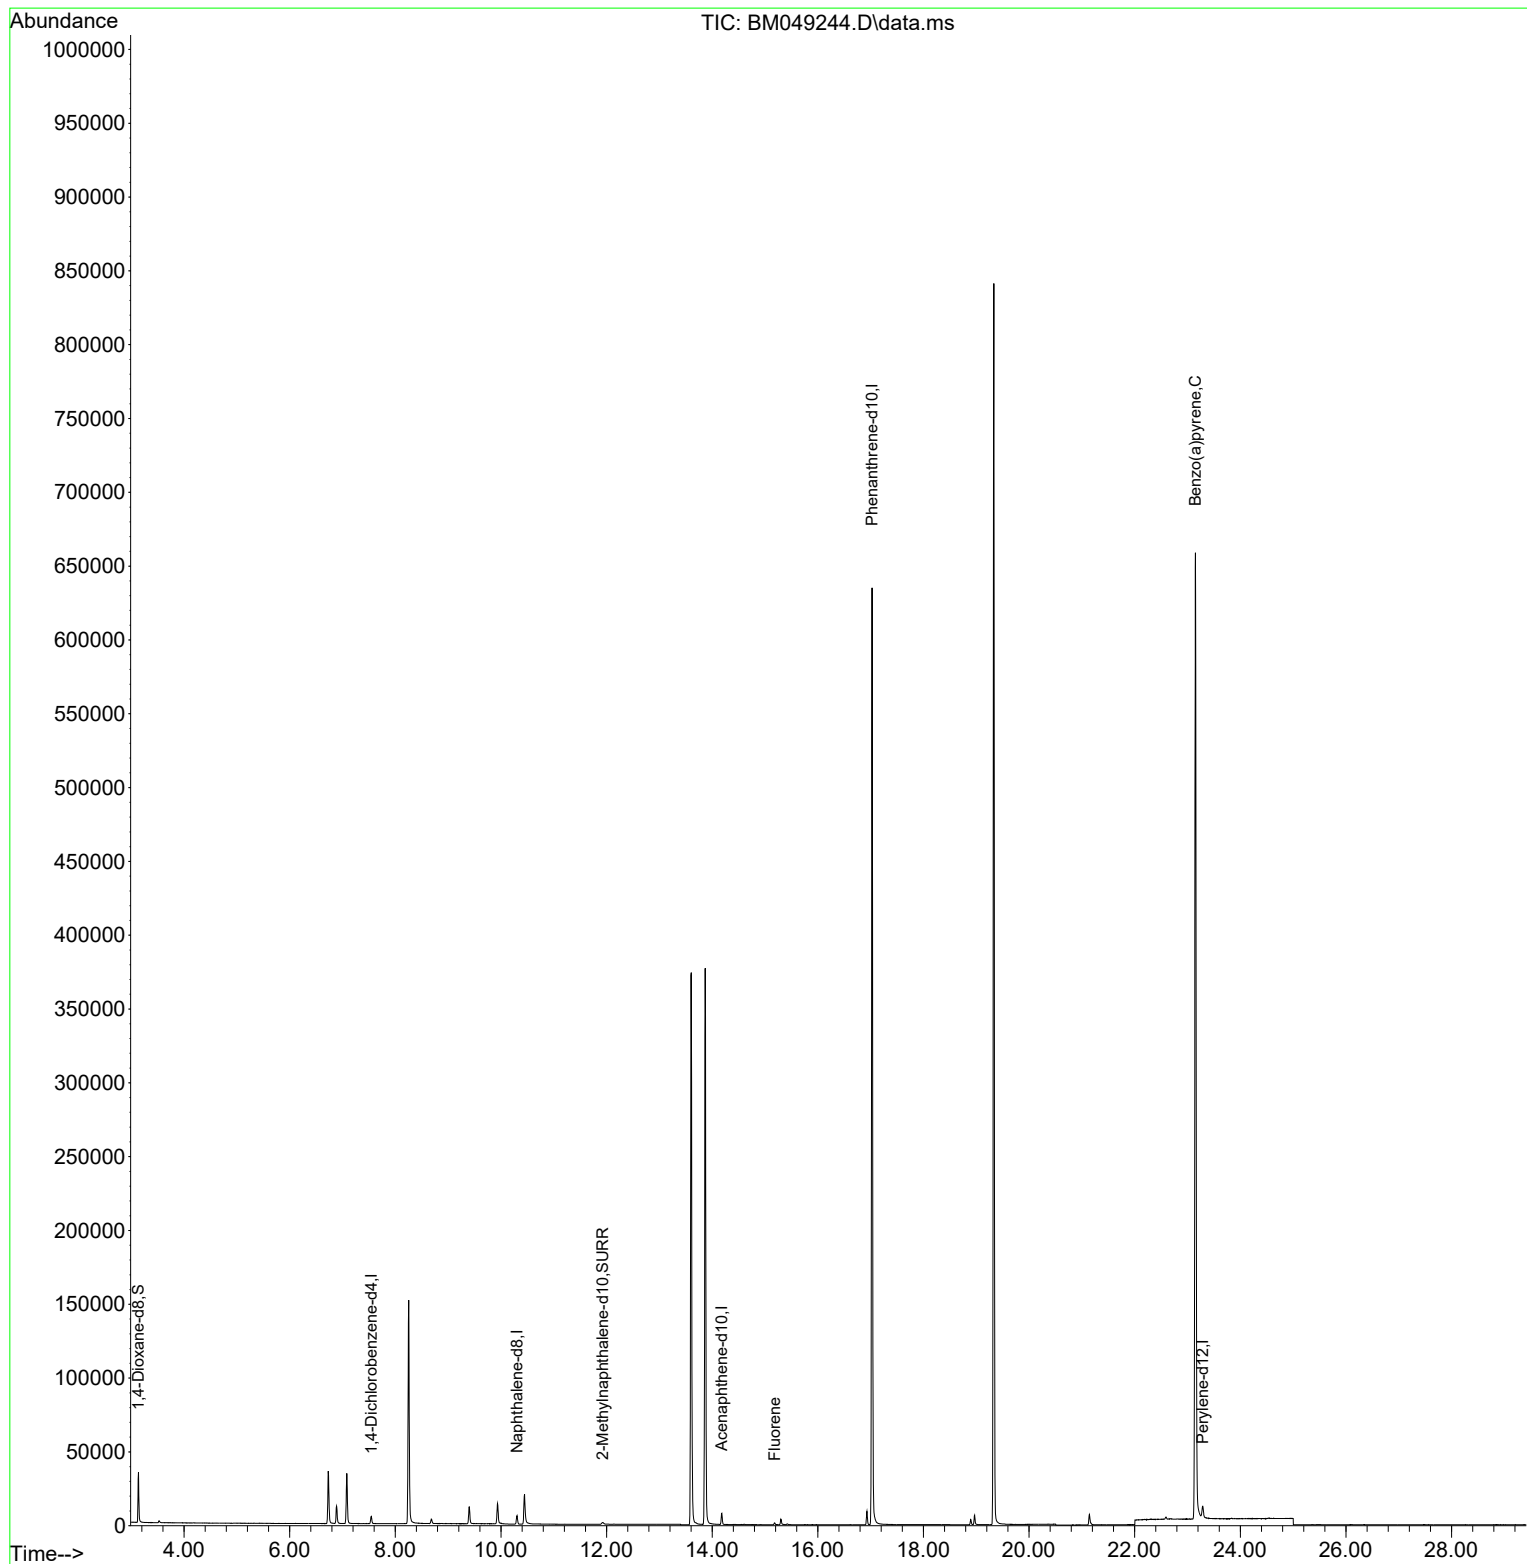


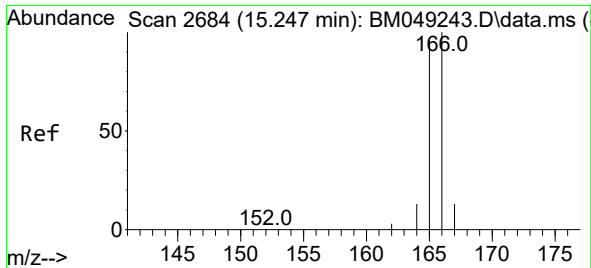

#12
Fluorene
Concen: 0.076 ng/ul
RT: 15.181 min Scan# 20
Delta R.T. -0.060 min
Lab File: BM049244.D
Acq: 27 Dec 2024 08:07

Instrument :
BNA_M
ClientSampleId :
SBLK797

Tgt Ion:166 Resp: 1133
Ion Ratio Lower Upper
166 100
165 14.4 79.7 119.5#
167 37.0 11.4 17.0#

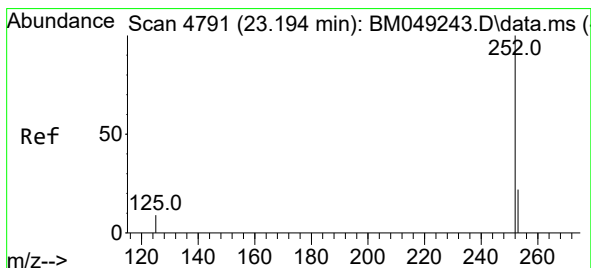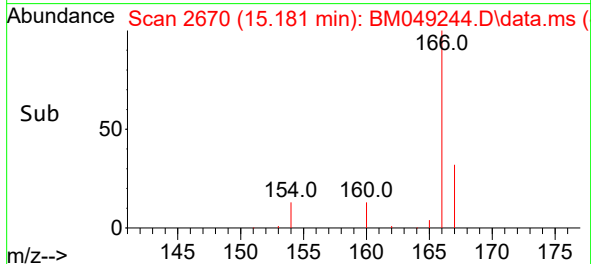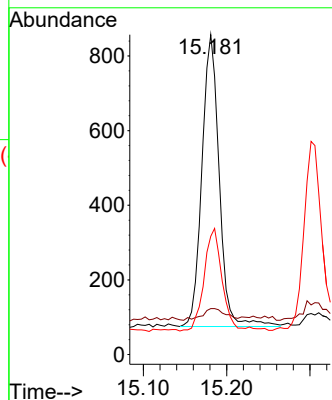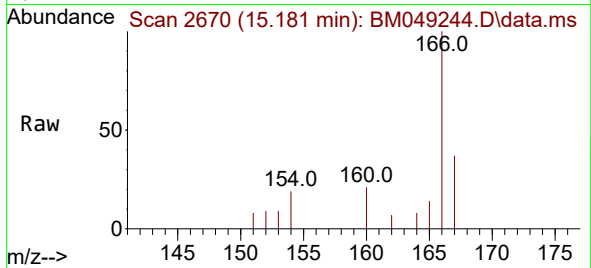

#26
Benzo(a)pyrene
Concen: 0.075 ng/ul
RT: 23.148 min Scan# 4775
Delta R.T. -0.044 min
Lab File: BM049244.D
Acq: 27 Dec 2024 08:07

Tgt Ion:252 Resp: 3146
Ion Ratio Lower Upper
252 100
253 47.2 22.4 33.6#
125 35.7 14.8 22.2#

