

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122724\
 Data File : BM049251.D
 Acq On : 27 Dec 2024 12:53
 Operator : RC/JU
 Sample : P5324-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YE5Y1

Quant Time: Dec 27 22:12:09 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 26 11:35:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.544	152	3261	0.400	ng/ul	0.00
4) Naphthalene-d8	10.303	136	9740	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.182	164	5698	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.030	188	1171599	0.400	ng/ul	# 0.10
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.13
23) Perylene-d12	23.286	264	20074	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.139	96	21531	5.725	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.909	152	4994	0.382	ng/ul	0.00
18) Fluoranthene-d10	18.968	212	12879	0.000	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.172	88	332	0.076	ng/ul#	73
26) Benzo(a)pyrene	23.151	252	5251	0.085	ng/ul#	17


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122724\
Data File : BM049251.D
Acq On : 27 Dec 2024 12:53
Operator : RC/JU
Sample : P5324-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YE5Y1

Quant Time: Dec 27 22:12:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 26 11:35:38 2024
Response via : Initial Calibration




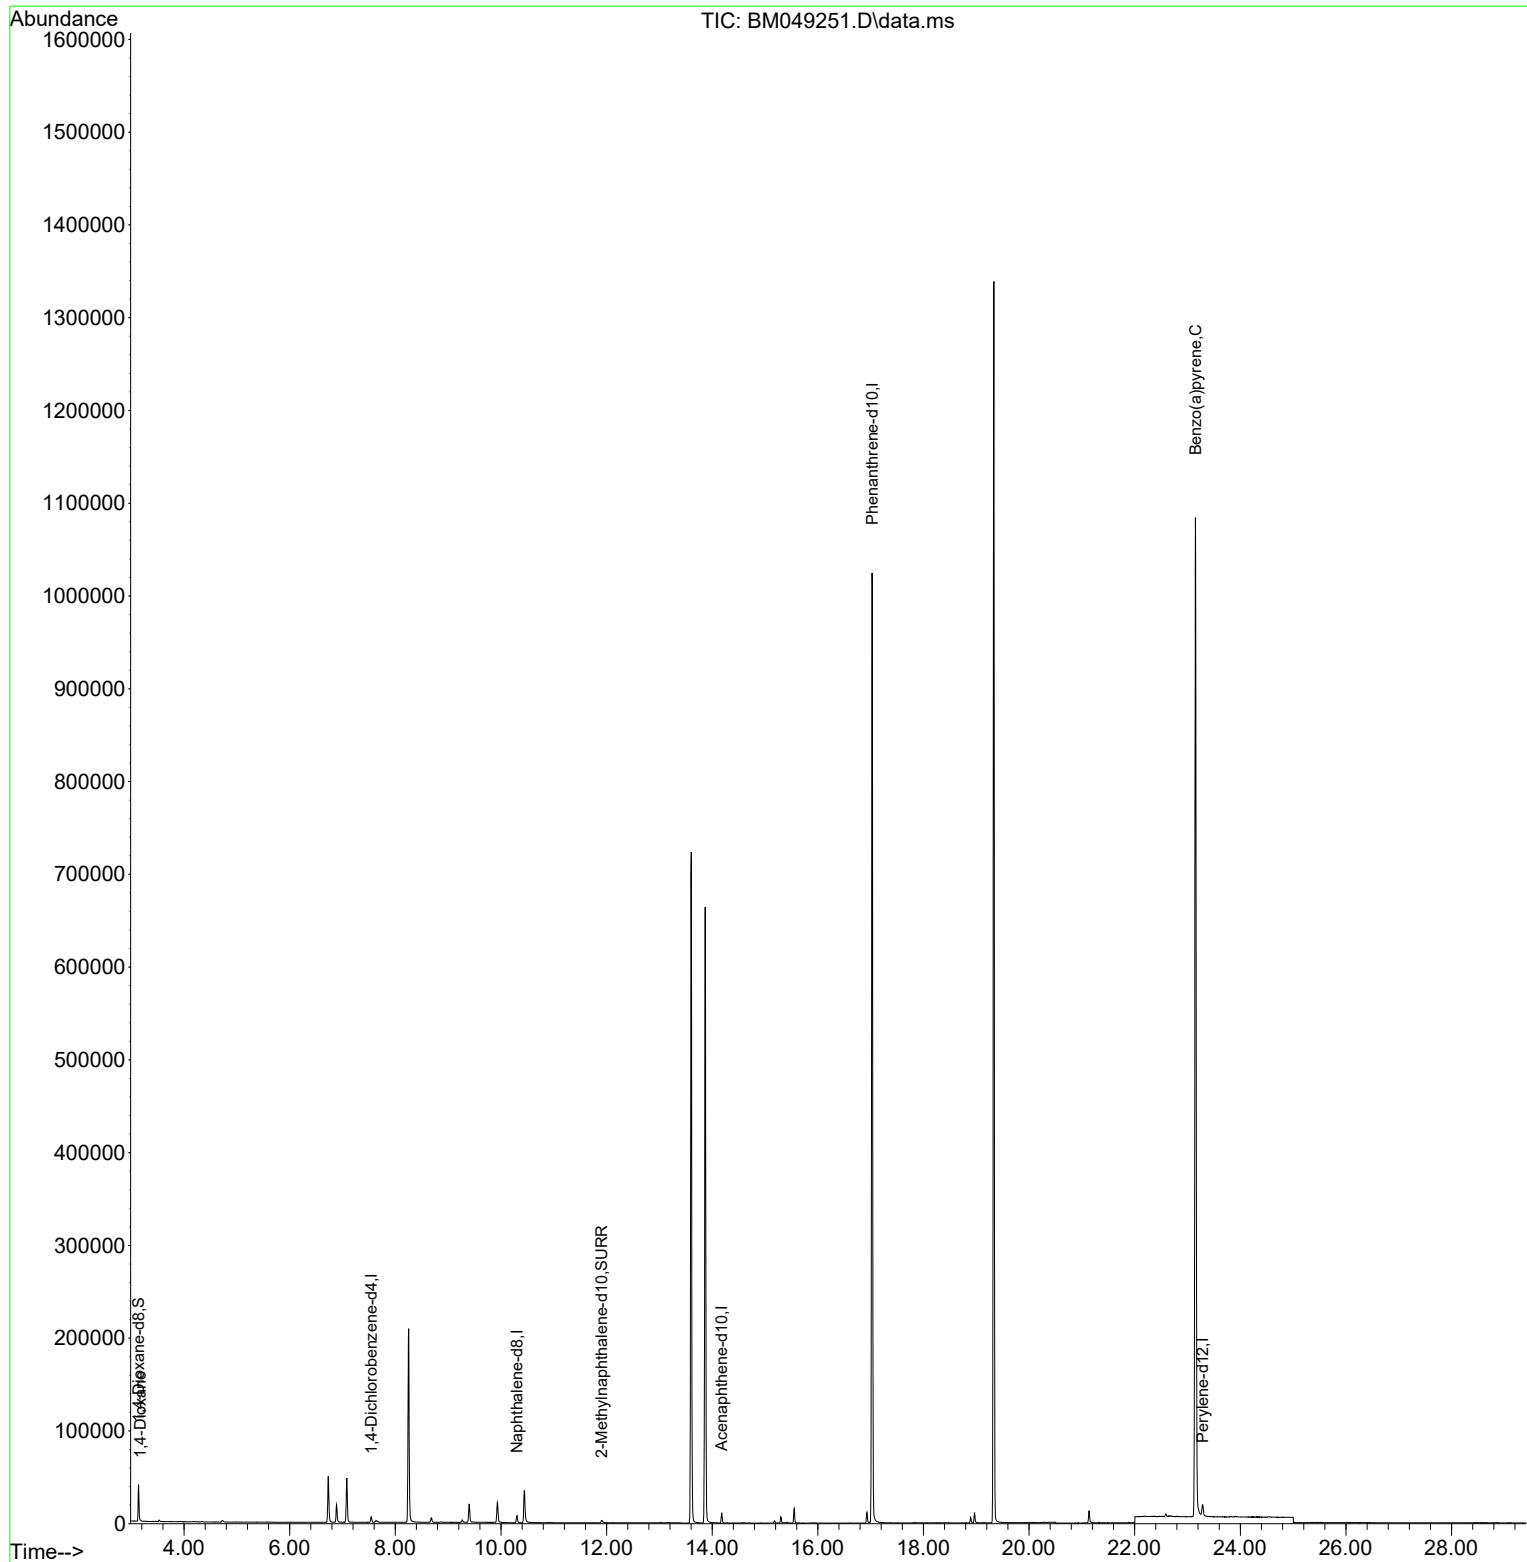


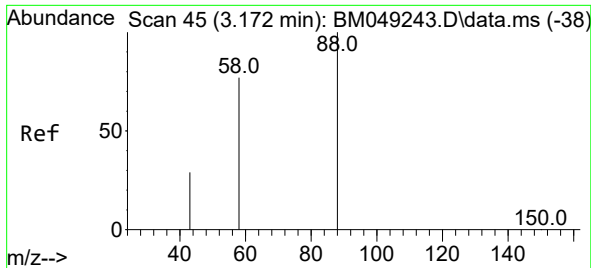

#2
1,4-Dioxane
Concen: 0.076 ng/ul
RT: 3.172 min Scan# 41
Delta R.T. -0.004 min
Lab File: BM049251.D
Acq: 27 Dec 2024 12:53

Instrument :
BNA_M
ClientSampleId :
YE5Y1

Tgt Ion: 88 Resp: 332
Ion Ratio Lower Upper
88 100
43 50.0 45.4 68.2
58 21.2 43.6 65.4#

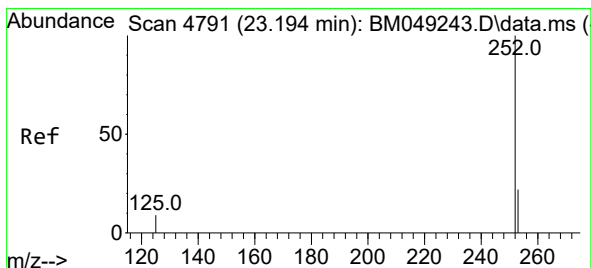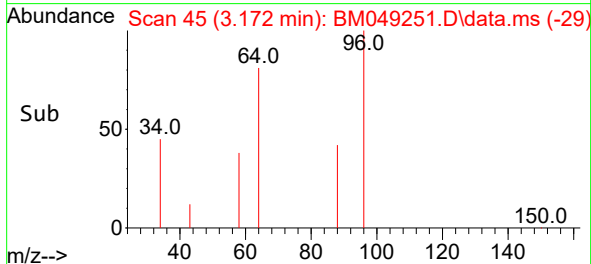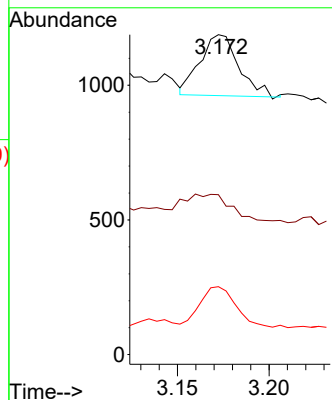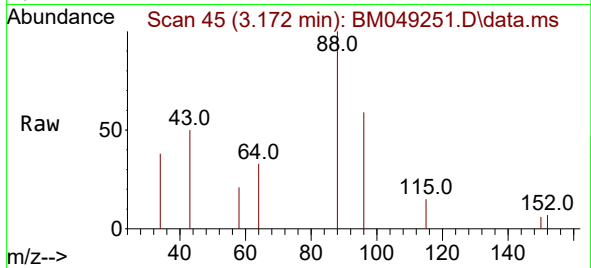

#26
Benzo(a)pyrene
Concen: 0.085 ng/ul
RT: 23.151 min Scan# 4776
Delta R.T. -0.041 min
Lab File: BM049251.D
Acq: 27 Dec 2024 12:53

Tgt Ion: 252 Resp: 5251
Ion Ratio Lower Upper
252 100
253 44.8 22.4 33.6#
125 90.0 14.8 22.2#

