

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122724\
 Data File : BM049260.D
 Acq On : 27 Dec 2024 18:50
 Operator : RC/JU
 Sample : P5324-12
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YE5Z9

Quant Time: Dec 27 22:13:22 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 26 11:35:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.543	152	3289	0.400	ng/ul	0.00
4) Naphthalene-d8	10.303	136	9818	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.181	164	5809	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.026	188	1374294	0.400	ng/ul	0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.13
23) Perylene-d12	23.285	264	16137	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.138	96	16425	4.330	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.914	152	3693	0.280	ng/ul	0.00
18) Fluoranthene-d10	18.968	212	15213	0.000	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.172	88	1067	0.241	ng/ul#	79
12) Fluorene	15.181	166	1979	0.100	ng/ul#	15
26) Benzo(a)pyrene	23.151	252	5480	0.111	ng/ul#	79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122724\
Data File : BM049260.D
Acq On : 27 Dec 2024 18:50
Operator : RC/JU
Sample : P5324-12
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YE5Z9

Quant Time: Dec 27 22:13:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 26 11:35:38 2024
Response via : Initial Calibration




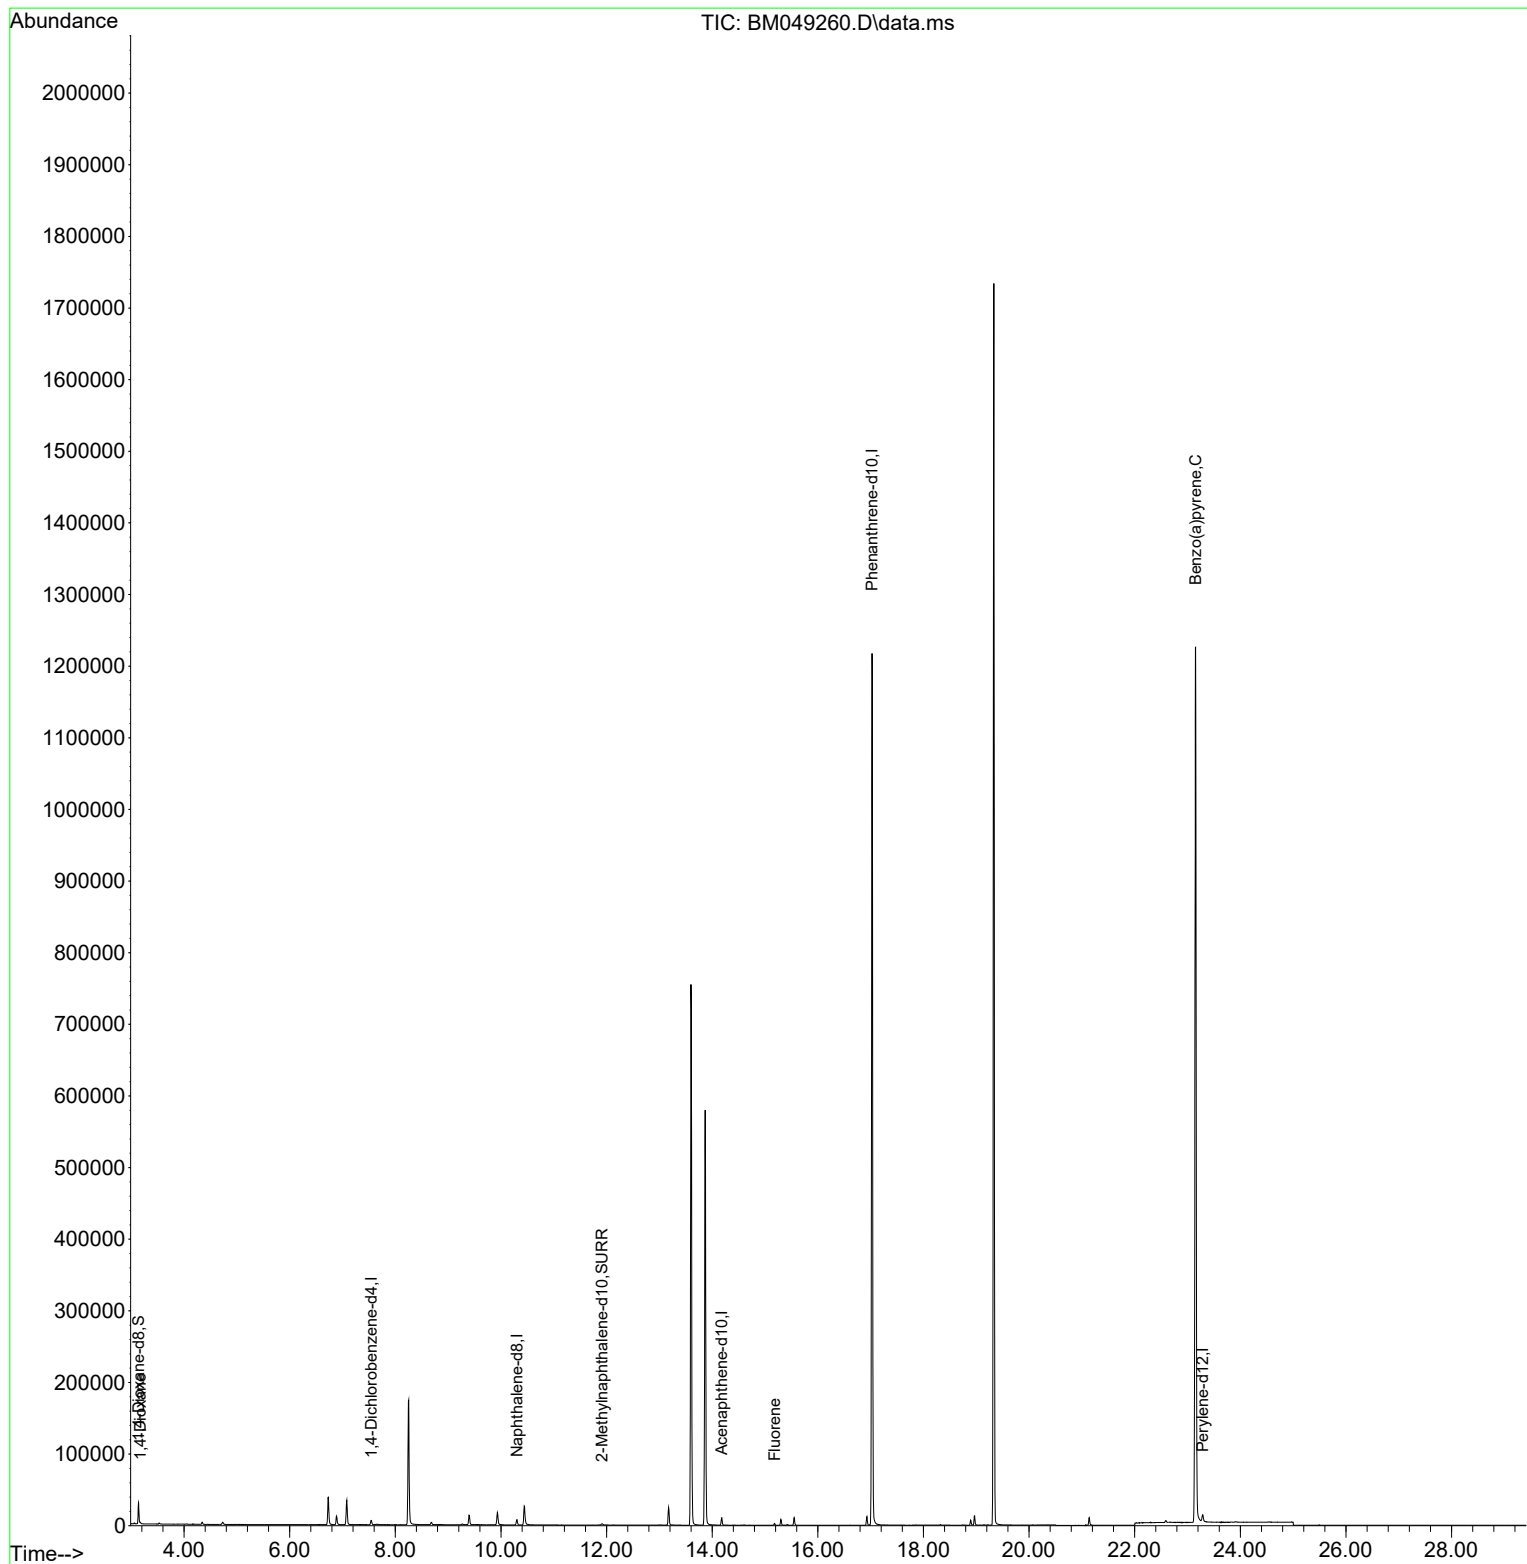


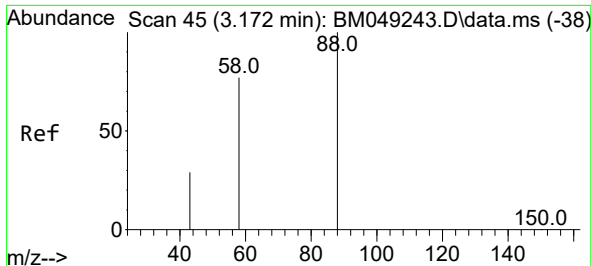

#2
1,4-Dioxane
Concen: 0.241 ng/ul
RT: 3.172 min Scan# 41
Delta R.T. -0.004 min
Lab File: BM049260.D
Acq: 27 Dec 2024 18:50




Instrument :
BNA_M
ClientSampleId :
YE5Z9


Tgt Ion: 88 Resp: 1067
Ion Ratio Lower Upper
88 100
43 40.6 45.4 68.2#
58 39.9 43.6 65.4#

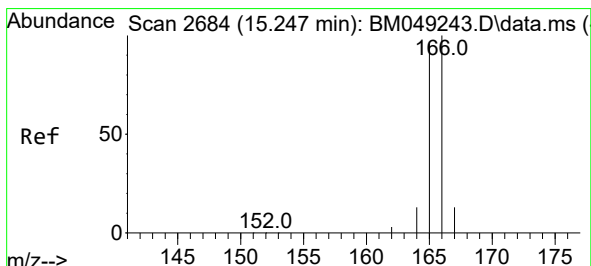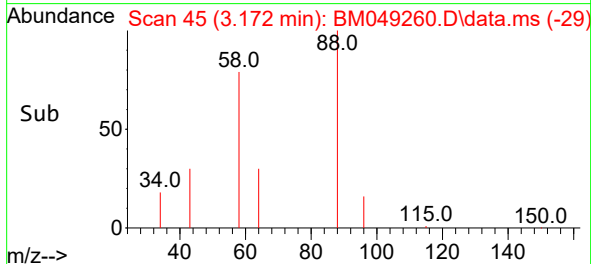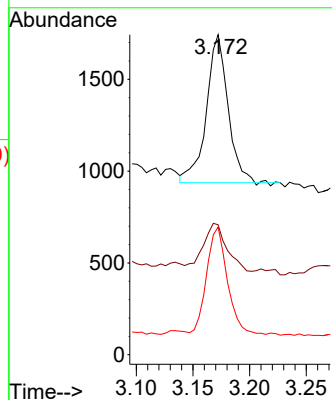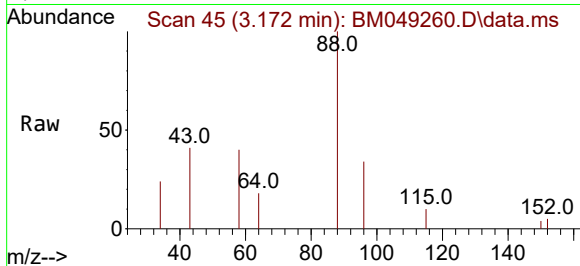

#12
Fluorene
Concen: 0.100 ng/ul
RT: 15.181 min Scan# 2670
Delta R.T. -0.060 min
Lab File: BM049260.D
Acq: 27 Dec 2024 18:50


Tgt Ion: 166 Resp: 1979
Ion Ratio Lower Upper
166 100
165 10.2 79.7 119.5#
167 37.0 11.4 17.0#

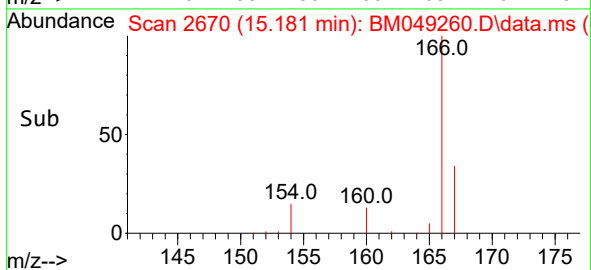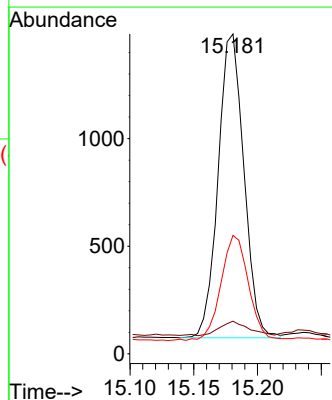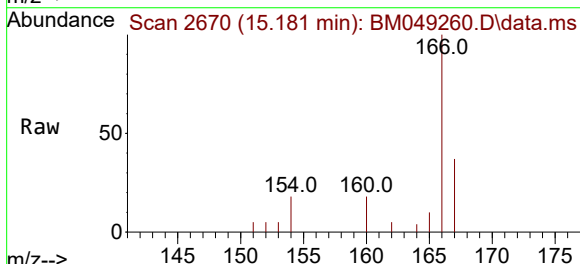

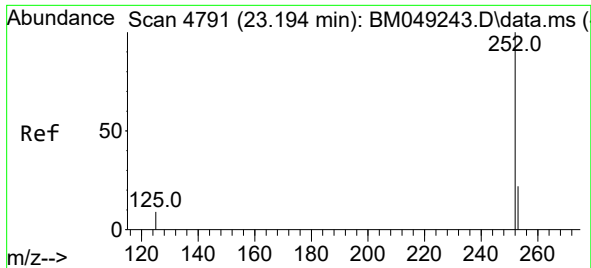

#26
Benzo(a)pyrene
Concen: 0.111 ng/ul
RT: 23.151 min Scan# 41
Delta R.T. -0.041 min
Lab File: BM049260.D
Acq: 27 Dec 2024 18:50

Instrument :
BNA_M
ClientSampleId :
YE5Z9

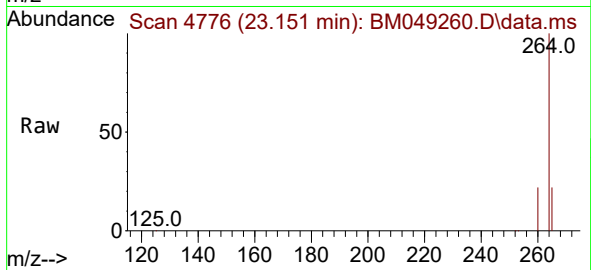

Tgt Ion:252 Resp: 5480
Ion Ratio Lower Upper
252 100
253 39.5 22.4 33.6#
125 27.7 14.8 22.2#

