

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122724\
 Data File : BM049279.D
 Acq On : 28 Dec 2024 06:46
 Operator : RC/JU
 Sample : P5325-01
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YE680

Quant Time: Dec 29 21:55:20 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 26 11:35:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.539	152	5215	0.400	ng/ul	0.00
4) Naphthalene-d8	10.297	136	17018	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.177	164	10127	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.026	188	1593561	0.400	ng/ul	0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.13
23) Perylene-d12	23.285	264	28267	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.138	96	30465	5.065	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.903	152	7732	0.338	ng/ul	0.00
18) Fluoranthene-d10	18.964	212	20092	0.000	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.172	88	388	0.055	ng/ul#	42
26) Benzo(a)pyrene	23.151	252	5878	0.068	ng/ul#	24


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122724\
Data File : BM049279.D
Acq On : 28 Dec 2024 06:46
Operator : RC/JU
Sample : P5325-01
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YE680

Quant Time: Dec 29 21:55:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 26 11:35:38 2024
Response via : Initial Calibration




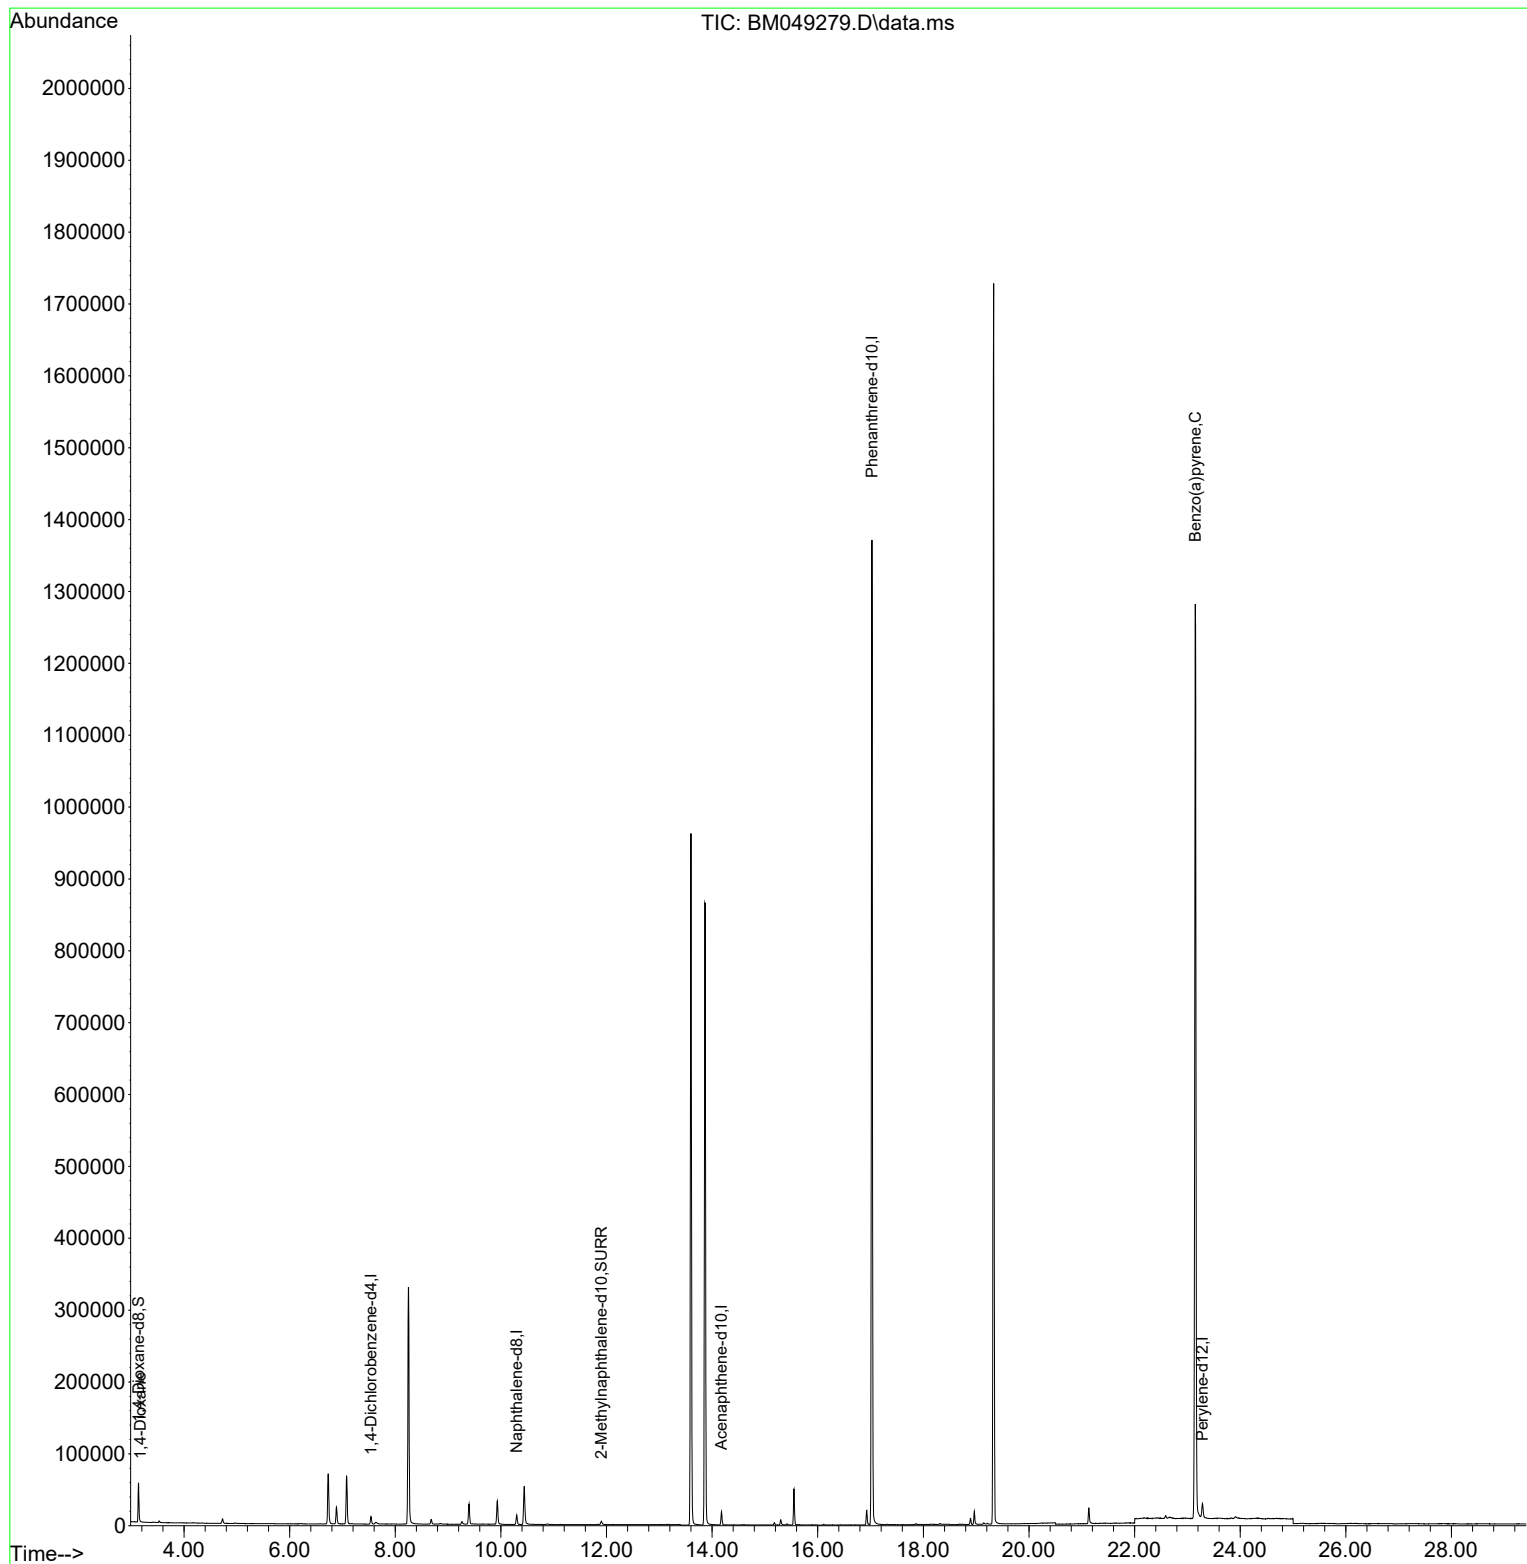


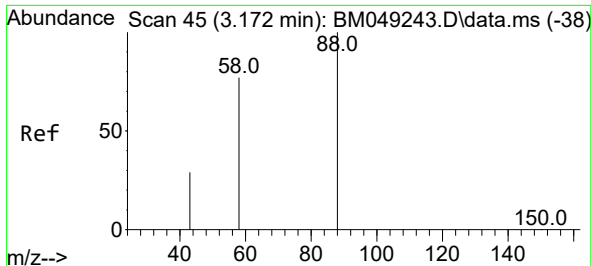

#2
1,4-Dioxane
Concen: 0.055 ng/ul
RT: 3.172 min Scan# 41
Delta R.T. -0.004 min
Lab File: BM049279.D
Acq: 28 Dec 2024 06:46

Instrument :
BNA_M
ClientSampleId :
YE680

Tgt Ion: 88 Resp: 388
Ion Ratio Lower Upper
88 100
43 115.9 45.4 68.2#
58 29.4 43.6 65.4#

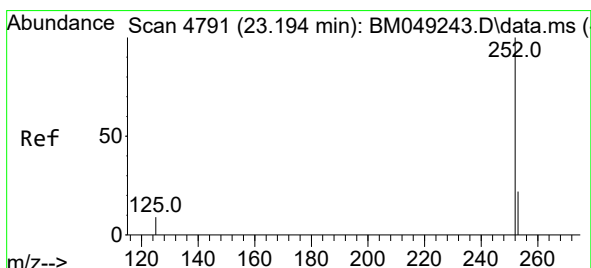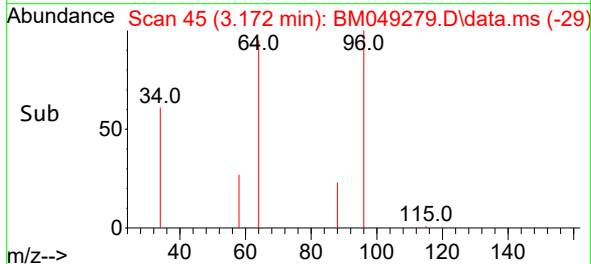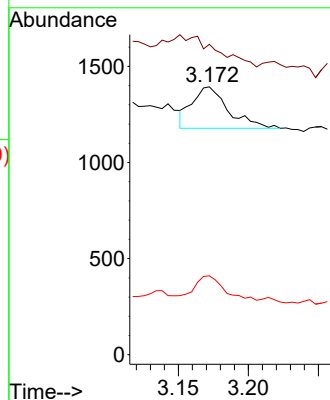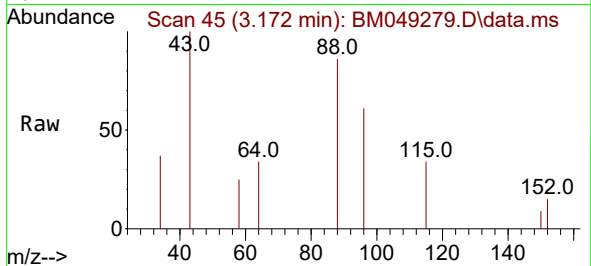

#26
Benzo(a)pyrene
Concen: 0.068 ng/ul
RT: 23.151 min Scan# 4776
Delta R.T. -0.041 min
Lab File: BM049279.D
Acq: 28 Dec 2024 06:46

Tgt Ion: 252 Resp: 5878
Ion Ratio Lower Upper
252 100
253 52.3 22.4 33.6#
125 73.0 14.8 22.2#

