

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122724\
 Data File : BM049290.D
 Acq On : 28 Dec 2024 13:20
 Operator : RC/JU
 Sample : P5324-14
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YE601

Quant Time: Dec 29 21:57:25 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 26 11:35:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.539	152	7279	0.400	ng/ul	0.00
4) Naphthalene-d8	10.299	136	23246	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.178	164	13264	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.023	188	2004884	0.400	ng/ul	0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.13
23) Perylene-d12	23.282	264	28265	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.134	96	34505	4.110	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.899	152	9139	0.293	ng/ul	0.00
18) Fluoranthene-d10	18.965	212	25751	0.000	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.164	88	208	0.021	ng/ul#	37
26) Benzo(a)pyrene	23.150	252	5954	0.069	ng/ul#	16


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122724\
Data File : BM049290.D
Acq On : 28 Dec 2024 13:20
Operator : RC/JU
Sample : P5324-14
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YE601


Quant Time: Dec 29 21:57:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 26 11:35:38 2024
Response via : Initial Calibration

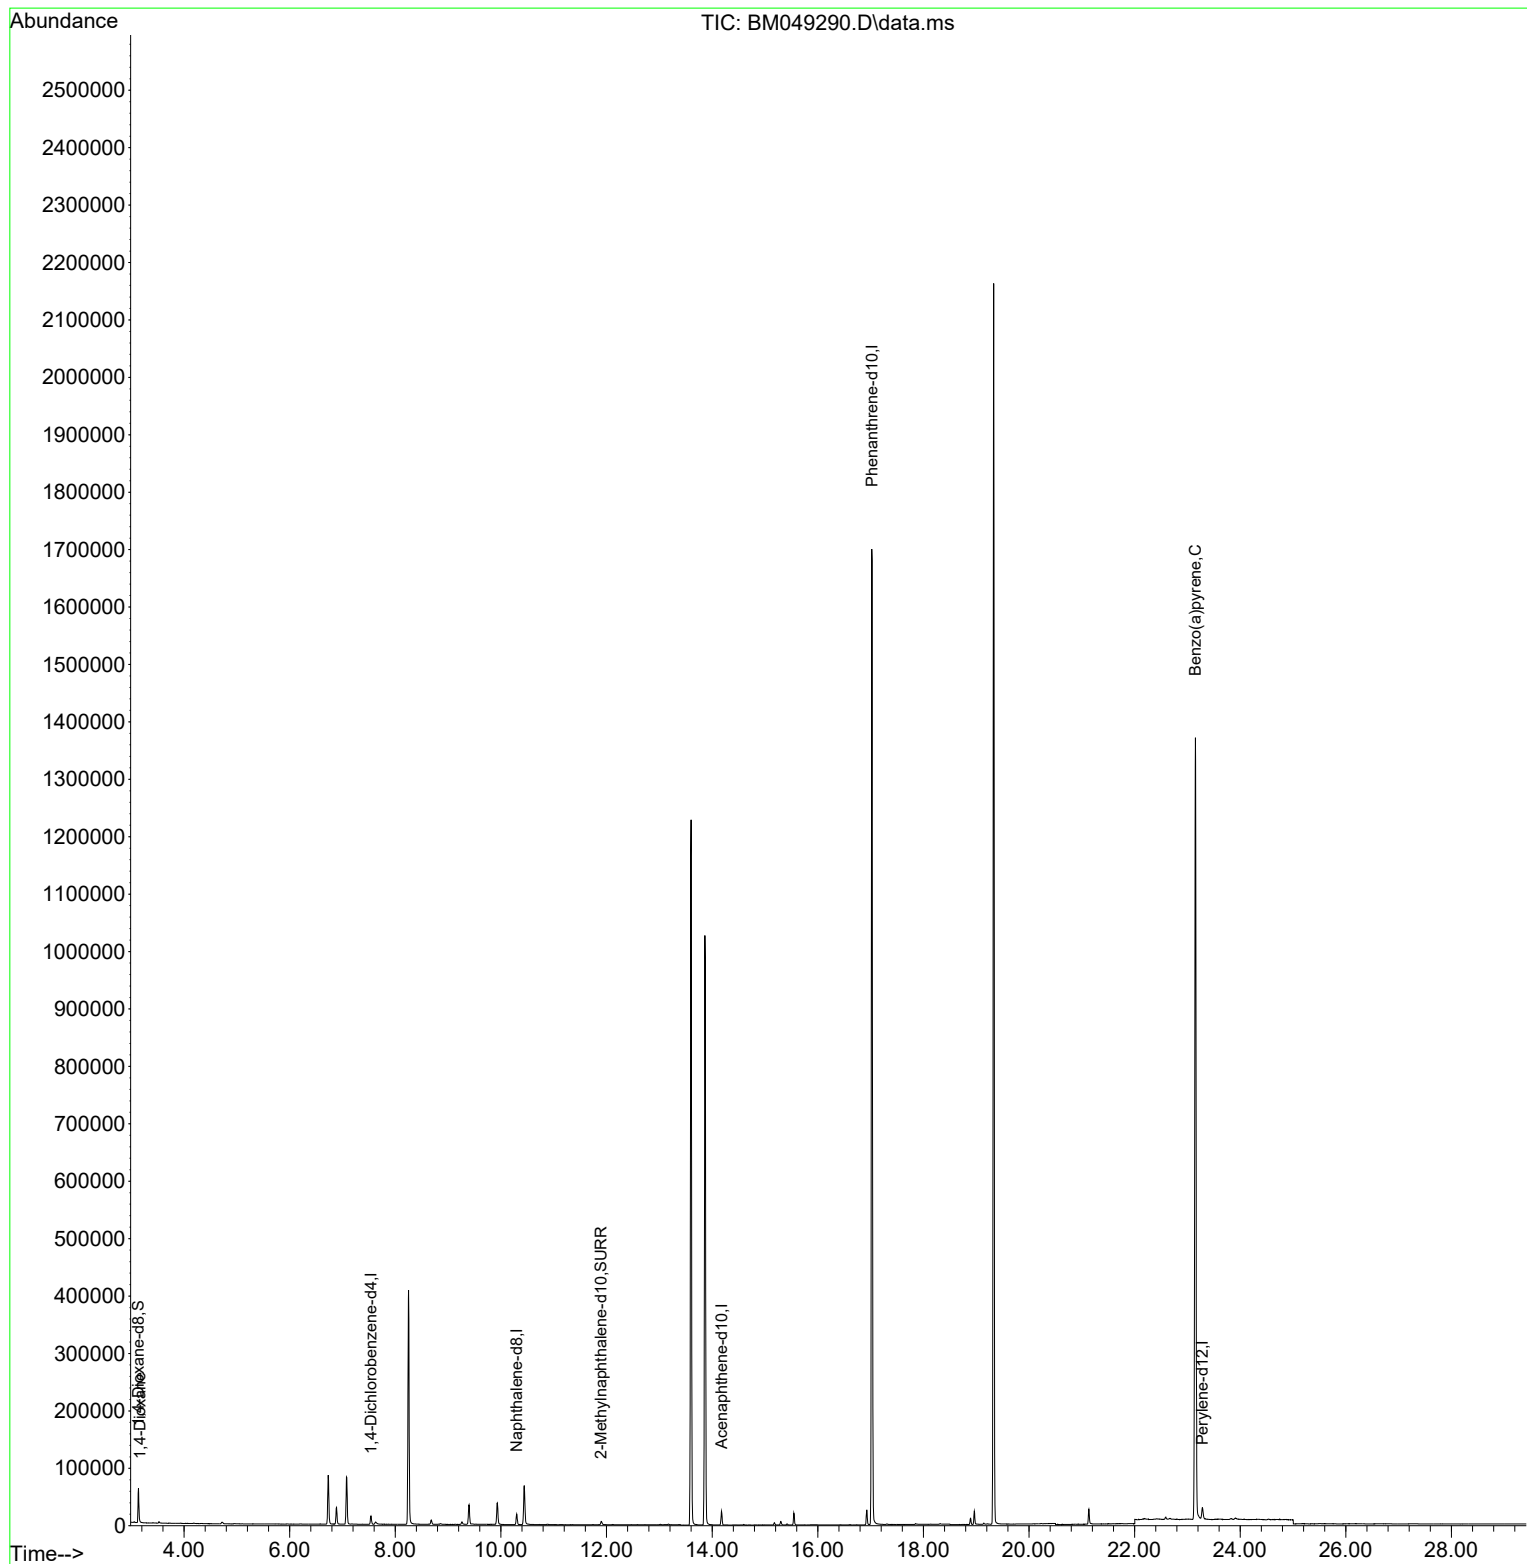



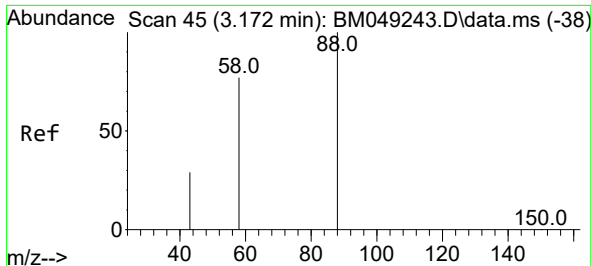


#2
1,4-Dioxane
Concen: 0.021 ng/ul
RT: 3.164 min Scan# 41
Delta R.T. -0.013 min
Lab File: BM049290.D
Acq: 28 Dec 2024 13:20


Instrument :
BNA_M
ClientSampleId :
YE601

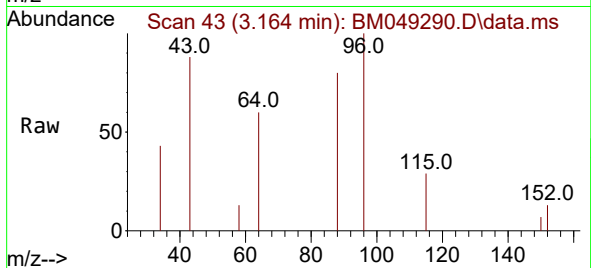

Tgt Ion: 88 Resp: 208
Ion Ratio Lower Upper
88 100
43 111.0 45.4 68.2#
58 16.6 43.6 65.4#

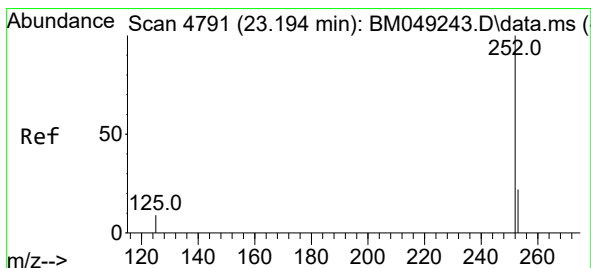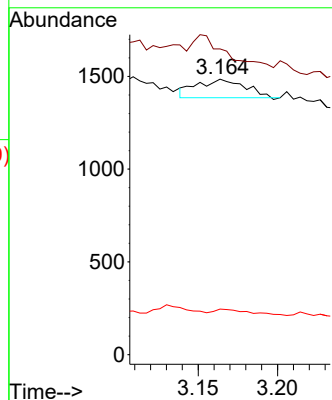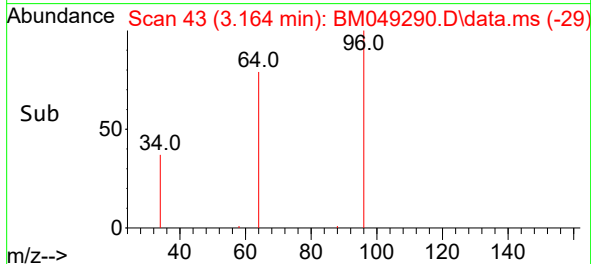

#26
Benzo(a)pyrene
Concen: 0.069 ng/ul
RT: 23.150 min Scan# 4776
Delta R.T. -0.041 min
Lab File: BM049290.D
Acq: 28 Dec 2024 13:20

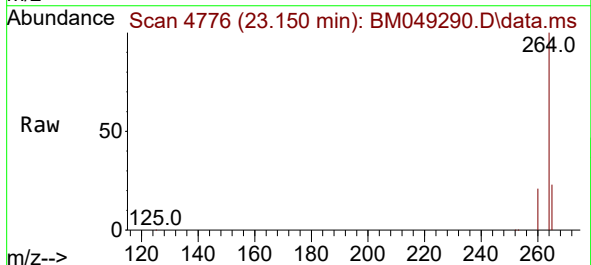

Tgt Ion: 252 Resp: 5954
Ion Ratio Lower Upper
252 100
253 53.7 22.4 33.6#
125 80.2 14.8 22.2#

