




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122724\
Data File : BM049274.D
Acq On : 28 Dec 2024 03:11
Operator : RC/JU
Sample : P5378-02
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YE633

Manual IntegrationsAPPROVED

Quant Time: Dec 28 03:45:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 26 11:35:38 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/30/2024
Supervised By :mohammad ahmed 12/30/2024

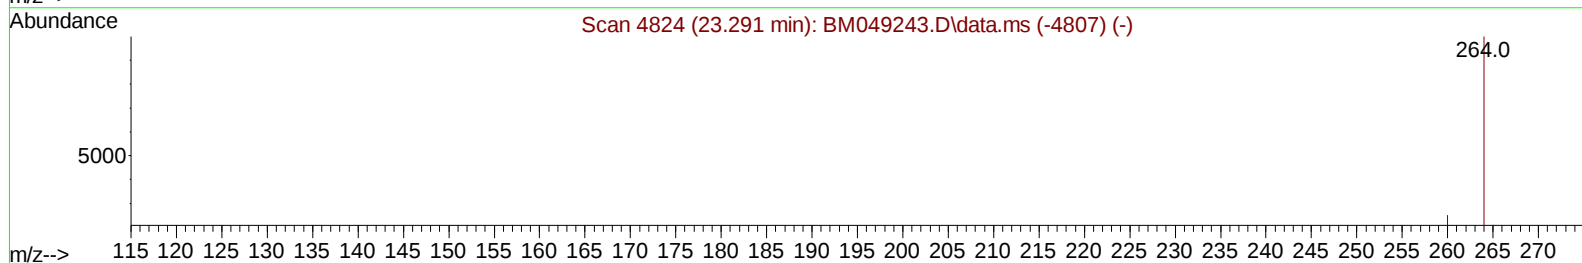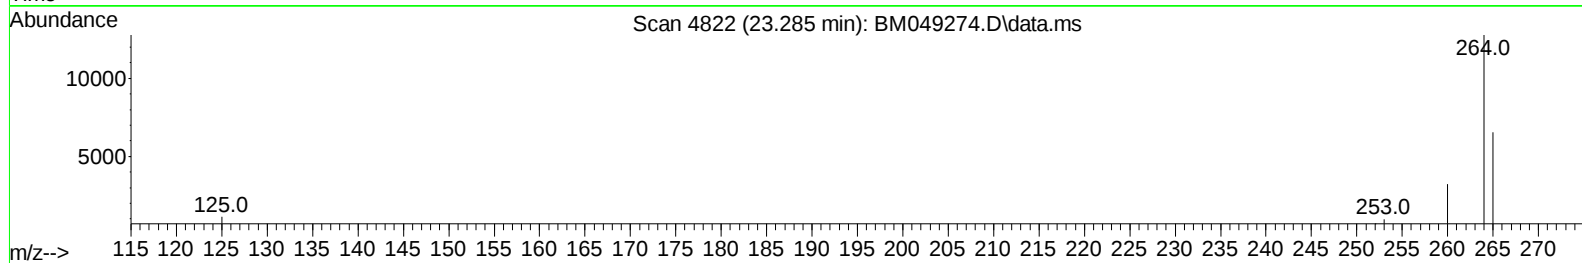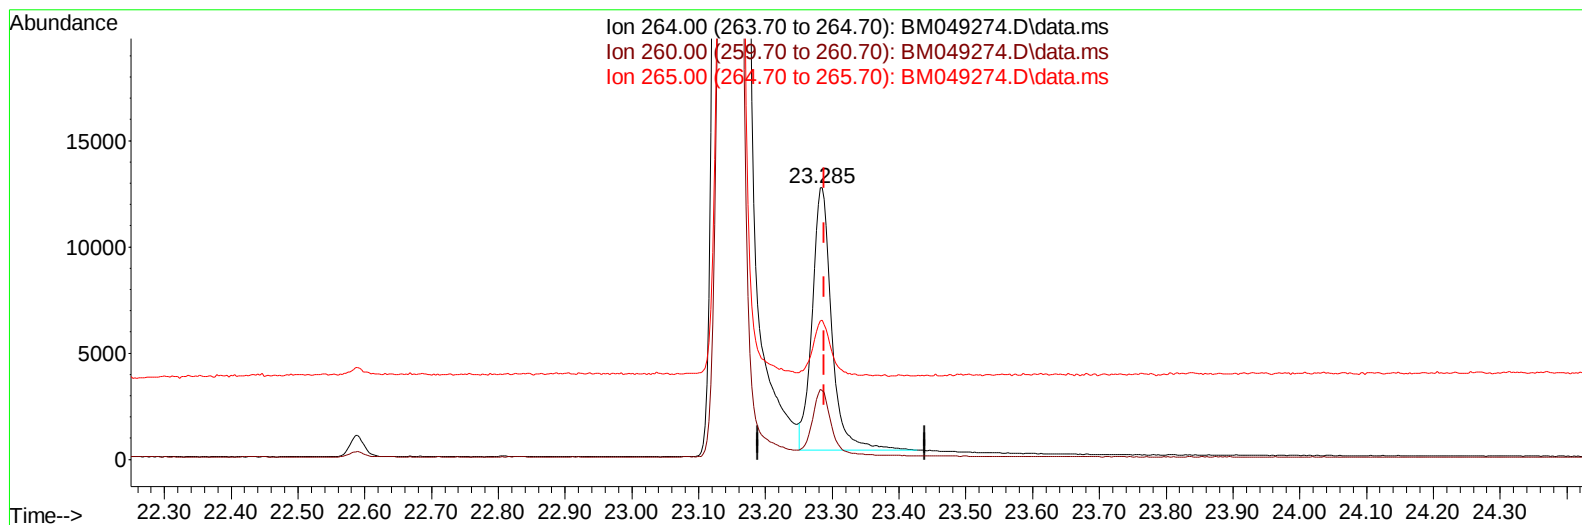

TIC: BM049274.D\data.ms

(23) Perylene-d12 (I)

23.285min (-0.003) 0.40 ng/u1

response 25446

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.80	25.43
265.00	78.30	51.18#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122724\
Data File : BM049274.D
Acq On : 28 Dec 2024 03:11
Operator : RC/JU
Sample : P5378-02
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YE633

Manual IntegrationsAPPROVED

Quant Time: Dec 28 03:45:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 26 11:35:38 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/30/2024
Supervised By :mohammad ahmed 12/30/2024

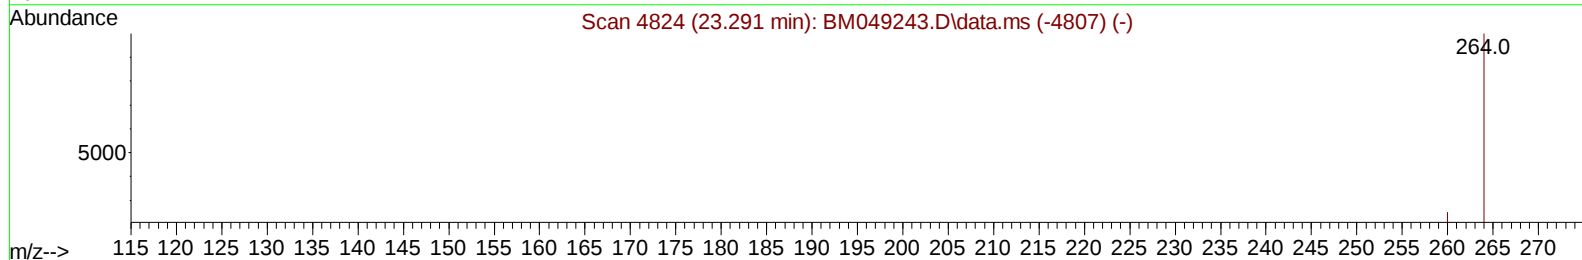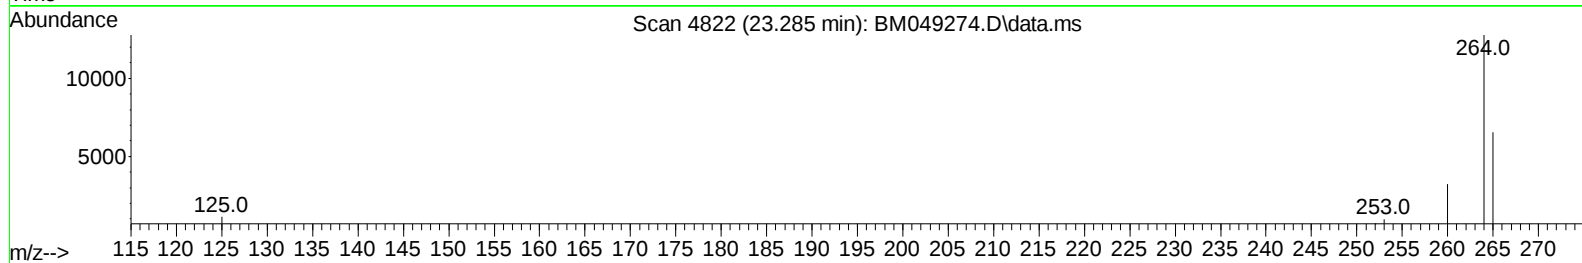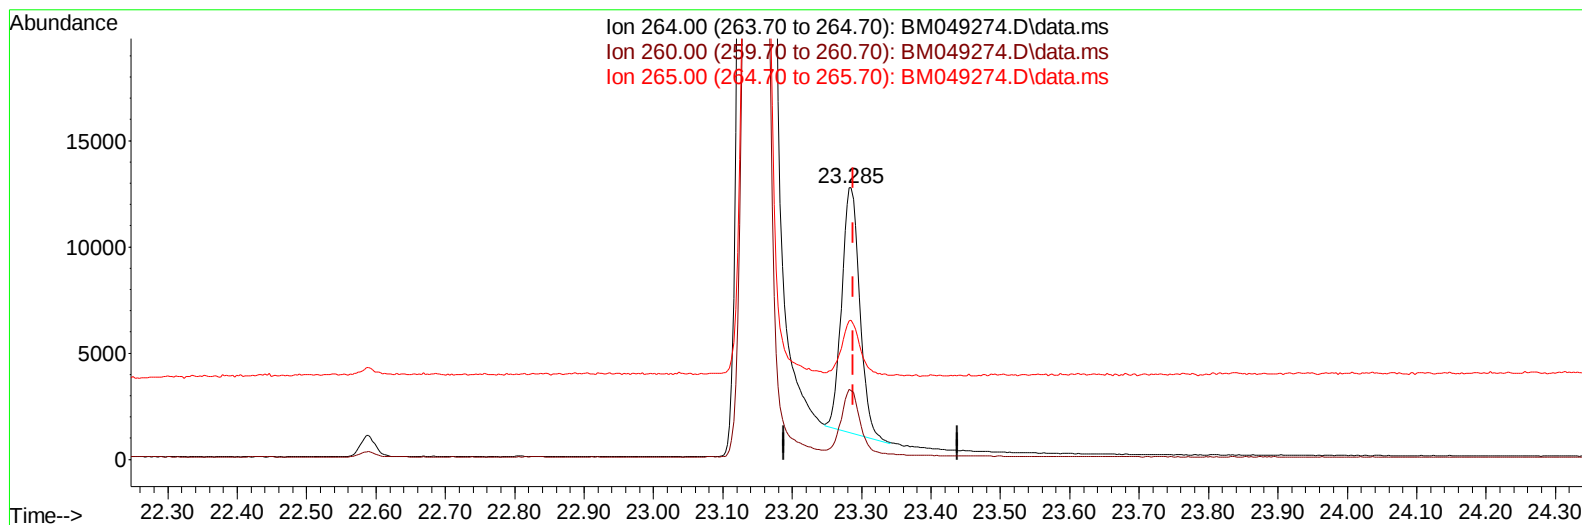

TIC: BM049274.D\data.ms

(23) Perylene-d12 (I)

23.285min (-0.003) 0.40 ng/ul m

response 20837

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.80	25.43
265.00	78.30	51.18#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122724\
 Data File : BM049274.D
 Acq On : 28 Dec 2024 03:11
 Operator : RC/JU
 Sample : P5378-02
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YE633

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/30/2024
 Supervised By :mohammad ahmed 12/30/2024

Quant Time: Dec 28 03:45:34 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 26 11:35:38 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.539	152		5457	0.400	ng/ul	0.00
4) Naphthalene-d8	10.299	136		17319	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.178	164		10640	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.926	188		25195	0.400	ng/ul	0.00
17) Chrysene-d12	21.134	240		22214	0.400	ng/ul	0.00
23) Perylene-d12	23.285	264		20837m	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.139	96		14743	2.343	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.899	152		3504	0.151	ng/ul	0.00
18) Fluoranthene-d10	18.965	212		9299	0.148	ng/ul	0.00
Target Compounds							
							Qvalue
2) 1,4-Dioxane	3.172	88		4101	0.557	ng/ul#	86

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122724\
Data File : BM049274.D
Acq On : 28 Dec 2024 03:11
Operator : RC/JU
Sample : P5378-02
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YE633

Manual IntegrationsAPPROVED

Quant Time: Dec 28 03:45:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 26 11:35:38 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/30/2024
Supervised By :mohammad ahmed 12/30/2024

