

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122724\
 Data File : BM049247.D
 Acq On : 27 Dec 2024 09:54
 Operator : RC/JU
 Sample : P5333-12DL 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E2914DL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/30/2024
 Supervised By :mohammad ahmed 12/30/2024

Quant Time: Dec 27 22:11:24 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 26 11:35:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.544	152	3234	0.400	ng/ul	0.00
4) Naphthalene-d8	10.308	136	9579	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.182	164	5888	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.929	188	13196	0.400	ng/ul	0.00
17) Chrysene-d12	21.135	240	11818	0.400	ng/ul	0.00
23) Perylene-d12	23.286	264	12851	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.139	96	2417	0.648	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.914	152	505	0.039	ng/ul	0.00
18) Fluoranthene-d10	18.968	212	961	0.029	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.358	128	3537	0.148	ng/ul#	93
7) 2-Methylnaphthalene	11.986	142	2974	0.196	ng/ul	99
8) 1-Methylnaphthalene	12.206	142	1336	0.086	ng/ul	97
11) Acenaphthene	14.242	153	391	0.022	ng/ul#	87
15) Phenanthrene	16.971	178	11232	0.326	ng/ul	100
16) Anthracene	17.064	178	1462	0.046	ng/ul#	83
19) Fluoranthene	18.996	202	18139	0.425	ng/ul	99
20) Pyrene	19.359	202	16792	0.368	ng/ul	99
21) Benzo(a)anthracene	21.117	228	12662	0.308	ng/ul	97
22) Chrysene	21.170	228	18641	0.423	ng/ul	96
24) Benzo(b)fluoranthene	22.645	252	31404m	0.765	ng/ul	
25) Benzo(k)fluoranthene	22.683	252	12315m	0.273	ng/ul	
26) Benzo(a)pyrene	23.189	252	12269	0.312	ng/ul	98
27) Indeno(1,2,3-cd)pyrene	25.414	276	14392	0.258	ng/ul#	92
28) Dibenzo(a,h)anthracene	25.424	278	4067	0.094	ng/ul#	80
29) Benzo(g,h,i)perylene	26.061	276	2282	0.051	ng/ul#	73

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122724\
Data File : BM049247.D
Acq On : 27 Dec 2024 09:54
Operator : RC/JU
Sample : P5333-12DL 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
E2914DL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/30/2024
Supervised By :mohammad ahmed 12/30/2024


Quant Time: Dec 27 22:11:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 26 11:35:38 2024
Response via : Initial Calibration

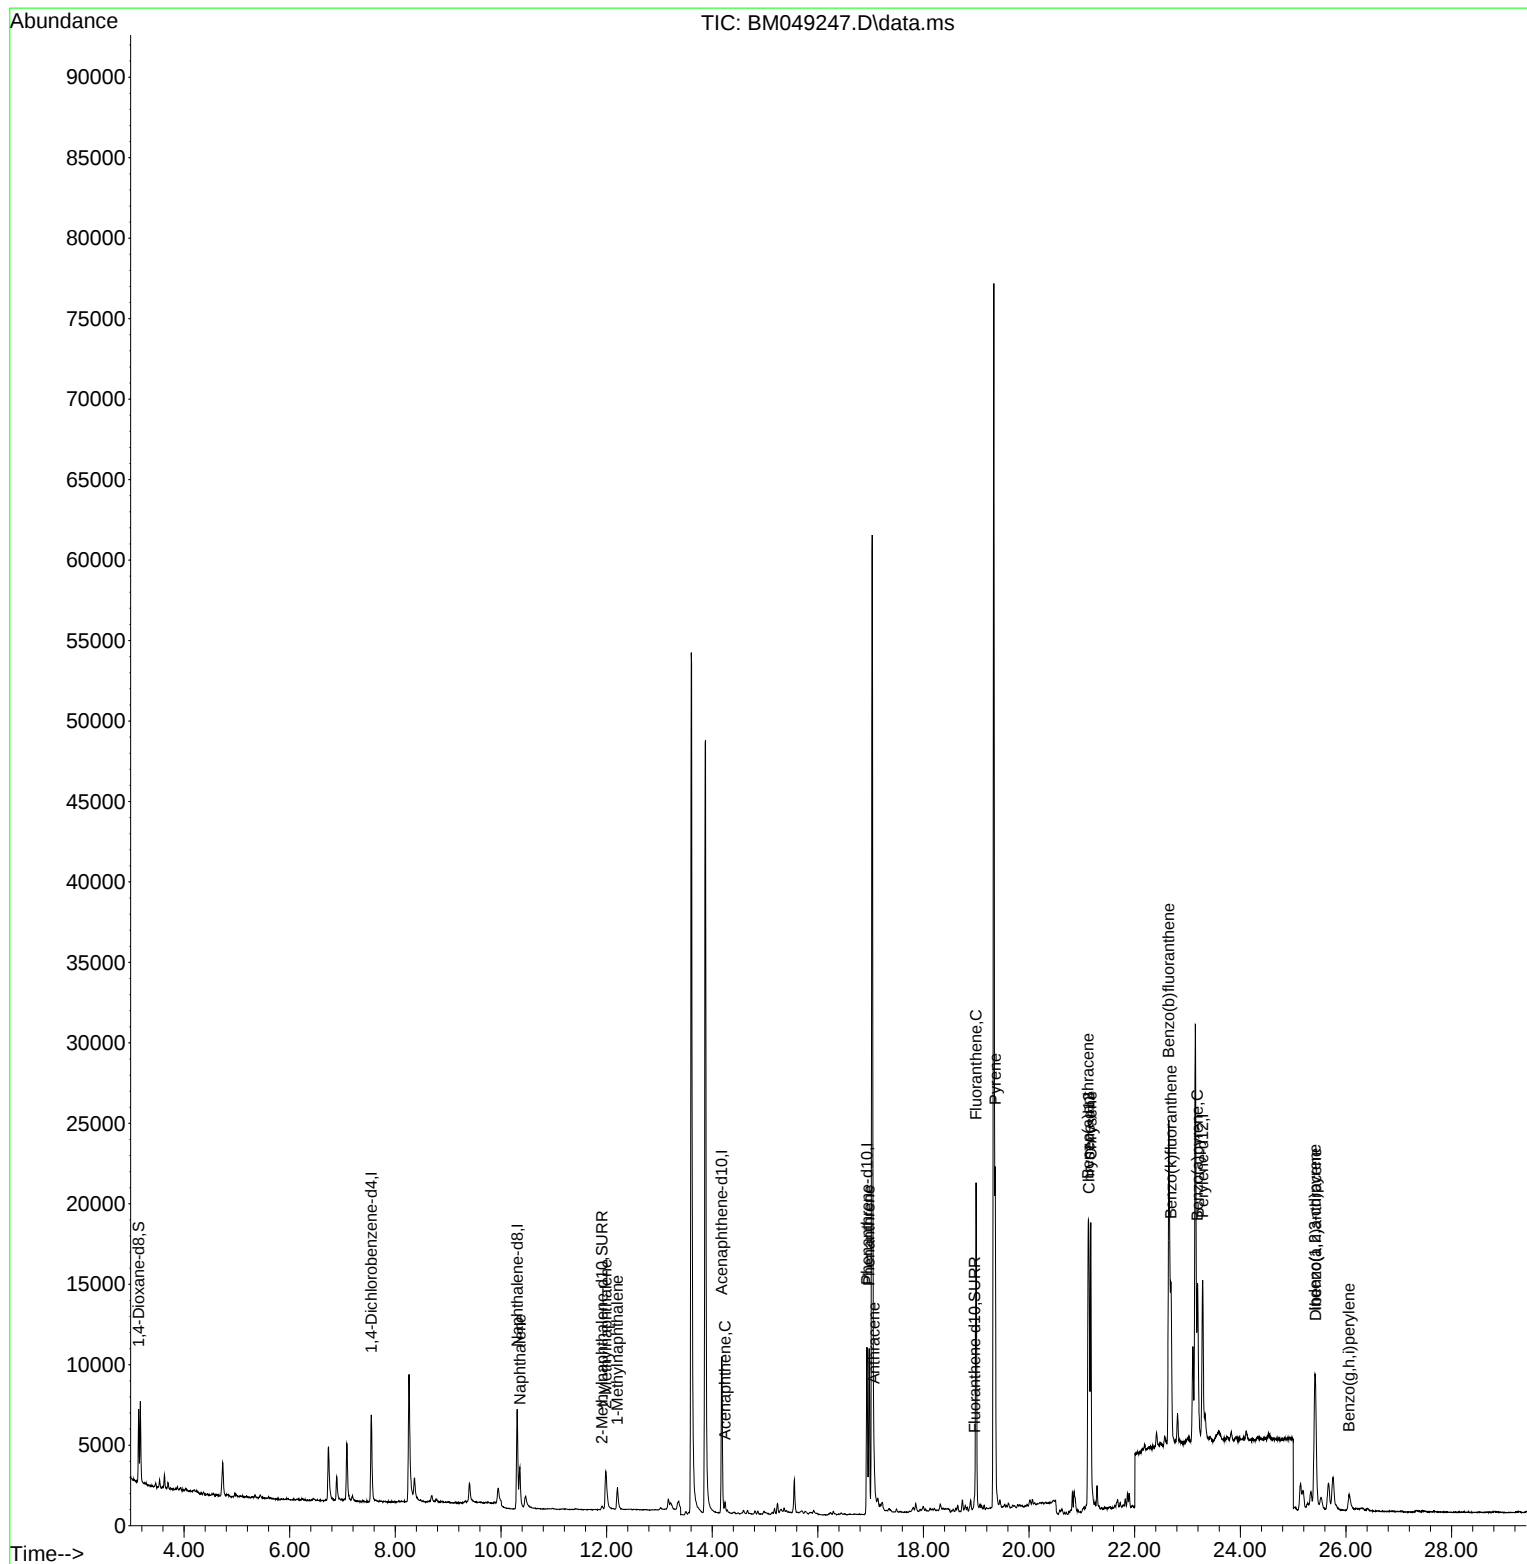



#5
Naphthalene
Concen: 0.148 ng/ul
RT: 10.358 min Scan# 1732
Delta R.T. 0.000 min
Lab File: BM049247.D
Acq: 27 Dec 2024 09:54




Instrument :
BNA_M
ClientSampleId :
E2914DL



Tgt Ion:128 Resp: 3537
Ion Ratio Lower Upper
128 100
129 14.9 9.7 14.5
127 16.0 10.6 16.0




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 12/30/2024
Supervised By :mohammad ahmed 12/30/2024

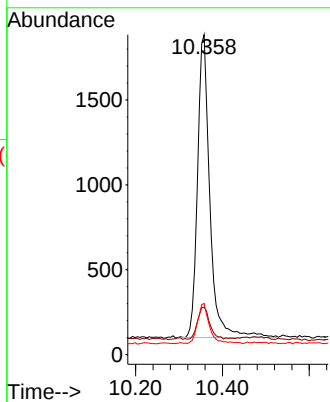

#7
2-Methylnaphthalene
Concen: 0.196 ng/ul
RT: 11.986 min Scan# 2028
Delta R.T. 0.006 min
Lab File: BM049247.D
Acq: 27 Dec 2024 09:54

Tgt Ion:142 Resp: 2974
Ion Ratio Lower Upper
142 100
141 90.9 71.7 107.5

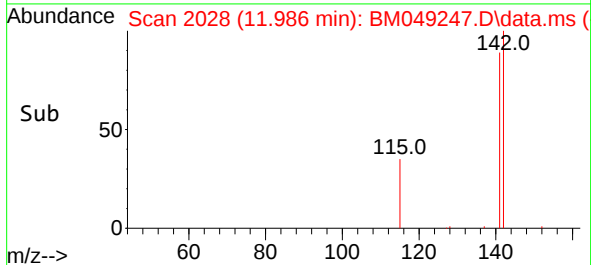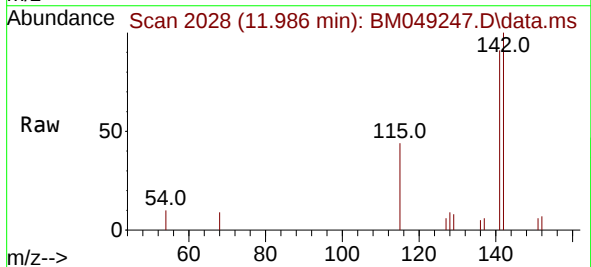



#8

1-Methylnaphthalene

Concen: 0.086 ng/ul

RT: 12.206 min Scan# 2067

Delta R.T. 0.000 min

Lab File: BM049247.D

Acq: 27 Dec 2024 09:54

Instrument :

BNA_M

ClientSampleId :

E2914DL

Tgt Ion:142 Resp: 1330

Ion Ratio Lower Upper

142 100





141 88.5 72.7 109.1

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 12/30/2024

Supervised By :mohammad ahmed 12/30/2024



#11

Acenaphthene

Concen: 0.022 ng/ul

RT: 14.242 min Scan# 2467

Delta R.T. -0.004 min

Lab File: BM049247.D

Acq: 27 Dec 2024 09:54




Tgt Ion:153 Resp: 391


Ion Ratio Lower Upper

153 100

152 68.3 40.7 61.1#


154 94.1 70.8 106.2

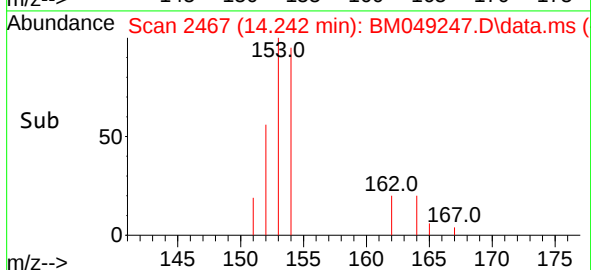



#15
Phenanthrene
Concen: 0.326 ng/ul
RT: 16.971 min Scan# 3077
Delta R.T. -0.004 min
Lab File: BM049247.D
Acq: 27 Dec 2024 09:54




Instrument :
BNA_M
ClientSampleId :
E2914DL



Tgt Ion:178 Resp: 1123
Ion Ratio Lower Upper
178 100
179 16.5 13.0 19.4
176 20.3 16.2 24.2




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 12/30/2024
Supervised By :mohammad ahmed 12/30/2024



#16
Anthracene
Concen: 0.046 ng/ul
RT: 17.064 min Scan# 3099
Delta R.T. -0.004 min
Lab File: BM049247.D
Acq: 27 Dec 2024 09:54


Tgt Ion:178 Resp: 1462
Ion Ratio Lower Upper
178 100
179 24.8 12.9 19.3#
176 25.4 15.3 22.9#

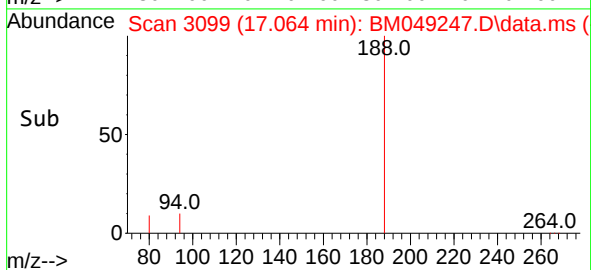



#19
Fluoranthene
Concen: 0.425 ng/ul
RT: 18.996 min Scan# 3547
Delta R.T. -0.004 min
Lab File: BM049247.D
Acq: 27 Dec 2024 09:54




Instrument :
BNA_M
ClientSampleId :
E2914DL




Tgt Ion:202 Resp: 18139
Ion Ratio Lower Upper
202 100
101 9.1 7.6 11.4
100 7.3 5.5 8.3

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 12/30/2024
Supervised By :mohammad ahmed 12/30/2024




#20
Pyrene
Concen: 0.368 ng/ul
RT: 19.359 min Scan# 3624
Delta R.T. -0.004 min
Lab File: BM049247.D
Acq: 27 Dec 2024 09:54




Tgt Ion:202 Resp: 16792
Ion Ratio Lower Upper
202 100
101 11.3 8.9 13.3
100 9.1 6.9 10.3

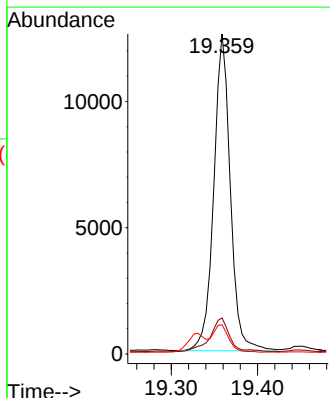



#21
Benzo(a)anthracene
Concen: 0.308 ng/ul
RT: 21.117 min Scan# 4080
Delta R.T. -0.003 min
Lab File: BM049247.D
Acq: 27 Dec 2024 09:54




Instrument :
BNA_M
ClientSampleId :
E2914DL




Tgt Ion:228 Resp: 12662
Ion Ratio Lower Upper
228 100
229 22.7 15.9 23.9
226 28.8 22.6 34.0

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 12/30/2024
Supervised By :mohammad ahmed 12/30/2024




#22
Chrysene
Concen: 0.423 ng/ul
RT: 21.170 min Scan# 4098
Delta R.T. -0.003 min
Lab File: BM049247.D
Acq: 27 Dec 2024 09:54

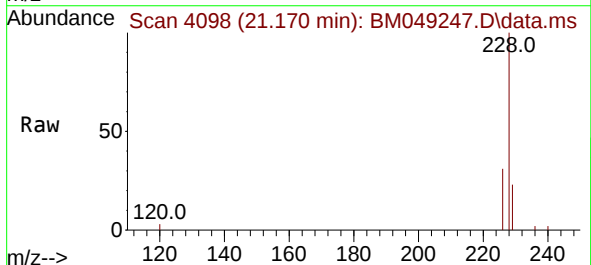


Tgt Ion:228 Resp: 18641
Ion Ratio Lower Upper
228 100
226 30.9 24.1 36.1
229 22.9 15.8 23.8

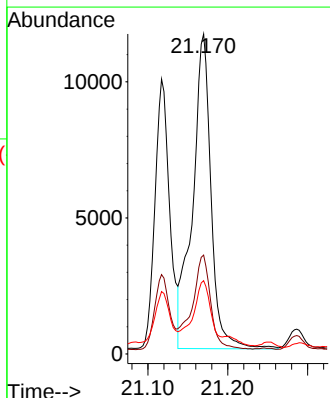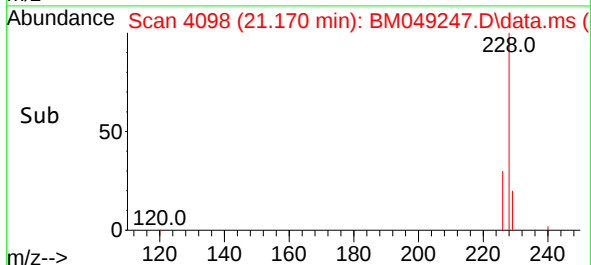



#24
Benzo(b)fluoranthene
Concen: 0.765 ng/ul m
RT: 22.645 min Scan# 4603
Delta R.T. -0.003 min
Lab File: BM049247.D
Acq: 27 Dec 2024 09:54




Instrument :
BNA_M
ClientSampleId :
E2914DL



Tgt Ion:252 Resp: 31404
Ion Ratio Lower Upper
252 100
253 25.7 0.0 52.6
125 13.0 0.0 30.8




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 12/30/2024
Supervised By :mohammad ahmed 12/30/2024



#25
Benzo(k)fluoranthene
Concen: 0.273 ng/ul m
RT: 22.683 min Scan# 4616
Delta R.T. -0.009 min
Lab File: BM049247.D
Acq: 27 Dec 2024 09:54


Tgt Ion:252 Resp: 12315
Ion Ratio Lower Upper
252 100
253 29.0 21.3 31.9
125 19.6 12.6 18.8#

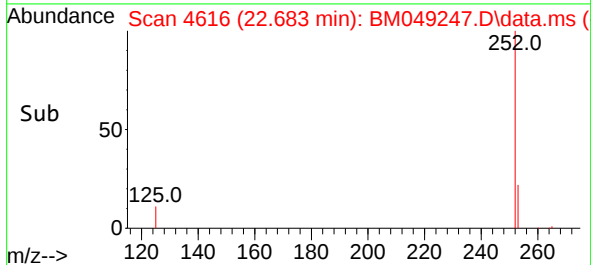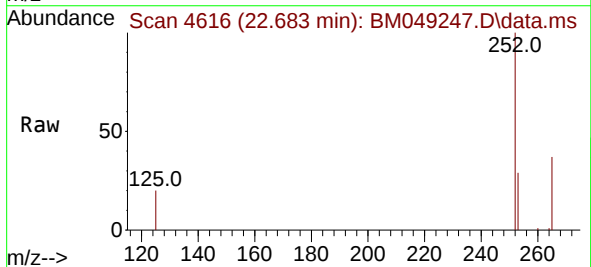



#26
Benzo(a)pyrene
Concen: 0.312 ng/ul
RT: 23.189 min Scan# 4789
Delta R.T. -0.003 min
Lab File: BM049247.D
Acq: 27 Dec 2024 09:54




Instrument :
BNA_M
ClientSampleId :
E2914DL




Tgt Ion:252 Resp: 12269
Ion Ratio Lower Upper
252 100
253 29.0 22.4 33.6
125 19.0 14.8 22.2

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 12/30/2024
Supervised By :mohammad ahmed 12/30/2024

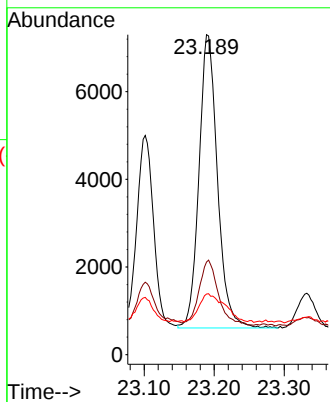


#27
Indeno(1,2,3-cd)pyrene
Concen: 0.258 ng/ul
RT: 25.414 min Scan# 5532
Delta R.T. -0.003 min
Lab File: BM049247.D
Acq: 27 Dec 2024 09:54

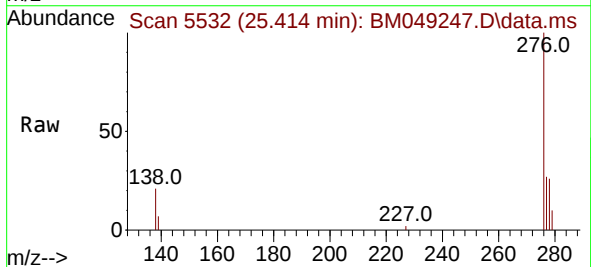


Tgt Ion:276 Resp: 14392
Ion Ratio Lower Upper
276 100
138 17.9 17.4 26.2
227 0.3 0.2 0.2#

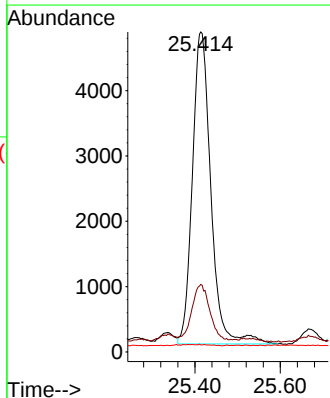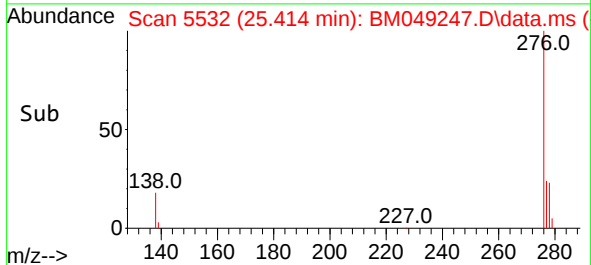



#28
Dibenzo(a,h)anthracene
Concen: 0.094 ng/ul
RT: 25.424 min Scan# 51
Delta R.T. -0.013 min
Lab File: BM049247.D
Acq: 27 Dec 2024 09:54




Instrument :
BNA_M
ClientSampleId :
E2914DL




Tgt Ion:278 Resp: 406
Ion Ratio Lower Upper
278 100
139 23.3 13.5 20.3
279 38.6 21.5 32.3

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/30/2024
Supervised By :mohammad ahmed 12/30/2024

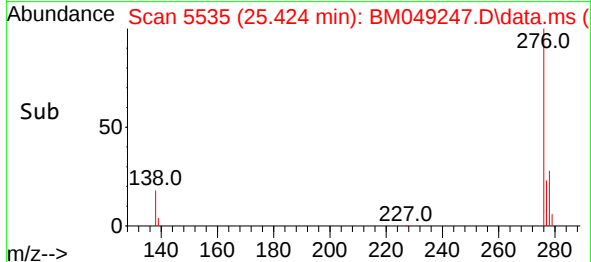

#29
Benzo(g,h,i)perylene
Concen: 0.051 ng/ul
RT: 26.061 min Scan# 5725
Delta R.T. -0.007 min
Lab File: BM049247.D
Acq: 27 Dec 2024 09:54



Tgt Ion:276 Resp: 2282
Ion Ratio Lower Upper
276 100
138 35.6 16.7 25.1#
277 36.6 19.9 29.9#

