

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122724\
 Data File : BM049262.D
 Acq On : 27 Dec 2024 20:02
 Operator : RC/JU
 Sample : P5324-15
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YE630

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/30/2024
 Supervised By :mohammad ahmed 12/30/2024

Quant Time: Dec 27 22:13:36 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 26 11:35:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.539	152	3971	0.400	ng/ul	0.00
4) Naphthalene-d8	10.303	136	11604	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.177	164	7351	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.929	188	18354m	0.400	ng/ul	0.00
17) Chrysene-d12	21.132	240	17565m	0.400	ng/ul	0.00
23) Perylene-d12	23.285	264	15901m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.139	96	17115	3.737	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.898	152	4389	0.281	ng/ul	-0.01
18) Fluoranthene-d10	18.964	212	12800	0.257	ng/ul	0.00
Target Compounds					Qvalue	
2) 1,4-Dioxane	3.172	88	1140	0.213	ng/ul#	82

(#) = qualifier out of range (m) = manual integration (+) = signals summed


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122724\
Data File : BM049262.D
Acq On    : 27 Dec 2024   20:02
Operator  : RC/JU
Sample    : P5324-15
Misc      :
ALS Vial  : 22   Sample Multiplier: 1
```


Instrument :
BNA_M
ClientSampleId :
YE630

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/30/2024
Supervised By :mohammad ahmed 12/30/2024


Quant Time: Dec 27 22:13:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 26 11:35:38 2024
Response via : Initial Calibration

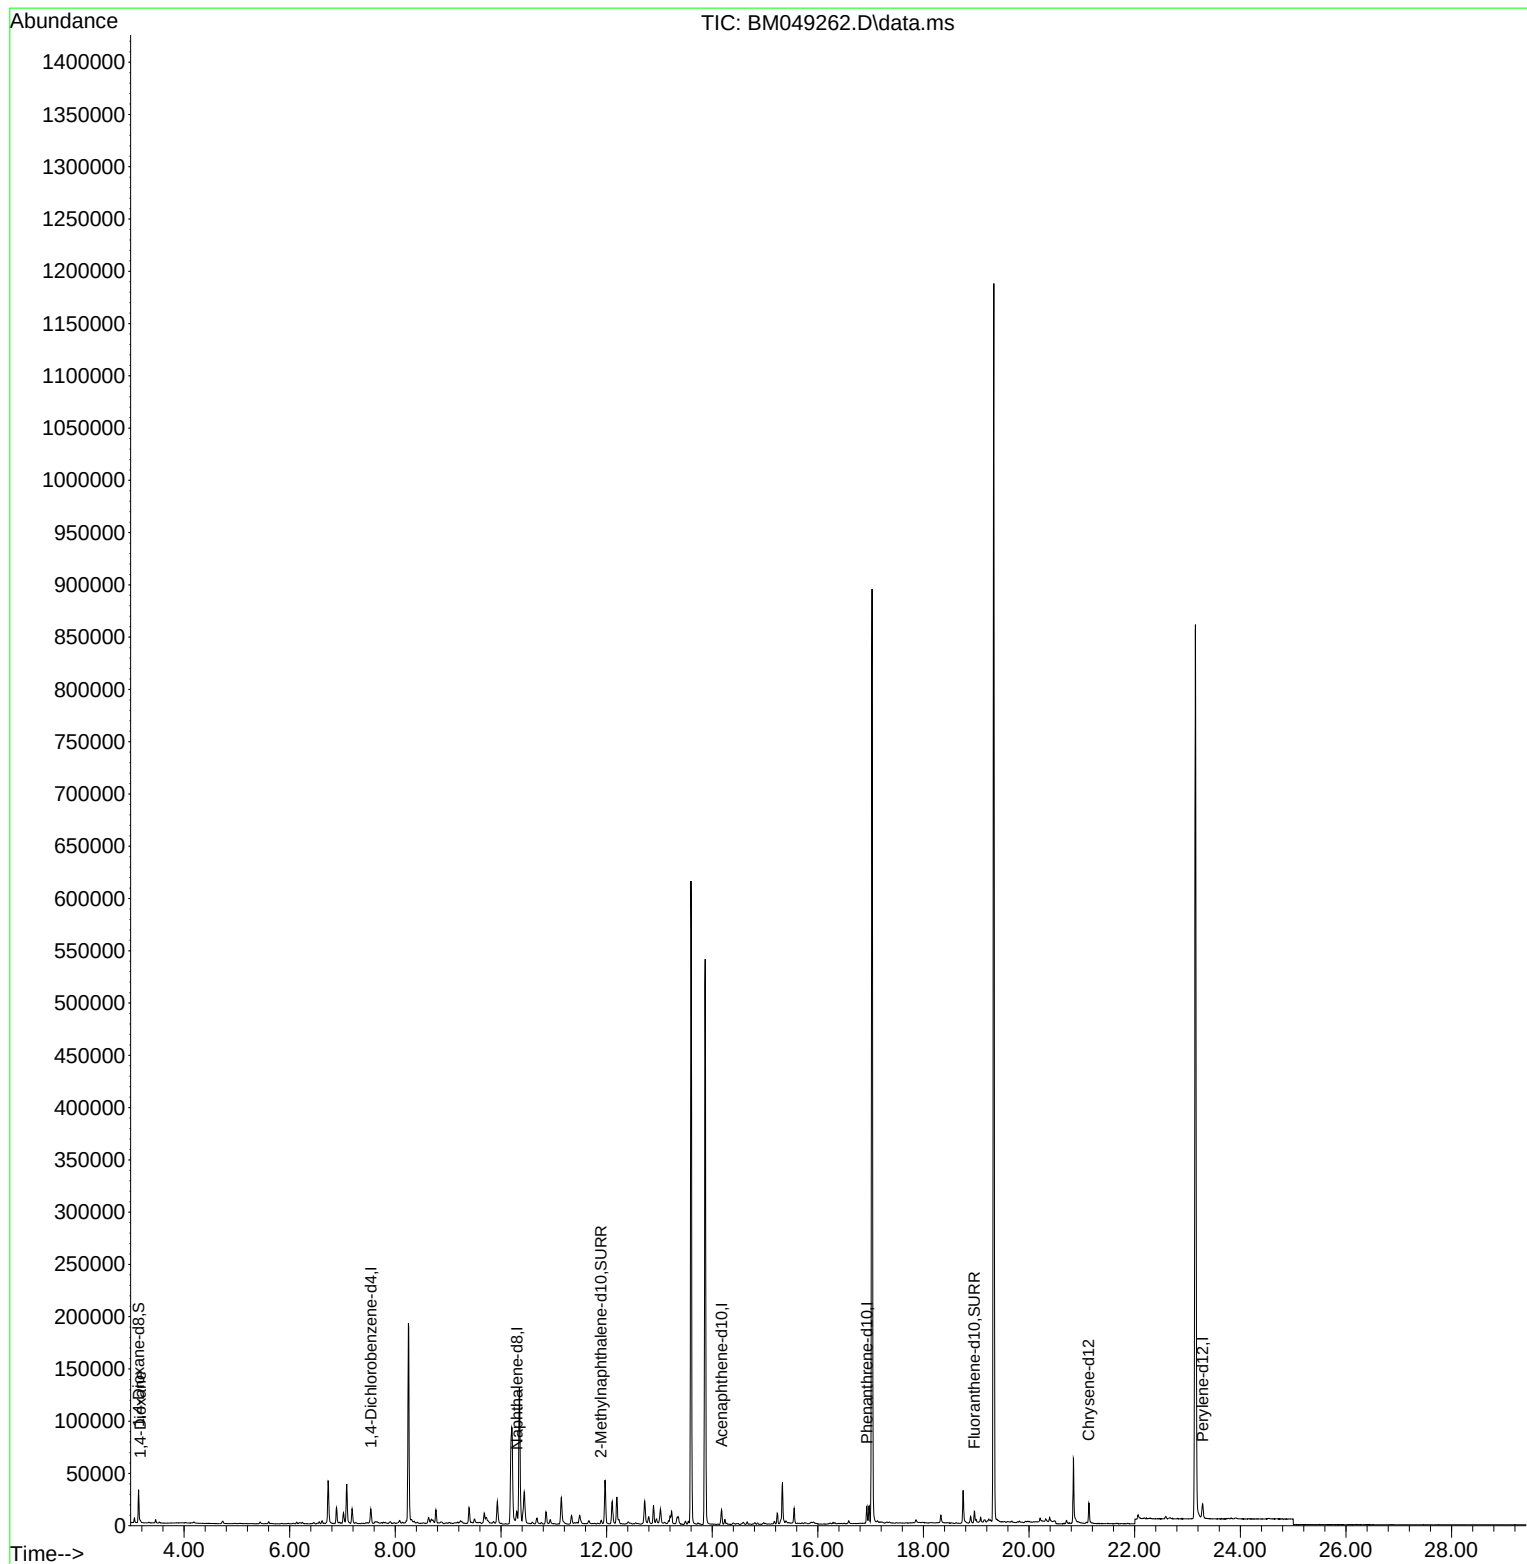

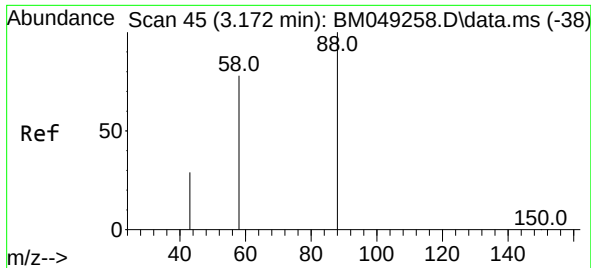

#2
 1,4-Dioxane
 Concen: 0.213 ng/ul
 RT: 3.172 min Scan# 41
 Delta R.T. -0.004 min
 Lab File: BM049262.D
 Acq: 27 Dec 2024 20:02

Instrument :
 BNA_M
 ClientSampleId :
 YE630

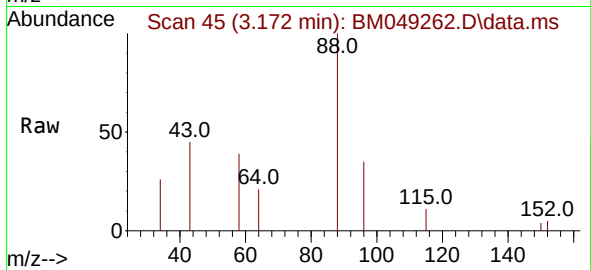

Tgt Ion: 88 Resp: 1140

Ion	Ratio	Lower	Upper
88	100		
43	45.2	45.4	68.2
58	39.3	43.6	65.4

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/30/2024
 Supervised By :mohammad ahmed 12/30/2024

