
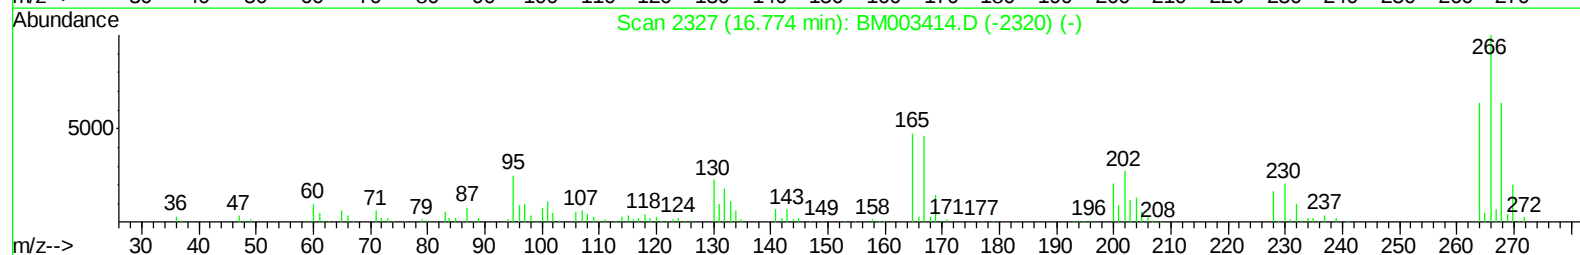
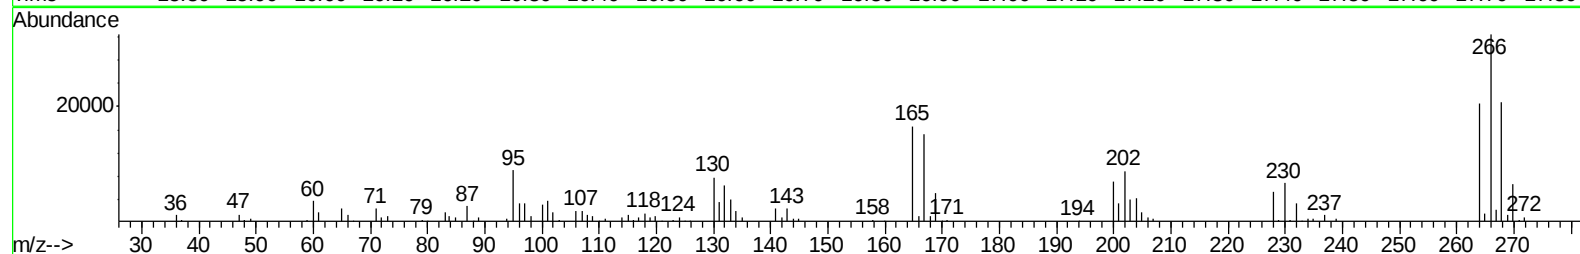


Data Path : Z:\HPCHEM1\BNA_M\Data\BM122815\
Data File : BM003819.D
Acq On : 28 Dec 2015 08:46
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 29 07:09:32 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM120915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 09 18:52:47 2015
Response via : Initial Calibration

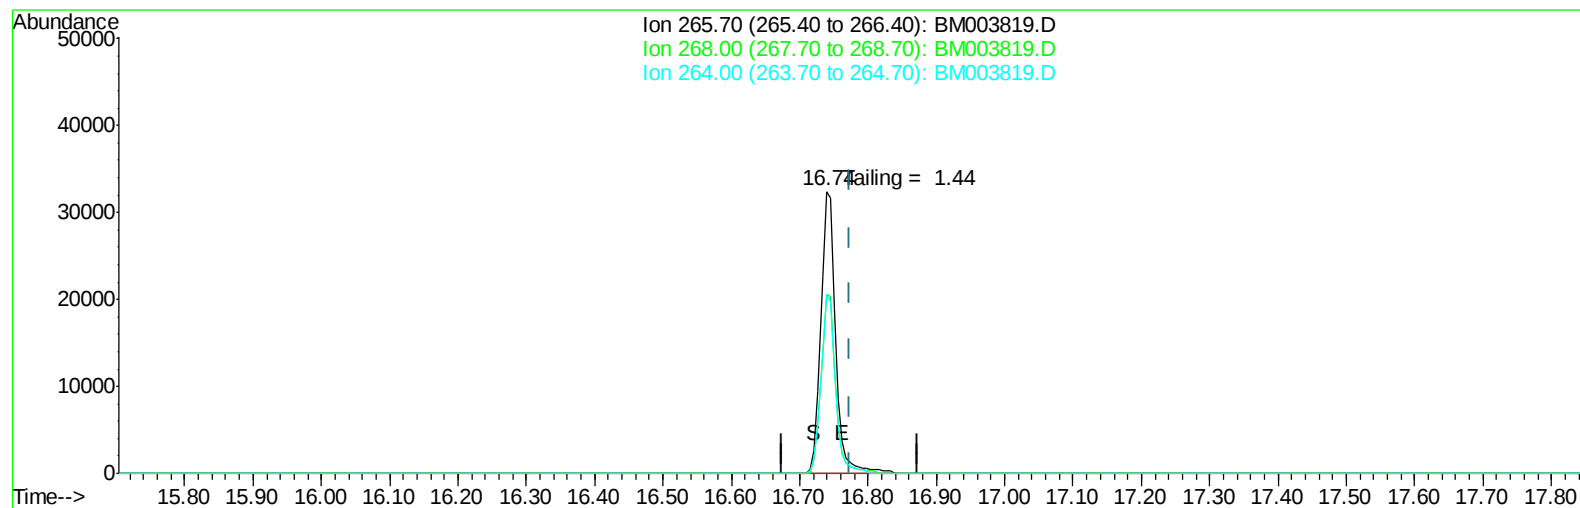

TIC: BM003819.D

(69) Pentachlorophenol (C)




16.739min (-0.035) 0.00ng

response 48806

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	63.83
264.00	61.20	63.69
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\Data\BM122815\
Data File : BM003819.D
Acq On : 28 Dec 2015 08:46
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 29 07:09:32 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM120915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 09 18:52:47 2015
Response via : Initial Calibration

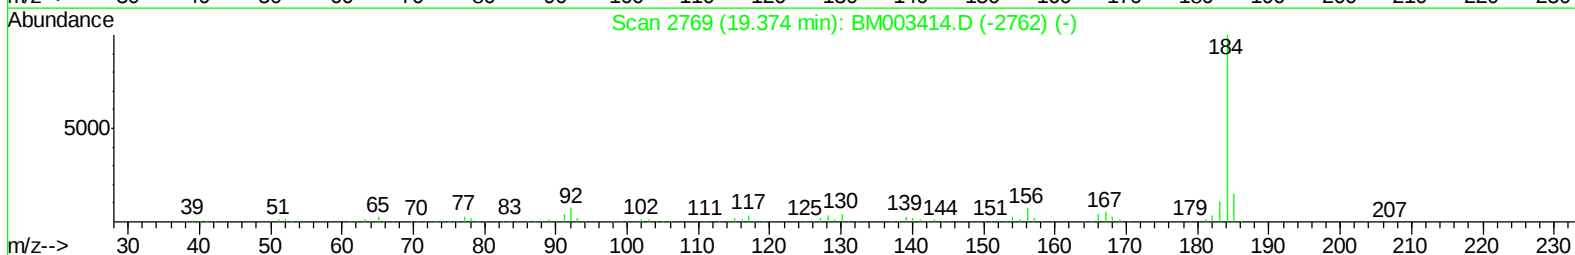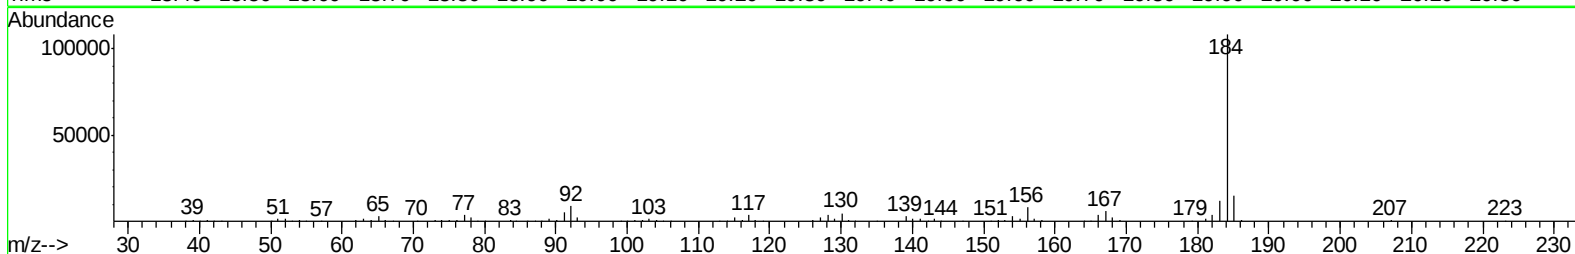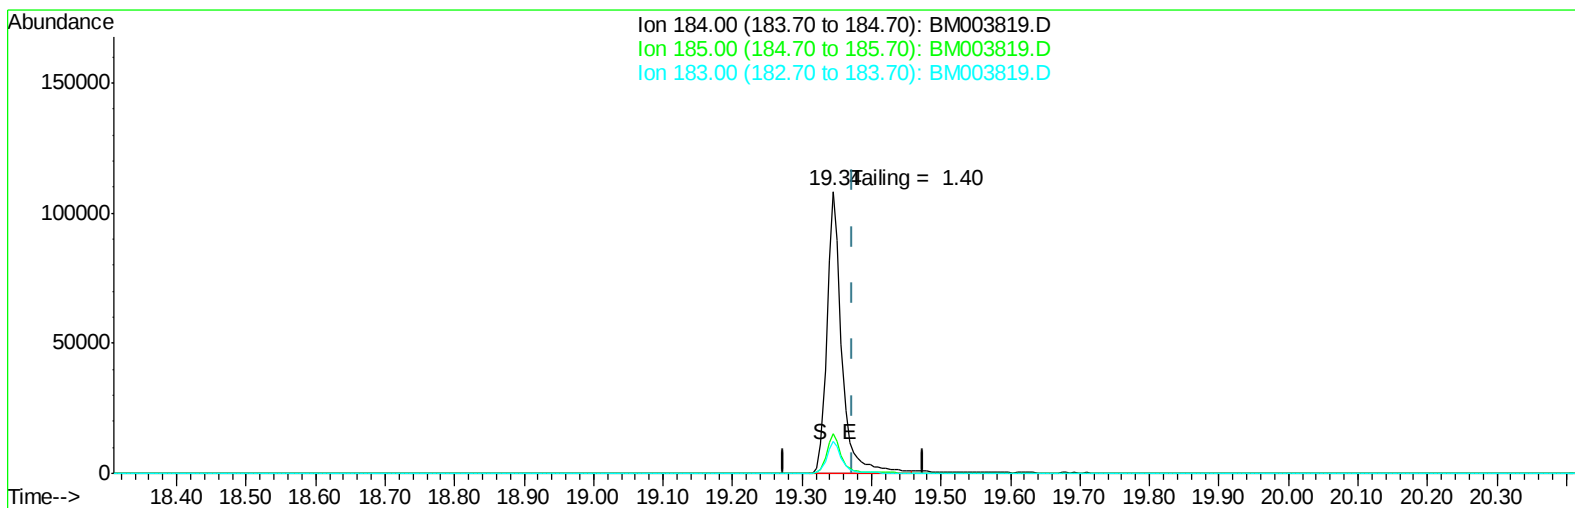

TIC: BM003819.D

(76) Benzidine

19.345min (-0.029) 642.61ng

response 158640

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.08
183.00	11.10	11.48
0.00	0.00	0.00