

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122816\
 Data File : BM008707.D
 Acq On : 28 Dec 2016 23:21
 Operator : UM/SJ
 Sample : H6067-05
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA7F6

Quant Time: Dec 29 03:34:30 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 29 03:29:39 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ng/ul	-7.82
2) Naphthalene-d8	10.43	136	1519	0.40	ng/ul	-0.13
6) Acenaphthene-d10	14.28	164	923	0.40	ng/ul	-0.07
10) Phenanthrene-d10	17.12	188	64052	0.40	ng/ul	0.02
16) Chrysene-d12	21.29	240	525	0.40	ng/ul	0.00
20) Perylene-d12	23.54	264	4142	0.40	ng/ul	0.01


System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.05	152	314	0.13	ng/ul	-0.11
14) Fluoranthene-d10	19.08	212	1065	0.01	ng/ul	-0.06


Target Compounds						Qvalue
3) Naphthalene	10.48	128	2543	0.60	ng/ul	97
5) 2-Methylnaphthalene	12.12	142	588	0.20	ng/ul	100
7) Acenaphthylene	14.00	152	47825	11.45	ng/ul#	94
8) Acenaphthene	14.35	153	1338	0.43	ng/ul#	89
9) Fluorene	15.34	166	3976	1.11	ng/ul	87

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122816\
Data File : BM008707.D
Acq On : 28 Dec 2016 23:21
Operator : UM/SJ
Sample : H6067-05
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA7F6

Quant Time: Dec 29 03:34:30 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 29 03:29:39 2016
Response via : Initial Calibration

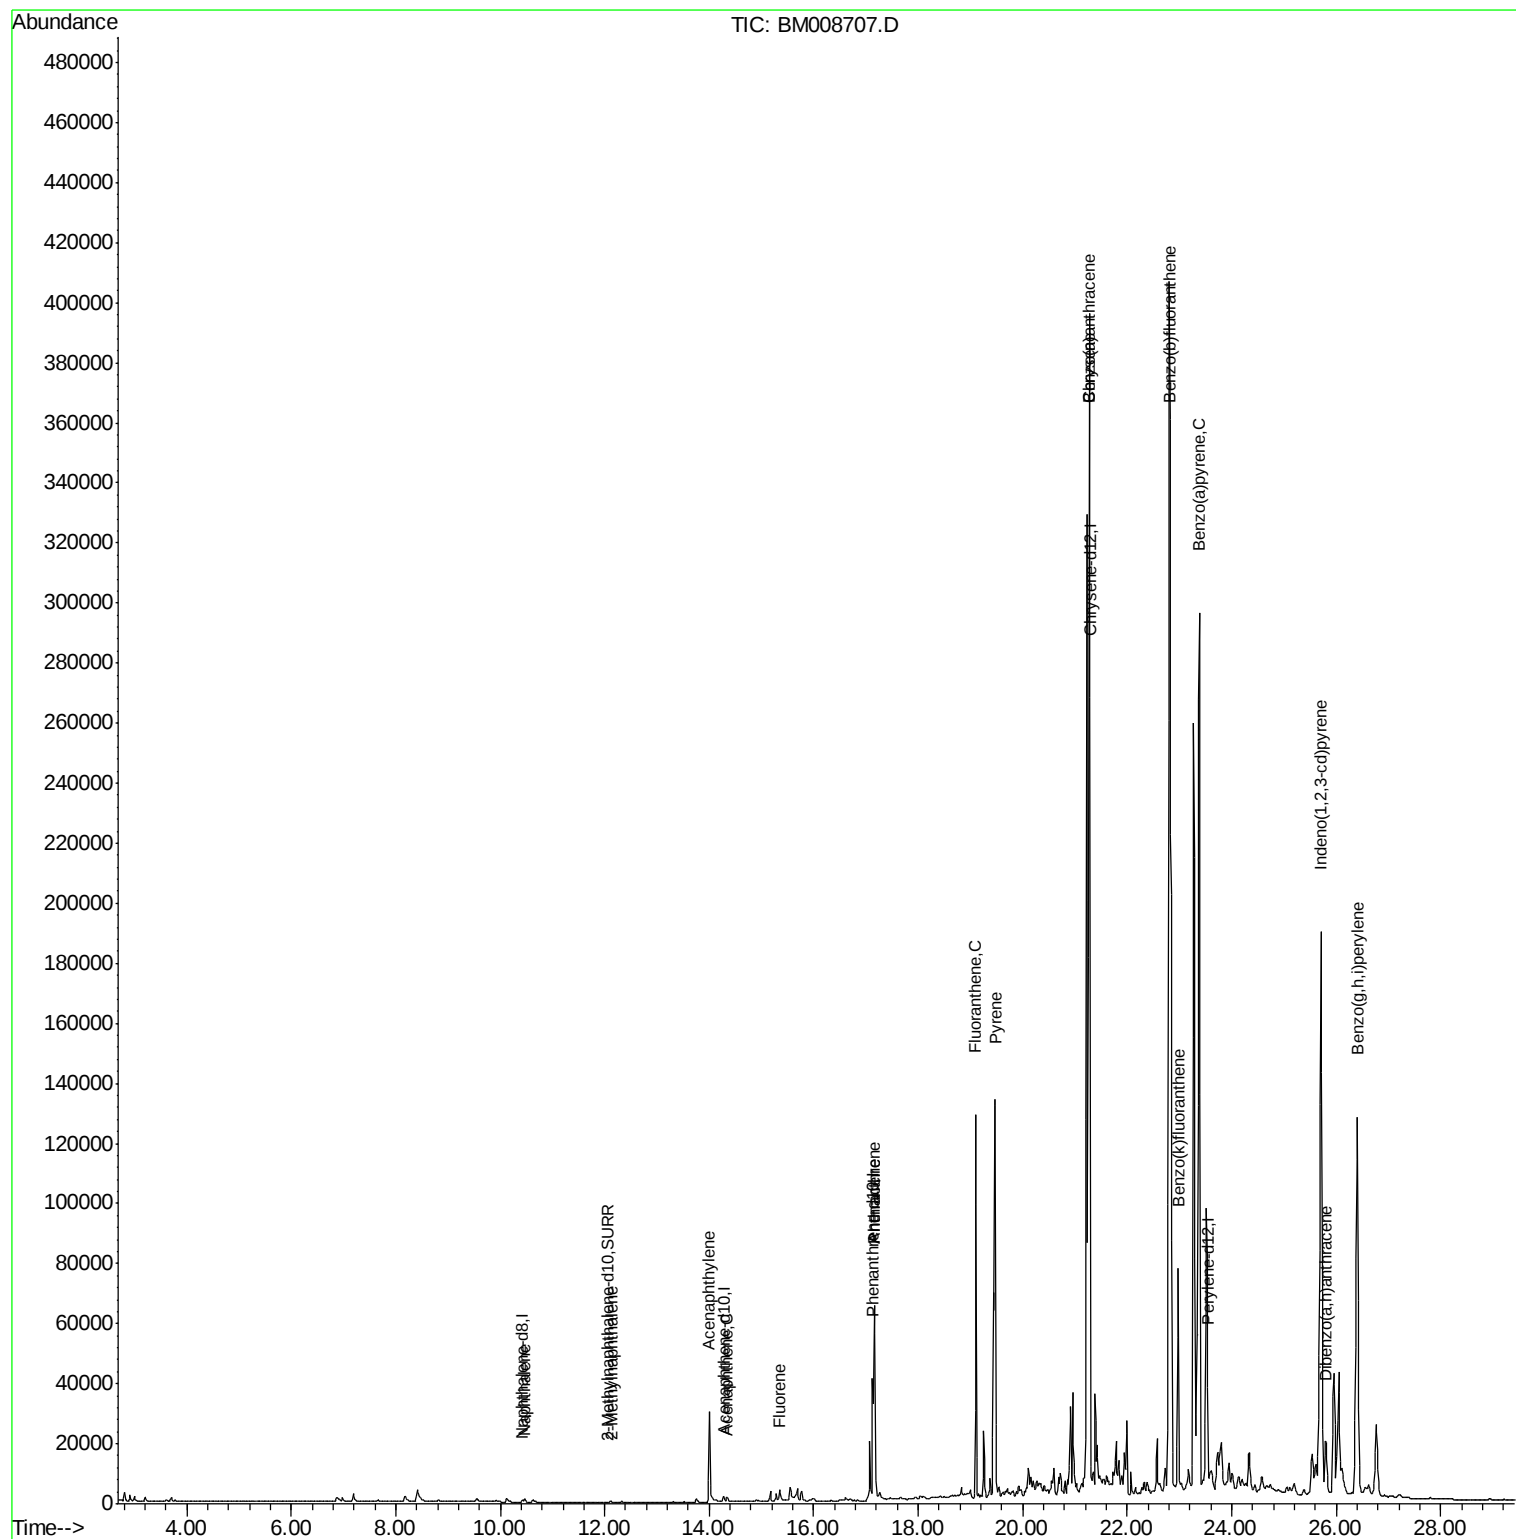

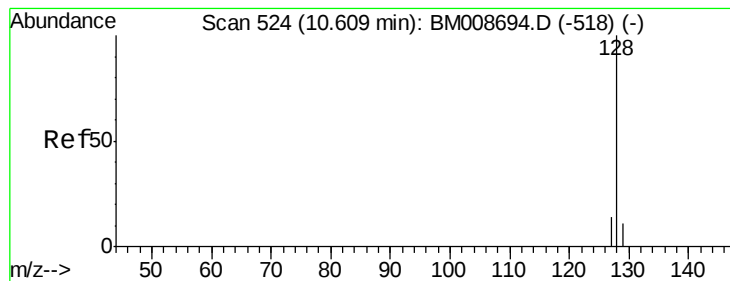

#3

Naphthalene

Concen: 0.60 ng/ul

RT: 10.48 min Scan# 513

Delta R.T. -0.13 min

Lab File: BM008707.D

Acq: 28 Dec 2016 23:21

Instrument :

BNA_M

ClientSampleId :

DA7F6


Tgt Ion:128 Resp: 2543

Ion Ratio Lower Upper

128 100

129 15.5 11.3 16.9




127 16.8 12.8 19.2

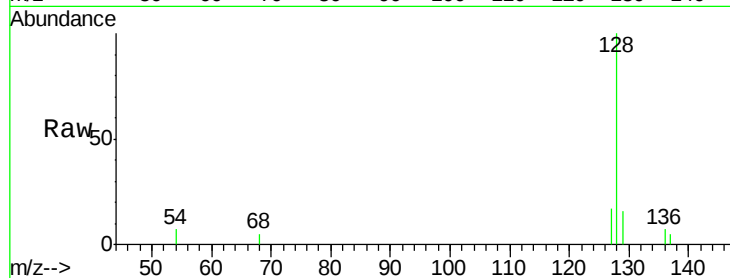

Abundance Ion 128.00 (127.70 to 128.70): E


Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

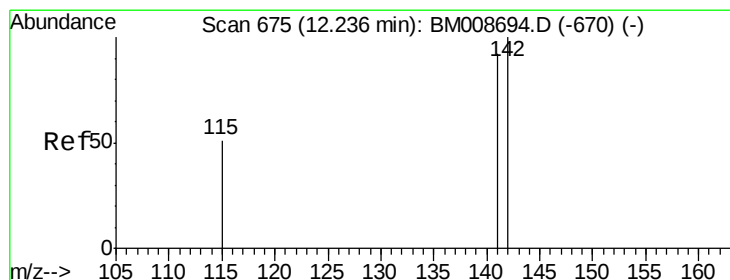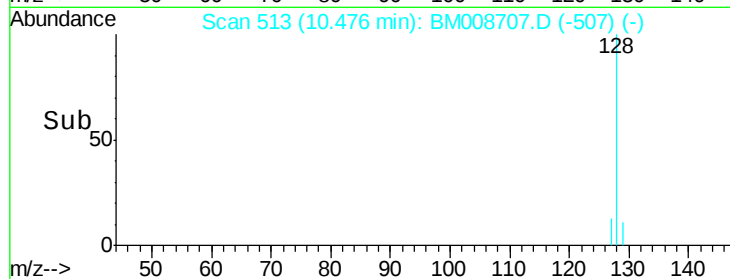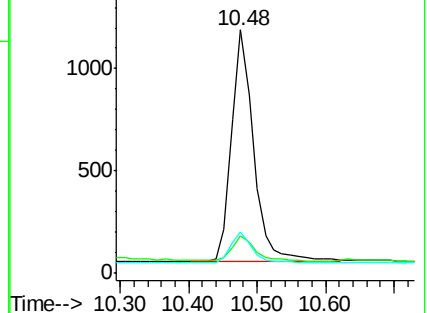

#5

</

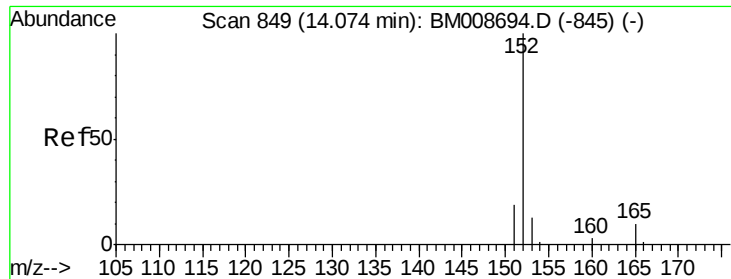

#7

Acenaphthylene

Concen: 11.45 ng/ul

RT: 14.00 min Scan# 844

Delta R.T. -0.08 min

Lab File: BM008707.D

Acq: 28 Dec 2016 23:21

Instrument :

BNA_M

ClientSampleId :

DA7F6


Tgt Ion:152 Resp: 47825

Ion Ratio Lower Upper

152 100

151 23.1 17.1 25.7



153 11.8 12.8 19.2#




Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E



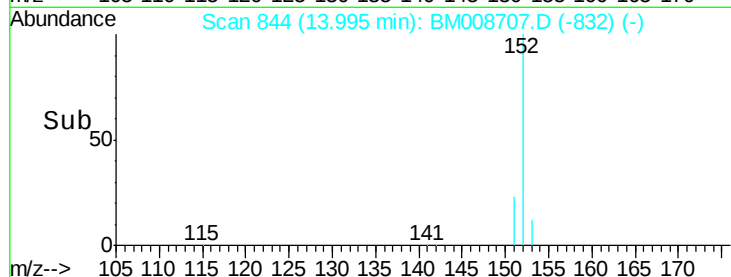
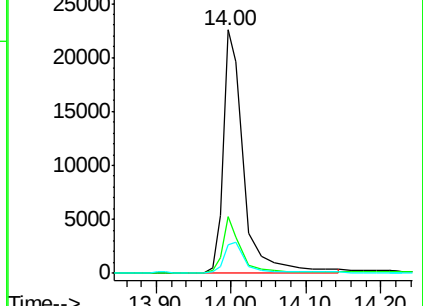


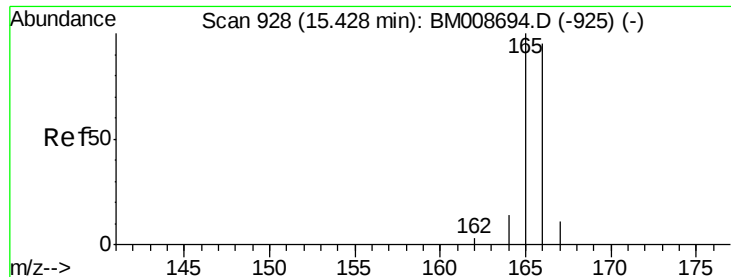

#9
Fluorene
 Concen: 1.11 ng/ul
 RT: 15.34 min Scan# 923
 Delta R.T. -0.09 min
 Lab File: BM008707.D
 Acq: 28 Dec 2016 23:21



Instrument :
 BNA_M
 ClientSampleId :
 DA7F6


Tgt Ion:166 Resp: 3976
 Ion Ratio Lower Upper
 166 100
 165 106.0 73.4 110.2
 167 16.7 14.6 22.0

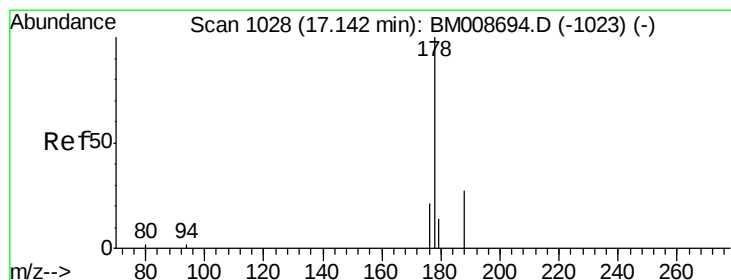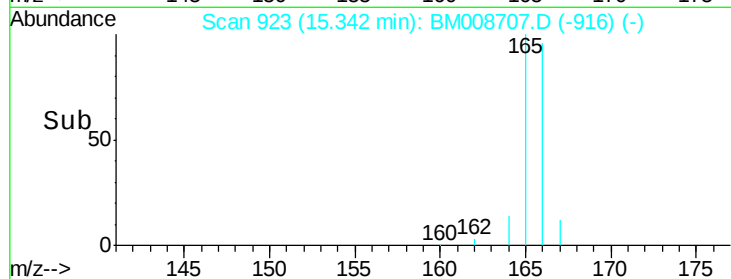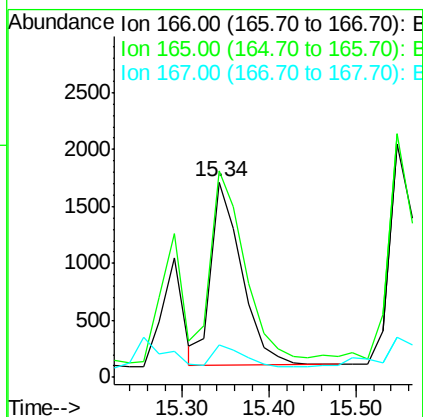

#12
Phenanthrene
 Concen: 0.52 ng/ul
 RT: 17.16 min Scan# 1029
 Delta R.T. 0.02 min
 Lab File: BM008707.D
 Acq: 28 Dec 2016 23:21

Tgt Ion:178 Resp: 100998
 Ion Ratio Lower Upper
 178 100
 176 21.5 18.4 27.6
 179 13.9 13.6 20.4

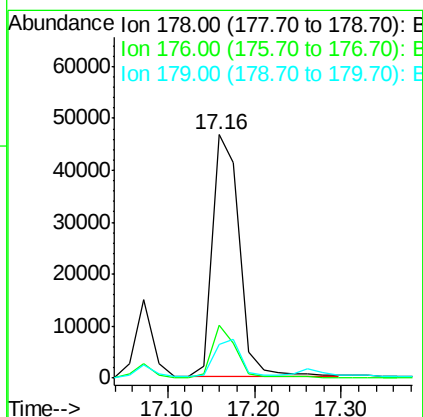

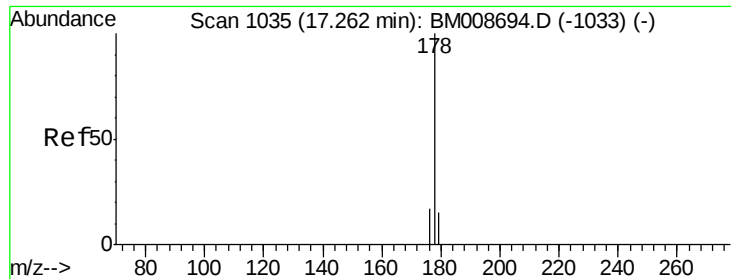

#13

Anthracene

Concen: 0.54 ng/ul

RT: 17.16 min Scan# 1029

Delta R.T. -0.10 min

Lab File: BM008707.D

Acq: 28 Dec 2016 23:21

Instrument :

BNA_M

ClientSampleId :

DA7F6





Tgt Ion:178 Resp: 101822

Ion Ratio Lower Upper

178 100

176 21.5 18.1 27.1

179 13.9 14.7 22.1#

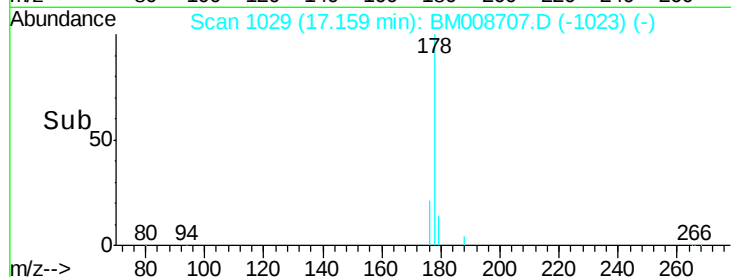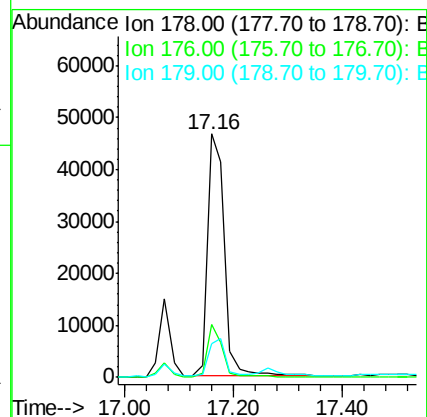


#15

Fluoranthene

Concen: 0.57 ng/ul





RT: 19.10 min Scan# 1144

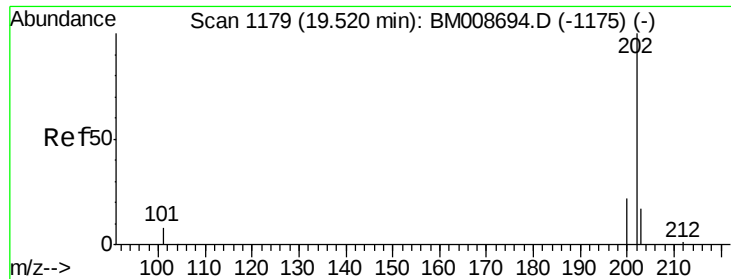

#17
 Pyrene
 Concen: 75.80 ng/ul
 RT: 19.48 min Scan# 1175
 Delta R.T. -0.04 min
 Lab File: BM008707.D
 Acq: 28 Dec 2016 23:21


Instrument :
 BNA_M
 ClientSampleId :
 DA7F6


Tgt Ion	Ratio	Lower	Upper
202	100		
200	18.3	18.2	27.4
203	19.9	15.6	23.4

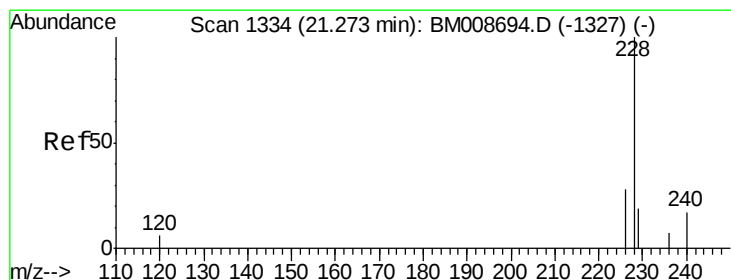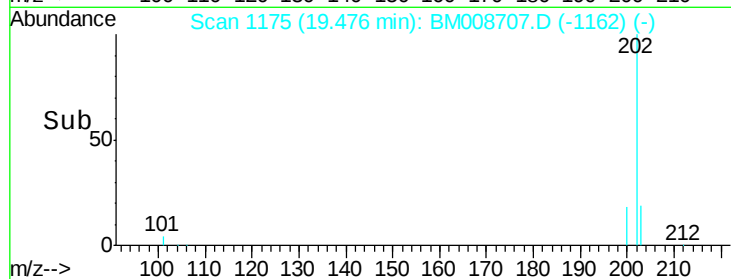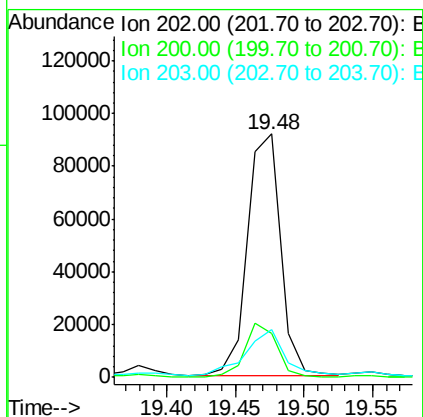

#18
 Benzo(a)anthracene
 Concen: 237.08 ng/ul
 RT: 21.28 min Scan# 1334
 Delta R.T. 0.00 min
 Lab File: BM008707.D
 Acq: 28 Dec 2016 23:21

Tgt Ion	Ratio	Lower	Upper
228	100		
226	33.3	22.8	34.2
229	18.6	17.0	25.6

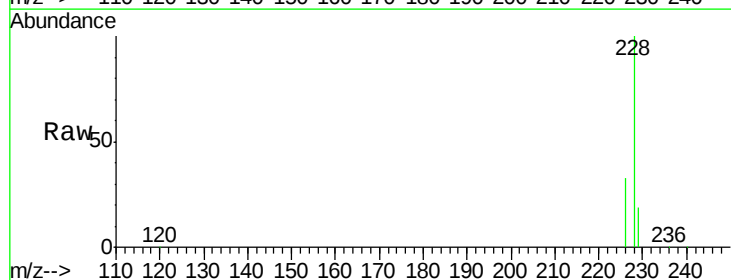

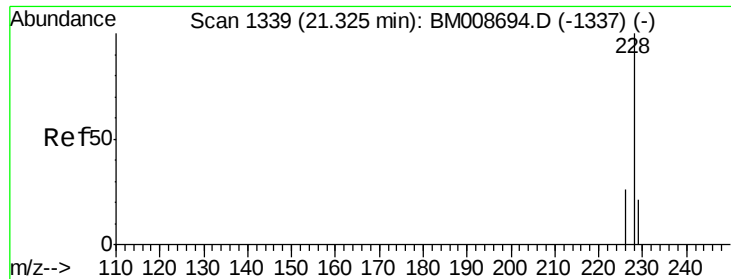

#19

Chrysene

Concen: 216.78 ng/ul

RT: 21.28 min Scan# 1334

Delta R.T. -0.05 min

Lab File: BM008707.D

Acq: 28 Dec 2016 23:21

Instrument :

BNA_M

ClientSampleId :

DA7F6


Tgt Ion:228 Resp: 409163

Ion Ratio Lower Upper

228 100

226 33.3 23.4 35.0




229 18.6 17.7 26.5




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

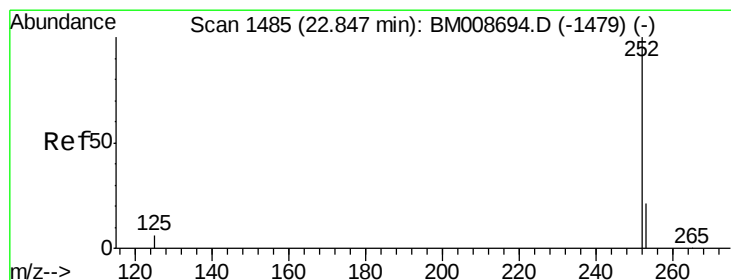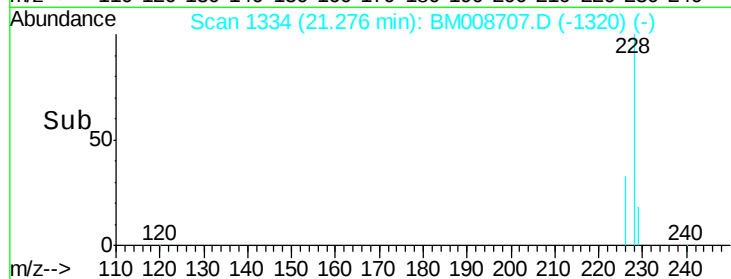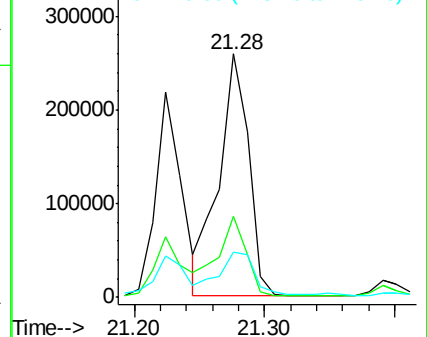

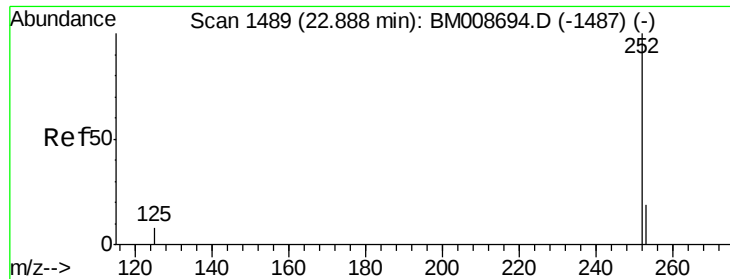

#22

Benzo(k)fluoranthene

Concen: 6.08 ng/u1

RT: 22.98 min Scan# 1497

Delta R.T. 0.09 min

Lab File: BM008707.D

Acq: 28 Dec 2016 23:21

Instrument :

BNA_M

ClientSampleId :

DA7F6


Tgt Ion:252 Resp: 96786

Ion Ratio Lower Upper

252 100

253 25.0 24.5 36.7




125 9.1 13.7 20.5#

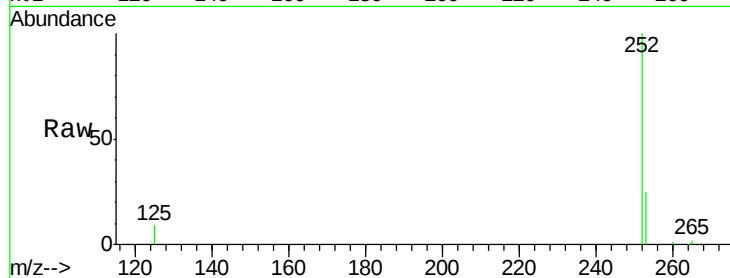


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

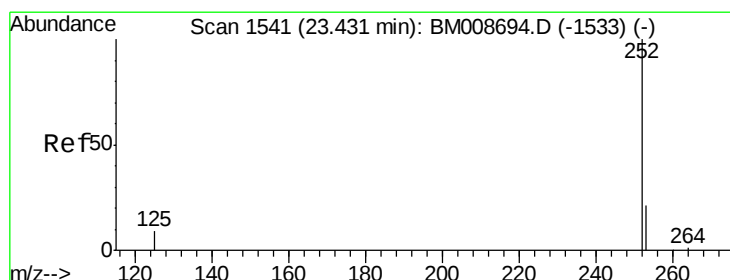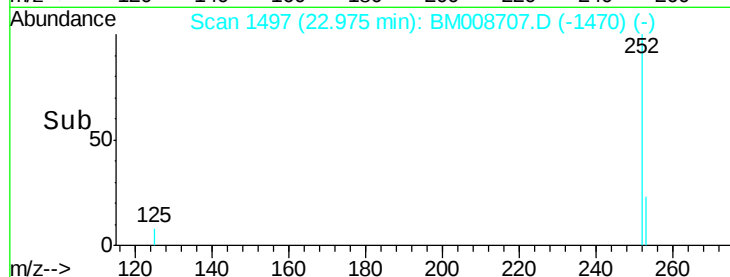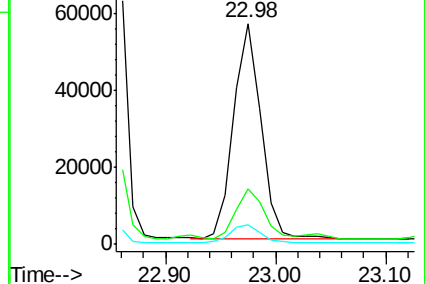




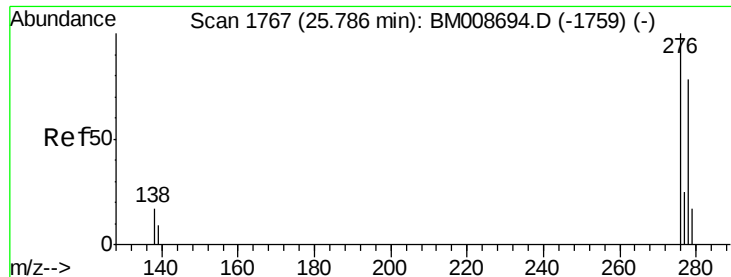


#24

Indeno(1,2,3-cd)pyrene
Concen: 16.65 ng/ul
RT: 25.72 min Scan# 1760
Delta R.T. -0.07 min
Lab File: BM008707.D
Acq: 28 Dec 2016 23:21

Instrument :
BNA_M
ClientSampleId :
DA7F6


Tgt Ion	Ratio	Lower	Upper
276	100		
138	15.1	19.1	28.7#
277	23.7	19.6	29.4

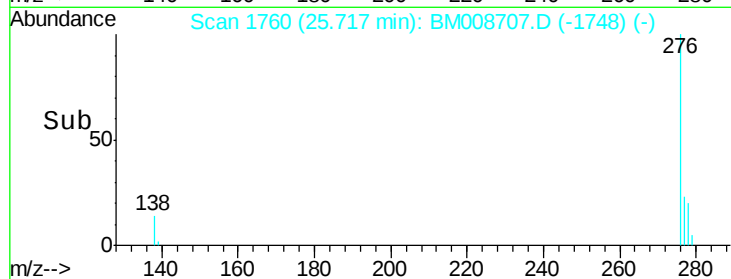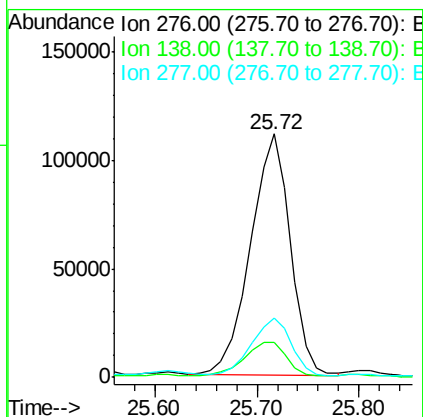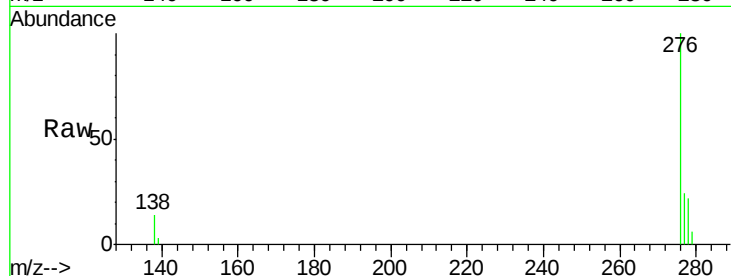


#25

Dibenzo(a,h)anthracene
Concen: 1.84 ng/ul
RT: 25.81 min Scan# 1769
Delta R.T. 0.02 min
Lab File: BM008707.D
Acq: 28 Dec 2016 23:21

Tgt Ion	Ratio	Lower	Upper
278	100		
139	14.3	17.4	26.0#
279	32.5	25.9	38.9



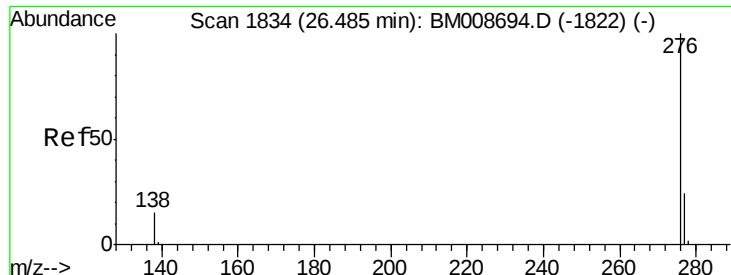

#26

Benzo(g,h,i)perylene

Concen: 17.22 ng/ul

RT: 26.40 min Scan# 1826

Delta R.T. -0.08 min

Lab File: BM008707.D


Acq: 28 Dec 2016 23:21

Instrument :

BNA_M

ClientSampleId :

DA7F6




Tgt Ion: 276 Resp: 266092

Ion Ratio Lower Upper

276 100

277 24.2 21.8 32.8

138 15.3 20.5 30.7#

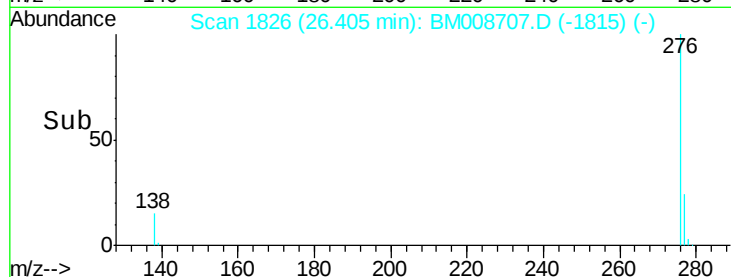

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

