
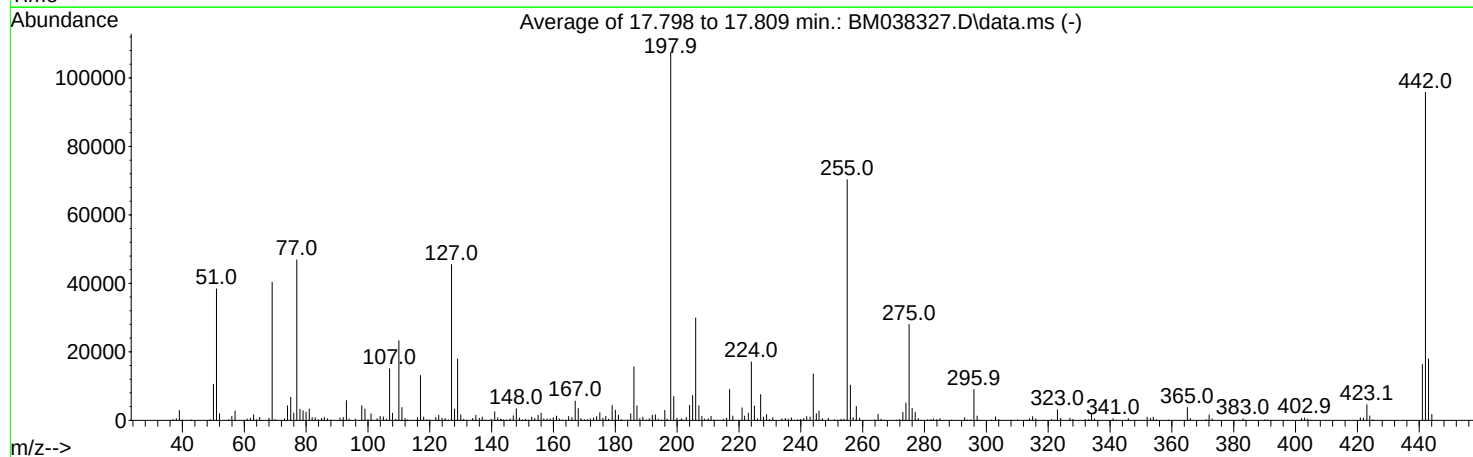


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122822\
 Data File : BM038327.D
 Acq On : 28 Dec 2022 09:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM122722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 28 01:33:07 2022

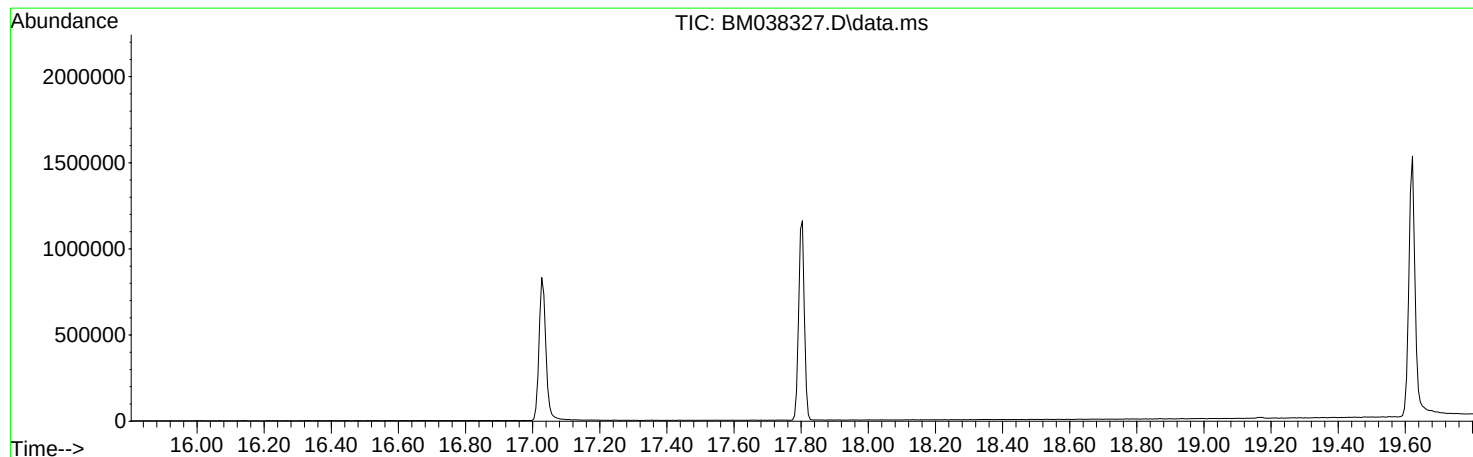




AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.7	38389	PASS
68	69	0.00	2	1.4	573	PASS
69	198	0.00	100	37.5	40336	PASS
70	69	0.00	2	0.5	200	PASS
127	198	10	80	42.4	45517	PASS
197	198	0.00	2	0.3	364	PASS
198	198	100	100	100.0	107461	PASS
199	198	5	9	6.5	6952	PASS
275	198	10	60	26.1	28000	PASS
365	198	1	100	3.5	3751	PASS
441	198	0.01	100	15.2	16311	PASS
442	442	50	100	100.0	95819	PASS
443	442	15	24	18.7	17922	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122822\
Data File : BM038327.D
Acq On : 28 Dec 2022 09:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Dec 29 05:04:30 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 28 01:33:07 2022
Response via : Initial Calibration

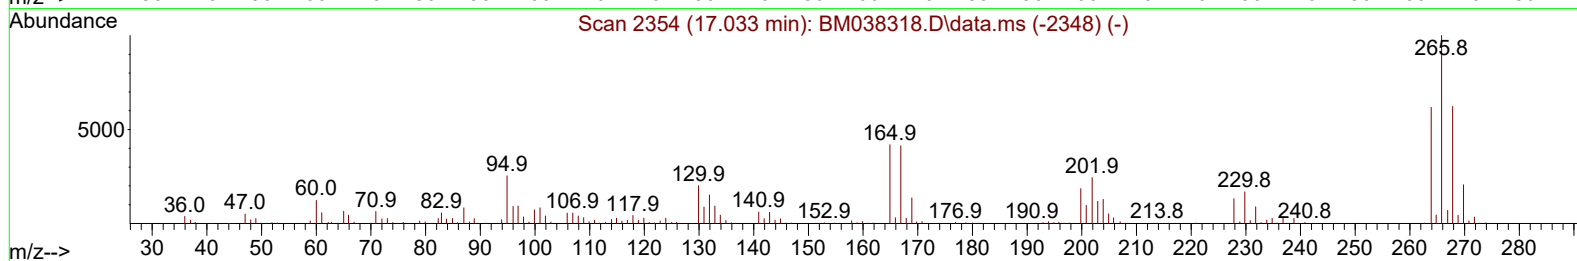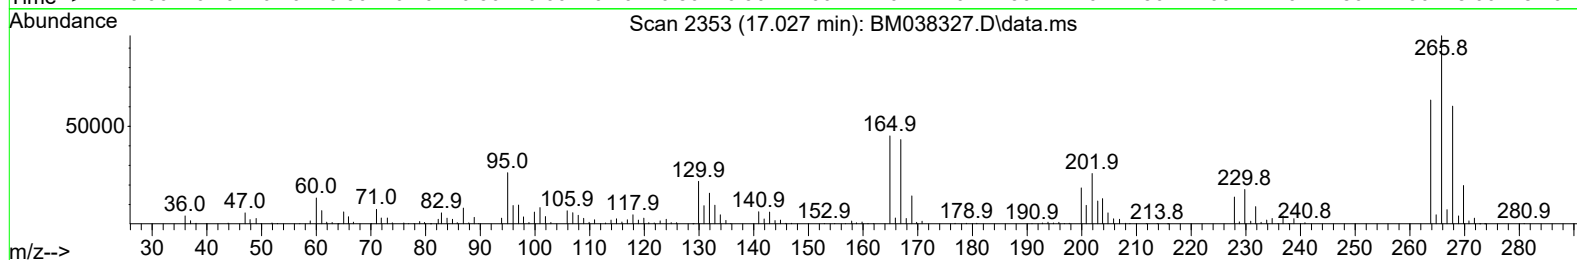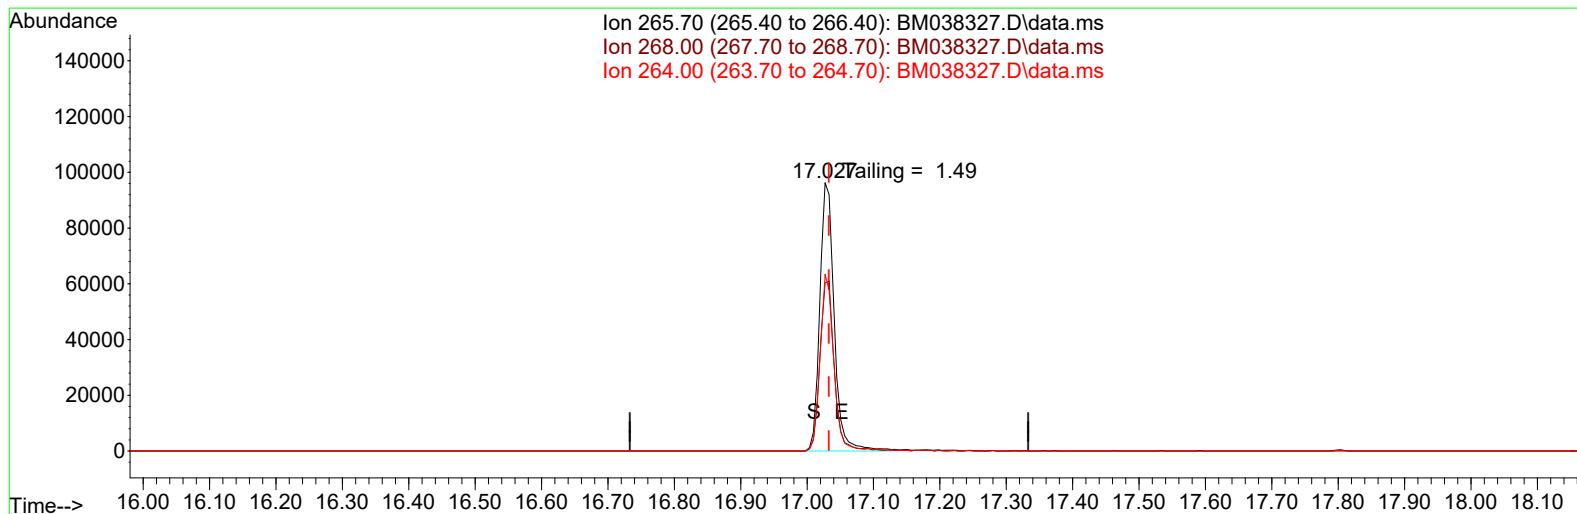

TIC: BM038327.D\data.ms

(70) Pentachlorophenol (C)

17.027min (-0.006) 0.00 ng




response 146001

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.60
264.00	61.80	65.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122822\
 Data File : BM038327.D
 Acq On : 28 Dec 2022 09:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Dec 29 05:04:30 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM122722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 28 01:33:07 2022
 Response via : Initial Calibration

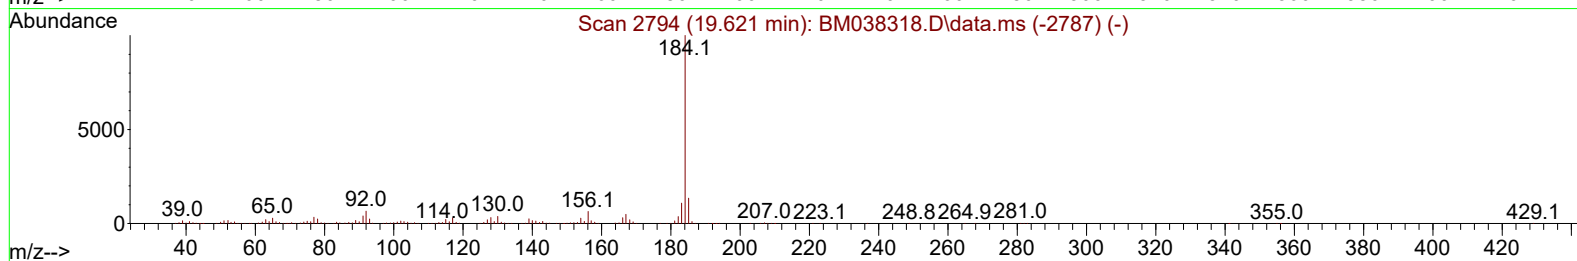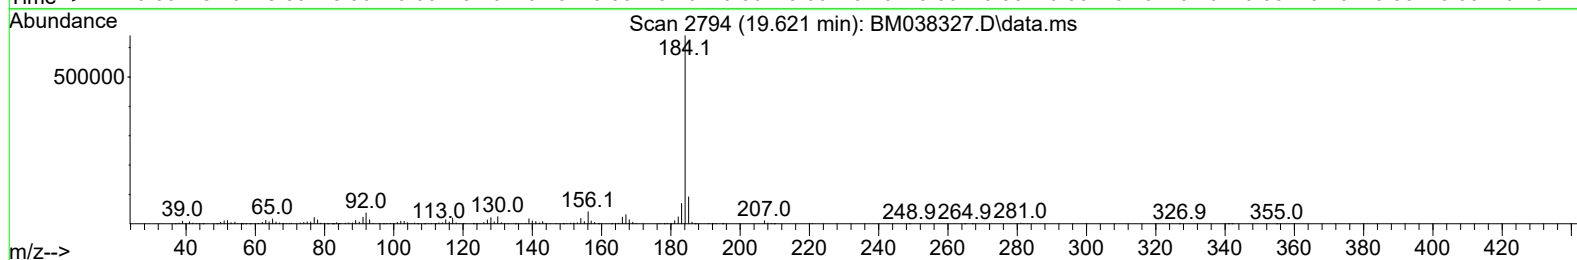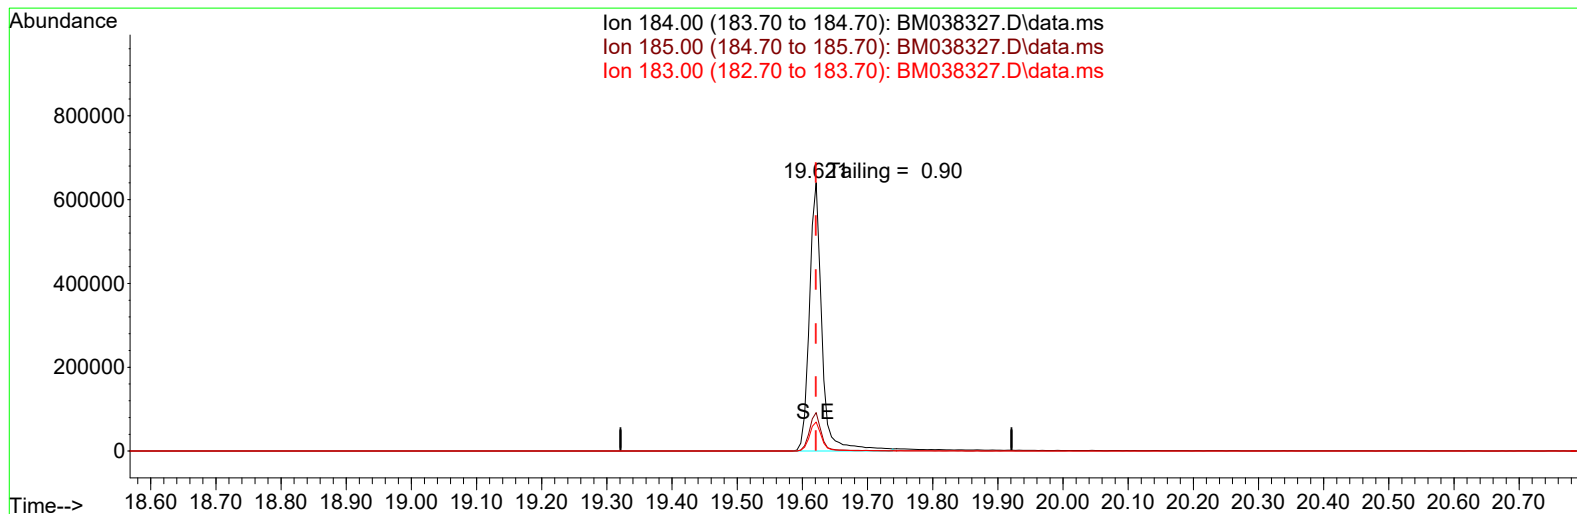

TIC: BM038327.D\data.ms

(77) Benzidine

19.621min (-0.000) 0.00 ng

response 868606

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.31
183.00	10.80	10.81
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/28/2022	BNA_M	<u>BM038327.D</u>
Compound Name	Response	Retention Time
DDT	455300	20.839
DDD	5161	20.45
DDE	70	19.898
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5231	460531	1.14

Instrument :
BNA_M
ClientSampleId :
DFTPP