

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122823\
 Data File : BM043645.D
 Acq On : 28 Dec 2023 19:01
 Operator : MA/JU
 Sample : PB158094BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK094

Quant Time: Dec 28 23:00:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 26 22:58:31 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.967	152	3752	0.400	ng/ul	0.00
4) Naphthalene-d8	10.768	136	11140	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.601	164	5233	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.443	188	848539	0.400	ng/ul	# 0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.53
23) Perylene-d12	23.936	264	9889	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.372	96	35140	7.412	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.368	152	4950	0.314	ng/ul	0.00
18) Fluoranthene-d10	19.371	212	7096	0.000	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.591	166	1746	0.074	ng/ul#	14
26) Benzo(a)pyrene	23.781	252	3148	0.085	ng/ul#	34


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122823\
Data File : BM043645.D
Acq On : 28 Dec 2023 19:01
Operator : MA/JU
Sample : PB158094BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK094

Quant Time: Dec 28 23:00:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 26 22:58:31 2023
Response via : Initial Calibration




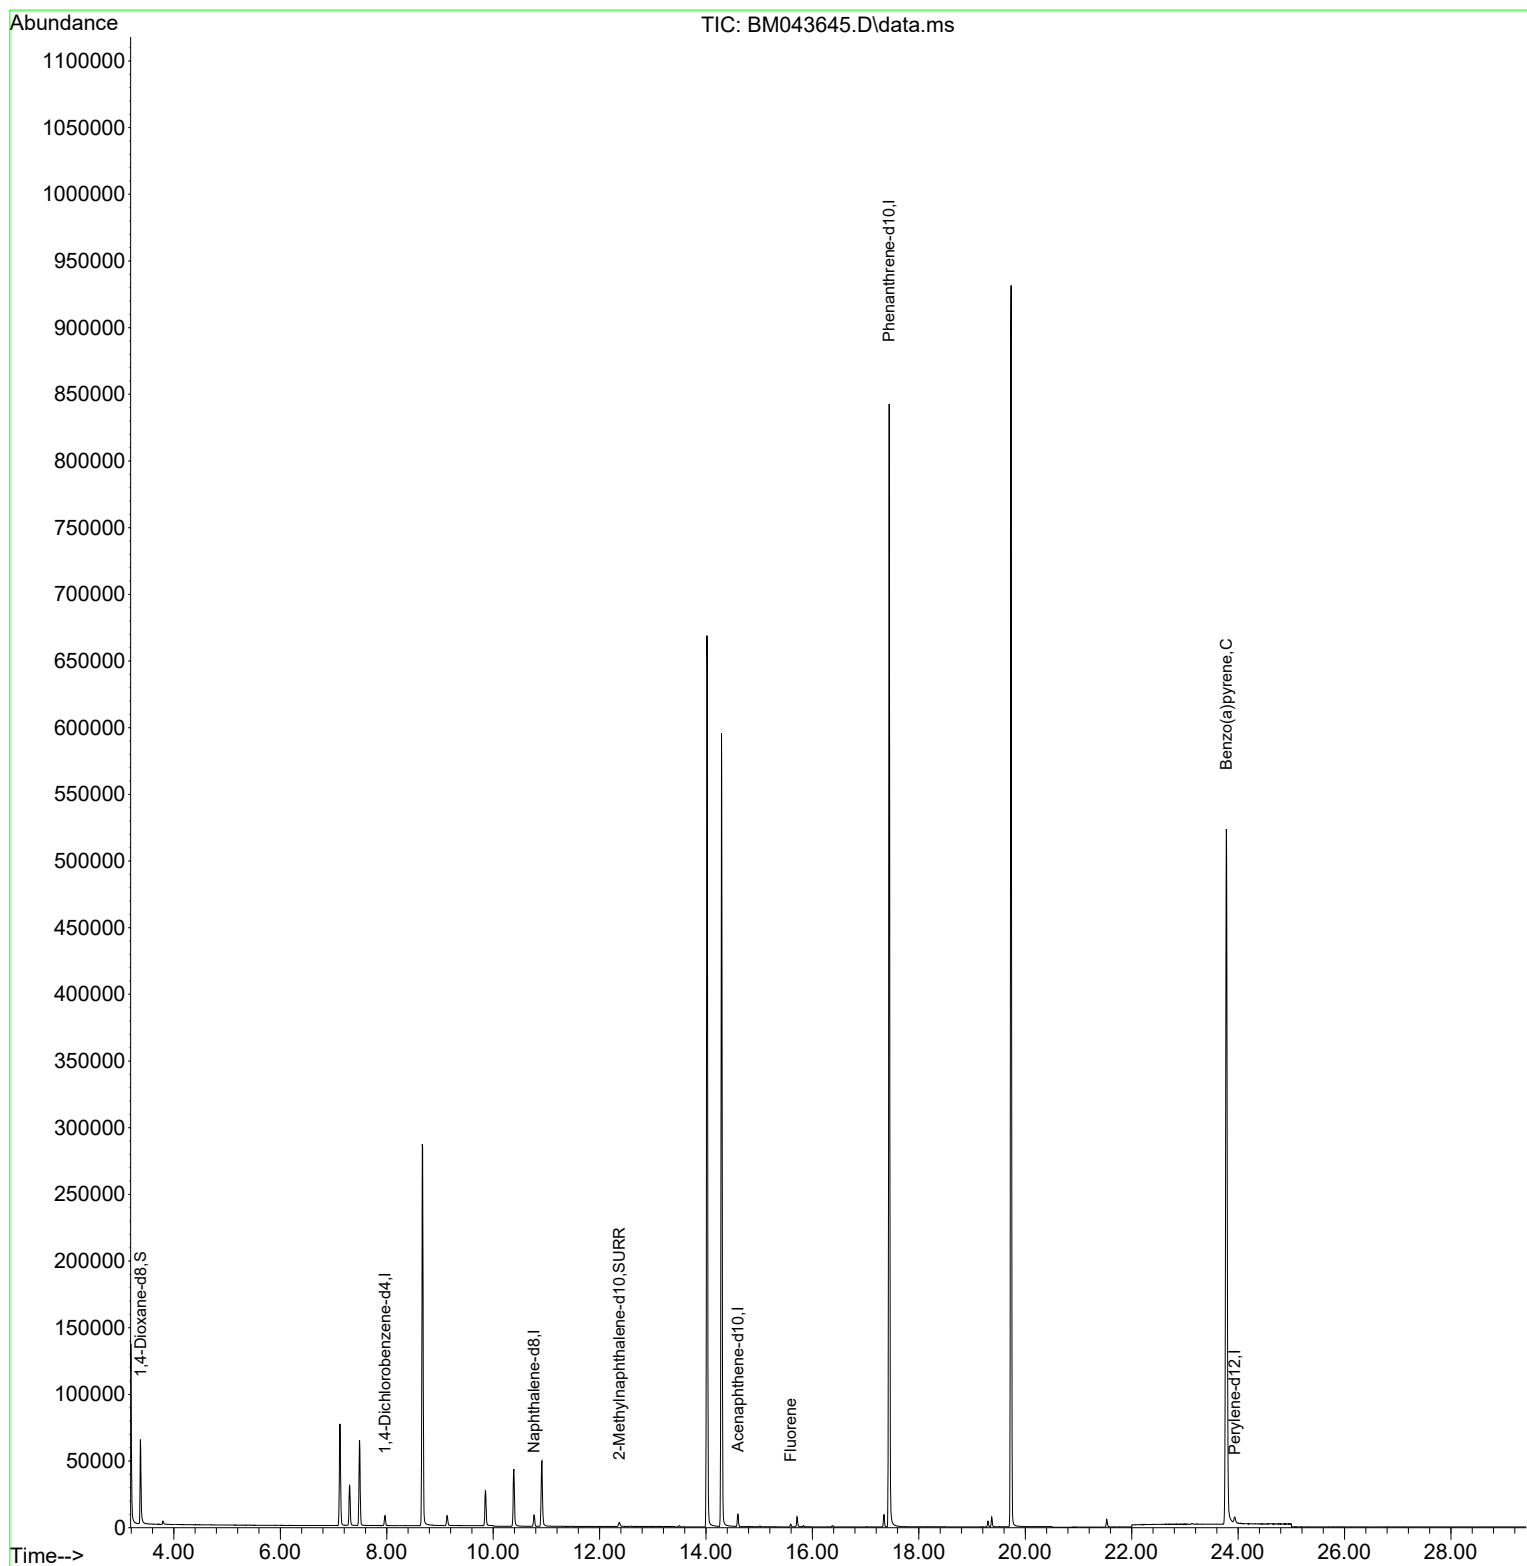


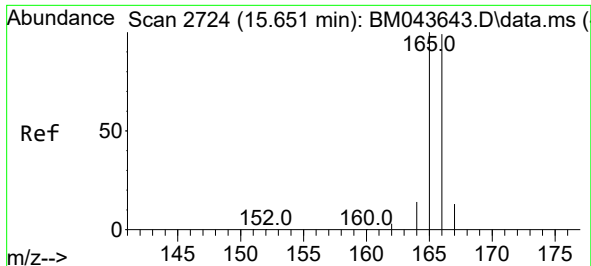

#12
 Fluorene
 Concen: 0.074 ng/ul
 RT: 15.591 min Scan# 21
 Delta R.T. -0.065 min
 Lab File: BM043645.D
 Acq: 28 Dec 2023 19:01

Instrument :
 BNA_M
 ClientSampleId :
 SBLK094

Tgt Ion:166 Resp: 1746
 Ion Ratio Lower Upper
 166 100
 165 9.9 80.3 120.5#
 167 33.9 10.8 16.2#

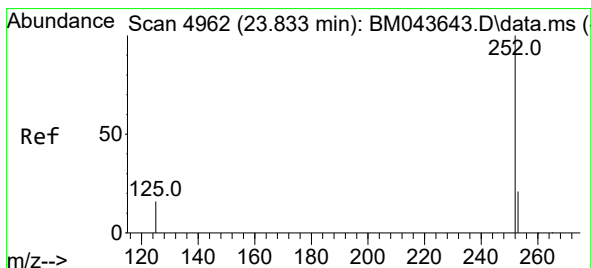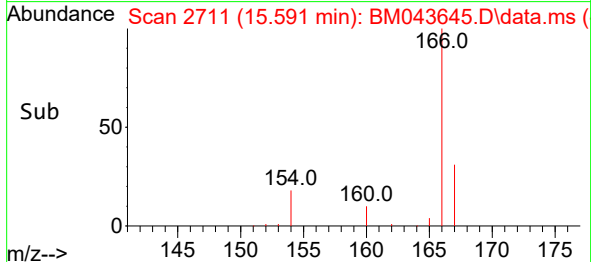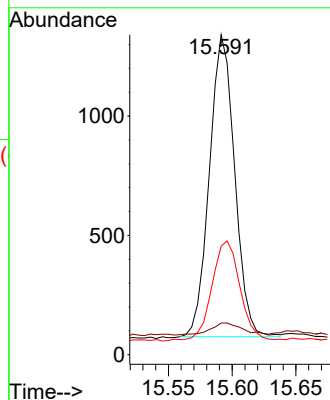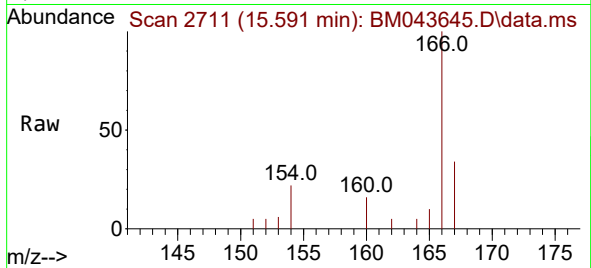

#26
 Benzo(a)pyrene
 Concen: 0.085 ng/ul
 RT: 23.781 min Scan# 4944
 Delta R.T. -0.052 min
 Lab File: BM043645.D
 Acq: 28 Dec 2023 19:01

Tgt Ion:252 Resp: 3148
 Ion Ratio Lower Upper
 252 100
 253 51.4 20.2 30.2#
 125 54.9 13.5 20.3#

