

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122823\
 Data File : BM043646.D
 Acq On : 28 Dec 2023 19:37
 Operator : MA/JU
 Sample : 05986-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AG0

Quant Time: Dec 28 23:00:09 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 26 22:58:31 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.967	152	4716	0.400	ng/ul	0.00
4) Naphthalene-d8	10.768	136	14483	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.597	164	6808	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.443	188	1043080	0.400	ng/ul	# 0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.53
23) Perylene-d12	23.933	264	12751	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.372	96	22776	3.822	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.363	152	4932	0.240	ng/ul	0.00
18) Fluoranthene-d10	19.366	212	9470	0.000	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.410	88	420	0.070	ng/ul#	60
26) Benzo(a)pyrene	23.778	252	4147	0.087	ng/ul#	45


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122823\
Data File : BM043646.D
Acq On : 28 Dec 2023 19:37
Operator : MA/JU
Sample : 05986-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG0

Quant Time: Dec 28 23:00:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 26 22:58:31 2023
Response via : Initial Calibration




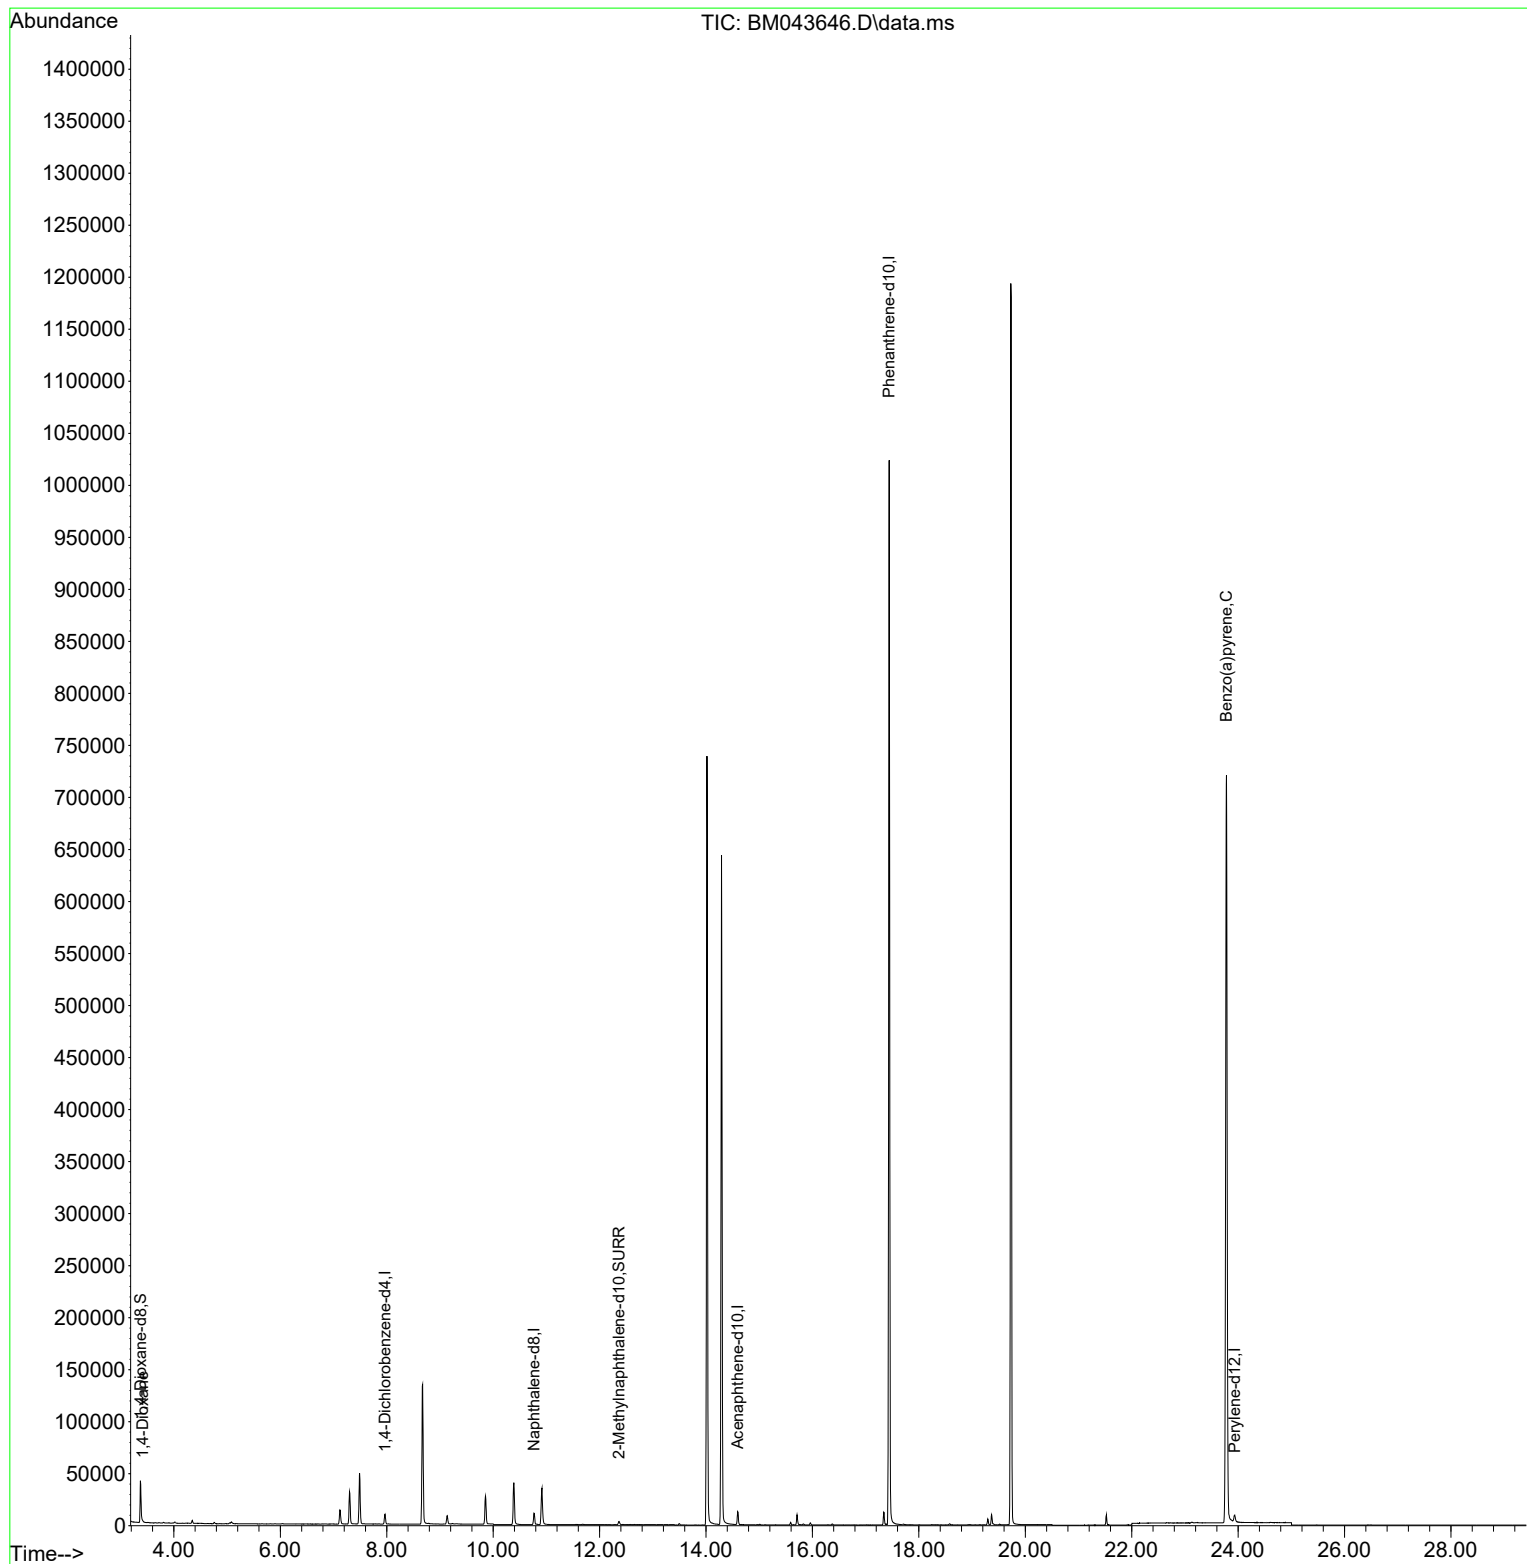


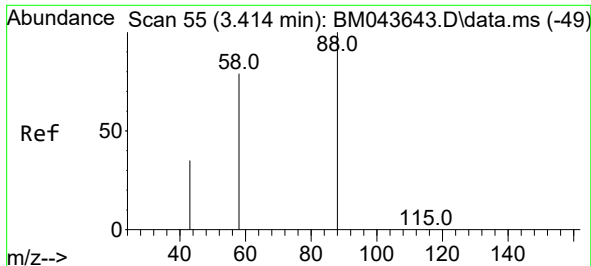

#2
1,4-Dioxane
Concen: 0.070 ng/ul
RT: 3.410 min Scan# 54
Delta R.T. -0.004 min
Lab File: BM043646.D
Acq: 28 Dec 2023 19:37

Instrument :
BNA_M
ClientSampleId :
C0AG0

Tgt Ion: 88 Resp: 420
Ion Ratio Lower Upper
88 100
43 50.7 27.9 41.9#
58 19.6 43.4 65.2#

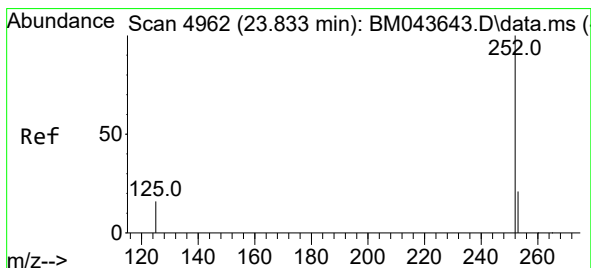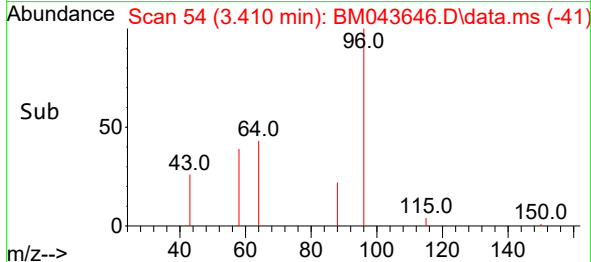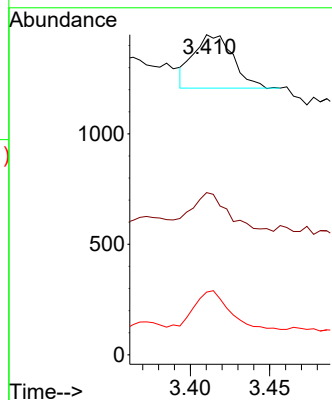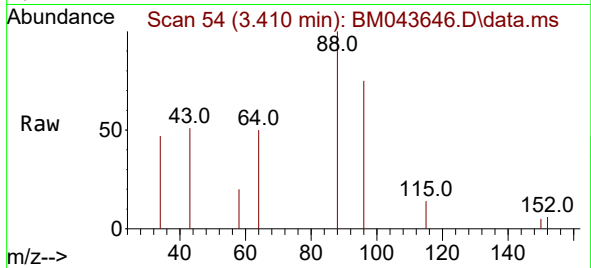

#26
Benzo(a)pyrene
Concen: 0.087 ng/ul
RT: 23.778 min Scan# 4943
Delta R.T. -0.055 min
Lab File: BM043646.D
Acq: 28 Dec 2023 19:37

Tgt Ion: 252 Resp: 4147
Ion Ratio Lower Upper
252 100
253 46.1 20.2 30.2#
125 49.1 13.5 20.3#

