

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122823\
 Data File : BM043649.D
 Acq On : 28 Dec 2023 21:26
 Operator : MA/JU
 Sample : 06021-17
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH7Z9

Quant Time: Dec 28 23:00:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 26 22:58:31 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.967	152	4651	0.400	ng/ul	0.00
4) Naphthalene-d8	10.768	136	14237	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.597	164	6662	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.443	188	1260246	0.400	ng/ul	# 0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.53
23) Perylene-d12	23.933	264	12649	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.372	96	27607	4.698	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.363	152	6534	0.324	ng/ul	0.00
18) Fluoranthene-d10	19.371	212	11037	0.000	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.591	166	2630	0.087	ng/ul#	12
26) Benzo(a)pyrene	23.781	252	4843	0.102	ng/ul#	49


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122823\
Data File : BM043649.D
Acq On : 28 Dec 2023 21:26
Operator : MA/JU
Sample : 06021-17
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH7Z9

Quant Time: Dec 28 23:00:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 26 22:58:31 2023
Response via : Initial Calibration




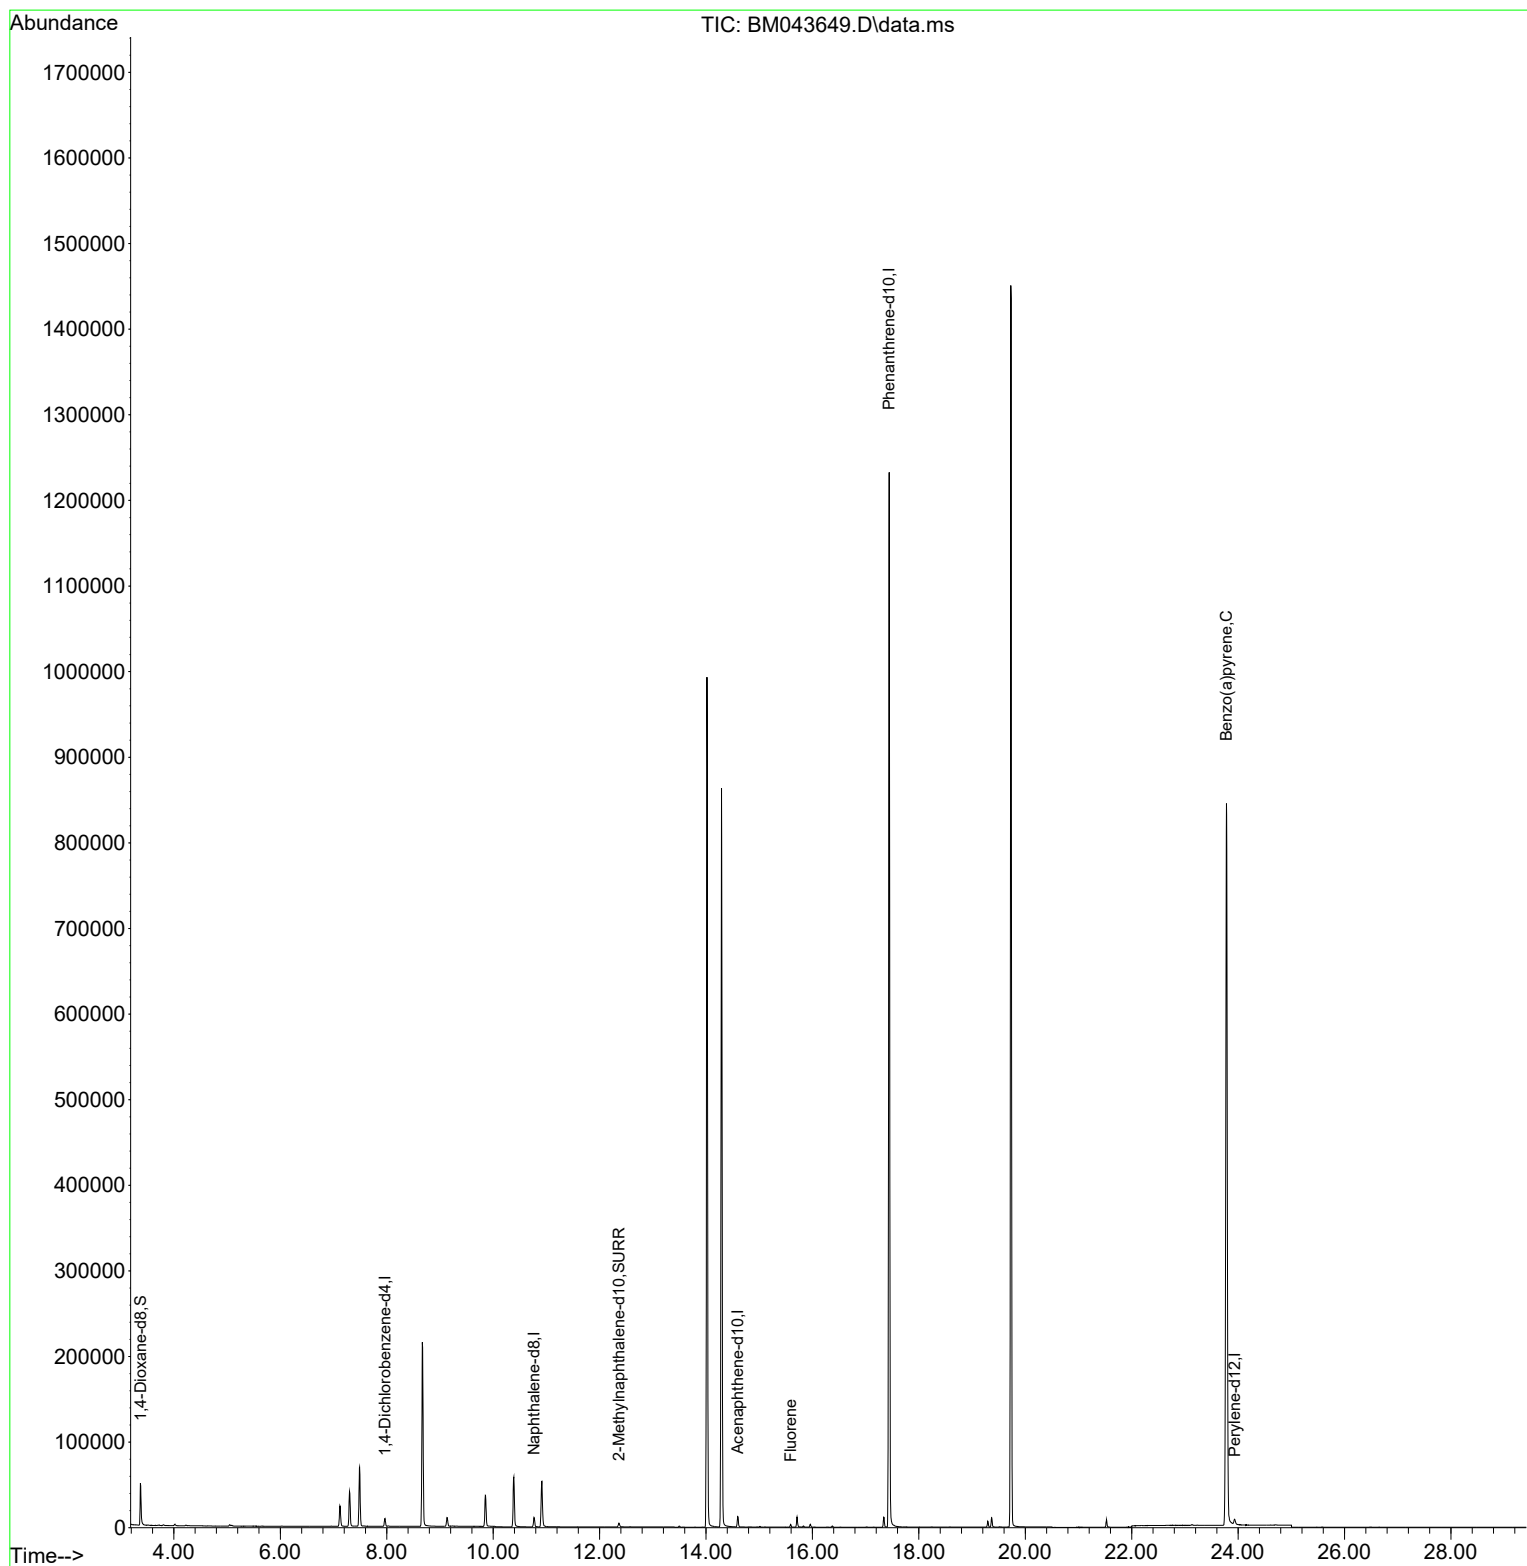


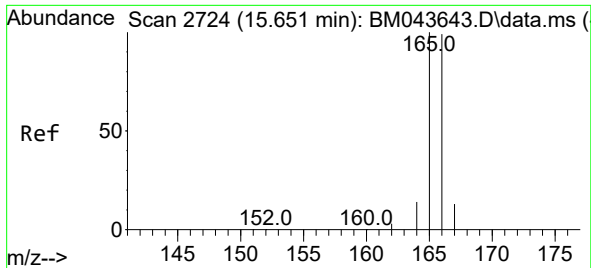

#12
Fluorene
Concen: 0.087 ng/ul
RT: 15.591 min Scan# 21
Delta R.T. -0.065 min
Lab File: BM043649.D
Acq: 28 Dec 2023 21:26

Instrument :
BNA_M
ClientSampleId :
BH7Z9

Tgt Ion:166 Resp: 2630
Ion Ratio Lower Upper
166 100
165 7.9 80.3 120.5#
167 34.6 10.8 16.2#

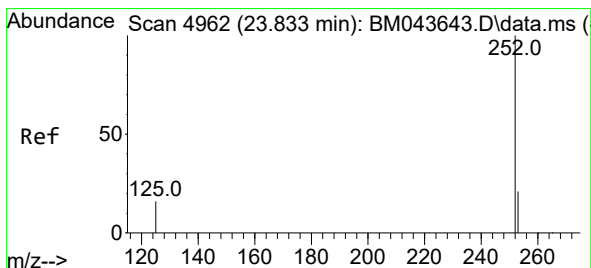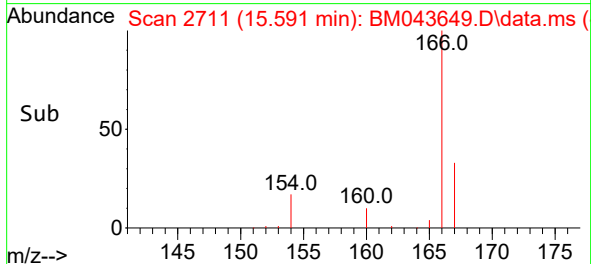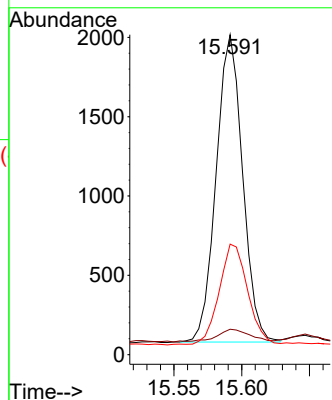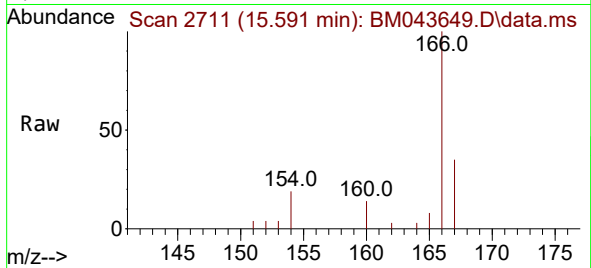

#26
Benzo(a)pyrene
Concen: 0.102 ng/ul
RT: 23.781 min Scan# 4944
Delta R.T. -0.052 min
Lab File: BM043649.D
Acq: 28 Dec 2023 21:26

Tgt Ion:252 Resp: 4843
Ion Ratio Lower Upper
252 100
253 44.5 20.2 30.2#
125 47.1 13.5 20.3#

