

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122823\
 Data File : BM043661.D
 Acq On : 29 Dec 2023 05:17
 Operator : MA/JU
 Sample : 05986-09
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AG4

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/29/2023
 Supervised By :mohammad ahmed 12/29/2023

Quant Time: Dec 29 05:48:33 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 26 22:58:31 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.963	152	4688	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.768	136	15007	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.597	164	9806	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.341	188	17067m	0.400	ng/ul	0.00
17) Chrysene-d12	21.521	240	10288m	0.400	ng/ul	0.00
23) Perylene-d12	23.930	264	14751	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.372	96	21214	3.581	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.357	152	6748	0.317	ng/ul	-0.01
18) Fluoranthene-d10	19.366	212	14475	0.394	ng/ul	0.00
Target Compounds						
11) Acenaphthene	14.657	153	9810	0.250	ng/ul	Qvalue 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122823\
Data File : BM043661.D
Acq On : 29 Dec 2023 05:17
Operator : MA/JU
Sample : 05986-09
Misc :
ALS Vial : 21 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0AG4

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/29/2023
Supervised By :mohammad ahmed 12/29/2023


Quant Time: Dec 29 05:48:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 26 22:58:31 2023
Response via : Initial Calibration

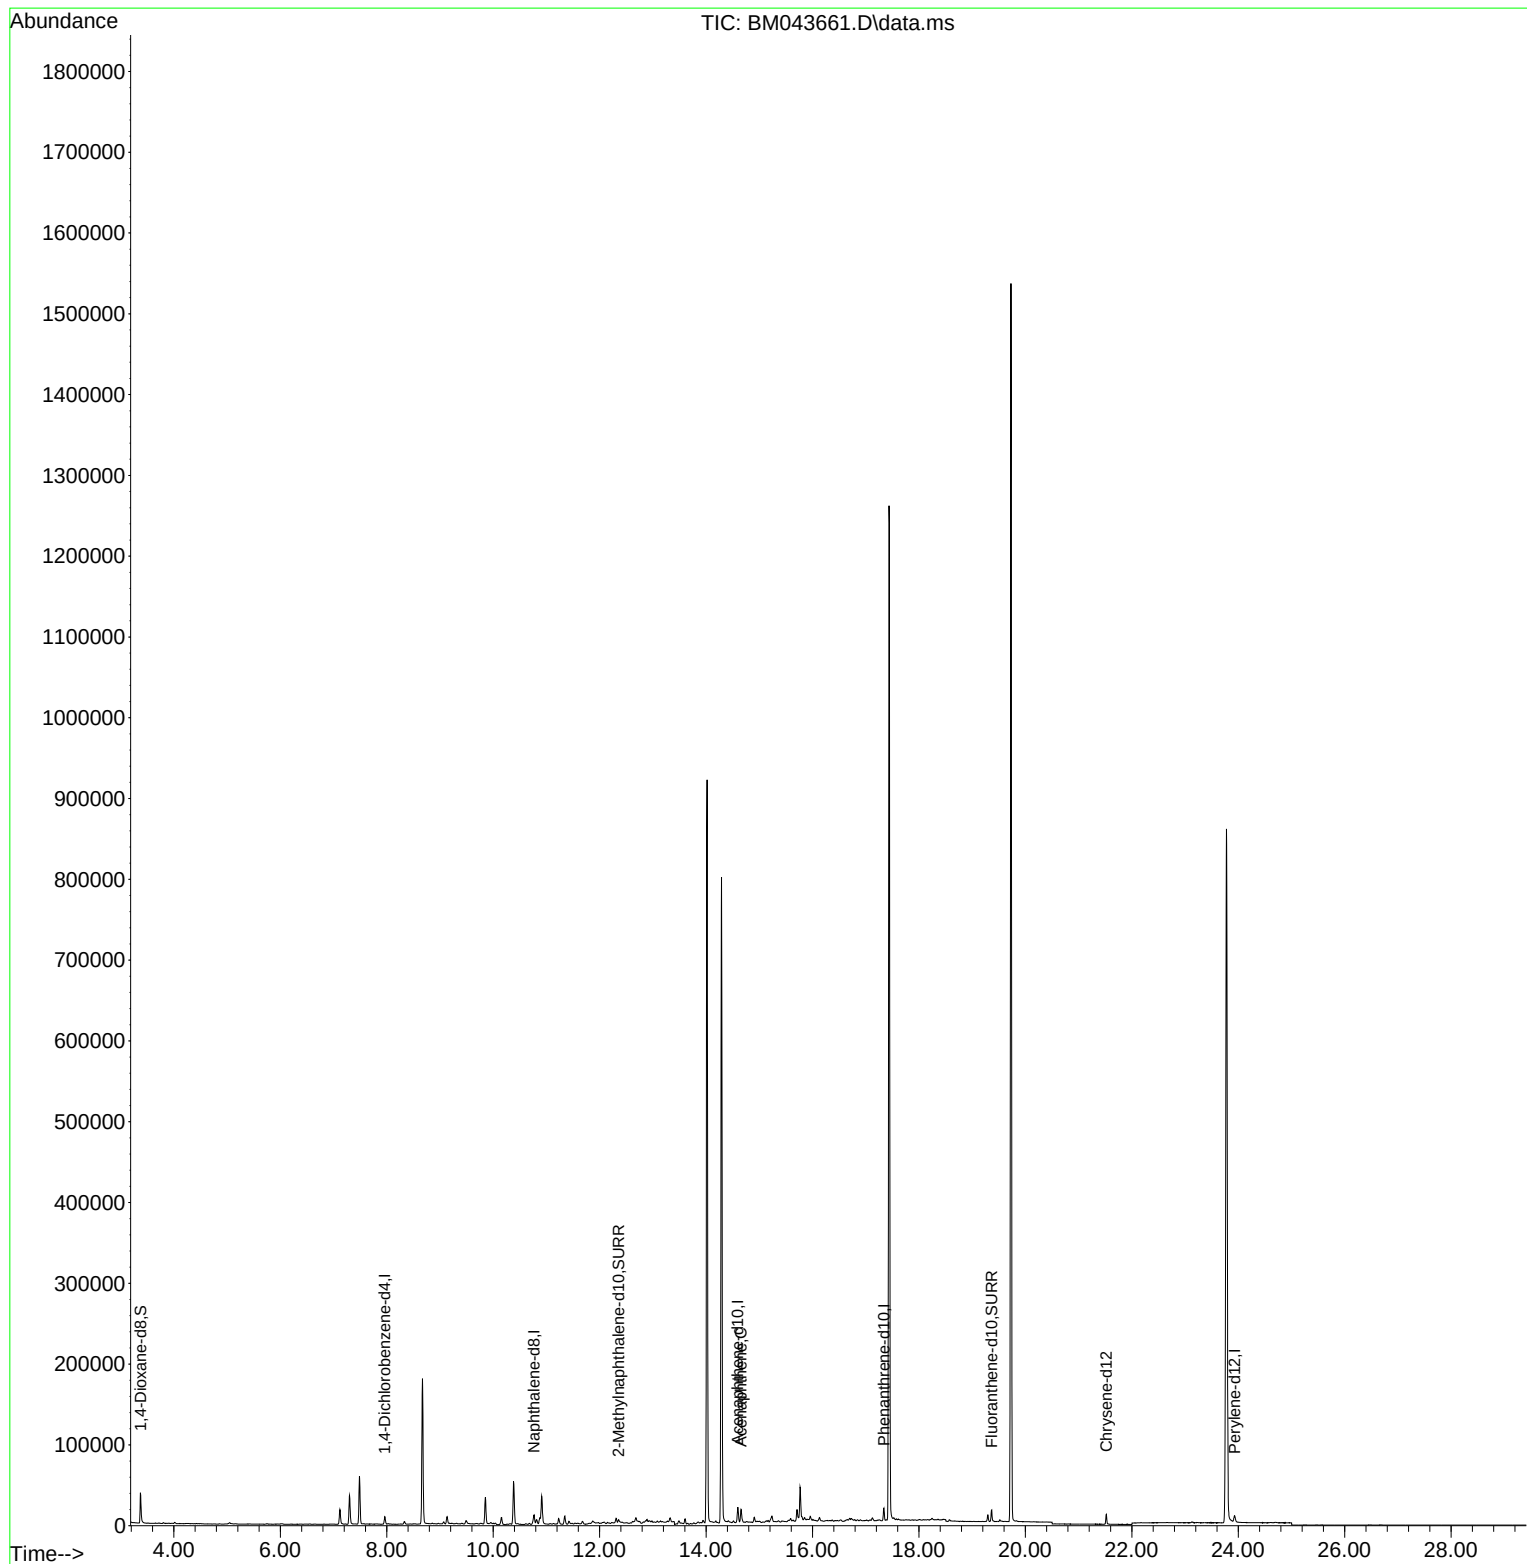

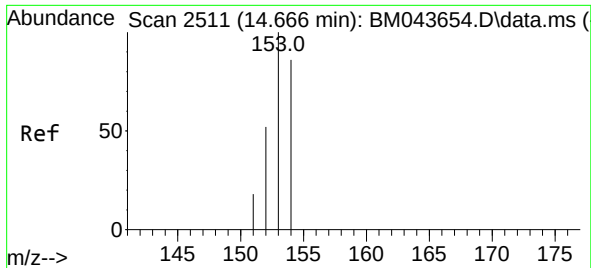

#11
Acenaphthene
Concen: 0.250 ng/ul
RT: 14.657 min Scan# 2509
Delta R.T. -0.009 min
Lab File: BM043661.D
Acq: 29 Dec 2023 05:17

Instrument :
BNA_M
ClientSampleId :
C0AG4

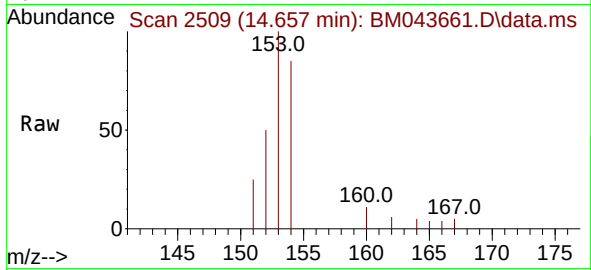

Tgt Ion:153 Resp: 9810
Ion Ratio Lower Upper
153 100
152 50.1 42.1 63.1
154 84.8 71.3 106.9

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/29/2023
Supervised By :mohammad ahmed 12/29/2023

