

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122823\
 Data File : BM043663.D
 Acq On : 29 Dec 2023 06:29
 Operator : MA/JU
 Sample : 05986-11
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AM7

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/29/2023
 Supervised By :mohammad ahmed 12/29/2023

Quant Time: Dec 29 07:00:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 26 22:58:31 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.962	152	4998	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.768	136	15361	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.597	164	7778	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.341	188	14759m	0.400	ng/ul	0.00
17) Chrysene-d12	21.524	240	9002m	0.400	ng/ul	0.00
23) Perylene-d12	23.927	264	15090	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.376	96	27252	4.315	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.357	152	6806	0.313	ng/ul	-0.01
18) Fluoranthene-d10	19.366	212	12947	0.403	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.818	128	1632	0.035	ng/ul#	84

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122823\
Data File : BM043663.D
Acq On : 29 Dec 2023 06:29
Operator : MA/JU
Sample : 05986-11
Misc :
ALS Vial : 23 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0AM7

Quant Time: Dec 29 07:00:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 26 22:58:31 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 12/29/2023
Supervised By :mohammad ahmed 12/29/2023

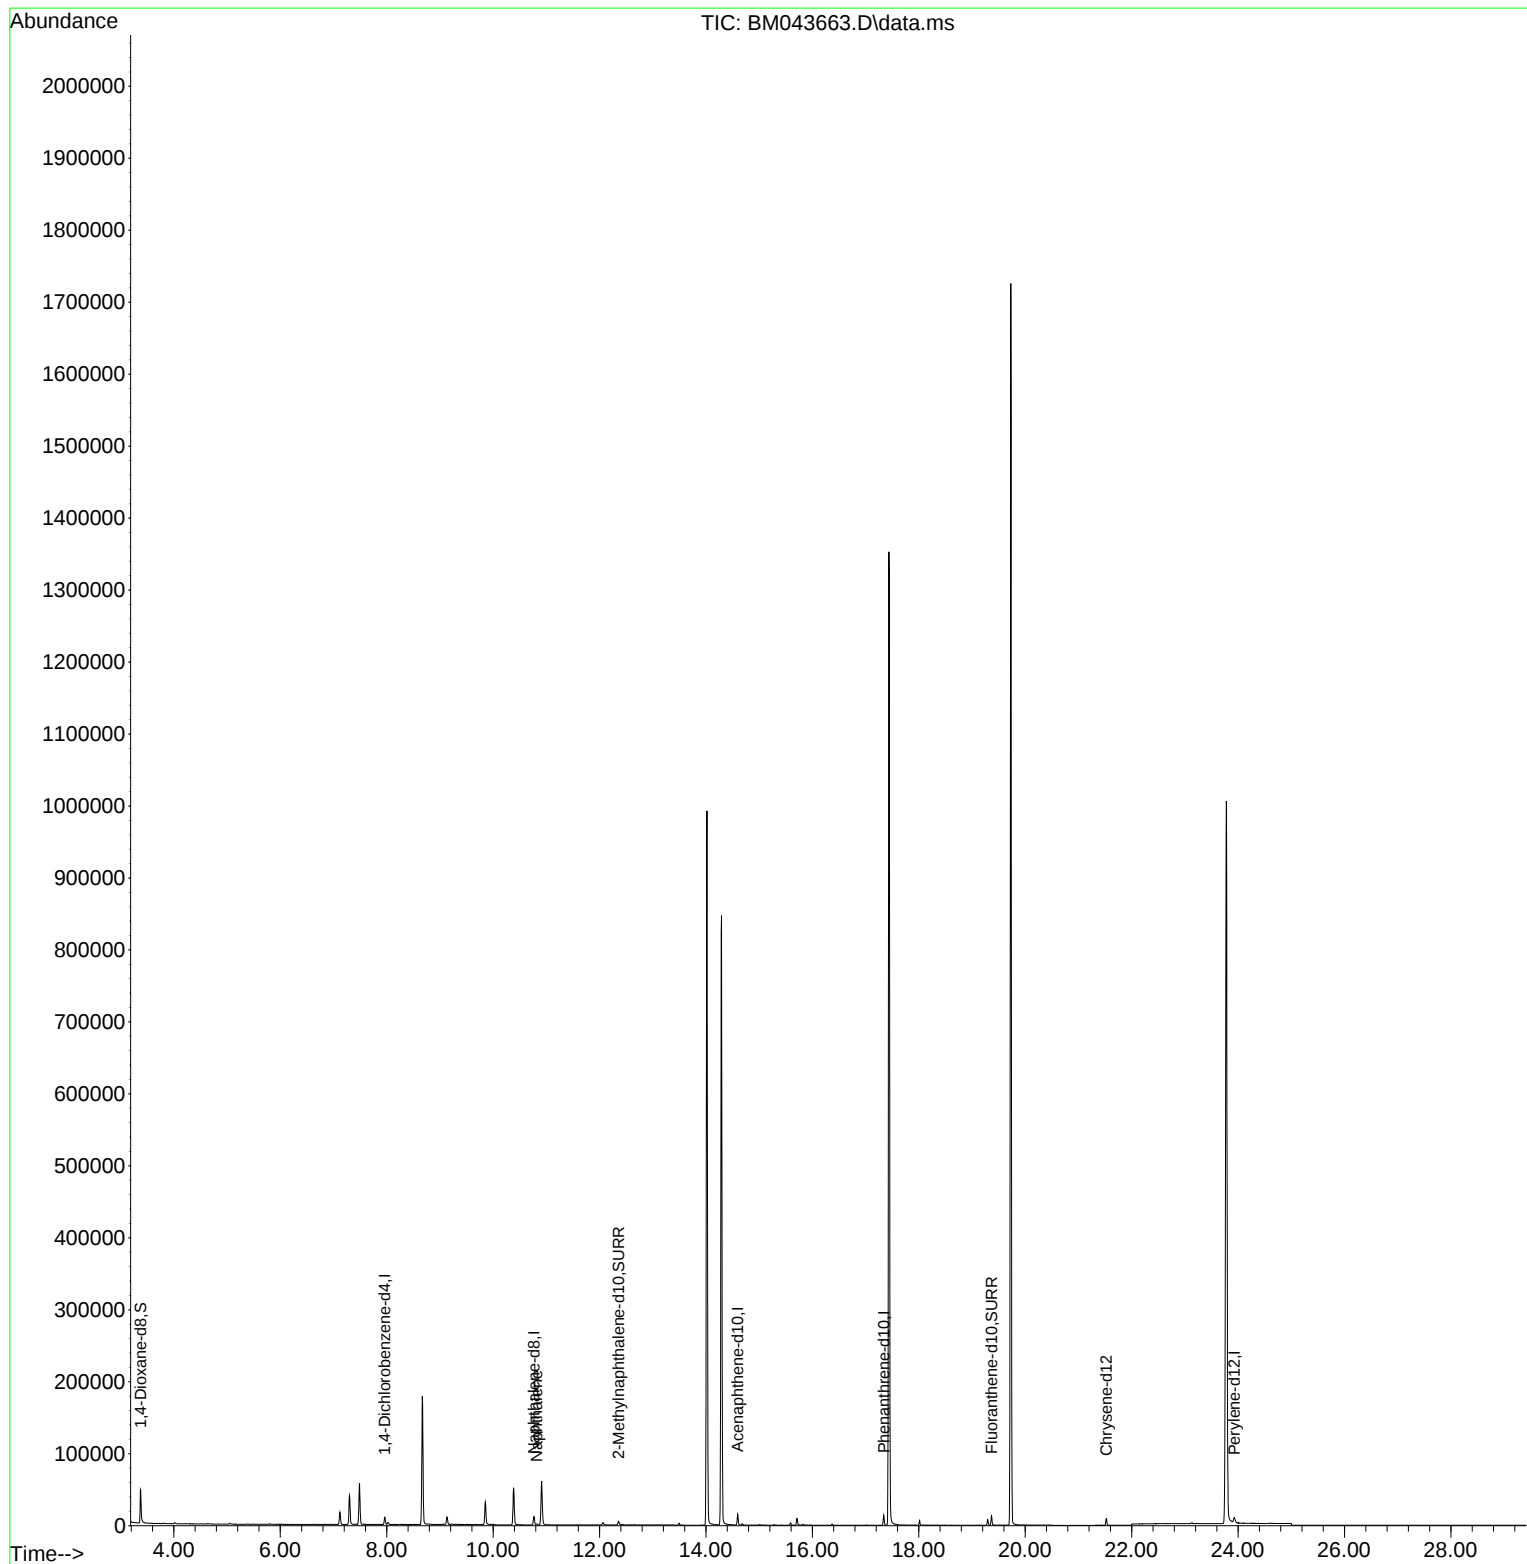

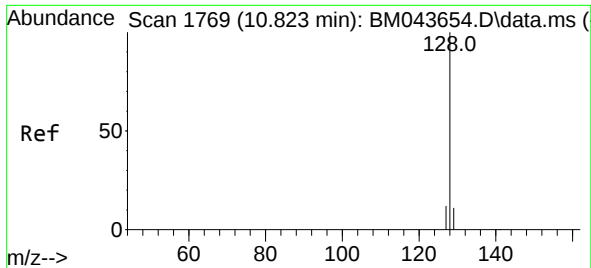

#5
Naphthalene
Concen: 0.035 ng/ul
RT: 10.818 min Scan# 1768
Delta R.T. -0.011 min
Lab File: BM043663.D
Acq: 29 Dec 2023 06:29

Instrument :
BNA_M
ClientSampleId :
C0AM7

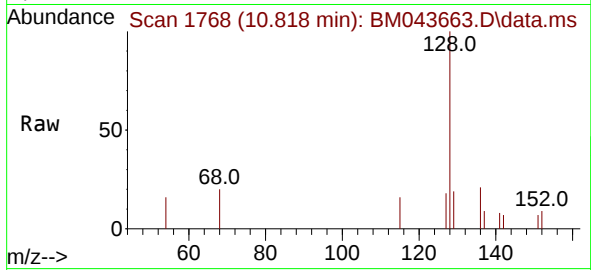

Tgt Ion:128 Resp: 1632
Ion Ratio Lower Upper
128 100
129 19.2 9.0 13.4
127 17.8 10.3 15.5

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/29/2023
Supervised By :mohammad ahmed 12/29/2023

