


Data Path : Z:\HPCHEM1\BNA_M\Data\BM122914\
Data File : BM000050.D
Acq On : 29 Dec 2014 08:56
Operator : TP
Sample : DFTPP01
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP01

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM122914.M
Title : SVOA CALIBRATION
Last Update : Wed Dec 31 02:57:11 2014

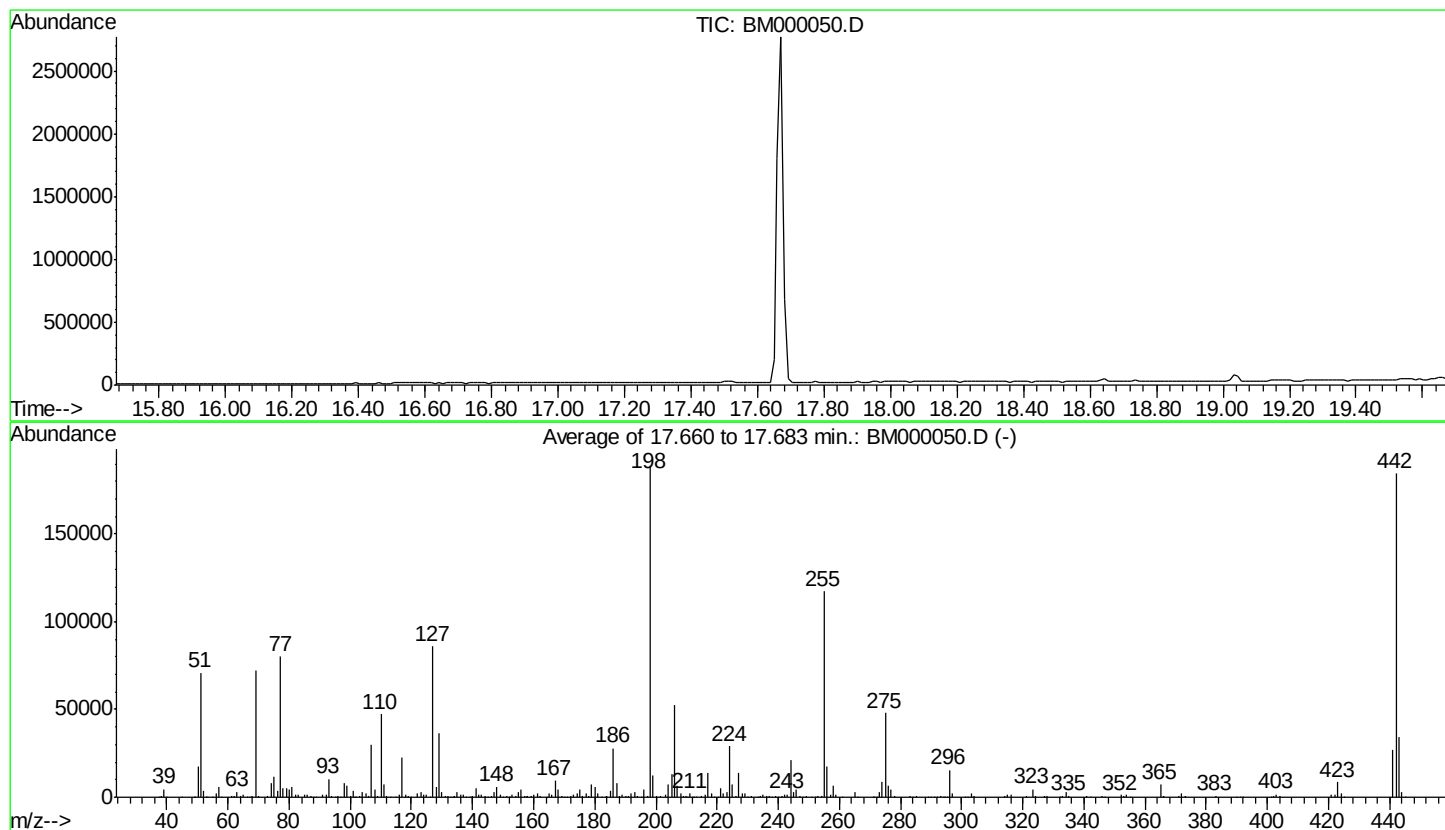

AutoFind: Scans 1310, 1311, 1312; Background Corrected with Scan 1307

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.5	70899	PASS
68	69	0.00	2	1.5	1105	PASS
69	198	0.00	100	38.4	72585	PASS
70	69	0.00	2	0.8	558	PASS
127	198	10	80	45.4	85888	PASS
197	198	0.00	2	0.4	825	PASS
198	198	100	100	100.0	189000	PASS
199	198	5	9	6.7	12733	PASS
275	198	10	60	25.4	48074	PASS
365	198	1	100	3.9	7288	PASS
441	443	0.01	100	77.9	26907	PASS
442	198	50	100	97.5	184320	PASS
443	442	15	24	18.7	34546	PASS