

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM122920\
 Data File : BM028277.D
 Acq On : 29 Dec 2020 11:25
 Operator : JU/CG
 Sample : PB133821BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK821

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120820.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.398	32	36	46	rVB	25354	35628	1.97%	0.177%
2	3.857	110	114	132	rBV	313962	505485	27.97%	2.513%
3	4.204	169	173	179	rVB2	6513	11232	0.62%	0.056%
4	7.322	691	703	716	rBV	393005	615470	34.06%	3.059%
5	7.498	725	733	741	rBV	296252	463424	25.65%	2.304%
6	7.704	761	768	781	rVB	410637	637263	35.27%	3.168%
7	8.181	843	849	857	rBV	295884	462023	25.57%	2.297%
8	8.886	962	969	981	rBV	460672	721725	39.94%	3.588%
9	9.357	1042	1049	1058	rVB	361728	578919	32.04%	2.878%
10	10.086	1165	1173	1180	rBV	287923	470949	26.06%	2.341%
11	10.622	1257	1264	1275	rVB	454288	732664	40.54%	3.642%
12	11.010	1323	1330	1337	rVB	394477	643095	35.59%	3.197%
13	11.139	1345	1352	1364	rBV	457755	752103	41.62%	3.739%
14	12.580	1592	1597	1602	rVB2	6476	9588	0.53%	0.048%
15	14.210	1868	1874	1880	rBV	757445	990125	54.79%	4.922%
16	14.510	1918	1925	1936	rBV	856489	1219110	67.46%	6.060%
17	14.810	1970	1976	1983	rBV	556808	815707	45.14%	4.055%
18	14.980	1999	2005	2014	rBV	353507	500946	27.72%	2.490%
19	15.792	2137	2143	2151	rVB	1060091	1461230	80.86%	7.264%
20	15.904	2157	2162	2173	rBV	337189	439824	24.34%	2.186%
21	16.033	2177	2184	2188	rVV2	10175	13429	0.74%	0.067%
22	16.568	2272	2275	2279	rVB4	2902	4058	0.22%	0.020%
23	17.327	2400	2404	2405	rBV3	1810	2559	0.14%	0.013%
24	17.533	2433	2439	2446	rVB	659983	905056	50.08%	4.499%
25	17.627	2449	2455	2464	rBV	1085725	1543971	85.44%	7.675%
26	17.939	2504	2508	2512	rVB6	1835	2536	0.14%	0.013%
27	19.527	2775	2778	2781	rVB2	11031	11945	0.66%	0.059%
28	19.780	2818	2821	2824	rBV	9265	9628	0.53%	0.048%
29	19.892	2834	2840	2845	rBV	1302076	1752955	97.01%	8.714%
30	21.644	3133	3138	3144	rBV	798400	1012005	56.00%	5.031%
31	23.850	3507	3513	3523	rVB	948251	1807053	100.00%	8.983%
32	24.003	3533	3539	3547	rVB2	518261	985013	54.51%	4.896%

LSC Area Percent Report

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM122920\
Data File : BM028277.D
Acq On : 29 Dec 2020 11:25
Operator : JU/CG
Sample : PB133821BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK821

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120820.M
Title : SVOA CALIBRATION


Sum of corrected areas: 20116718

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM122920\
Data File : BM028277.D
Acq On : 29 Dec 2020 11:25
Operator : JU/CG
Sample : PB133821BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK821

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120820.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

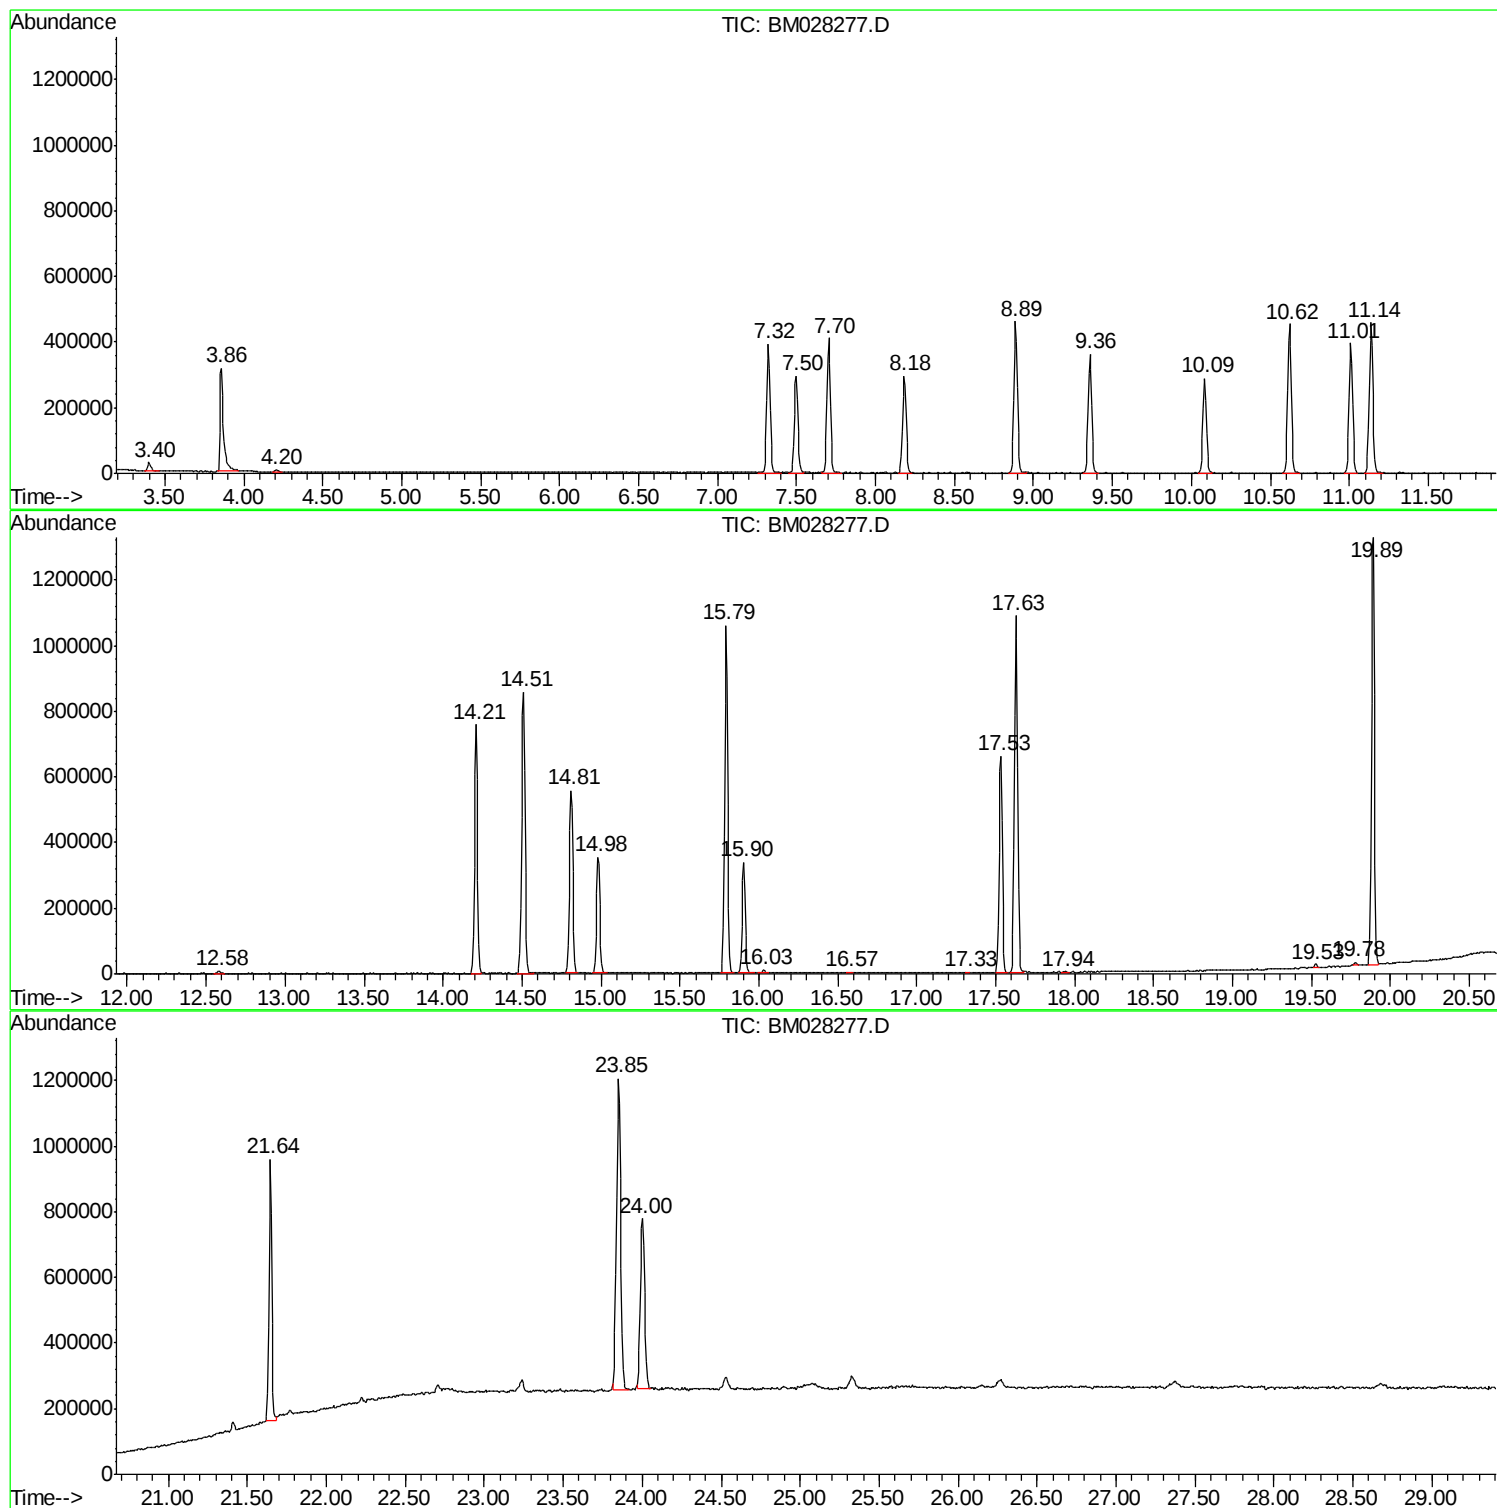

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM122920\
Data File : BM028277.D
Acq On : 29 Dec 2020 11:25
Operator : JU/CG
Sample : PB133821BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK821

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120820.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM122920\
Data File : BM028277.D
Acq On : 29 Dec 2020 11:25
Operator : JU/CG
Sample : PB133821BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK821

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120820.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc