

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122922\
 Data File : BM038337.D
 Acq On : 28 Dec 2022 20:11
 Operator : CG/JU
 Sample : SSTD16014
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD160017

Quant Time: Dec 29 01:57:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM122922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 29 01:45:50 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.004	152	82022	20.000	ng/u1	0.00
20) Naphthalene-d8	10.822	136	329133	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.639	164	211300	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.380	188	469739	20.000	ng/u1	0.00
79) Chrysene-d12	21.556	240	503226	20.000	ng/u1	0.00
88) Perylene-d12	23.991	264	536922	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.363	96	134187	74.282	ng/uL	0.00
4) Pyridine-d5	3.798	84	1065926	198.911	ng/u1	0.00
7) Phenol-d5	7.181	99	1198987	179.888	ng/u1	0.01
9) Bis-(2-Chloroethyl)eth...	7.339	67	744449	183.427	ng/u1	0.00
11) 2-Chlorophenol-d4	7.539	132	964188	176.344	ng/u1	0.00
15) 4-Methylphenol-d8	8.739	113	953539	183.276	ng/u1	0.02
21) Nitrobenzene-d5	9.186	128	478965	183.798	ng/u1	0.00
24) 2-Nitrophenol-d4	9.910	143	567749	207.897	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.451	165	1145911	220.916	ng/u1	0.01
31) 4-Chloroaniline-d4	10.974	131	1359387	189.855	ng/u1	0.01
46) Dimethylphthalate-d6	14.057	166	2974481	197.453	ng/u1	0.00
49) Acenaphthylene-d8	14.339	160	3673148	199.505	ng/u1	0.00
54) 4-Nitrophenol-d4	14.868	143	533965	207.984	ng/u1	0.02
60) Fluorene-d10	15.633	176	2666781	198.699	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.768	200	640381	254.987	ng/u1	0.02
73) Anthracene-d10	17.486	188	4191502	191.190	ng/u1	0.00
81) Pyrene-d10	19.768	212	5014021	165.869	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.844	264	5031182	187.604	ng/u1	0.02
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.398	88	142941	75.431	ng/uL	99
5) Pyridine	3.816	79	1070268	198.736	ng/u1	96
6) Benzaldehyde	7.145	77	309118	123.999	ng/u1	98
8) Phenol	7.210	94	1244318	186.144	ng/u1	98
10) Bis(2-Chloroethyl)ether	7.439	93	975196	177.658	ng/u1	94
12) 2-Chlorophenol	7.575	128	987665	176.625	ng/u1	95
13) 2-Methylphenol	8.463	108	925964	181.010	ng/u1	100
14) 2,2'-oxybis(1-Chloropr...	8.545	45	1271666	128.298	ng/u1	99
16) Acetophenone	8.851	105	1662417	203.163	ng/u1	96
17) N-Nitroso-di-n-propyla...	8.851	70	857390	222.430	ng/u1#	93
18) 4-Methylphenol	8.810	108	1011594	182.800	ng/u1	94
19) Hexachloroethane	9.092	117	463446	207.311	ng/u1	95
22) Nitrobenzene	9.233	77	1292254	230.465	ng/u1	96
23) Isophorone	9.769	82	2328394	226.609	ng/u1	97
25) 2-Nitrophenol	9.945	139	583009	203.631	ng/u1	93
26) 2,4-Dimethylphenol	10.004	107	1205984	217.818	ng/u1	94
27) Bis(2-Chloroethoxy)met...	10.239	93	1370244	200.616	ng/u1	98
29) 2,4-Dichlorophenol	10.480	162	1093459	214.859	ng/u1	97
30) Naphthalene	10.874	128	3233260	182.036	ng/u1	98
32) 4-Chloroaniline	10.998	127	1414418	198.093	ng/u1	98
33) Hexachlorobutadiene	11.145	225	787637	235.262	ng/u1	99
34) Caprolactam	11.821	113	149425	114.462	ng/u1	94
35) 4-Chloro-3-methylphenol	12.121	107	1043344	225.227	ng/u1	93
36) 2-Methylnaphthalene	12.480	142	2243230	194.721	ng/u1	98

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122922\
 Data File : BM038337.D
 Acq On : 28 Dec 2022 20:11
 Operator : CG/JU
 Sample : SSTD16014
 Misc :
 ALS Vial : 7 Sample Multiplier: 1


Instrument :
 BNA_M
 ClientSampleId :
 SSTD160017


Quant Time: Dec 29 01:57:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM122922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 29 01:45:50 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.698	142	2299757	195.229	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.845	216	1478042	214.084	ng/ul	100
40) Hexachlorocyclopentadiene	12.816	237	1089635	275.896	ng/ul	98
41) 2,4,6-Trichlorophenol	13.086	196	956083	227.348	ng/ul	99
42) 2,4,5-Trichlorophenol	13.163	196	1015516	231.544	ng/ul	97
43) 1,1'-Biphenyl	13.480	154	3134221	184.534	ng/ul	98
44) 2-Chloronaphthalene	13.527	162	2489517	190.004	ng/ul	98
45) 2-Nitroaniline	13.745	65	718262	227.512	ng/ul	92
47) Dimethylphthalate	14.110	163	3002263	201.999	ng/ul	99
48) 2,6-Dinitrotoluene	14.239	165	636298	220.405	ng/ul	93
50) Acenaphthylene	14.374	152	3811270	188.260	ng/ul	99
51) 3-Nitroaniline	14.568	138	509250	176.801	ng/ul	85
52) Acenaphthene	14.710	153	2616871	186.883	ng/ul	100
53) 2,4-Dinitrophenol	14.774	184	477627	337.157	ng/ul	96
55) 4-Nitrophenol	14.886	109	509009	300.637	ng/ul	92
56) Dibenzofuran	15.045	168	3593569	187.972	ng/ul	97
57) 2,4-Dinitrotoluene	15.021	165	905748	231.669	ng/ul	94
58) 2,3,4,6-Tetrachlorophenol	15.268	232	891834	241.735	ng/ul	97
59) Diethylphthalate	15.462	149	2968363	200.479	ng/ul	98
61) Fluorene	15.692	166	3011668	193.169	ng/ul	98
62) 4-Chlorophenyl-phenyle...	15.680	204	1532531	201.138	ng/ul	97
63) 4-Nitroaniline	15.733	138	383189	146.721	ng/ul	95
66) 4,6-Dinitro-2-methylph...	15.786	198	617348	253.916	ng/ul#	94
67) N-Nitrosodiphenylamine	15.898	169	2496270	176.171	ng/ul	98
68) 4-Bromophenyl-phenylether	16.574	248	990384	192.336	ng/ul	98
69) Hexachlorobenzene	16.692	284	1146179	186.475	ng/ul	97
70) Atrazine	16.851	200	991040	204.667	ng/ul	99
71) Pentachlorophenol	17.033	266	748593	219.056	ng/ul	98
72) Phenanthrene	17.427	178	4748678	185.116	ng/ul	100
74) Anthracene	17.521	178	4870525	186.830	ng/ul	98
75) 1,2,3,4-Tetrachloroben...	13.451	216	1435706	189.056	ng/ul	98
76) Pentachlorobenzene	14.962	250	1356048	180.262	ng/ul	99
77) Carbazole	17.792	167	4247401	188.055	ng/ul	99
78) Di-n-butylphthalate	18.339	149	5223369	194.563	ng/ul	99
80) Fluoranthene	19.439	202	5751208	161.208	ng/ul	98
82) Pyrene	19.803	202	5966778	160.703	ng/ul	99
83) Butylbenzylphthalate	20.680	149	2431214	176.095	ng/ul	97
84) 3,3'-Dichlorobenzidine	21.468	252	1694363	170.153	ng/ul	98
85) Benzo(a)anthracene	21.538	228	5779499	170.593	ng/ul	98
86) Bis(2-ethylhexyl)phtha...	21.444	149	3532363	175.870	ng/ul	96
87) Chrysene	21.597	228	5334104	167.808	ng/ul	98
89) Di-n-octyl phthalate	22.380	149	6149066	178.733	ng/ul	100
90) Benzo(b)fluoranthene	23.250	252	6183697	185.769	ng/ul	98
91) Benzo(k)fluoranthene	23.303	252	6067393	188.077	ng/ul	99
93) Benzo(a)pyrene	23.897	252	5491714	187.612	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.568	276	7077425	187.736	ng/ul	97
95) Dibenzo(a,h)anthracene	26.585	278	5862633	184.469	ng/ul	100
96) Benzo(g,h,i)perylene	27.362	276	5900772	196.045	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Dec 29 01:57:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM122922.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 29 01:45:50 2022
Response via : Initial Calibration









#2
1,4-Dioxane
Concen: 75.431 ng/uL
RT: 3.398 min Scan# 30
Delta R.T. -0.006 min
Lab File: BM038337.D
Acq: 28 Dec 2022 20:11




Instrument :
BNA_M
ClientSampleId :
SSTD160017


Tgt Ion: 88 Resp: 142941
Ion Ratio Lower Upper
88 100
43 33.7 26.6 40.0
58 76.1 59.9 89.9

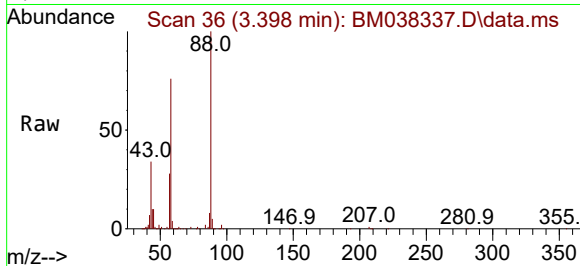

#5
Pyridine
Concen: 198.736 ng/uL
RT: 3.816 min Scan# 107
Delta R.T. -0.006 min
Lab File: BM038337.D
Acq: 28 Dec 2022 20:11

Tgt Ion: 79 Resp: 1070268
Ion Ratio Lower Upper
79 100
52 74.7 62.2 93.4
51 37.7 31.9 47.9




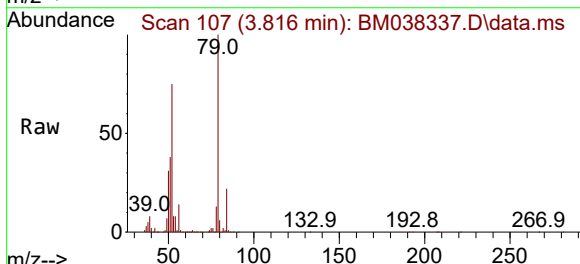




#6
Benzaldehyde
Concen: 123.999 ng/ul
RT: 7.145 min Scan# 611
Delta R.T. -0.000 min
Lab File: BM038337.D
Acq: 28 Dec 2022 20:11




Instrument :
BNA_M
ClientSampleId :
SSTD160017


Tgt Ion: 77 Resp: 309118
Ion Ratio Lower Upper
77 100
105 91.6 72.9 109.3
106 86.2 67.0 100.4



#8
Phenol
Concen: 186.144 ng/ul
RT: 7.210 min Scan# 684
Delta R.T. 0.011 min
Lab File: BM038337.D
Acq: 28 Dec 2022 20:11

Tgt Ion: 94 Resp: 1244318
Ion Ratio Lower Upper
94 100
65 31.5 26.3 39.5
66 42.5 35.2 52.8


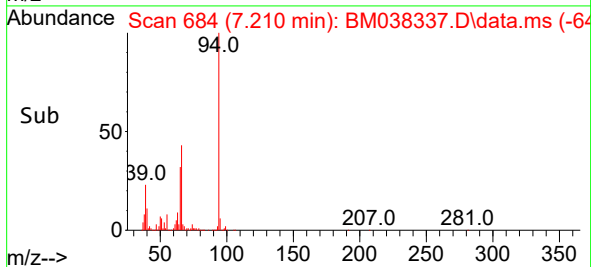

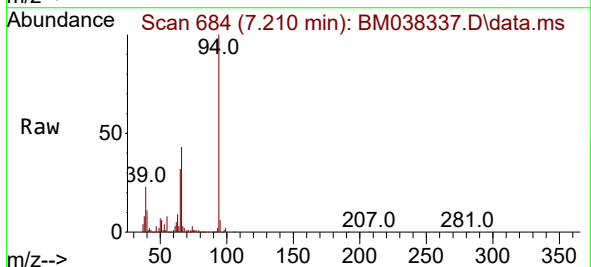




#10
Bis(2-Chloroethyl)ether
Concen: 177.658 ng/ul
RT: 7.439 min Scan# 721
Delta R.T. 0.011 min
Lab File: BM038337.D
Acq: 28 Dec 2022 20:11




Instrument :
BNA_M
ClientSampleId :
SSTD160017


Tgt Ion: 93 Resp: 975196
Ion Ratio Lower Upper
93 100
63 77.1 67.7 101.5
95 32.7 26.7 40.1

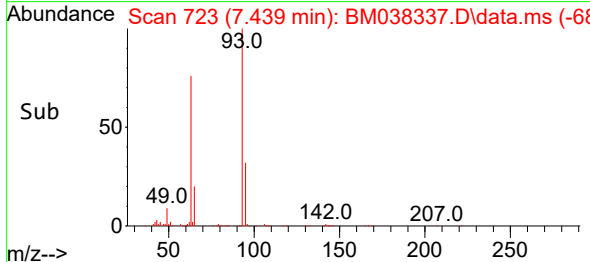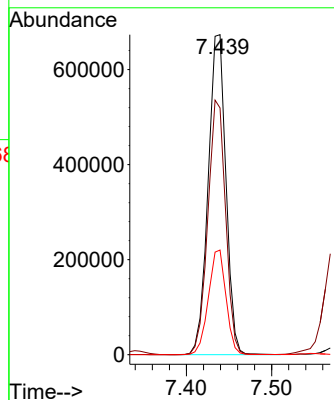

#12
2-Chlorophenol
Concen: 176.625 ng/ul
RT: 7.575 min Scan# 746
Delta R.T. 0.005 min
Lab File: BM038337.D
Acq: 28 Dec 2022 20:11

Tgt Ion:128 Resp: 987665
Ion Ratio Lower Upper
128 100
64 48.7 42.6 63.8
130 32.7 27.7 41.5

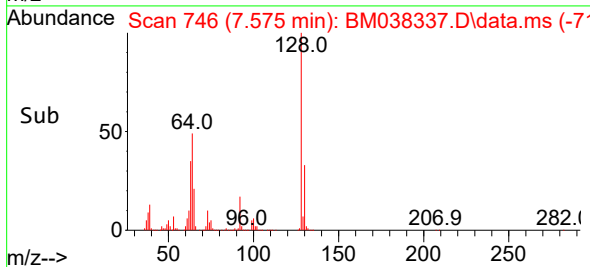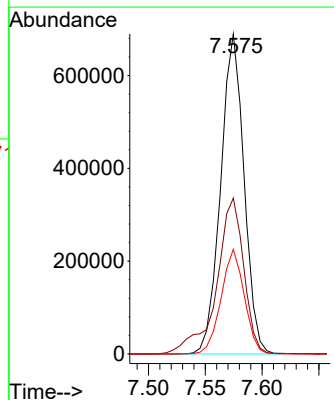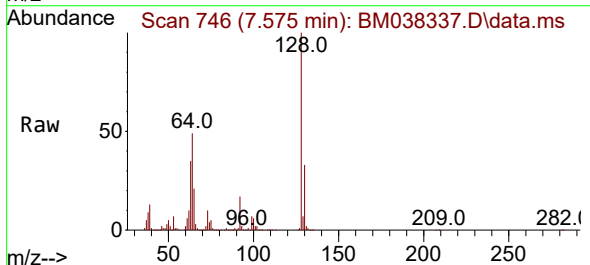



#13

2-Methylphenol

Concen: 181.010 ng/ul

RT: 8.463 min Scan# 896

Delta R.T. 0.005 min

Lab File: BM038337.D

Acq: 28 Dec 2022 20:11

Instrument :

BNA_M

ClientSampleId :





SSTD160017

Tgt Ion:108 Resp: 925964

Ion Ratio Lower Upper

108 100

107 88.8 71.4 107.0

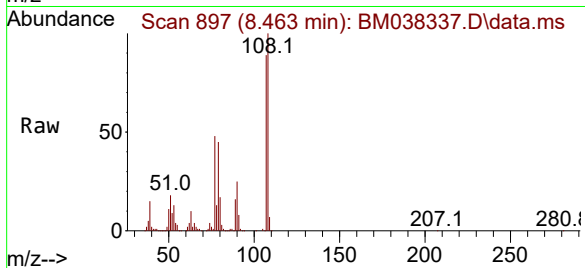

#14

2,2'-oxybis(1-Chloropropane)

Concen: 128.298 ng/ul

RT: 8.545 min Scan# 911

Delta R.T. 0.005 min

Lab File: BM038337.D

Acq: 28 Dec 2022 20:11




Tgt Ion: 45 Resp: 1271666


Ion Ratio Lower Upper

45 100

77 15.2 12.4 18.6

79 12.5 9.3 13.9




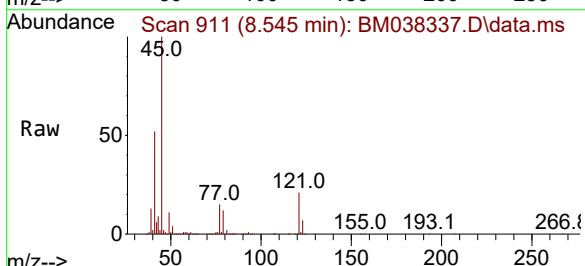




#16
Acetophenone
Concen: 203.163 ng/ul
RT: 8.851 min Scan# 961
Delta R.T. 0.011 min
Lab File: BM038337.D
Acq: 28 Dec 2022 20:11




Instrument :
BNA_M
ClientSampleId :
SSTD160017


Tgt Ion:105 Resp: 1662417
Ion Ratio Lower Upper
105 100
77 78.2 64.6 97.0
51 26.8 23.9 35.9



#17
N-Nitroso-di-n-propylamine
Concen: 222.430 ng/ul
RT: 8.851 min Scan# 963
Delta R.T. 0.035 min
Lab File: BM038337.D
Acq: 28 Dec 2022 20:11

Tgt Ion: 70 Resp: 857390
Ion Ratio Lower Upper
70 100
42 55.2 49.0 73.4
101 9.6 7.0 10.6
130 20.2 13.3 19.9









#18
4-Methylphenol
Concen: 182.800 ng/ul
RT: 8.810 min Scan# 91
Delta R.T. 0.023 min
Lab File: BM038337.D
Acq: 28 Dec 2022 20:11




Instrument :
BNA_M
ClientSampleId :
SSTD160017


Tgt Ion:108 Resp: 1011594
Ion Ratio Lower Upper
108 100
107 111.3 94.3 141.5

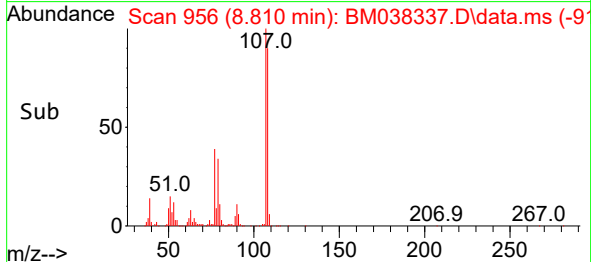

#19
Hexachloroethane
Concen: 207.311 ng/ul
RT: 9.092 min Scan# 1004
Delta R.T. 0.005 min
Lab File: BM038337.D
Acq: 28 Dec 2022 20:11

Tgt Ion:117 Resp: 463446
Ion Ratio Lower Upper
117 100
201 120.7 92.0 138.0
199 74.7 56.1 84.1


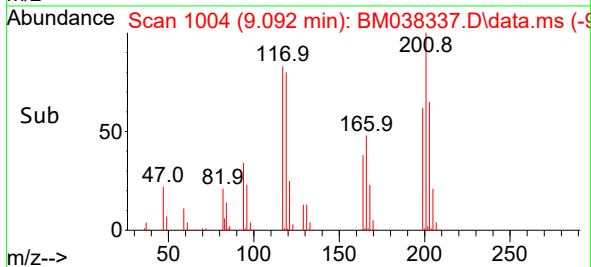

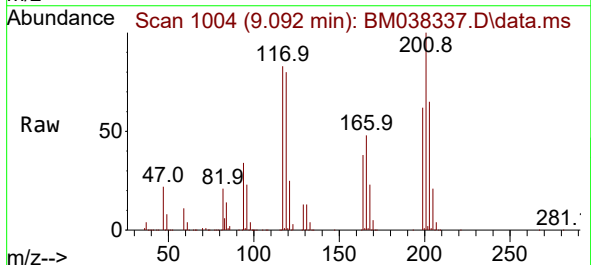




#22
Nitrobenzene
Concen: 230.465 ng/ul
RT: 9.233 min Scan# 1026
Delta R.T. 0.011 min
Lab File: BM038337.D
Acq: 28 Dec 2022 20:11




Instrument :
BNA_M
ClientSampleId :
SSTD160017


Tgt Ion: 77 Resp: 1292254
Ion Ratio Lower Upper
77 100
123 41.1 30.2 45.4
65 13.5 11.3 16.9

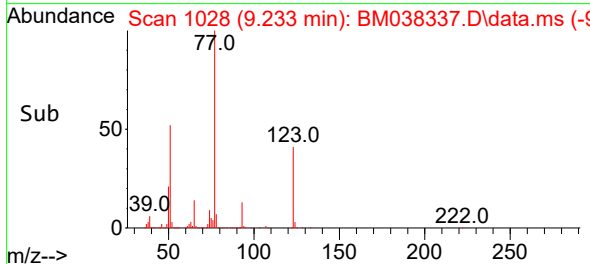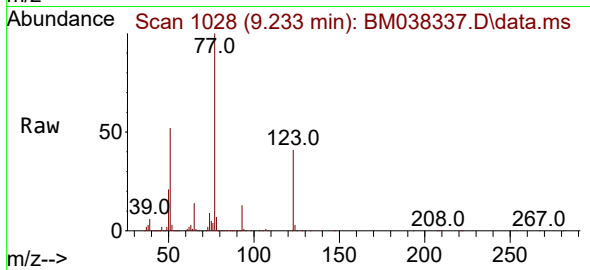

#23
Isophorone
Concen: 226.609 ng/ul
RT: 9.769 min Scan# 1119
Delta R.T. 0.023 min
Lab File: BM038337.D
Acq: 28 Dec 2022 20:11

Tgt Ion: 82 Resp: 2328394
Ion Ratio Lower Upper
82 100
95 7.4 5.3 7.9
138 16.5 12.3 18.5


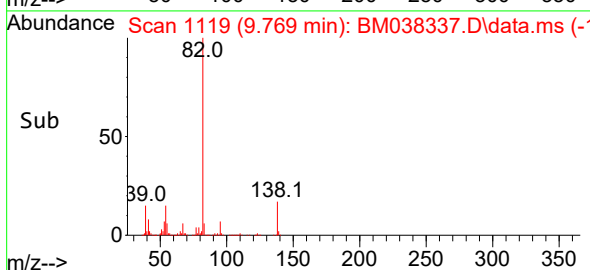

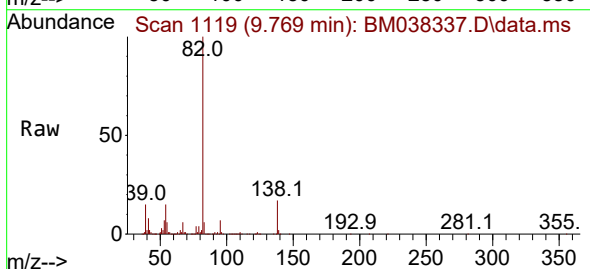




#25
2-Nitrophenol
Concen: 203.631 ng/ul
RT: 9.945 min Scan# 1147
Delta R.T. 0.011 min
Lab File: BM038337.D
Acq: 28 Dec 2022 20:11




Instrument :
BNA_M
ClientSampleId :
SSTD160017


Tgt Ion:139 Resp: 583009
Ion Ratio Lower Upper
139 100
65 56.3 51.4 77.0
109 35.9 29.8 44.8

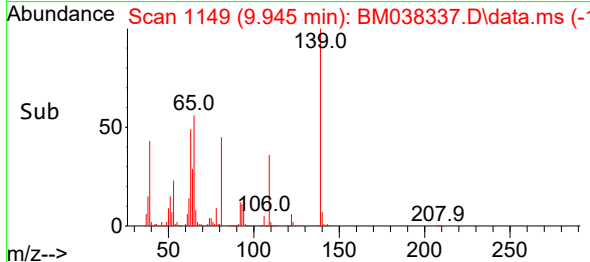

#26
2,4-Dimethylphenol
Concen: 217.818 ng/ul
RT: 10.004 min Scan# 1159
Delta R.T. 0.011 min
Lab File: BM038337.D
Acq: 28 Dec 2022 20:11

Tgt Ion:107 Resp: 1205984
Ion Ratio Lower Upper
107 100
121 48.2 35.4 53.0
122 82.3 61.4 92.2

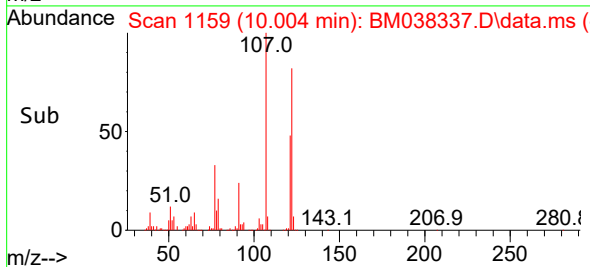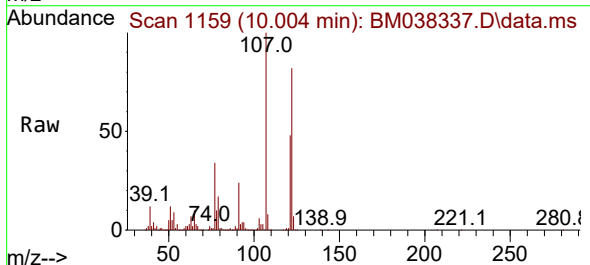



#27

Bis(2-Chloroethoxy)methane

Concen: 200.616 ng/ul

RT: 10.239 min Scan# 1199

Delta R.T. 0.011 min

Lab File: BM038337.D

Acq: 28 Dec 2022 20:11

Instrument :





BNA_M

ClientSampleId :

SSTD160017

Tgt Ion: 93 Resp: 1370244

Ion	Ratio	Lower	Upper
93	100		
95	32.3	25.3	37.9
123	10.7	7.8	11.8

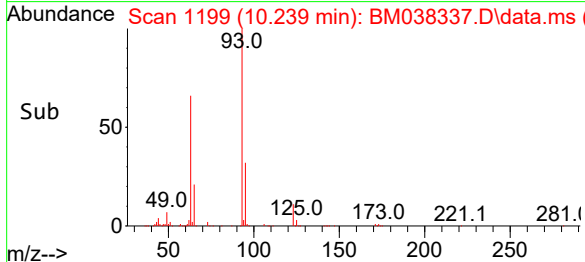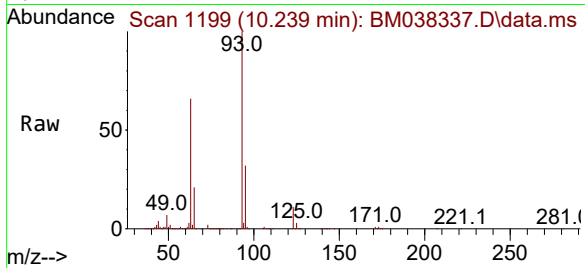

#29

2,4-Dichlorophenol

Concen: 214.859 ng/ul

RT: 10.480 min Scan# 1240




Delta R.T. 0.011 min


Lab File: BM038337.D

Acq: 28 Dec 2022 20:11

Tgt Ion:162 Resp: 1093459

Ion	Ratio	Lower	Upper
162	100		
164	66.1	52.4	78.6
98	33.2	29.6	44.4

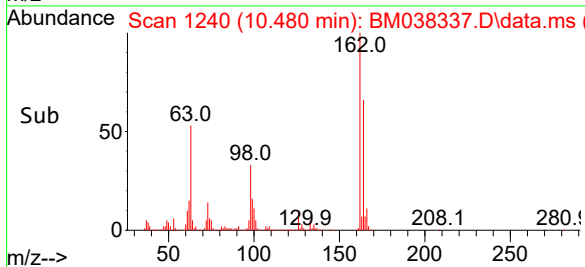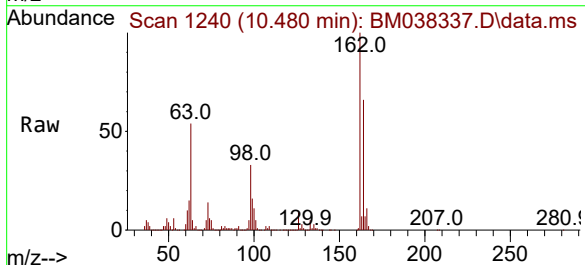



#30

Naphthalene

Concen: 182.036 ng/ul

RT: 10.874 min Scan# 11

Delta R.T. 0.006 min

Lab File: BM038337.D

Acq: 28 Dec 2022 20:11

Instrument :

BNA_M

ClientSampleId :

SSTD160017





Tgt Ion:128 Resp: 3233260

Ion Ratio Lower Upper

128 100

129 11.2 8.6 12.8

127 12.9 10.9 16.3

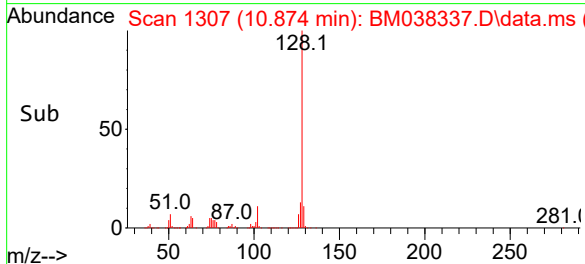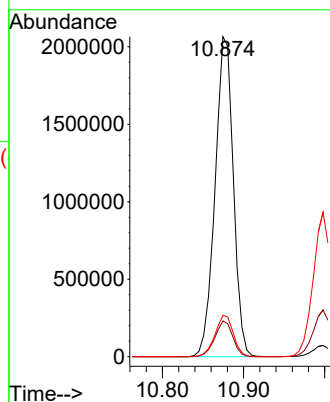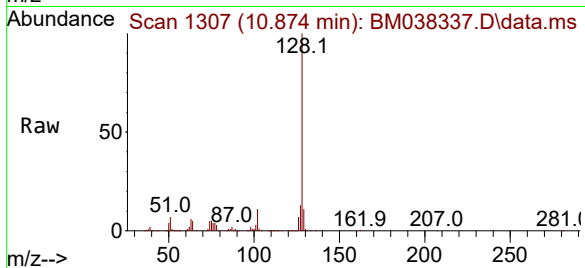

#32

4-Chloroaniline

Concen: 198.093 ng/ul

RT: 10.998 min Scan# 1328

Delta R.T. 0.011 min

Lab File: BM038337.D




Acq: 28 Dec 2022 20:11


Tgt Ion:127 Resp: 1414418

Ion Ratio Lower Upper

127 100

129 32.3 24.7 37.1

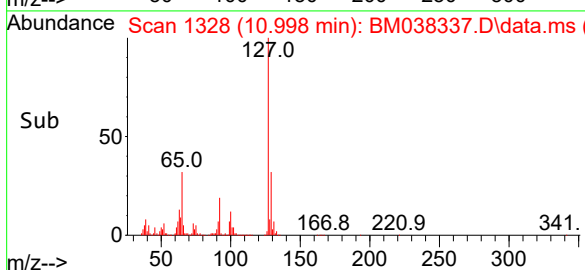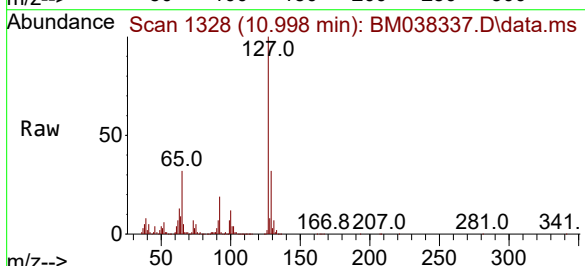



#33

Hexachlorobutadiene

Concen: 235.262 ng/ul

RT: 11.145 min Scan# 1

Delta R.T. -0.000 min

Lab File: BM038337.D

Acq: 28 Dec 2022 20:11

Instrument :

BNA_M

ClientSampleId :

SSTD160017





Tgt Ion:225 Resp: 787637

Ion Ratio Lower Upper

225 100

223 63.1 50.6 76.0

227 63.9 49.7 74.5

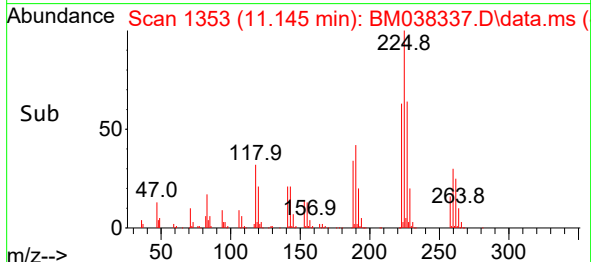

#34

Caprolactam

Concen: 114.462 ng/ul

RT: 11.821 min Scan# 1468

Delta R.T. 0.047 min

Lab File: BM038337.D

Acq: 28 Dec 2022 20:11




Tgt Ion:113 Resp: 149425


Ion Ratio Lower Upper

113 100

55 186.9 160.5 240.7

56 147.1 119.0 178.6









#35
4-Chloro-3-methylphenol
Concen: 225.227 ng/ul
RT: 12.121 min Scan# 1519
Delta R.T. 0.017 min
Lab File: BM038337.D
Acq: 28 Dec 2022 20:11




Instrument :
BNA_M
ClientSampleId :
SSTD160017


Tgt Ion:107 Resp: 1043344
Ion Ratio Lower Upper
107 100
144 26.5 20.1 30.1
142 81.5 59.4 89.2



#36
2-Methylnaphthalene
Concen: 194.721 ng/ul
RT: 12.480 min Scan# 1580
Delta R.T. 0.005 min
Lab File: BM038337.D
Acq: 28 Dec 2022 20:11

Tgt Ion:142 Resp: 2243230
Ion Ratio Lower Upper
142 100
141 87.6 71.3 106.9


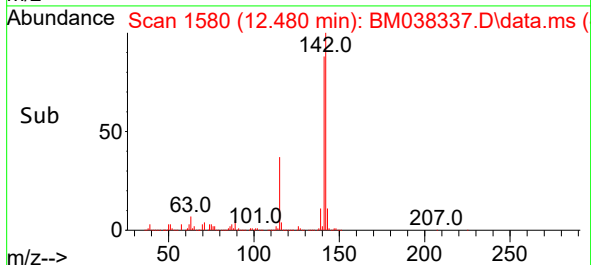

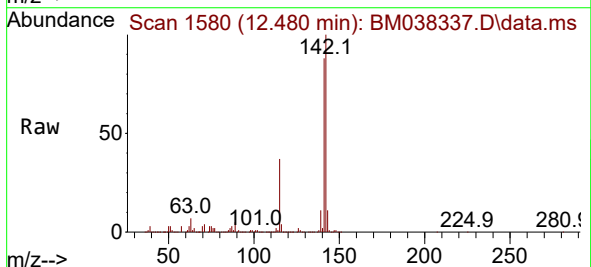




#37
1-Methylnaphthalene
Concen: 195.229 ng/ul
RT: 12.698 min Scan# 1
Delta R.T. 0.005 min
Lab File: BM038337.D
Acq: 28 Dec 2022 20:11




Instrument :
BNA_M
ClientSampleId :
SSTD160017


Tgt Ion:142 Resp: 2299757
Ion Ratio Lower Upper
142 100
141 91.5 74.0 111.0
116 4.1 3.7 5.5

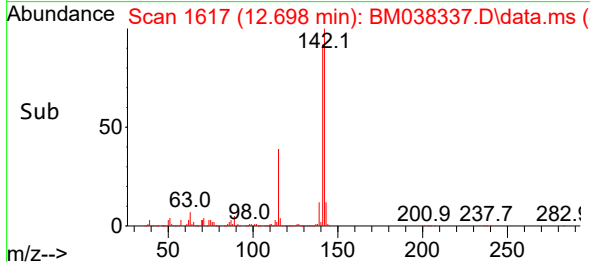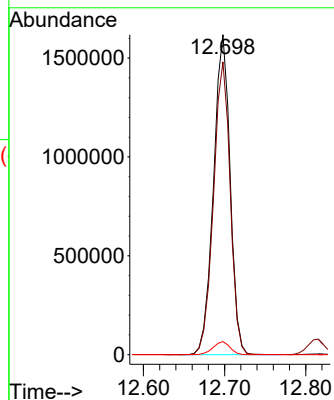

#39
1,2,4,5-Tetrachlorobenzene
Concen: 214.084 ng/ul
RT: 12.845 min Scan# 1642
Delta R.T. 0.005 min
Lab File: BM038337.D
Acq: 28 Dec 2022 20:11

Tgt Ion:216 Resp: 1478042
Ion Ratio Lower Upper
216 100
214 77.9 62.2 93.4
179 19.5 15.5 23.3
108 14.0 11.4 17.2


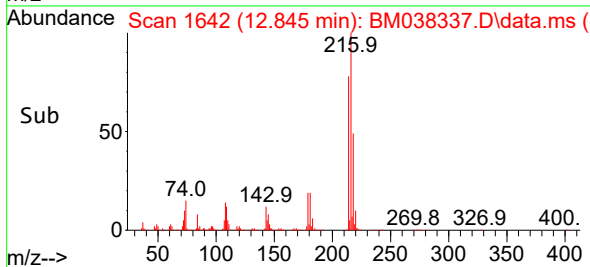
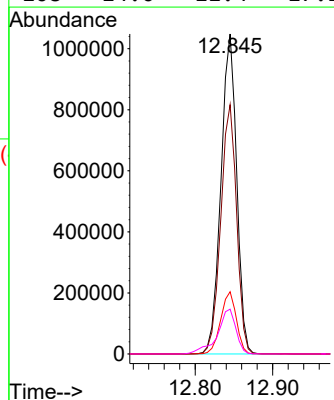
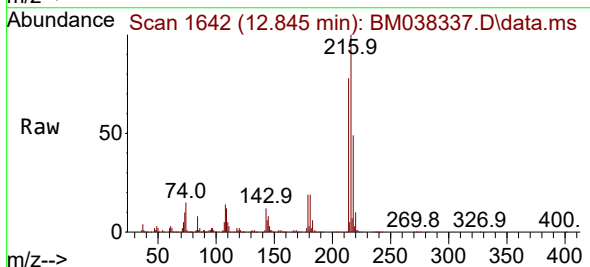




#40
Hexachlorocyclopentadiene
Concen: 275.896 ng/ul
RT: 12.816 min Scan# 1637
Delta R.T. 0.005 min
Lab File: BM038337.D
Acq: 28 Dec 2022 20:11




Instrument :
BNA_M
ClientSampleId :
SSTD160017


Tgt Ion:237 Resp: 1089635
Ion Ratio Lower Upper
237 100
235 62.3 51.0 76.6
272 13.1 10.7 16.1

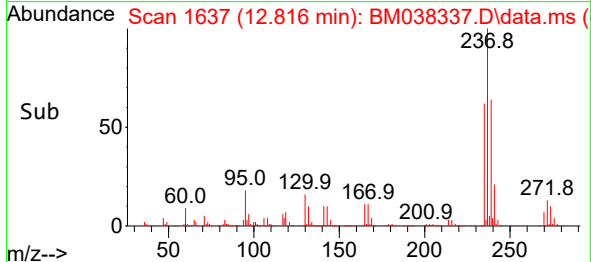

#41
2,4,6-Trichlorophenol
Concen: 227.348 ng/ul
RT: 13.086 min Scan# 1683
Delta R.T. 0.005 min
Lab File: BM038337.D
Acq: 28 Dec 2022 20:11

Tgt Ion:196 Resp: 956083
Ion Ratio Lower Upper
196 100
198 97.0 77.3 115.9
200 31.5 24.7 37.1

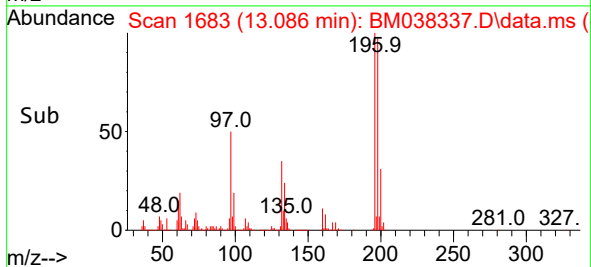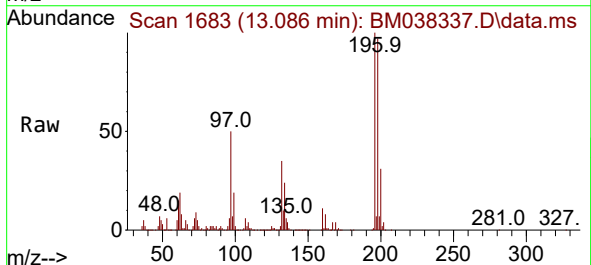



#42

2,4,5-Trichlorophenol

Concen: 231.544 ng/ul

RT: 13.163 min Scan# 1

Delta R.T. 0.011 min

Lab File: BM038337.D

Acq: 28 Dec 2022 20:11

Instrument :

BNA_M

ClientSampleId :

SSTD160017





Tgt Ion:196 Resp: 1015516

Ion Ratio Lower Upper

196 100

198 96.6 80.1 120.1

200 32.1 26.2 39.4

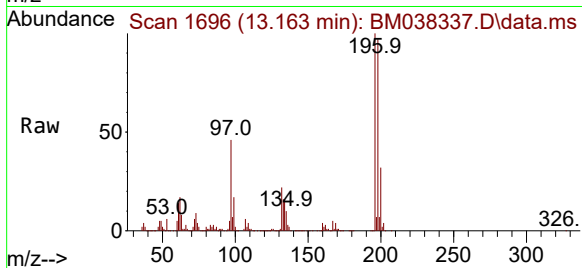

#43

1,1'-Biphenyl

Concen: 184.534 ng/ul

RT: 13.480 min Scan# 1750

Delta R.T. 0.005 min

Lab File: BM038337.D

Acq: 28 Dec 2022 20:11




Tgt Ion:154 Resp: 3134221


Ion Ratio Lower Upper

154 100

153 39.8 32.6 49.0

76 10.9 9.7 14.5


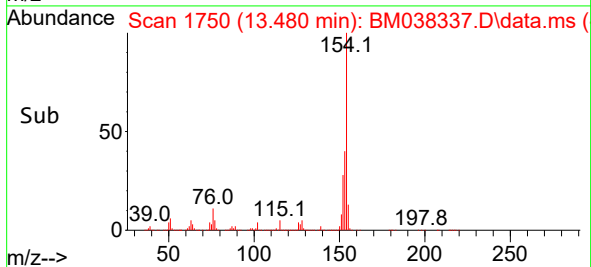

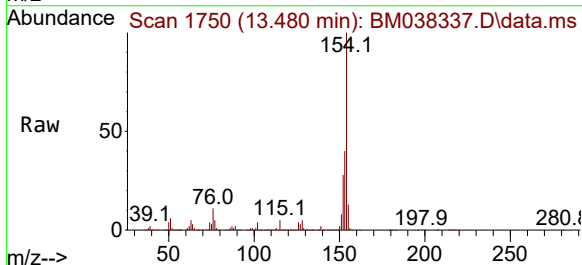




#44
2-Chloronaphthalene
Concen: 190.004 ng/ul
RT: 13.527 min Scan# 1757
Delta R.T. 0.005 min
Lab File: BM038337.D
Acq: 28 Dec 2022 20:11




Instrument :
BNA_M
ClientSampleId :
SSTD160017


Tgt Ion:162 Resp: 2489517
Ion Ratio Lower Upper
162 100
164 33.7 27.3 40.9
127 35.4 30.1 45.1

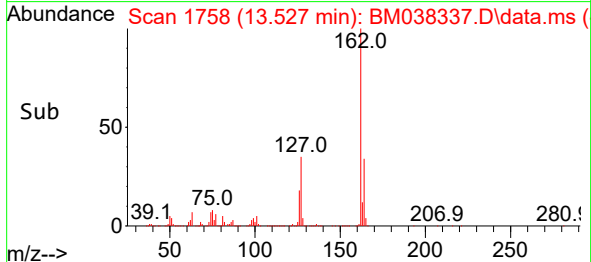

#45
2-Nitroaniline
Concen: 227.512 ng/ul
RT: 13.745 min Scan# 1795
Delta R.T. 0.011 min
Lab File: BM038337.D
Acq: 28 Dec 2022 20:11

Tgt Ion: 65 Resp: 718262
Ion Ratio Lower Upper
65 100
92 65.9 51.7 77.5
138 102.5 72.0 108.0









#47
Dimethylphthalate
Concen: 201.999 ng/ul
RT: 14.110 min Scan# 1857
Delta R.T. 0.017 min
Lab File: BM038337.D
Acq: 28 Dec 2022 20:11




Instrument :
BNA_M
ClientSampleId :
SSTD160017


Tgt Ion:163 Resp: 3002263
Ion Ratio Lower Upper
163 100
194 4.2 3.0 4.6
164 10.1 8.3 12.5

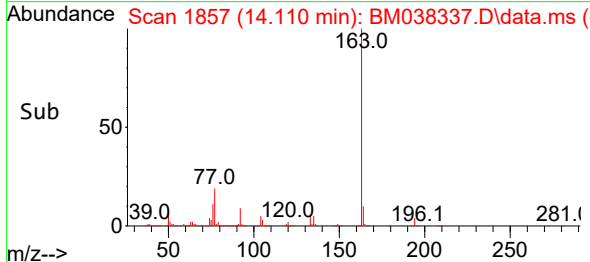

#48
2,6-Dinitrotoluene
Concen: 220.405 ng/ul
RT: 14.239 min Scan# 1879
Delta R.T. 0.017 min
Lab File: BM038337.D
Acq: 28 Dec 2022 20:11

Tgt Ion:165 Resp: 636298
Ion Ratio Lower Upper
165 100
89 58.8 52.3 78.5
121 19.8 17.7 26.5


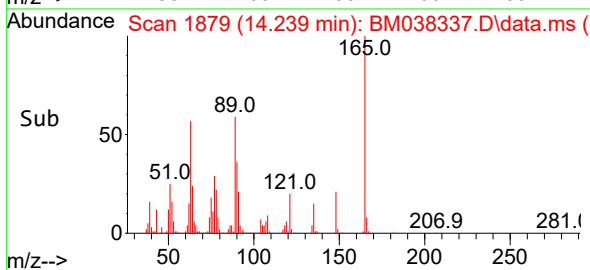

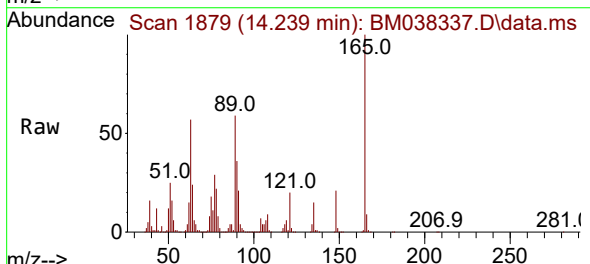




#50
Acenaphthylene
Concen: 188.260 ng/ul
RT: 14.374 min Scan# 1902
Delta R.T. 0.011 min
Lab File: BM038337.D
Acq: 28 Dec 2022 20:11




Instrument :
BNA_M
ClientSampleId :
SSTD160017


Tgt Ion:152 Resp: 3811270
Ion Ratio Lower Upper
152 100
151 19.7 15.8 23.6
153 13.4 10.1 15.1

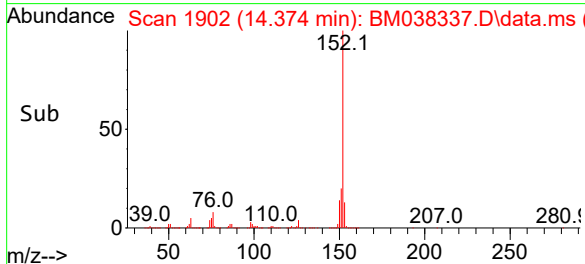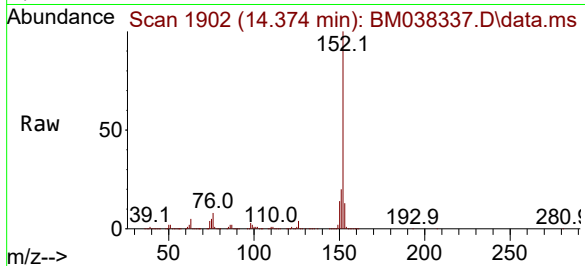

#51
3-Nitroaniline
Concen: 176.801 ng/ul
RT: 14.568 min Scan# 1935
Delta R.T. 0.017 min
Lab File: BM038337.D
Acq: 28 Dec 2022 20:11

Tgt Ion:138 Resp: 509250
Ion Ratio Lower Upper
138 100
108 9.7 8.6 13.0
92 115.7 108.0 162.0

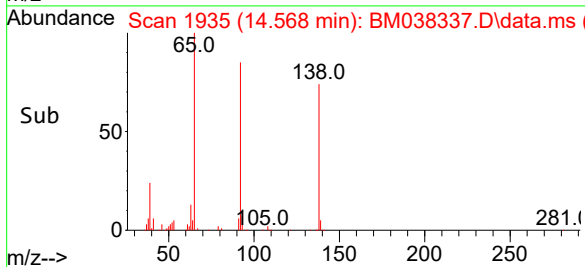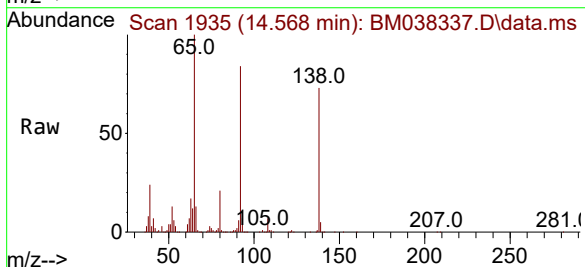



#52

Acenaphthene

Concen: 186.883 ng/ul

RT: 14.710 min Scan# 1958

Delta R.T. 0.006 min

Lab File: BM038337.D

Acq: 28 Dec 2022 20:11

Instrument :

BNA_M

ClientSampleId :

SSTD160017





Tgt Ion:153 Resp: 2616871

Ion Ratio Lower Upper

153 100

152 47.6 38.5 57.7

154 89.0 71.4 107.2

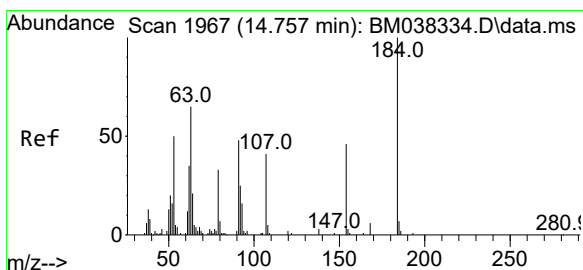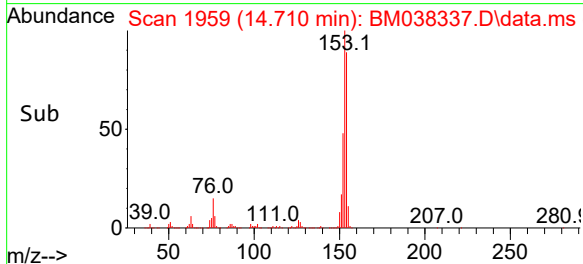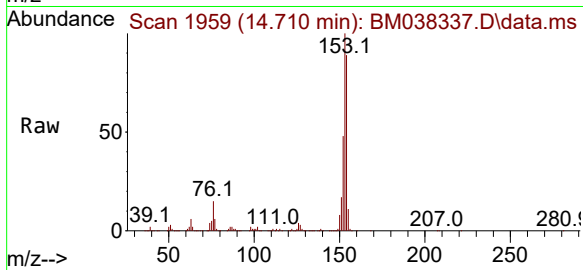

#53

2,4-Dinitrophenol

Concen: 337.157 ng/ul

RT: 14.774 min Scan# 1970

Delta R.T. 0.017 min

Lab File: BM038337.D

Acq: 28 Dec 2022 20:11




Tgt Ion:184 Resp: 477627


Ion Ratio Lower Upper

184 100

63 61.8 53.2 79.8

154 62.2 48.8 73.2


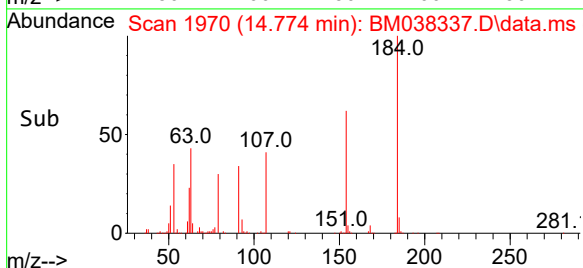
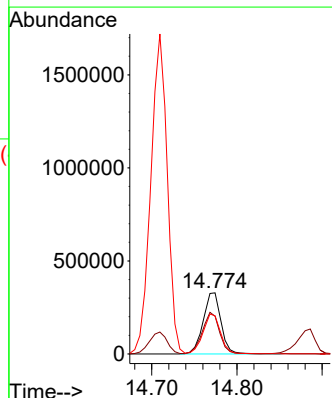
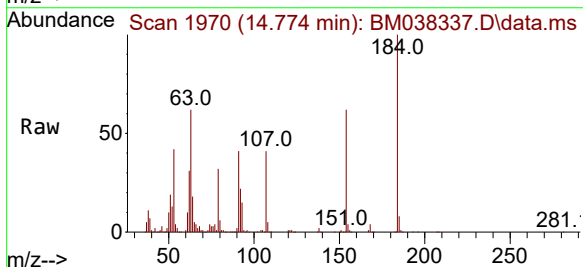




#55
4-Nitrophenol
Concen: 300.637 ng/ul
RT: 14.886 min Scan# 1984
Delta R.T. 0.029 min
Lab File: BM038337.D
Acq: 28 Dec 2022 20:11




Instrument :
BNA_M
ClientSampleId :
SSTD160017


Tgt Ion:109 Resp: 509009
Ion Ratio Lower Upper
109 100
139 110.9 85.0 127.4
65 114.4 101.0 151.4

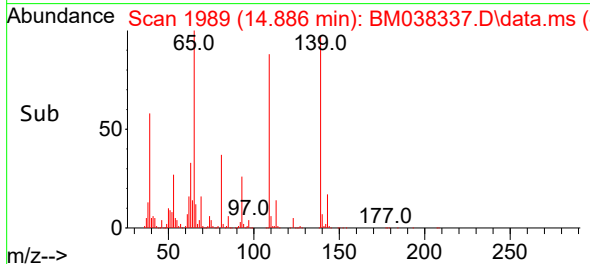

#56
Dibenzofuran
Concen: 187.972 ng/ul
RT: 15.045 min Scan# 2016
Delta R.T. 0.011 min
Lab File: BM038337.D
Acq: 28 Dec 2022 20:11

Tgt Ion:168 Resp: 3593569
Ion Ratio Lower Upper
168 100
139 36.0 30.4 45.6

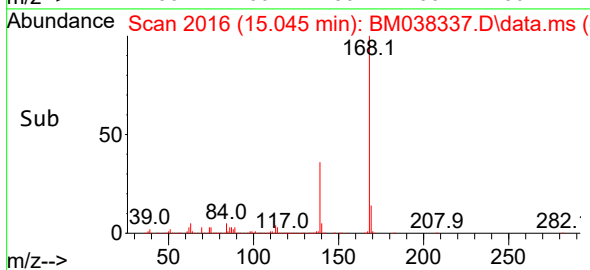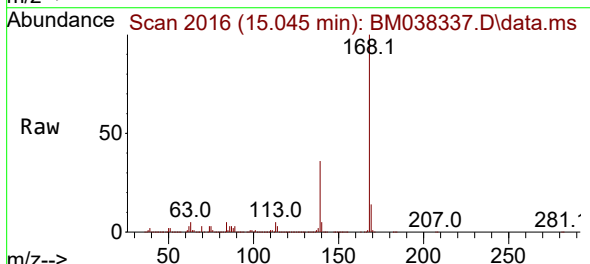



#57

2,4-Dinitrotoluene

Concen: 231.669 ng/ul

RT: 15.021 min Scan# 2012

Delta R.T. 0.017 min

Lab File: BM038337.D

Acq: 28 Dec 2022 20:11

Instrument :

BNA_M

ClientSampleId :

SSTD160017





Tgt Ion:165 Resp: 905748

Ion Ratio Lower Upper

165 100

63 46.4 40.4 60.6

182 2.4 1.8 2.8

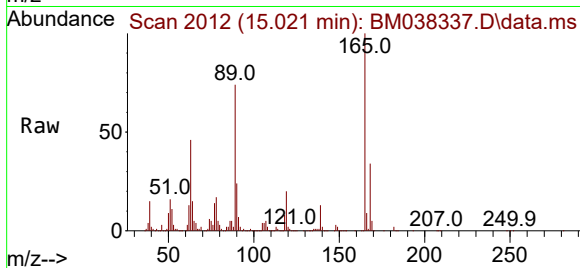

#58

2,3,4,6-Tetrachlorophenol

Concen: 241.735 ng/ul

RT: 15.268 min Scan# 2054

Delta R.T. 0.005 min

Lab File: BM038337.D

Acq: 28 Dec 2022 20:11

Tgt Ion:232 Resp: 891834




Ion Ratio Lower Upper


232 100

131 39.3 33.4 50.0

130 2.2 1.6 2.4

166 28.1 22.2 33.2




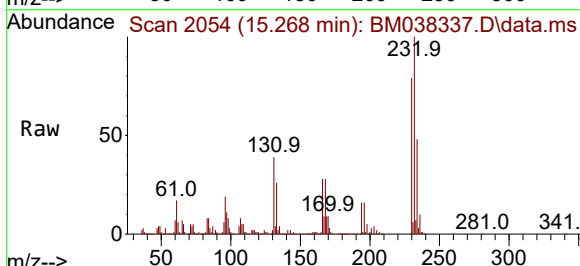




#59
Diethylphthalate
Concen: 200.479 ng/ul
RT: 15.462 min Scan# 2085
Delta R.T. 0.011 min
Lab File: BM038337.D
Acq: 28 Dec 2022 20:11




Instrument :
BNA_M
ClientSampleId :
SSTD160017


Tgt Ion:149 Resp: 2968363
Ion Ratio Lower Upper
149 100
177 22.8 17.4 26.0
150 12.0 9.6 14.4

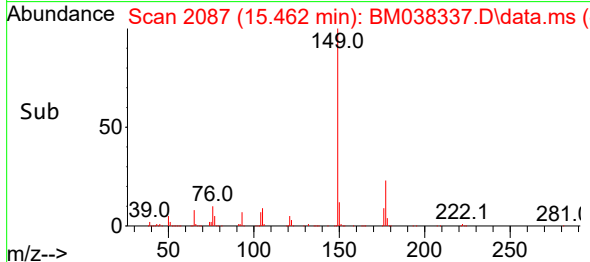

#61
Fluorene
Concen: 193.169 ng/ul
RT: 15.692 min Scan# 2126
Delta R.T. 0.011 min
Lab File: BM038337.D
Acq: 28 Dec 2022 20:11

Tgt Ion:166 Resp: 3011668
Ion Ratio Lower Upper
166 100
165 96.7 78.9 118.3
167 13.6 10.3 15.5


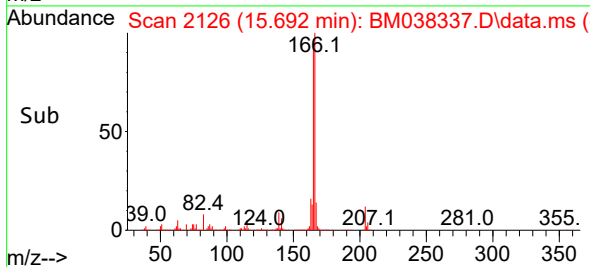

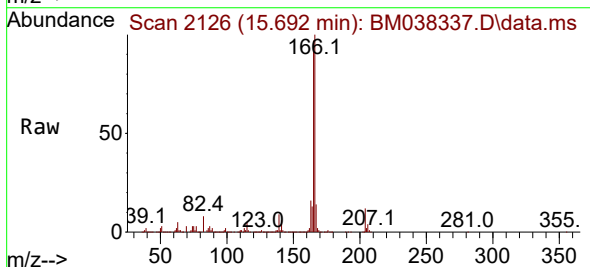




#62
4-Chlorophenyl-phenylether
Concen: 201.138 ng/ul
RT: 15.680 min Scan# 2124
Delta R.T. 0.005 min
Lab File: BM038337.D
Acq: 28 Dec 2022 20:11




Instrument :
BNA_M
ClientSampleId :
SSTD160017


Tgt Ion:204 Resp: 1532531
Ion Ratio Lower Upper
204 100
206 33.0 26.2 39.4
141 54.6 41.2 61.8

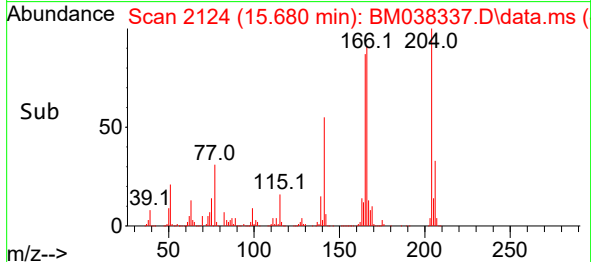

#63
4-Nitroaniline
Concen: 146.721 ng/ul
RT: 15.733 min Scan# 2133
Delta R.T. 0.023 min
Lab File: BM038337.D
Acq: 28 Dec 2022 20:11

Tgt Ion:138 Resp: 383189
Ion Ratio Lower Upper
138 100
92 53.9 42.6 63.8
108 100.2 75.0 112.6


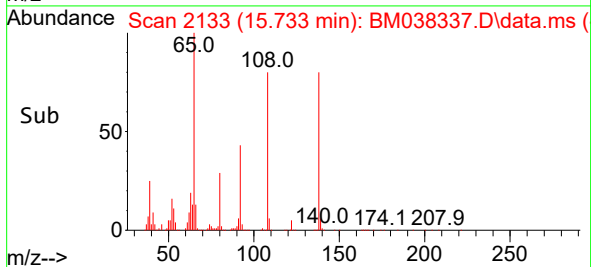

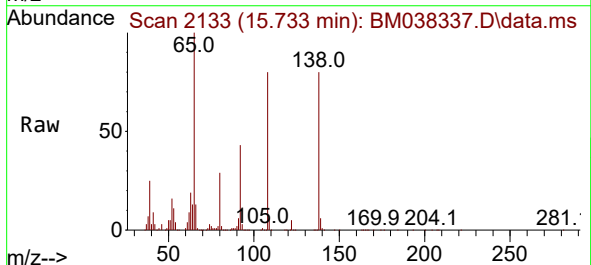




#66
4,6-Dinitro-2-methylphenol
Concen: 253.916 ng/ul
RT: 15.786 min Scan# 2142
Delta R.T. 0.017 min
Lab File: BM038337.D
Acq: 28 Dec 2022 20:11




Instrument :
BNA_M
ClientSampleId :
SSTD160017


Tgt Ion:198 Resp: 617348
Ion Ratio Lower Upper
198 100
182 2.9 3.1 4.7#
77 22.5 20.4 30.6

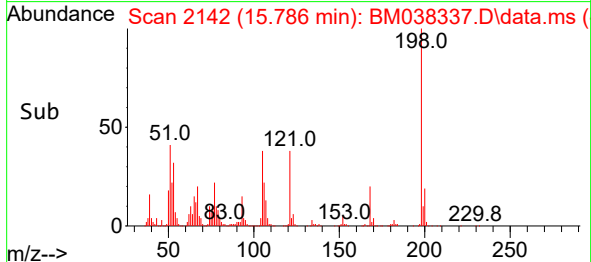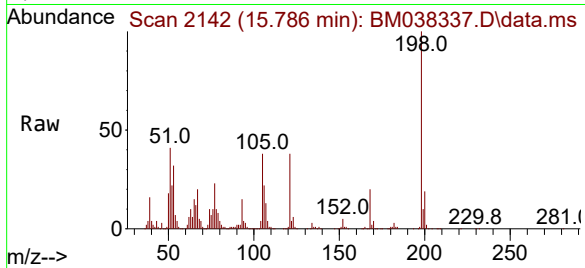

#67
N-Nitrosodiphenylamine
Concen: 176.171 ng/ul
RT: 15.898 min Scan# 2161
Delta R.T. 0.011 min
Lab File: BM038337.D
Acq: 28 Dec 2022 20:11

Tgt Ion:169 Resp: 2496270
Ion Ratio Lower Upper
169 100
168 67.0 54.7 82.1
167 36.9 30.0 45.0


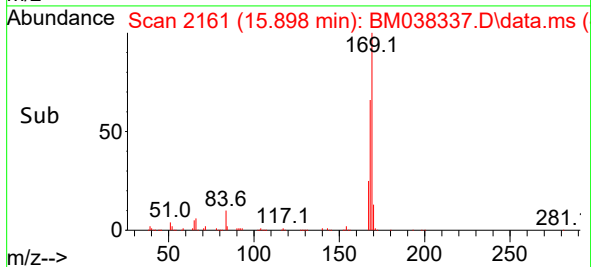

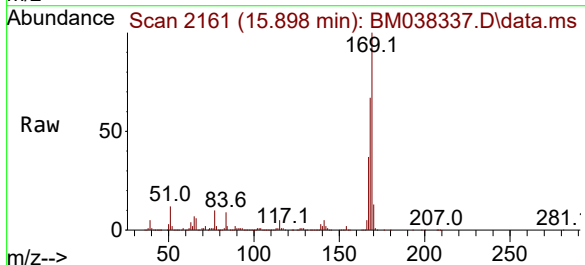




#68
4-Bromophenyl-phenylether
Concen: 192.336 ng/ul
RT: 16.574 min Scan# 2276
Delta R.T. 0.005 min
Lab File: BM038337.D
Acq: 28 Dec 2022 20:11




Instrument :
BNA_M
ClientSampleId :
SSTD160017


Tgt Ion:248 Resp: 990384
Ion Ratio Lower Upper
248 100
250 98.9 76.9 115.3
141 60.4 48.4 72.6



#69
Hexachlorobenzene
Concen: 186.475 ng/ul
RT: 16.692 min Scan# 2296
Delta R.T. 0.011 min
Lab File: BM038337.D
Acq: 28 Dec 2022 20:11

Tgt Ion:284 Resp: 1146179
Ion Ratio Lower Upper
284 100
142 28.6 25.3 37.9
249 29.7 24.2 36.4

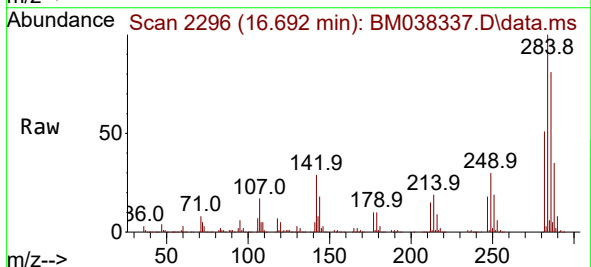



#70

Atrazine

Concen: 204.667 ng/ul

RT: 16.851 min Scan# 21

Delta R.T. 0.017 min

Lab File: BM038337.D

Acq: 28 Dec 2022 20:11

Instrument :

BNA_M

ClientSampleId :

SSTD160017





Tgt Ion:200 Resp: 991040

Ion Ratio Lower Upper

200 100

173 24.8 20.5 30.7

215 48.4 38.3 57.5

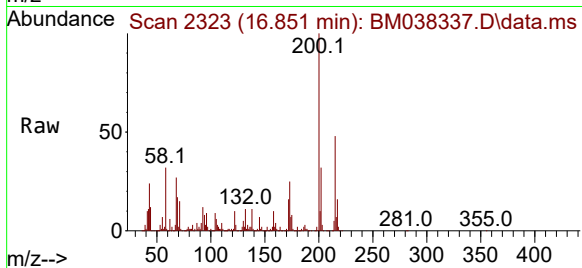

#71

Pentachlorophenol

Concen: 219.056 ng/ul

RT: 17.033 min Scan# 2354

Delta R.T. 0.006 min

Lab File: BM038337.D

Acq: 28 Dec 2022 20:11




Tgt Ion:266 Resp: 748593


Ion Ratio Lower Upper

266 100

264 63.4 50.6 76.0

268 64.5 49.0 73.6

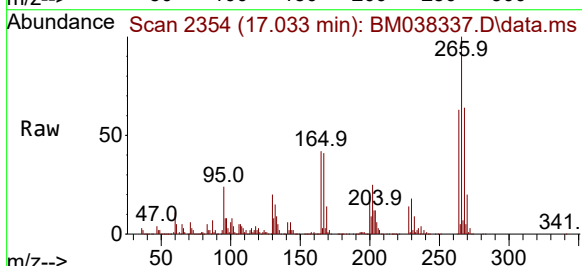



#72

Phenanthrene

Concen: 185.116 ng/ul

RT: 17.427 min Scan# 2420

Delta R.T. 0.005 min

Lab File: BM038337.D

Acq: 28 Dec 2022 20:11

Instrument :

BNA_M

ClientSampleId :

SSTD160017





Tgt Ion:178 Resp: 4748678

Ion Ratio Lower Upper

178 100

179 16.0 12.5 18.7

176 19.6 15.7 23.5

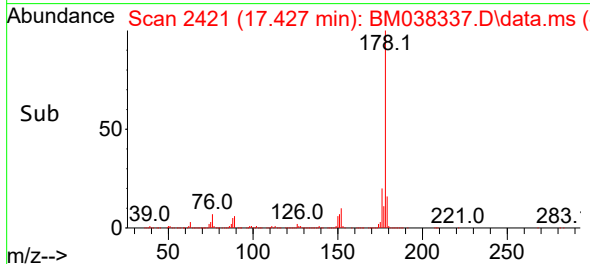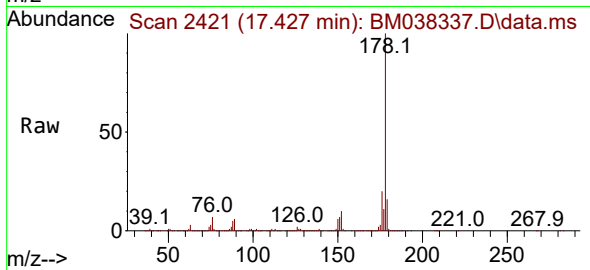

#74

Anthracene

Concen: 186.830 ng/ul

RT: 17.521 min Scan# 2437

Delta R.T. 0.011 min

Lab File: BM038337.D

Acq: 28 Dec 2022 20:11




Tgt Ion:178 Resp: 4870525


Ion Ratio Lower Upper

178 100

179 15.9 12.0 18.0

176 19.1 14.7 22.1

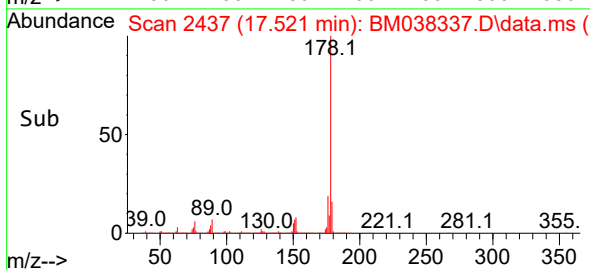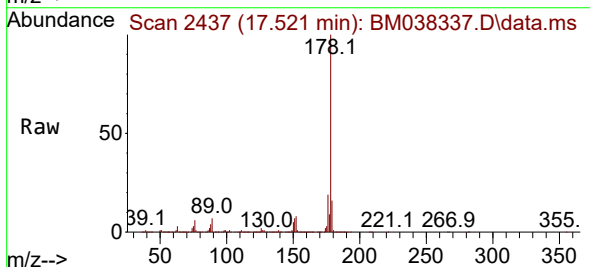



#75

1,2,3,4-Tetrachlorobenzene

Concen: 189.056 ng/uL

RT: 13.451 min Scan# 11

Delta R.T. 0.005 min

Lab File: BM038337.D

Acq: 28 Dec 2022 20:11

Instrument :

BNA_M

ClientSampleId :

SSTD160017





Tgt Ion:216 Resp: 1435706

Ion Ratio Lower Upper

216 100

214 78.4 61.4 92.2

218 48.9 38.3 57.5

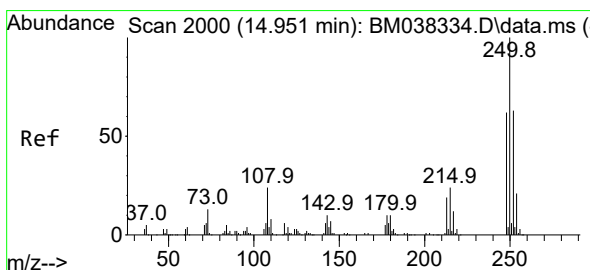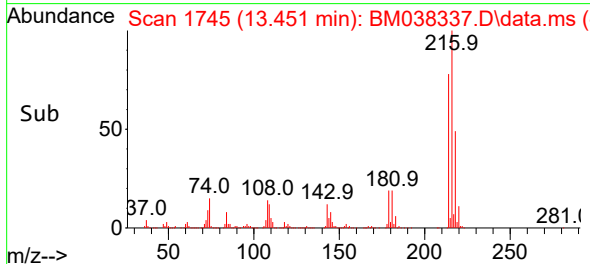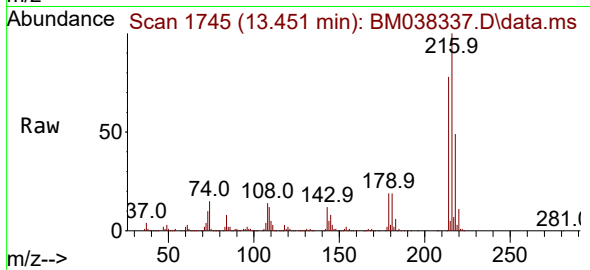

#76

Pentachlorobenzene

Concen: 180.262 ng/uL

RT: 14.962 min Scan# 2002

Delta R.T. 0.011 min

Lab File: BM038337.D

Acq: 28 Dec 2022 20:11




Tgt Ion:250 Resp: 1356048


Ion Ratio Lower Upper

250 100

248 62.4 49.3 73.9

252 64.5 50.8 76.2

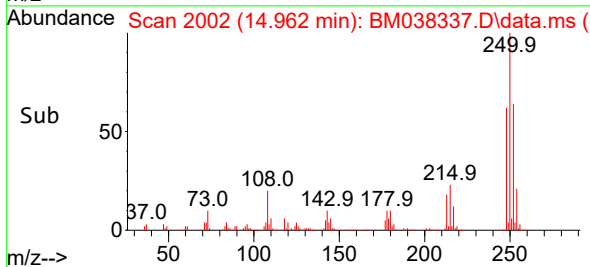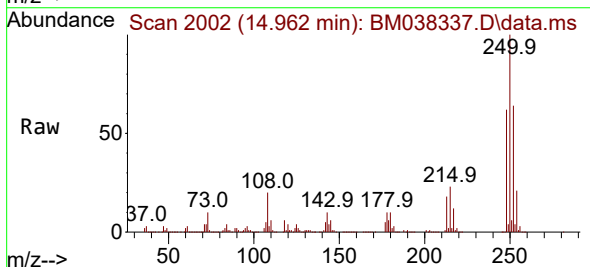



#77

Carbazole

Concen: 188.055 ng/ul

RT: 17.792 min Scan# 24

Delta R.T. 0.005 min

Lab File: BM038337.D

Acq: 28 Dec 2022 20:11

Instrument :

BNA_M

ClientSampleId :

SSTD160017





Tgt Ion:167 Resp: 4247401

Ion Ratio Lower Upper

167 100

166 21.8 17.2 25.8

139 12.3 10.2 15.4



#78

Di-n-butylphthalate

Concen: 194.563 ng/ul

RT: 18.339 min Scan# 2576

Delta R.T. 0.005 min

Lab File: BM038337.D

Acq: 28 Dec 2022 20:11




Tgt Ion:149 Resp: 5223369


Ion Ratio Lower Upper

149 100

150 9.4 7.7 11.5

104 5.2 4.6 6.8





#80

Fluoranthene

Concen: 161.208 ng/ul

RT: 19.439 min Scan# 21

Delta R.T. 0.011 min

Lab File: BM038337.D

Acq: 28 Dec 2022 20:11

Instrument :

BNA_M

ClientSampleId :

SSTD160017





Tgt Ion:202 Resp: 5751208

Ion Ratio Lower Upper

202 100

101 7.6 6.4 9.6

100 5.8 5.4 8.2

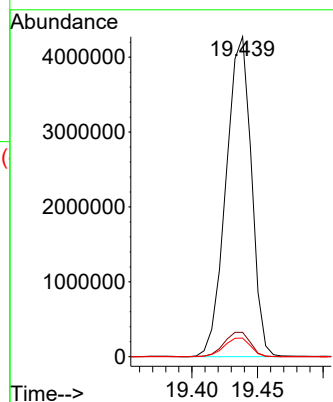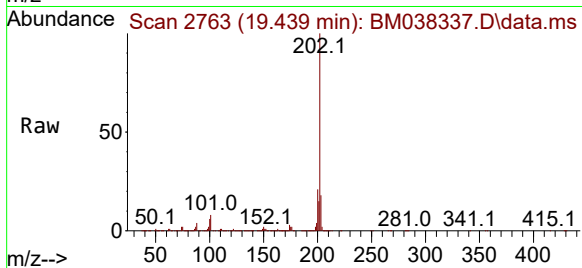

#82

Pyrene

Concen: 160.703 ng/ul

RT: 19.803 min Scan# 2825

Delta R.T. 0.011 min

Lab File: BM038337.D

Acq: 28 Dec 2022 20:11




Tgt Ion:202 Resp: 5966778


Ion Ratio Lower Upper

202 100

101 9.1 7.5 11.3

100 7.3 6.5 9.7

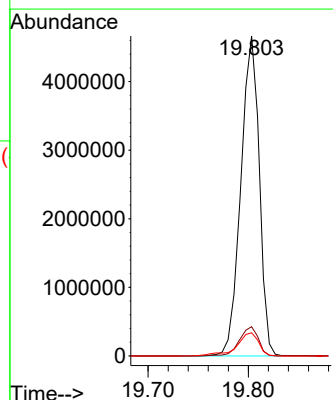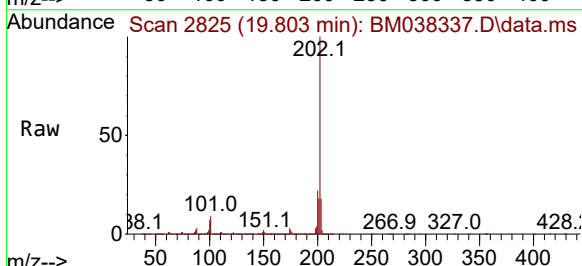



#83

Butylbenzylphthalate

Concen: 176.095 ng/ul

RT: 20.680 min Scan# 2974

Delta R.T. -0.000 min

Lab File: BM038337.D

Acq: 28 Dec 2022 20:11

Instrument :

BNA_M

ClientSampleId :

SSTD160017





Tgt Ion:149 Resp: 2431214

Ion Ratio Lower Upper

149 100

91 65.3 54.3 81.5

206 22.5 17.6 26.4

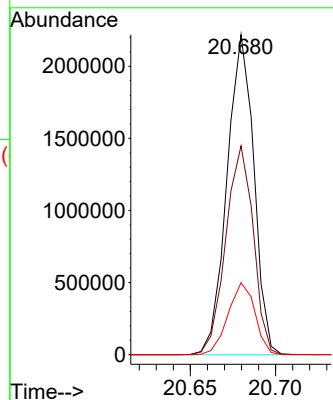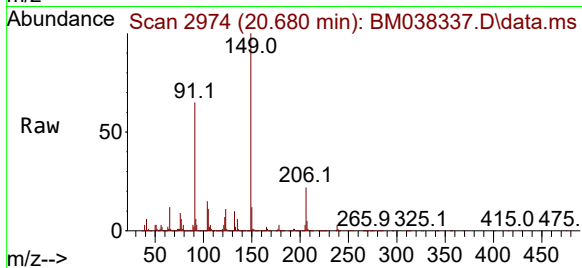

#84

3,3'-Dichlorobenzidine

Concen: 170.153 ng/ul

RT: 21.468 min Scan# 3108

Delta R.T. -0.000 min

Lab File: BM038337.D

Acq: 28 Dec 2022 20:11




Tgt Ion:252 Resp: 1694363


Ion Ratio Lower Upper

252 100

254 65.1 50.8 76.2

126 9.0 6.1 9.1



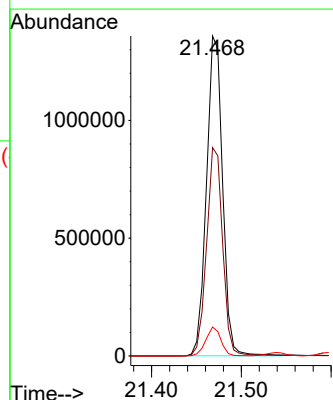
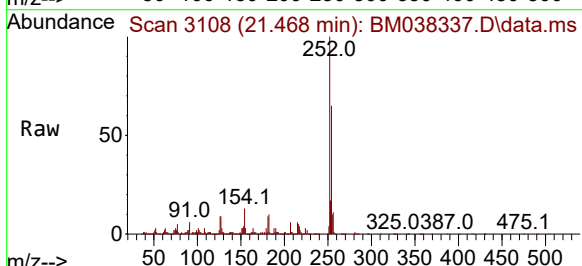




#85
Benzo(a)anthracene
Concen: 170.593 ng/ul
RT: 21.538 min Scan# 3119
Delta R.T. 0.005 min
Lab File: BM038337.D
Acq: 28 Dec 2022 20:11




Instrument :
BNA_M
ClientSampleId :
SSTD160017


Tgt Ion:228 Resp: 5779499
Ion Ratio Lower Upper
228 100
229 20.9 15.7 23.5
226 28.1 22.1 33.1

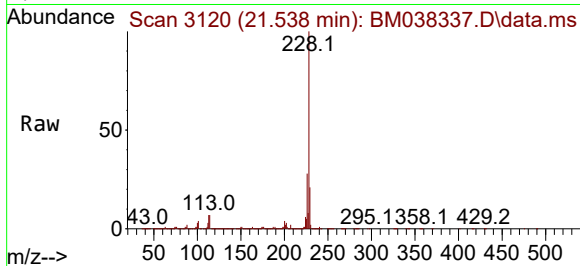

#86
Bis(2-ethylhexyl)phthalate
Concen: 175.870 ng/ul
RT: 21.444 min Scan# 3104
Delta R.T. -0.000 min
Lab File: BM038337.D
Acq: 28 Dec 2022 20:11

Tgt Ion:149 Resp: 3532363
Ion Ratio Lower Upper
149 100
167 28.5 21.0 31.6
279 4.4 3.4 5.0

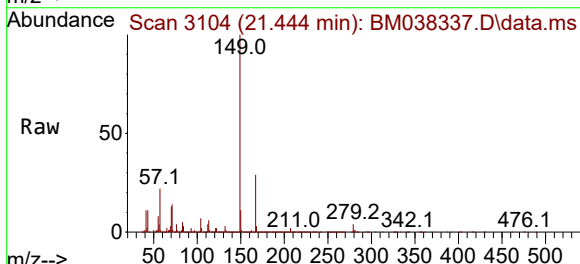



#87

Chrysene

Concen: 167.808 ng/ul

RT: 21.597 min Scan# 3128

Delta R.T. 0.011 min

Lab File: BM038337.D

Acq: 28 Dec 2022 20:11

Instrument :

BNA_M

ClientSampleId :

SSTD160017





Tgt Ion:228 Resp: 5334104

Ion Ratio Lower Upper

228 100

226 30.9 23.7 35.5

229 20.3 15.5 23.3



#89

Di-n-octyl phthalate

Concen: 178.733 ng/ul




RT: 22.380 min Scan# 3263


Delta R.T. 0.006 min

Lab File: BM038337.D

Acq: 28 Dec 2022 20:11

Tgt Ion:149 Resp: 6149066



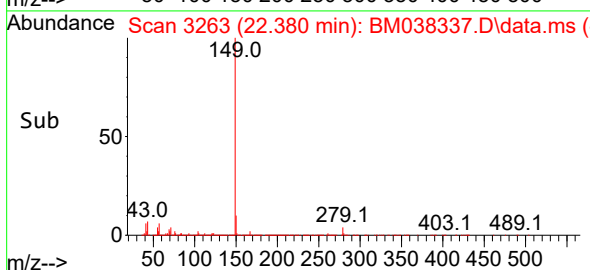





#90
Benzo(b)fluoranthene
Concen: 185.769 ng/ul
RT: 23.250 min Scan# 3409
Delta R.T. 0.011 min
Lab File: BM038337.D
Acq: 28 Dec 2022 20:11




Instrument :
BNA_M
ClientSampleId :
SSTD160017


Tgt Ion:252 Resp: 6183697
Ion Ratio Lower Upper
252 100
253 22.6 17.2 25.8
125 7.1 6.1 9.1

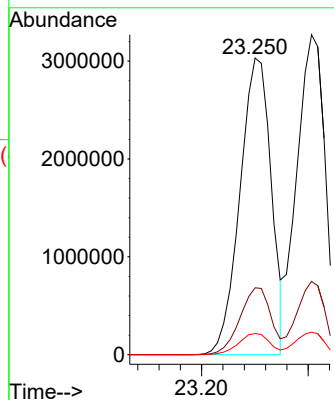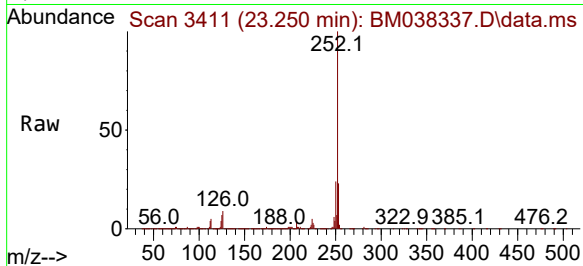

#91
Benzo(k)fluoranthene
Concen: 188.077 ng/ul
RT: 23.303 min Scan# 3420
Delta R.T. 0.017 min
Lab File: BM038337.D
Acq: 28 Dec 2022 20:11

Tgt Ion:252 Resp: 6067393
Ion Ratio Lower Upper
252 100
253 22.9 17.7 26.5
125 7.1 5.7 8.5

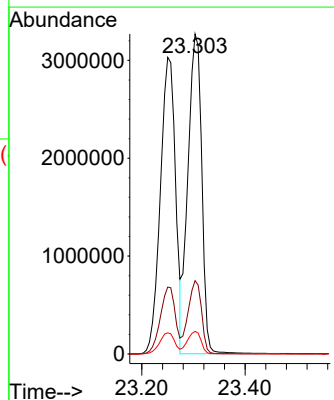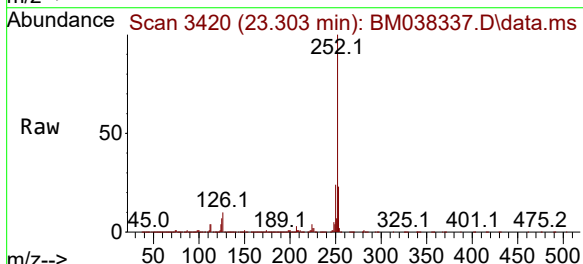



#93

Benzo(a)pyrene

Concen: 187.612 ng/ul

RT: 23.897 min Scan# 3

Delta R.T. 0.017 min

Lab File: BM038337.D

Acq: 28 Dec 2022 20:11

Instrument :

BNA_M

ClientSampleId :

SSTD160017





Tgt Ion:252 Resp: 5491714

Ion Ratio Lower Upper

252 100

253 22.5 17.4 26.0

125 8.1 6.4 9.6



#94

Indeno(1,2,3-cd)pyrene

Concen: 187.736 ng/ul

RT: 26.568 min Scan# 3975

Delta R.T. 0.041 min

Lab File: BM038337.D

Acq: 28 Dec 2022 20:11




Tgt Ion:276 Resp: 7077425


Ion Ratio Lower Upper

276 100

138 18.5 14.4 21.6

277 25.8 19.2 28.8

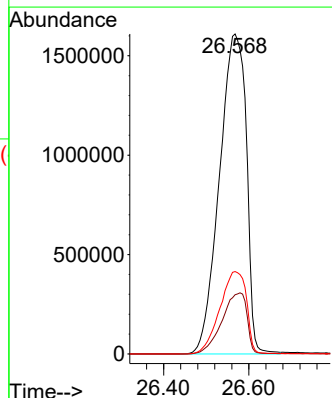



#95

Dibenzo(a,h)anthracene

Concen: 184.469 ng/ul

RT: 26.585 min Scan# 3970

Delta R.T. 0.047 min

Lab File: BM038337.D

Acq: 28 Dec 2022 20:11

Instrument :

BNA_M

ClientSampleId :

SSTD160017





Tgt Ion:278 Resp: 5862633

Ion Ratio Lower Upper

278 100

139 12.0 9.4 14.0

279 23.6 19.0 28.4

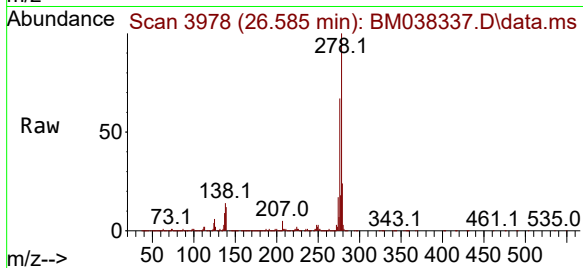

#96

Benzo(g,h,i)perylene

Concen: 196.045 ng/ul

RT: 27.362 min Scan# 4110

Delta R.T. 0.047 min

Lab File: BM038337.D

Acq: 28 Dec 2022 20:11

Tgt Ion:276 Resp: 5900772

Ion Ratio Lower Upper

276 100

138 15.1 13.0 19.4

277 24.7 19.6 29.4

