

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122923\
 Data File : BM043675.D
 Acq On : 29 Dec 2023 14:23
 Operator : MA/JU
 Sample : 05920-09
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GCF60

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/01/2024
 Supervised By :mohammad ahmed 01/01/2024

Quant Time: Dec 29 23:13:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 29 22:31:57 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.963	152	189170	20.000	ng/u1	0.00
20) Naphthalene-d8	10.769	136	817280	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.598	164	460914	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.345	188	931555	20.000	ng/u1	0.00
79) Chrysene-d12	21.527	240	770407	20.000	ng/u1	0.00
88) Perylene-d12	23.944	264	844667	20.000	ng/u1	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.369	96	27015	4.641	ng/uL	0.00
4) Pyridine-d5	3.816	84	35220m	2.102	ng/u1	0.03
7) Phenol-d5	7.122	99	501996	23.327	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.298	67	350612	25.726	ng/u1	0.00
11) 2-Chlorophenol-d4	7.487	132	420119	25.569	ng/u1	0.00
15) 4-Methylphenol-d8	8.669	113	347381	20.802	ng/u1	0.00
21) Nitrobenzene-d5	9.134	128	211389	26.733	ng/u1	0.00
24) 2-Nitrophenol-d4	9.851	143	218815	26.782	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.386	165	355430	24.644	ng/u1	0.00
31) 4-Chloroaniline-d4	10.922	131	3379	0.159	ng/u1	0.01
46) Dimethylphthalate-d6	14.016	166	1021902	24.629	ng/u1	0.00
49) Acenaphthylene-d8	14.292	160	1295671	26.324	ng/u1	0.00
54) 4-Nitrophenol-d4	14.804	143	106231m	13.527	ng/u1	0.01
60) Fluorene-d10	15.586	176	929656	27.096	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.710	200	90681	14.719	ng/u1	0.00
73) Anthracene-d10	17.439	188	1283834	24.574	ng/u1	0.00
81) Pyrene-d10	19.733	212	1452582	23.882	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.786	264	1335272	25.617	ng/u1	0.01
Target Compounds						
71) Pentachlorophenol	16.986	266	31216m	4.084	ng/u1	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122923\
Data File : BM043675.D
Acq On : 29 Dec 2023 14:23
Operator : MA/JU
Sample : 05920-09
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
GCF60

Quant Time: Dec 29 23:13:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 22:31:57 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 01/01/2024
Supervised By :mohammad ahmed 01/01/2024

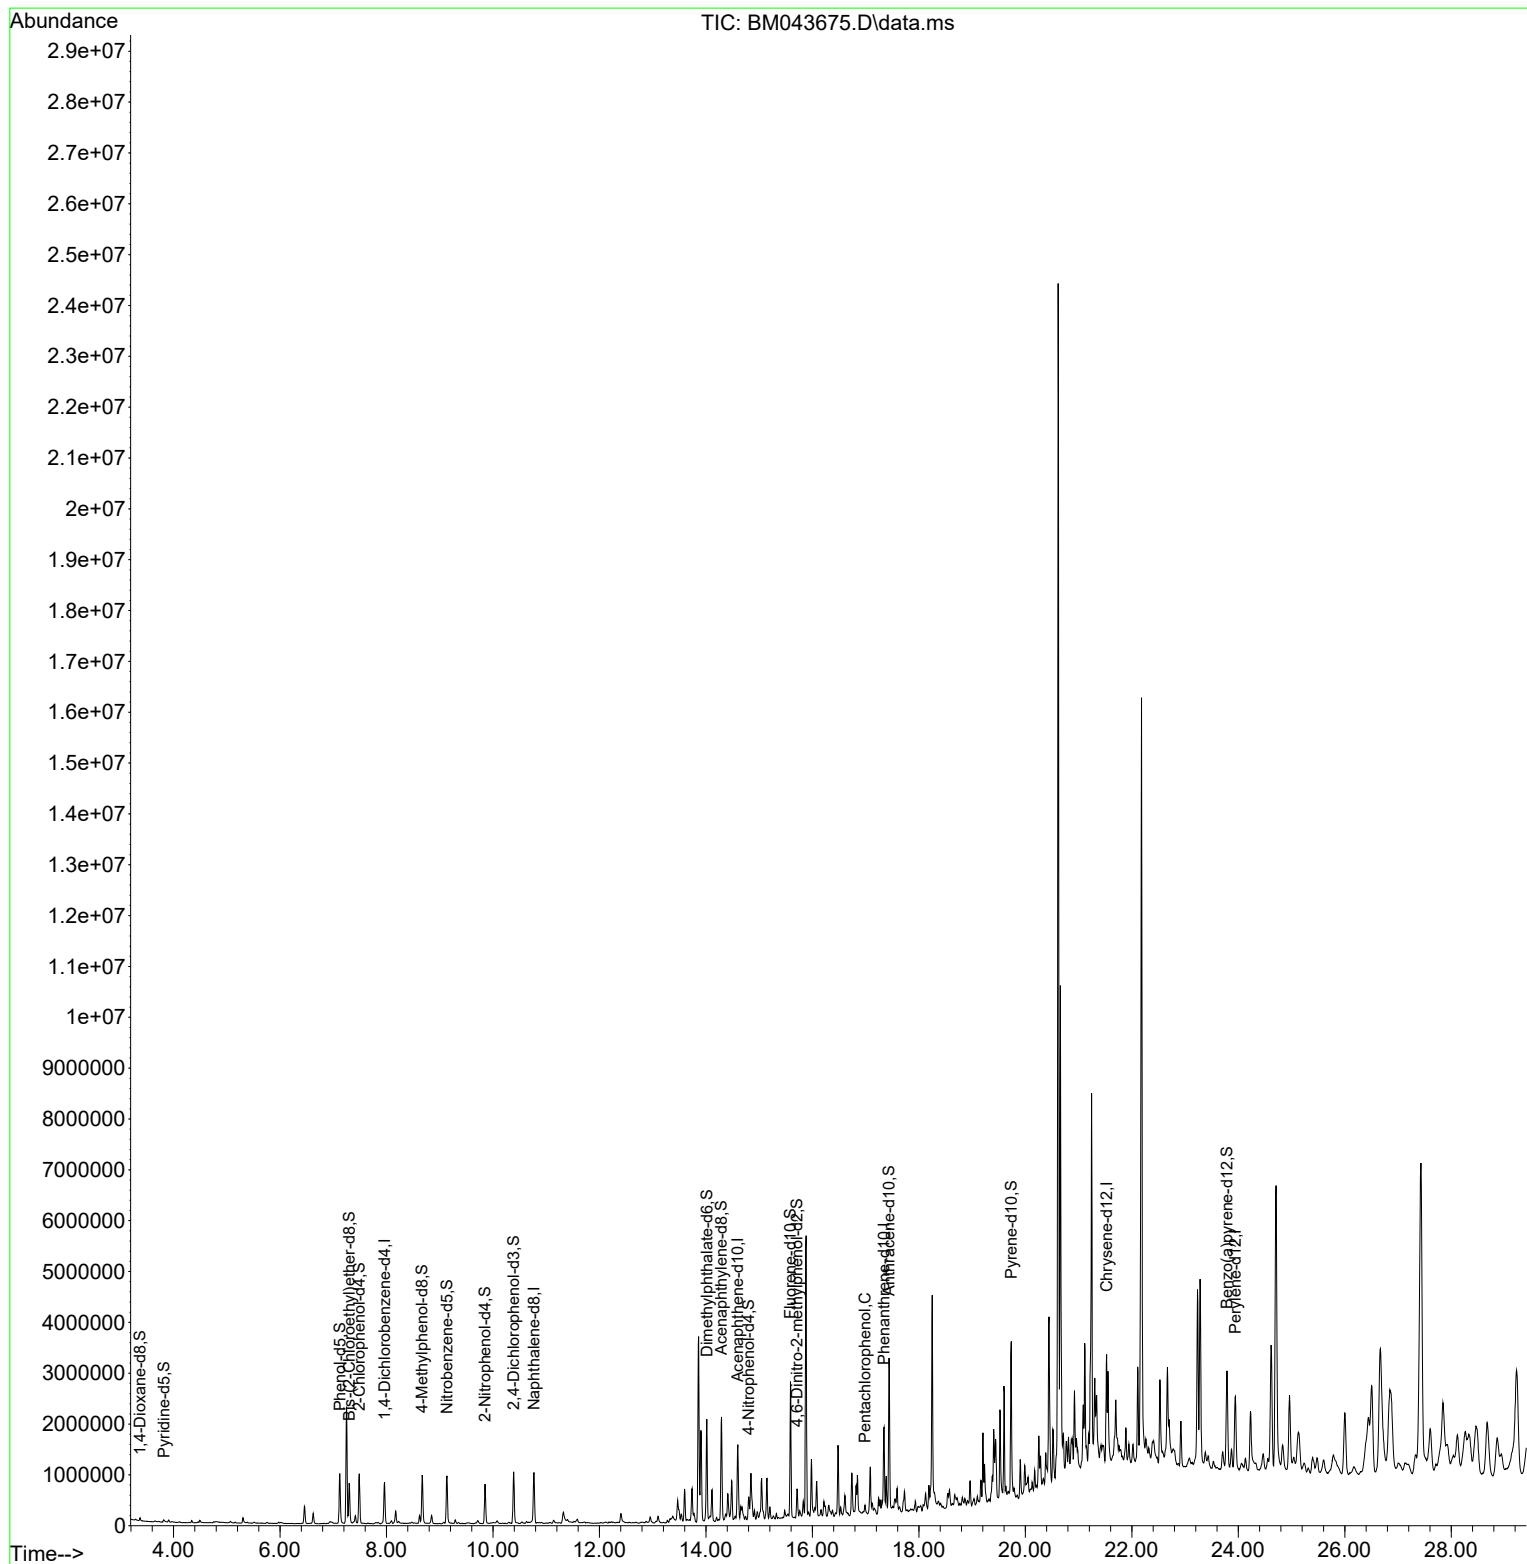

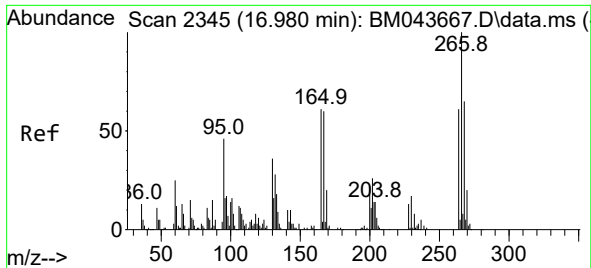

#71
 Pentachlorophenol
 Concen: 4.084 ng/ul m
 RT: 16.986 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: BM043675.D
 Acq: 29 Dec 2023 14:23

Instrument :
 BNA_M
 ClientSampleId :
 GCF60

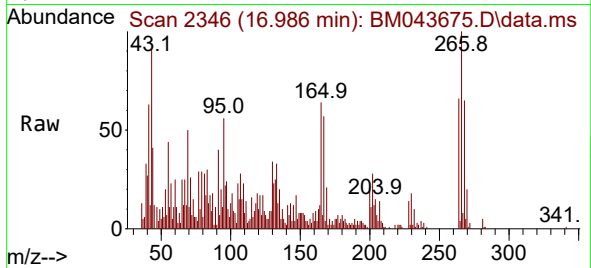

Tgt Ion:266 Resp: 31210
 Ion Ratio Lower Upper
 266 100
 264 65.8 49.9 74.9
 268 65.4 51.0 76.6

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/01/2024
 Supervised By :mohammad ahmed 01/01/2024

