

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122923\
 Data File : BM043668.D
 Acq On : 29 Dec 2023 10:09
 Operator : MA/JU
 Sample : PB158024BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK024

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043668.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	28	31	37	rVB	62992	78222	2.48%	0.202%
2	3.793	99	103	129	rBV	647654	1123539	35.68%	2.902%
3	4.116	155	158	163	rVB3	14765	19606	0.62%	0.051%
4	6.604	579	581	587	rBV6	1795	3546	0.11%	0.009%
5	7.116	661	668	680	rBV	813135	1287988	40.91%	3.326%
6	7.298	692	699	713	rVB	632299	1017917	32.33%	2.629%
7	7.487	724	731	740	rBV	750860	1218052	38.68%	3.146%
8	7.957	804	811	820	rBV	656626	1048262	33.29%	2.707%
9	8.669	921	932	949	rBV	864689	1455082	46.21%	3.758%
10	9.128	1003	1010	1024	rBV	700346	1191774	37.85%	3.078%
11	9.463	1064	1067	1069	rBV4	2526	3152	0.10%	0.008%
12	9.851	1126	1133	1146	rBV	536318	901417	28.63%	2.328%
13	10.381	1216	1223	1249	rBV	730393	1318965	41.89%	3.406%
14	10.763	1281	1288	1298	rBV	862491	1470163	46.69%	3.797%
15	10.910	1305	1313	1330	rBV	822398	1521901	48.33%	3.931%
16	11.016	1330	1331	1338	rVB7	3049	5595	0.18%	0.014%
17	12.357	1553	1559	1568	rVB6	11004	23571	0.75%	0.061%
18	13.492	1746	1752	1758	rVV3	9154	16016	0.51%	0.041%
19	13.574	1761	1766	1771	rVV9	3481	4753	0.15%	0.012%
20	14.016	1834	1841	1853	rBV	1291104	1864356	59.21%	4.815%
21	14.286	1880	1887	1900	rBV	1474176	2187875	69.49%	5.651%
22	14.592	1933	1939	1950	rBV	1195130	1730168	54.95%	4.468%
23	14.792	1967	1973	1991	rBV	564304	1060769	33.69%	2.740%
24	15.010	2008	2010	2018	rVB8	3183	6253	0.20%	0.016%
25	15.586	2101	2108	2116	rBV	1928013	2643997	83.97%	6.829%
26	15.710	2121	2129	2139	rBV	548311	808903	25.69%	2.089%
27	15.827	2144	2149	2153	rVB6	6929	13103	0.42%	0.034%
28	16.157	2199	2205	2208	rBV7	3210	4777	0.15%	0.012%
29	16.368	2237	2241	2244	rBV6	3811	5231	0.17%	0.014%
30	17.339	2399	2406	2416	rBV	1364266	1885955	59.90%	4.871%
31	17.439	2416	2423	2441	rVV2	1963319	2766525	87.86%	7.145%
32	18.239	2554	2559	2565	rBV7	9082	17969	0.57%	0.046%
33	19.292	2734	2738	2742	rVV4	18399	25821	0.82%	0.067%
34	19.362	2746	2750	2756	rBV	15466	23280	0.74%	0.060%
35	19.521	2773	2777	2783	rBV7	8283	13882	0.44%	0.036%
36	19.668	2800	2802	2805	rBV3	4601	4397	0.14%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122923\
Data File : BM043668.D
Acq On : 29 Dec 2023 10:09
Operator : MA/JU
Sample : PB158024BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK024

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Title : SVOA CALIBRATION

37	19.727	2806	2812	2820	rBV	2247174	2888081	91.72%	7.459%
38	20.262	2901	2903	2907	rBV5	5390	8395	0.27%	0.022%
39	21.521	3111	3117	3127	rBV	1399874	1847945	58.69%	4.773%
40	23.774	3493	3500	3510	rBV	1674097	3148663	100.00%	8.132%
41	23.933	3520	3527	3540	rVB	996055	2053591	65.22%	5.304%




Sum of corrected areas: 38719457

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122923\
Data File : BM043668.D
Acq On : 29 Dec 2023 10:09
Operator : MA/JU
Sample : PB158024BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK024

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

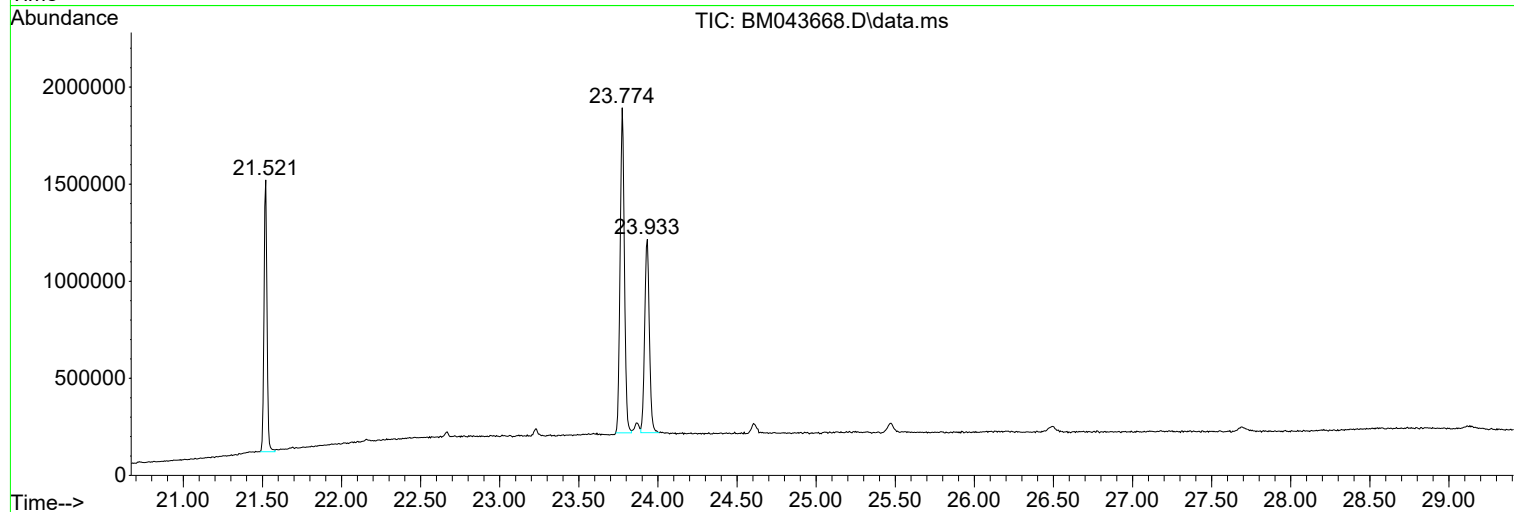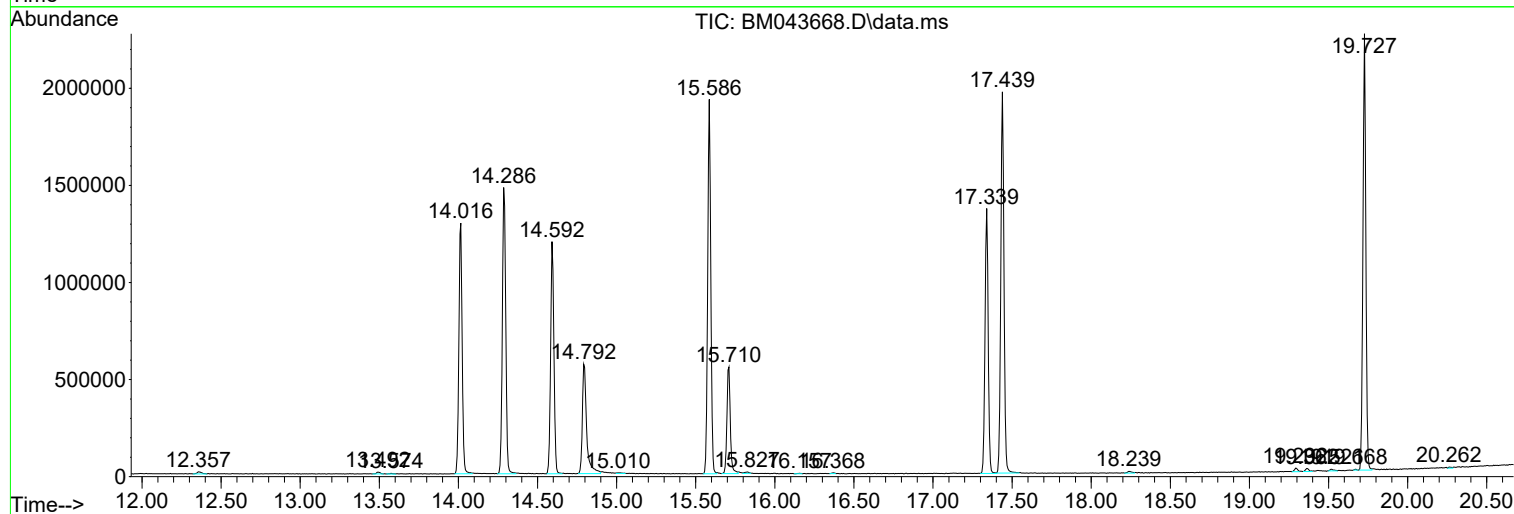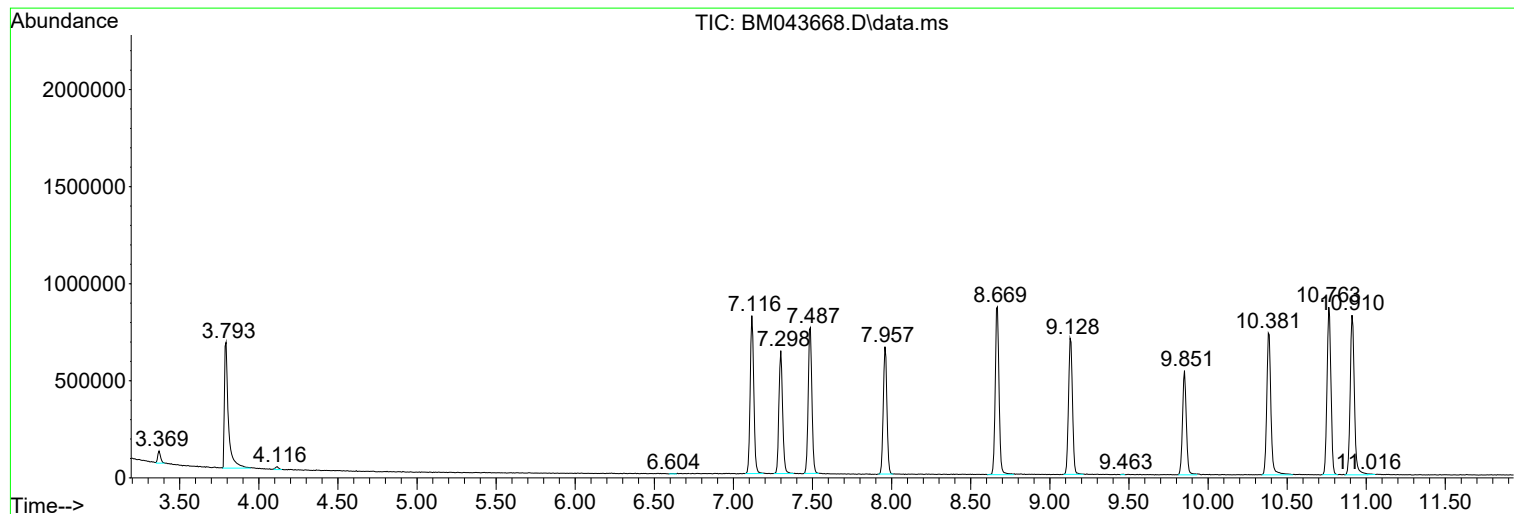

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122923\
Data File : BM043668.D
Acq On : 29 Dec 2023 10:09
Operator : MA/JU
Sample : PB158024BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK024

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122923\
Data File : BM043668.D
Acq On : 29 Dec 2023 10:09
Operator : MA/JU
Sample : PB158024BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK024

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc