

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122923\
 Data File : BM043680.D
 Acq On : 29 Dec 2023 20:52
 Operator : MA/JU
 Sample : PB158024BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK024

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043680.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	27	31	40	rVB	85265	118449	2.03%	0.183%
2	3.793	99	103	127	rVB	967260	1544660	26.47%	2.380%
3	4.110	154	157	162	rVB	17317	22253	0.38%	0.034%
4	7.122	660	669	681	rBV	1224736	1962501	33.63%	3.024%
5	7.298	692	699	710	rBV	874553	1385401	23.74%	2.135%
6	7.487	724	731	742	rVB	1172310	1833591	31.42%	2.825%
7	7.957	804	811	823	rBV	941673	1526405	26.16%	2.352%
8	8.675	925	933	945	rBV	1374932	2295078	39.33%	3.536%
9	9.134	1003	1011	1019	rBV	1089256	1795673	30.77%	2.767%
10	9.851	1126	1133	1144	rBV	911787	1495124	25.62%	2.304%
11	10.386	1215	1224	1245	rBV	1275039	2257207	38.68%	3.478%
12	10.769	1280	1289	1298	rBV	1329886	2276263	39.01%	3.507%
13	10.916	1302	1314	1335	rBV	1302770	2393398	41.02%	3.688%
14	12.357	1552	1559	1567	rVB	23356	45010	0.77%	0.069%
15	13.492	1748	1752	1760	rVB2	25875	45213	0.77%	0.070%
16	13.569	1760	1765	1767	rBV5	5788	8138	0.14%	0.013%
17	14.016	1834	1841	1856	rBV	2065734	2885580	49.45%	4.446%
18	14.292	1881	1888	1903	rBV	2555667	3719452	63.74%	5.731%
19	14.598	1931	1940	1949	rBV	1912874	2837622	48.63%	4.372%
20	14.804	1968	1975	2000	rBV	1070925	1906357	32.67%	2.937%
21	15.010	2005	2010	2019	rVB	9316	23808	0.41%	0.037%
22	15.263	2047	2053	2057	rBV9	3685	7977	0.14%	0.012%
23	15.586	2102	2108	2122	rBV	3077504	4440190	76.10%	6.841%
24	15.710	2123	2129	2145	rVV	863652	1228294	21.05%	1.893%
25	15.827	2145	2149	2153	rVB3	14885	23738	0.41%	0.037%
26	16.368	2238	2241	2246	rVB3	11690	15326	0.26%	0.024%
27	16.745	2301	2305	2306	rBV4	4788	5882	0.10%	0.009%
28	16.804	2309	2315	2316	rBV6	5061	6920	0.12%	0.011%
29	17.345	2400	2407	2416	rBV	2259122	3279369	56.20%	5.053%
30	17.445	2416	2424	2432	rBV	3373369	4804122	82.33%	7.402%
31	17.610	2449	2452	2455	rBV5	16843	26196	0.45%	0.040%
32	18.015	2517	2521	2524	rBV5	5160	8219	0.14%	0.013%
33	18.239	2555	2559	2564	rBV5	26205	41028	0.70%	0.063%
34	18.362	2576	2580	2587	rVB4	26683	37679	0.65%	0.058%
35	19.298	2735	2739	2743	rBV2	40063	47668	0.82%	0.073%
36	19.368	2747	2751	2755	rBV	33165	44826	0.77%	0.069%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122923\
Data File : BM043680.D
Acq On : 29 Dec 2023 20:52
Operator : MA/JU
Sample : PB158024BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK024

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Title : SVOA CALIBRATION

37	19.515	2774	2776	2781	rBV5	13916	17856	0.31%	0.028%
38	19.668	2800	2802	2806	rVB3	17220	14797	0.25%	0.023%
39	19.733	2806	2813	2820	rBV	4097474	5443438	93.29%	8.387%
40	21.521	3112	3117	3125	rVB	2744421	3421467	58.64%	5.272%
41	23.780	3494	3501	3510	rVB2	3045433	5834899	100.00%	8.990%
42	23.933	3521	3527	3537	rVB	1861442	3774763	64.69%	5.816%




Sum of corrected areas: 64901837

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122923\
Data File : BM043680.D
Acq On : 29 Dec 2023 20:52
Operator : MA/JU
Sample : PB158024BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK024

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

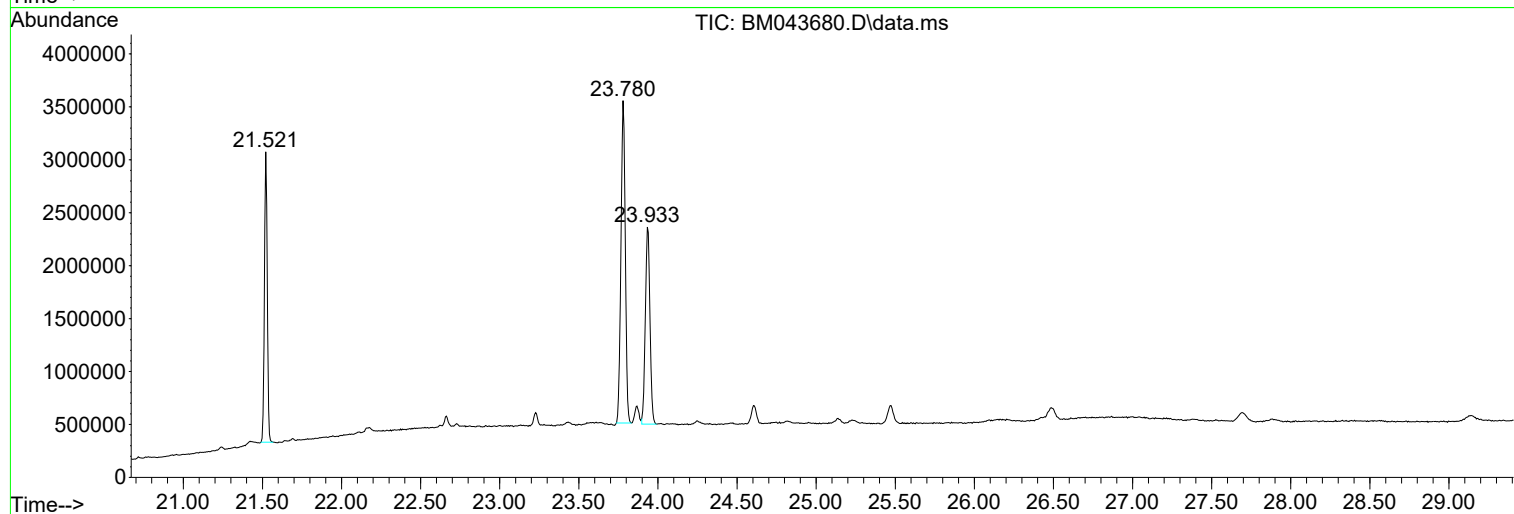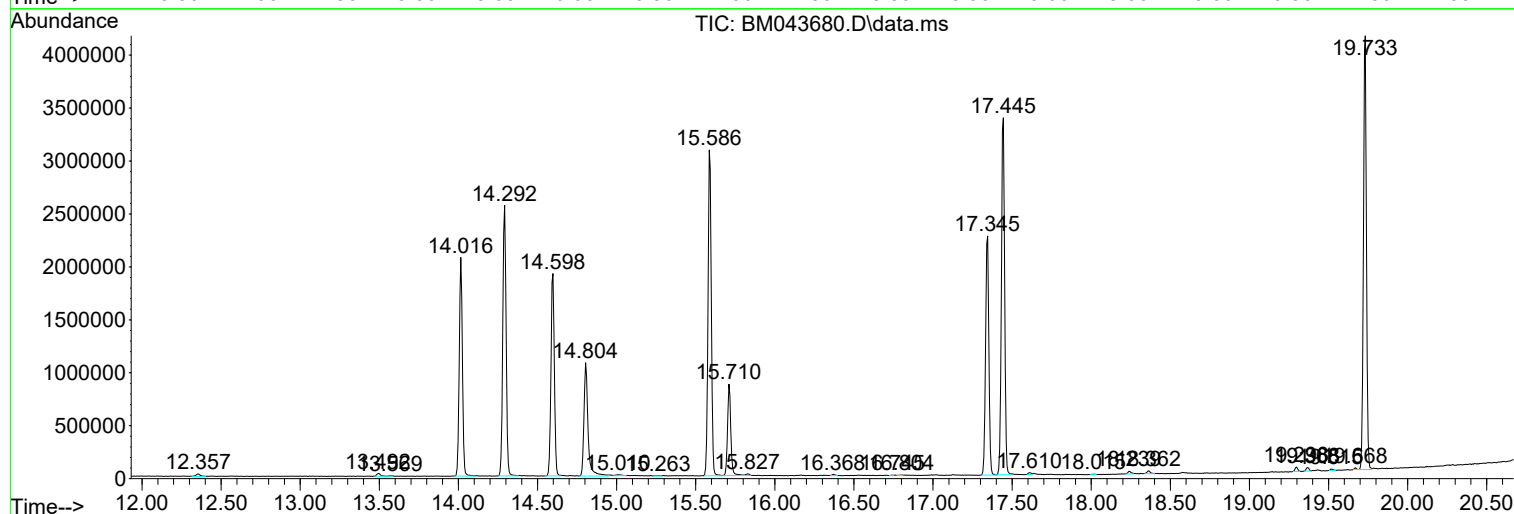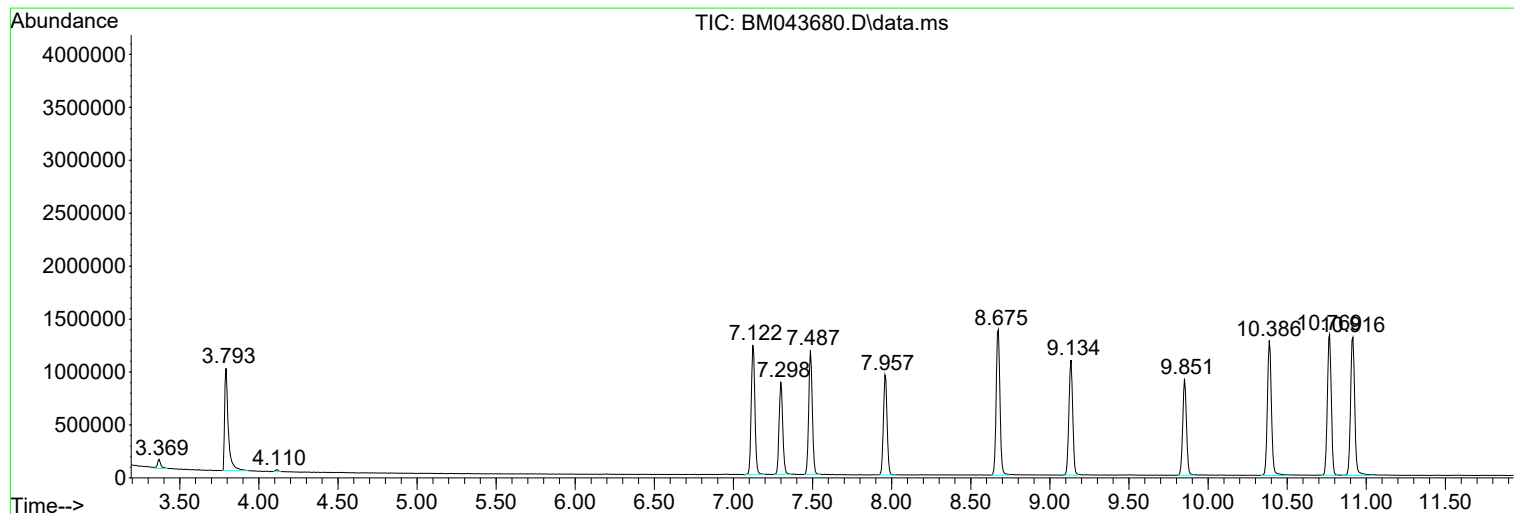

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122923\
Data File : BM043680.D
Acq On : 29 Dec 2023 20:52
Operator : MA/JU
Sample : PB158024BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK024

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122923\
Data File : BM043680.D
Acq On : 29 Dec 2023 20:52
Operator : MA/JU
Sample : PB158024BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK024

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc