

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122923\
 Data File : BM043685.D
 Acq On : 29 Dec 2023 23:55
 Operator : MA/JU
 Sample : 05920-10DL 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GCF61DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043685.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.116	155	158	162	rVB3	11225	14718	0.48%	0.078%
2	5.040	313	315	317	rBV3	4794	4184	0.14%	0.022%
3	5.510	393	395	400	rBV6	3454	6705	0.22%	0.035%
4	5.728	431	432	435	rBV3	4858	4955	0.16%	0.026%
5	6.057	485	488	489	rBV3	3320	3122	0.10%	0.017%
6	6.140	501	502	506	rBV4	2171	3320	0.11%	0.018%
7	6.181	508	509	511	rBV2	3728	3239	0.11%	0.017%
8	6.457	552	556	562	rVB5	8924	13693	0.45%	0.072%
9	6.622	580	584	588	rVB7	4097	5691	0.19%	0.030%
10	6.963	638	642	643	rBV4	2641	3485	0.11%	0.018%
11	7.040	654	655	660	rVB5	3518	3262	0.11%	0.017%
12	7.128	663	670	672	rBV2	19221	36790	1.20%	0.195%
13	7.257	686	692	695	rBV6	7866	13663	0.44%	0.072%
14	7.304	695	700	708	rVB	38591	66026	2.15%	0.349%
15	7.381	710	713	716	rBV5	2962	3201	0.10%	0.017%
16	7.493	727	732	739	rVB	38907	67645	2.20%	0.358%
17	7.963	804	812	819	rBV	731851	1169772	38.07%	6.188%
18	8.028	819	823	828	rVV6	7471	14983	0.49%	0.079%
19	8.087	830	833	837	rBV5	2378	3777	0.12%	0.020%
20	8.181	845	849	852	rVB6	4222	6098	0.20%	0.032%
21	8.222	852	856	857	rBV3	3058	3588	0.12%	0.019%
22	8.622	919	924	927	rVV6	7026	10451	0.34%	0.055%
23	8.681	928	934	947	rVB2	31085	66313	2.16%	0.351%
24	8.798	947	954	968	rBV	73995	146804	4.78%	0.777%
25	8.922	971	975	979	rVB5	6931	10089	0.33%	0.053%
26	9.134	1005	1011	1017	rBV	46715	78923	2.57%	0.418%
27	9.310	1038	1041	1043	rVB4	3624	3103	0.10%	0.016%
28	9.557	1081	1083	1087	rVB5	3187	4085	0.13%	0.022%
29	9.857	1126	1134	1140	rBV2	32979	62460	2.03%	0.330%
30	10.010	1154	1160	1162	rBV6	7486	13824	0.45%	0.073%
31	10.075	1170	1171	1176	rVB4	2631	3237	0.11%	0.017%
32	10.192	1189	1191	1193	rBV3	3699	3619	0.12%	0.019%
33	10.222	1193	1196	1199	rVV5	6989	8394	0.27%	0.044%
34	10.398	1220	1226	1239	rVB3	22894	50729	1.65%	0.268%
35	10.769	1280	1289	1298	rBV	1012496	1723164	56.09%	9.116%
36	10.928	1313	1316	1323	rVB8	5641	13521	0.44%	0.072%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122923\
 Data File : BM043685.D
 Acq On : 29 Dec 2023 23:55
 Operator : MA/JU
 Sample : 05920-10DL 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GCF61DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

37	10.998	1323	1328	1329	rVB5	2512	3343	0.11%	0.018%
38	11.139	1349	1352	1355	rVV5	2680	4433	0.14%	0.023%
39	11.257	1368	1372	1376	rBV7	5511	8241	0.27%	0.044%
40	11.322	1379	1383	1384	rBV4	4913	5138	0.17%	0.027%
41	11.451	1400	1405	1407	rBV6	2613	4516	0.15%	0.024%
42	11.592	1427	1429	1432	rVB4	4172	4339	0.14%	0.023%
43	11.992	1494	1497	1501	rBV6	3292	5372	0.17%	0.028%
44	12.269	1542	1544	1551	rVB6	2454	4321	0.14%	0.023%
45	12.327	1551	1554	1556	rBV3	3197	3688	0.12%	0.020%
46	12.569	1594	1595	1599	rVV2	4208	4135	0.13%	0.022%
47	12.710	1616	1619	1622	rBV4	2972	4372	0.14%	0.023%
48	12.833	1633	1640	1646	rBV3	37319	69777	2.27%	0.369%
49	13.010	1667	1670	1673	rBV5	3731	4795	0.16%	0.025%
50	13.098	1682	1685	1693	rVB10	6569	13054	0.42%	0.069%
51	13.180	1695	1699	1702	rVV6	3595	4682	0.15%	0.025%
52	13.274	1714	1715	1718	rVB3	5081	3118	0.10%	0.016%
53	13.416	1736	1739	1744	rVB7	3344	4492	0.15%	0.024%
54	13.498	1744	1753	1758	rBV	28384	53804	1.75%	0.285%
55	13.598	1766	1770	1774	rVB5	11841	14547	0.47%	0.077%
56	13.657	1778	1780	1785	rVB6	4290	6108	0.20%	0.032%
57	13.739	1788	1794	1797	rBV7	13119	24320	0.79%	0.129%
58	13.774	1797	1800	1804	rVB6	5220	8533	0.28%	0.045%
59	13.857	1808	1814	1819	rBV2	91260	143897	4.68%	0.761%
60	13.904	1819	1822	1827	rVB4	31214	46933	1.53%	0.248%
61	14.016	1837	1841	1847	rBV	83525	133060	4.33%	0.704%
62	14.110	1854	1857	1864	rVB7	14929	22266	0.72%	0.118%
63	14.251	1877	1881	1884	rBV6	11040	18487	0.60%	0.098%
64	14.292	1884	1888	1896	rVB	51118	87266	2.84%	0.462%
65	14.410	1905	1908	1915	rVB8	9292	16396	0.53%	0.087%
66	14.486	1915	1921	1926	rVB6	23517	37085	1.21%	0.196%
67	14.598	1933	1940	1948	rBV	1370995	2092978	68.12%	11.072%
68	14.845	1971	1982	1987	rBV	22061	62511	2.03%	0.331%
69	14.974	2000	2004	2007	rBV5	4441	6582	0.21%	0.035%
70	15.145	2028	2033	2037	rVB6	24250	31429	1.02%	0.166%
71	15.192	2037	2041	2042	rBV4	13454	16801	0.55%	0.089%
72	15.221	2042	2046	2051	rVB4	41075	63356	2.06%	0.335%
73	15.545	2095	2101	2103	rBV7	6989	9808	0.32%	0.052%
74	15.592	2103	2109	2115	rVV	127512	204828	6.67%	1.084%
75	15.710	2124	2129	2135	rBV4	29971	56632	1.84%	0.300%
76	15.874	2150	2157	2163	rVB2	83281	133211	4.34%	0.705%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122923\
 Data File : BM043685.D
 Acq On : 29 Dec 2023 23:55
 Operator : MA/JU
 Sample : 05920-10DL 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GCF61DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

77	15.963	2167	2172	2174	rBV5	5539	11168	0.36%	0.059%
78	16.215	2211	2215	2219	rBV6	11828	18150	0.59%	0.096%
79	16.327	2228	2234	2239	rVB4	22820	41454	1.35%	0.219%
80	16.986	2340	2346	2360	rBV	2023759	3072395	100.00%	16.254%
81	17.115	2365	2368	2372	rVB3	44798	65198	2.12%	0.345%
82	17.345	2401	2407	2418	rBV	1728670	2521280	82.06%	13.338%
83	17.439	2419	2423	2427	rBV	78398	113357	3.69%	0.600%
84	18.239	2556	2559	2570	rVB3	78074	133854	4.36%	0.708%
85	19.598	2788	2790	2796	rVB4	90679	114879	3.74%	0.608%
86	20.609	2959	2962	2966	rBV2	211970	251651	8.19%	1.331%
87	21.521	3113	3117	3127	rVB2	2061046	2625722	85.46%	13.891%
88	23.939	3522	3528	3539	rVB	1387965	2840251	92.44%	15.026%




Sum of corrected areas: 18902646

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122923\
Data File : BM043685.D
Acq On : 29 Dec 2023 23:55
Operator : MA/JU
Sample : 05920-10DL 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCF61DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

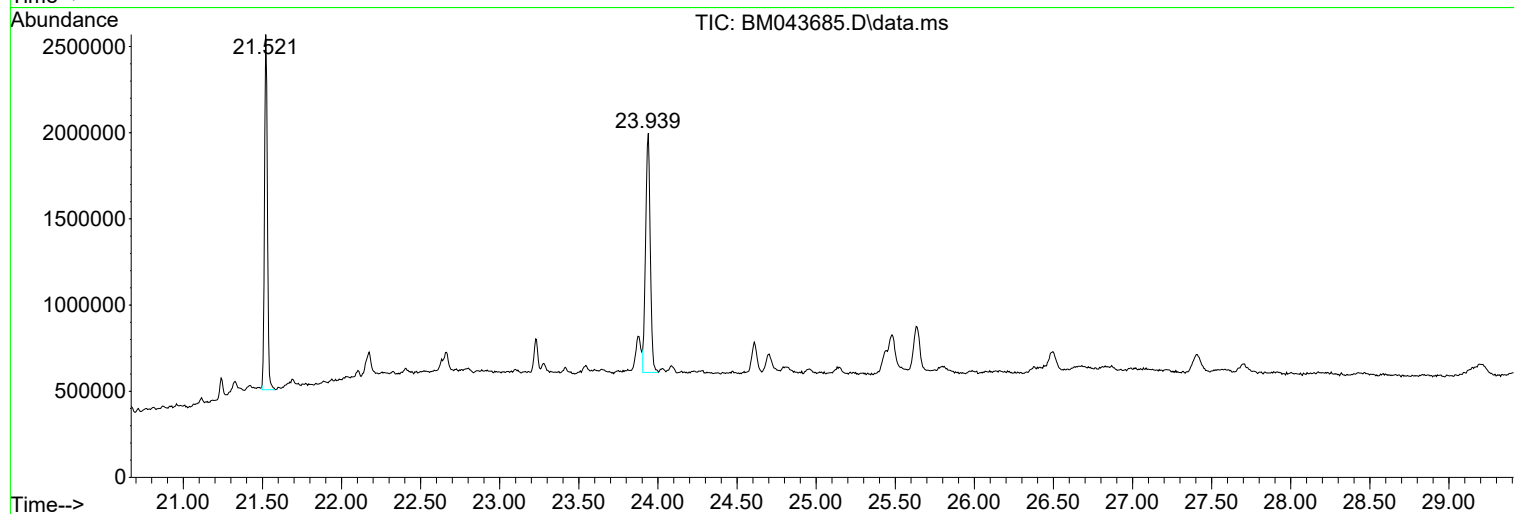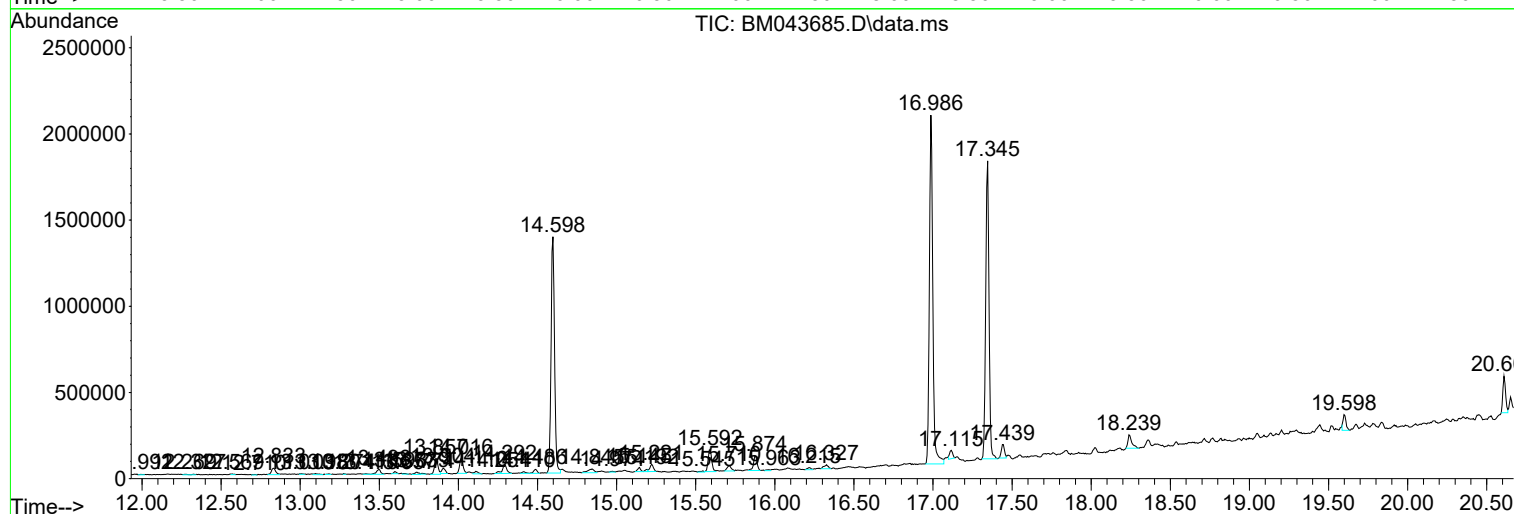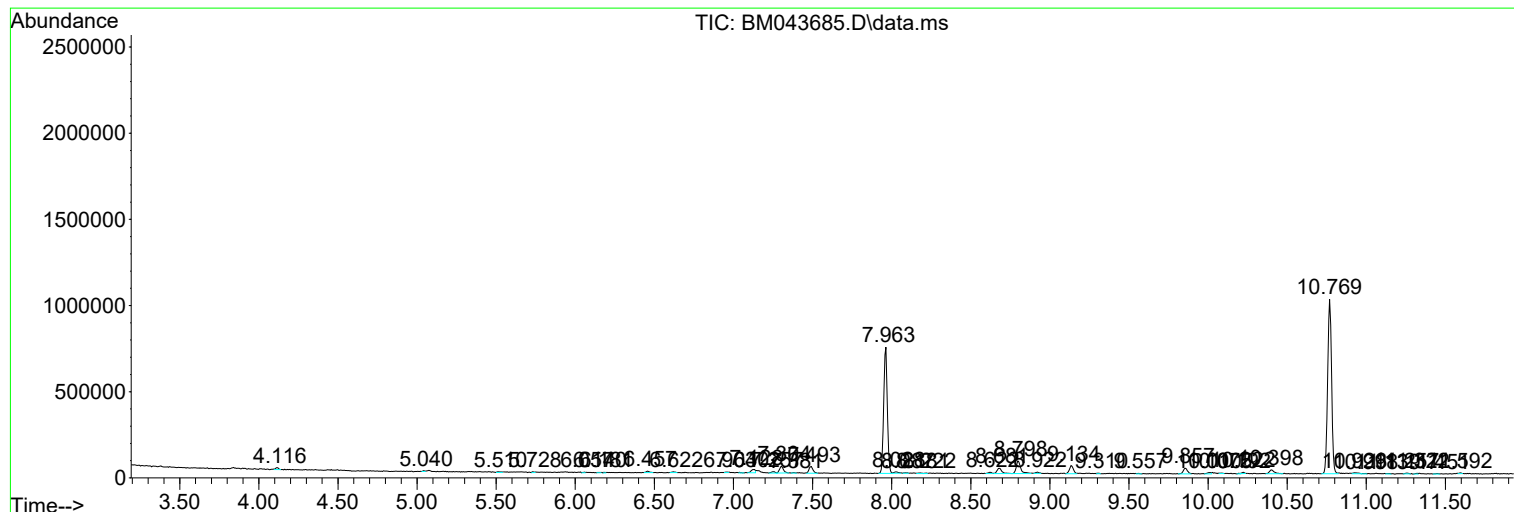

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122923\
Data File : BM043685.D
Acq On : 29 Dec 2023 23:55
Operator : MA/JU
Sample : 05920-10DL 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCF61DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122923\
Data File : BM043685.D
Acq On : 29 Dec 2023 23:55
Operator : MA/JU
Sample : 05920-10DL 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCF61DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc