


Data Path : Z:\HPCHEM1\BNA M\Data\BM123015\
 Data File : BM003831.D
 Acq On : 28 Dec 2015 16:44
 Operator : SJ/UM
 Sample : DFTPP64
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP64

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM121515.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 29 08:19:02 2015

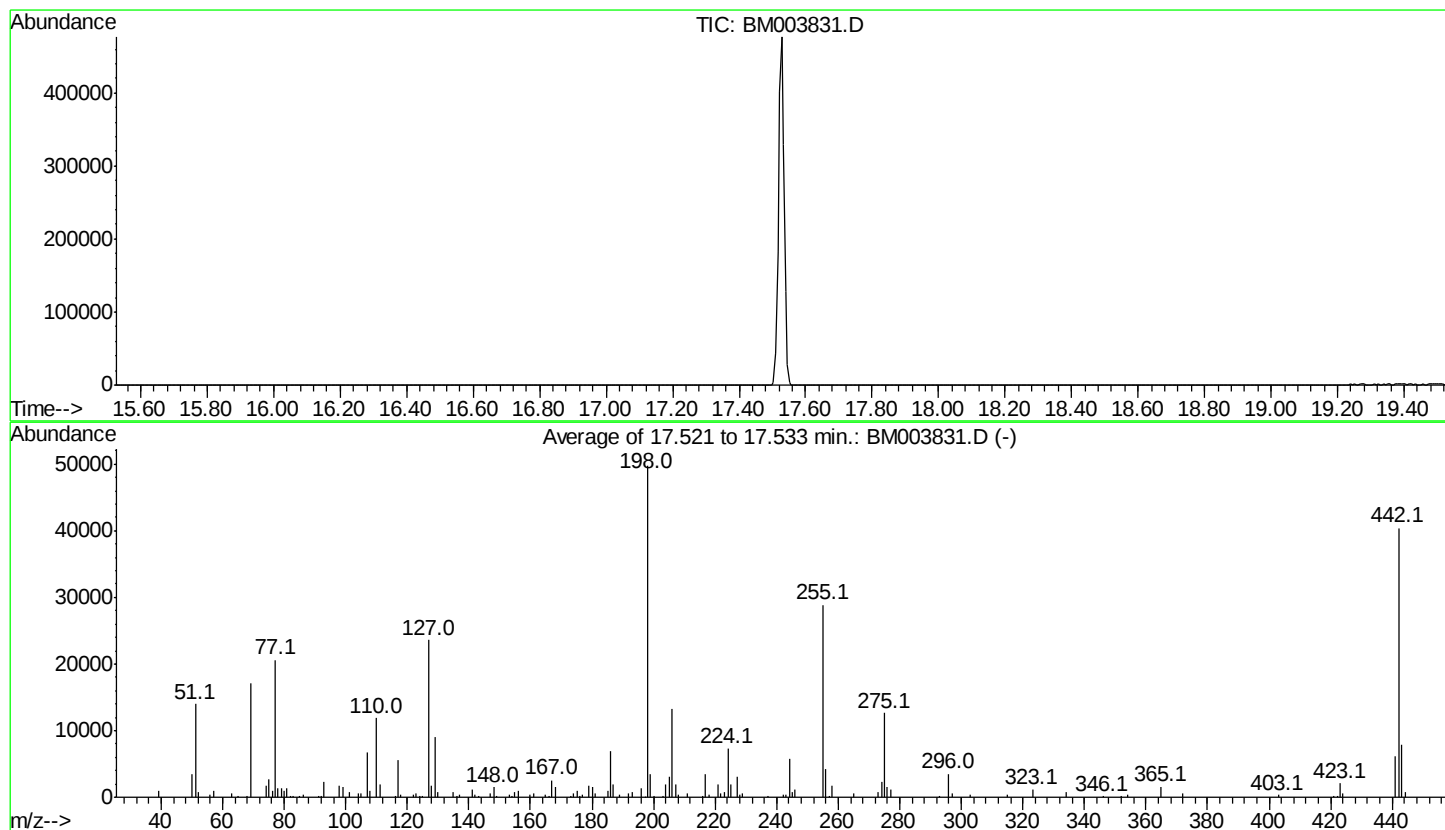

AutoFind: Scans 2454, 2455, 2456; Background Corrected with Scan 2448

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.1	13984	PASS
68	69	0.00	2	1.3	218	PASS
69	198	0.00	100	34.2	17048	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.3	23552	PASS
197	198	0.00	1	0.2	102	PASS
198	198	100	100	100.0	49778	PASS
199	198	5	9	6.8	3406	PASS
275	198	10	60	25.4	12642	PASS
365	198	1	100	3.1	1544	PASS
441	443	0.01	100	79.0	6173	PASS
442	198	50	100	81.2	40424	PASS
443	442	15	24	19.3	7813	PASS

m/z Abundance

Instrument :
BNA_M
ClientSampleId :
DFTPP64

m/z	Abundance
39.10	1185.0
50.10	3934.0
51.10	16030.0
52.00	809.0
56.00	501.0
57.00	1148.0
63.00	708.0
65.00	327.0
68.00	337.0
69.00	19120.0
74.00	1994.0
75.00	3086.0
76.10	1066.0
77.10	22992.0
78.00	1621.0
79.00	1483.0
80.00	1093.0
81.00	1521.0
82.00	350.0
83.00	355.0
85.00	388.0
86.00	475.0
91.00	407.0
91.90	433.0
93.00	2533.0
98.00	1827.0
99.00	1808.0
101.00	874.0
104.00	560.0
105.00	521.0
107.00	7164.0
108.00	1084.0
110.00	13050.0
111.00	2046.0
116.00	371.0
117.00	5892.0
118.00	452.0
122.00	468.0
123.00	711.0
124.00	304.0
125.00	320.0
127.00	24904.0
128.00	1829.0
129.00	10012.0
130.00	901.0
135.00	740.0
135.90	352.0
137.00	511.0
141.00	1218.0
142.00	486.0
147.00	719.0
148.00	1561.0
149.00	362.0
153.00	407.0
153.90	302.0
155.00	752.0
156.00	1024.0
160.00	422.0
161.00	586.0
165.00	438.0
166.10	335.0
167.00	2683.0
168.00	1747.0
174.00	525.0
175.00	1023.0
177.00	421.0
179.00	1791.0
180.00	1481.0
181.00	585.0
185.00	988.0
186.10	6860.0
187.00	2016.0
189.00	416.0
192.00	663.0
193.00	681.0
196.00	1451.0
198.00	49336.0
199.00	3521.0
203.00	317.0
204.00	1875.0
205.10	3074.0
206.10	13141.0
207.10	2005.0
208.10	474.0
211.00	507.0
217.00	3417.0
218.00	478.0
221.10	2032.0
221.80	484.0
223.00	776.0
224.10	6971.0
225.00	1939.0

Instrument :
BNA_M
ClientSampleId :
DFTPP64

227.00	3037.0
228.00	406.0
229.00	656.0
237.00	349.0
242.00	358.0
243.10	389.0
244.10	5399.0
245.00	698.0
246.00	1045.0
255.10	27304.0
256.00	4118.0
257.00	417.0
258.00	1556.0
265.00	610.0
273.00	770.0
274.10	2028.0
275.10	11803.0
276.00	1540.0
277.00	951.0
296.00	3345.0
297.00	464.0
303.00	346.0
315.00	352.0
323.10	1021.0
334.10	655.0
354.10	304.0
365.10	1342.0
372.10	530.0
403.10	326.0
423.10	1565.0
424.10	639.0
441.10	4763.0
442.10	31536.0
443.10	6259.0
444.10	628.0

Instrument :
BNA_M
ClientSampleId :
DFTPP64

m/z	Abundance
39.00	1079.0
50.10	4018.0
51.10	15847.0
52.00	807.0
56.00	464.0
57.00	1231.0
63.00	786.0
65.00	366.0
68.00	319.0
69.00	19768.0
74.00	2081.0
75.00	3282.0
76.10	1086.0
77.10	23872.0
78.10	1646.0
79.00	1424.0
80.00	1128.0
81.00	1645.0
82.00	391.0
83.00	385.0
85.00	380.0
86.00	535.0
91.00	436.0
92.00	445.0
93.00	2818.0
98.00	2175.0
99.00	1925.0
101.00	935.0
104.00	640.0
105.00	679.0
107.00	7606.0
108.00	1188.0
110.00	13422.0
111.00	2159.0
116.00	435.0
117.00	6302.0
118.00	438.0
122.00	503.0
123.00	778.0
123.90	383.0
125.00	344.0
127.00	27920.0
128.00	2126.0
129.00	10452.0
130.00	877.0
135.00	936.0
136.00	374.0
137.00	537.0
141.00	1337.0
142.00	411.0
143.00	350.0
147.00	810.0
148.00	1748.0
149.00	406.0
153.00	470.0
154.00	382.0
155.00	768.0
156.00	1126.0
160.00	464.0
161.00	769.0
165.00	488.0
166.00	472.0
167.00	3033.0
168.00	1909.0
173.00	333.0
174.00	609.0
175.00	1209.0
176.00	316.0
177.00	527.0
179.00	2134.0
180.00	1789.0
181.00	700.0
185.10	971.0
186.10	8413.0
187.00	2436.0
189.00	481.0
192.00	690.0
193.00	863.0
196.00	1552.0
197.10	308.0
198.00	58464.0
199.00	4080.0
200.00	338.0
203.00	437.0
204.00	2178.0
205.10	3523.0
206.10	15687.0
207.10	2219.0
208.00	585.0
211.00	578.0
216.00	347.0
217.00	4225.0

Instrument :
BNA_M
ClientSampleId :
DFTPP64

218.00	504.0
221.00	2337.0
221.80	573.0
223.00	968.0
224.10	8427.0
225.00	2064.0
227.00	3751.0
228.00	501.0
229.00	668.0
237.00	408.0
242.10	459.0
243.10	491.0
244.10	6844.0
245.10	911.0
246.00	1429.0
255.10	34368.0
256.10	4922.0
257.00	454.0
258.00	1954.0
265.00	705.0
273.00	999.0
274.00	2713.0
275.10	14916.0
276.10	1859.0
277.00	1388.0
293.00	327.0
296.00	4026.0
297.00	560.0
303.10	461.0
315.00	433.0
323.10	1290.0
334.10	849.0
346.10	362.0
352.10	357.0
354.10	401.0
365.00	1777.0
372.10	622.0
403.10	379.0
421.10	320.0
422.10	367.0
423.10	2508.0
424.10	827.0
441.10	7302.0
442.10	48376.0
443.10	9222.0
444.10	828.0

Instrument :
BNA_M
ClientSampleId :
DFTPP64

m/z	Abundance
39.00	764.0
50.00	2531.0
51.10	10077.0
52.00	523.0
57.00	770.0
63.00	451.0
69.00	12258.0
74.00	1251.0
75.00	2013.0
76.10	703.0
77.10	15025.0
78.00	1034.0
79.00	956.0
80.00	732.0
81.00	970.0
86.00	318.0
93.00	1600.0
98.00	1345.0
99.00	1115.0
101.00	599.0
104.00	401.0
105.00	332.0
107.00	5227.0
108.00	820.0
110.00	9007.0
111.00	1292.0
117.00	4296.0
121.90	327.0
123.00	515.0
127.00	17832.0
128.00	1468.0
129.00	6521.0
130.00	616.0
135.00	575.0
137.00	343.0
141.00	908.0
147.00	457.0
148.00	1112.0
153.00	314.0
155.00	587.0
156.00	816.0
160.00	342.0
161.10	461.0
165.00	357.0
167.00	1945.0
168.00	1238.0
174.00	440.0
175.00	730.0
177.00	347.0
179.00	1494.0
180.00	1118.0
181.10	490.0
185.00	778.0
186.00	5479.0
187.00	1619.0
188.90	371.0
192.00	556.0
193.00	644.0
196.10	1098.0
198.00	41536.0
199.00	2618.0
204.00	1548.0
205.10	2511.0
206.10	10954.0
207.10	1534.0
208.00	376.0
211.10	474.0
217.00	2964.0
218.00	335.0
221.10	1639.0
221.80	419.0
223.00	676.0
224.10	6463.0
225.10	1550.0
227.00	2633.0
228.00	350.0
229.00	548.0
242.10	324.0
243.10	355.0
244.10	4883.0
245.10	659.0
246.00	892.0
255.10	25104.0
256.10	3645.0
258.00	1497.0
265.00	579.0
273.00	740.0
274.00	2008.0
275.10	11208.0
276.10	1488.0
277.00	1052.0
296.00	3092.0

Instrument :
BNA_M
ClientSampleId :
DFTPP64

297.00	493.0
303.00	340.0
315.00	381.0
323.00	994.0
334.10	694.0
354.10	326.0
365.10	1515.0
372.10	583.0
403.10	352.0
422.10	301.0
423.10	2202.0
424.10	511.0
441.10	6454.0
442.10	41360.0
443.10	7958.0
444.10	736.0

Instrument :
BNA_M
ClientSampleId :
DFTPP64