
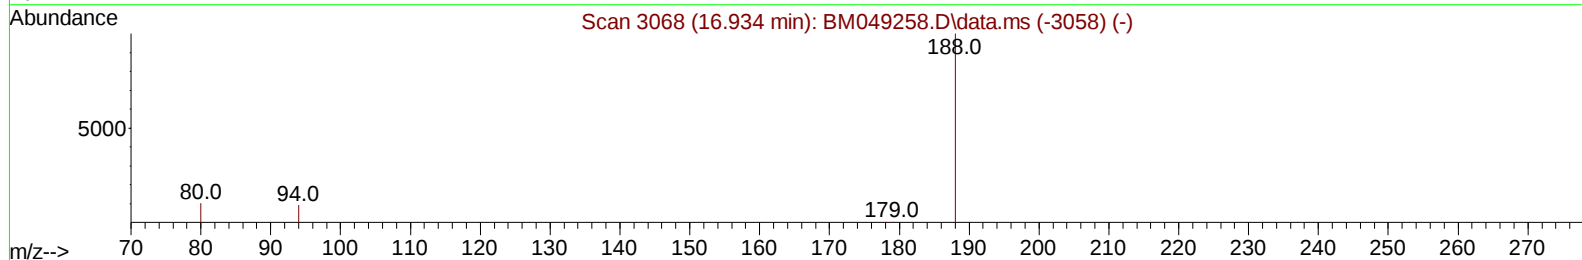
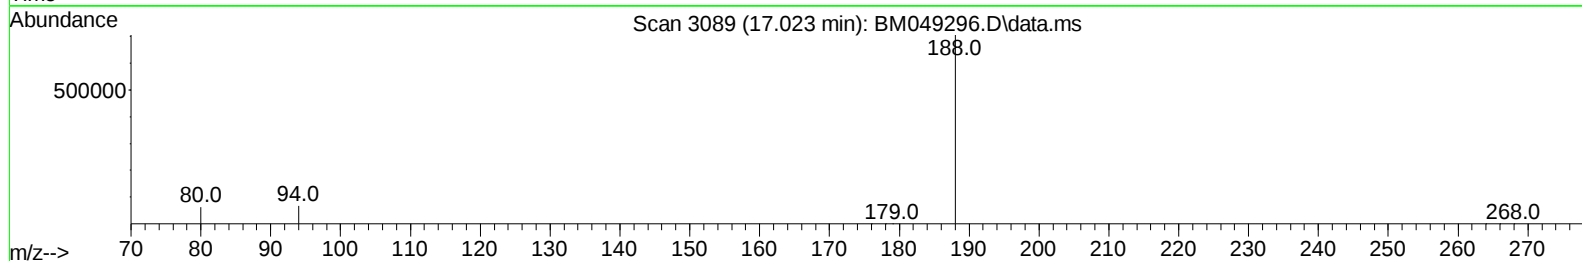


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM123024\
Data File : BM049296.D
Acq On : 30 Dec 2024 10:58
Operator : RC/JU
Sample : PB165848BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Dec 30 11:32:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 26 11:35:38 2024
Response via : Initial Calibration

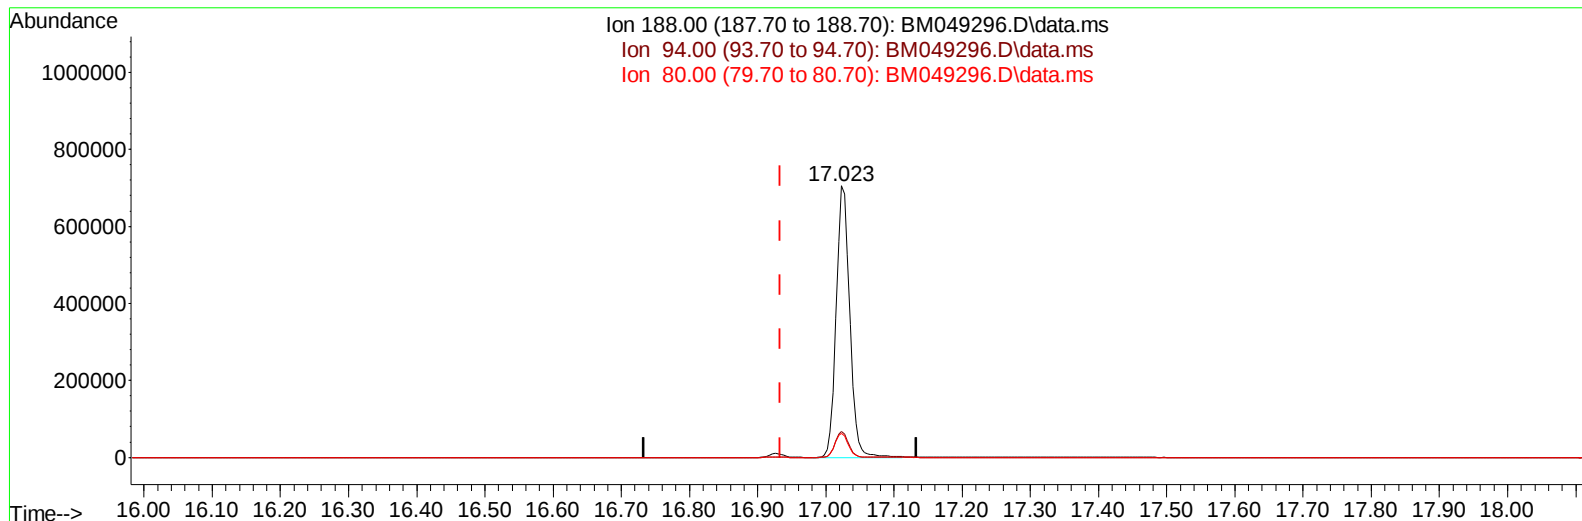




TIC: BM049296.D\data.ms

(13) Phenanthrene-d10 (I)**17.023min (+ 0.090) 0.40 ng/u1****response 974194**

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	9.80	9.59
80.00	10.70	8.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM123024\
Data File : BM049296.D
Acq On : 30 Dec 2024 10:58
Operator : RC/JU
Sample : PB165848BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Dec 30 11:32:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 26 11:35:38 2024
Response via : Initial Calibration

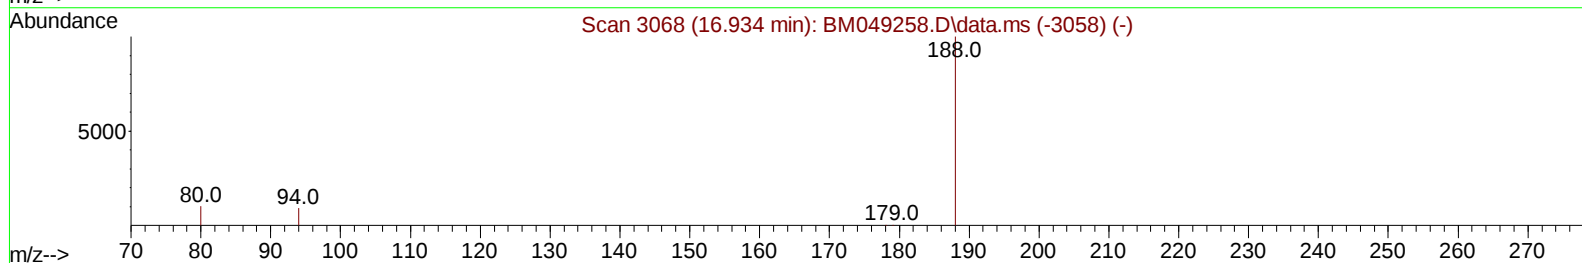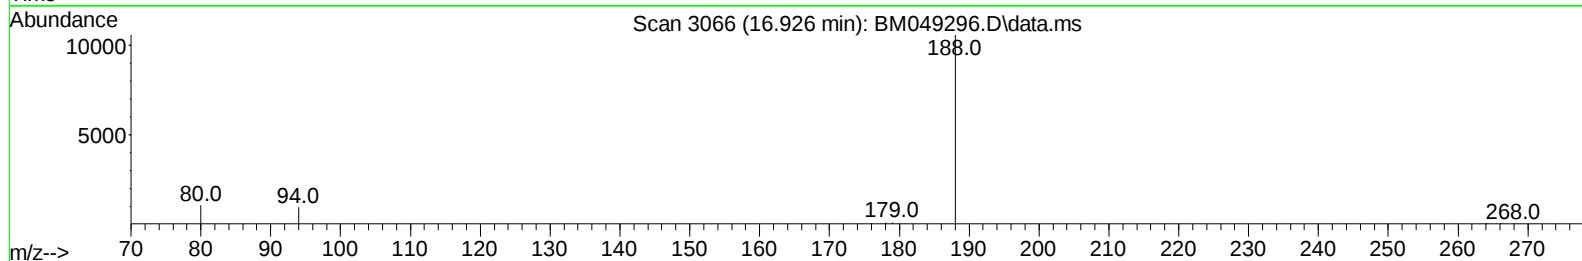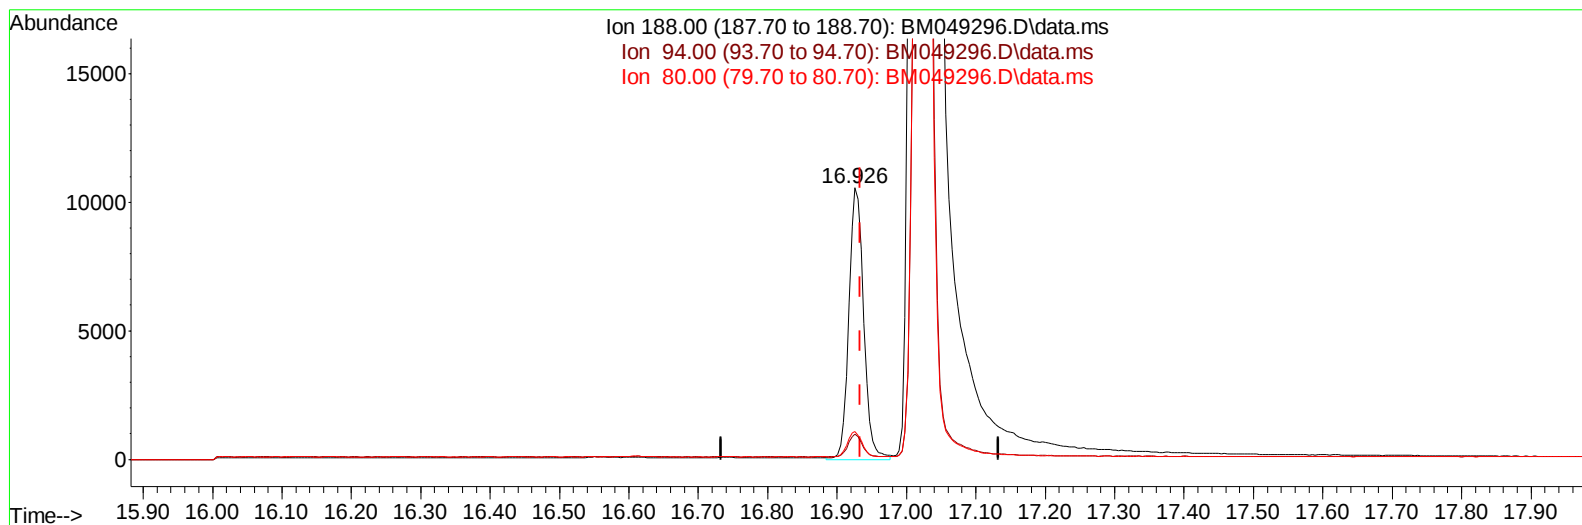




TIC: BM049296.D\data.ms

(13) Phenanthrene-d10 (I)**16.926min (-0.007) 0.40 ng/ul m****response 15577**

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	9.80	9.25
80.00	10.70	10.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM123024\
Data File : BM049296.D
Acq On : 30 Dec 2024 10:58
Operator : RC/JU
Sample : PB165848BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Dec 30 11:32:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 26 11:35:38 2024
Response via : Initial Calibration

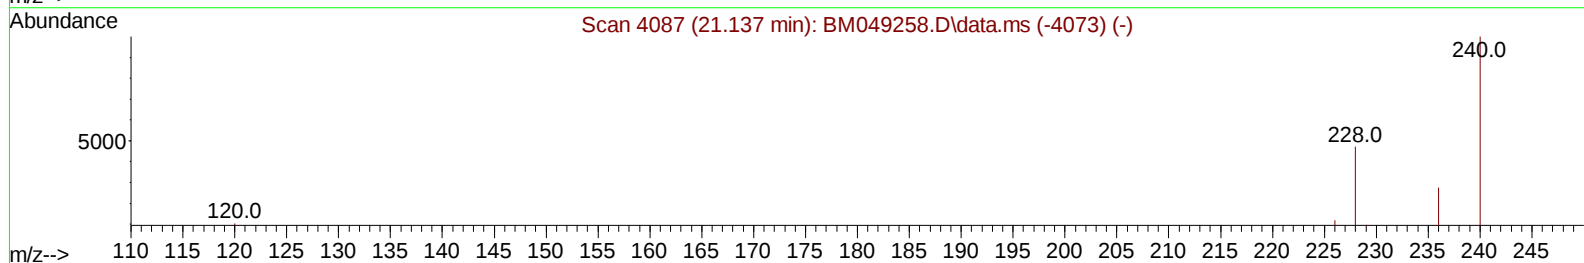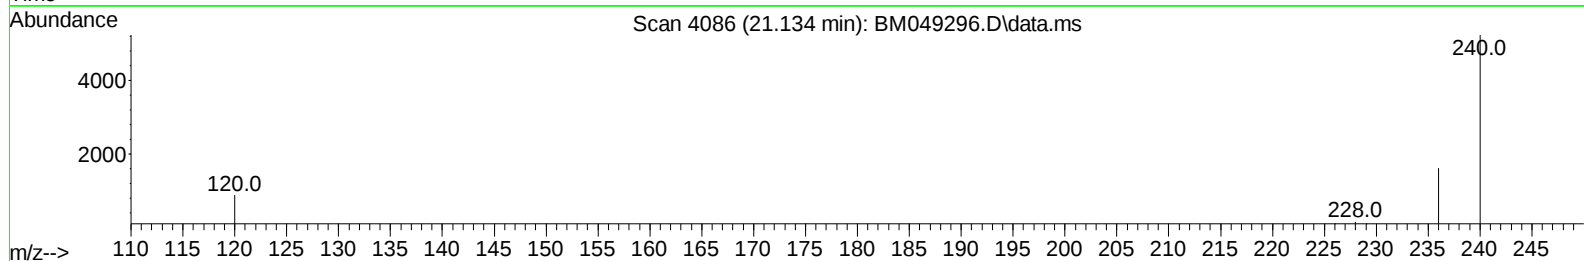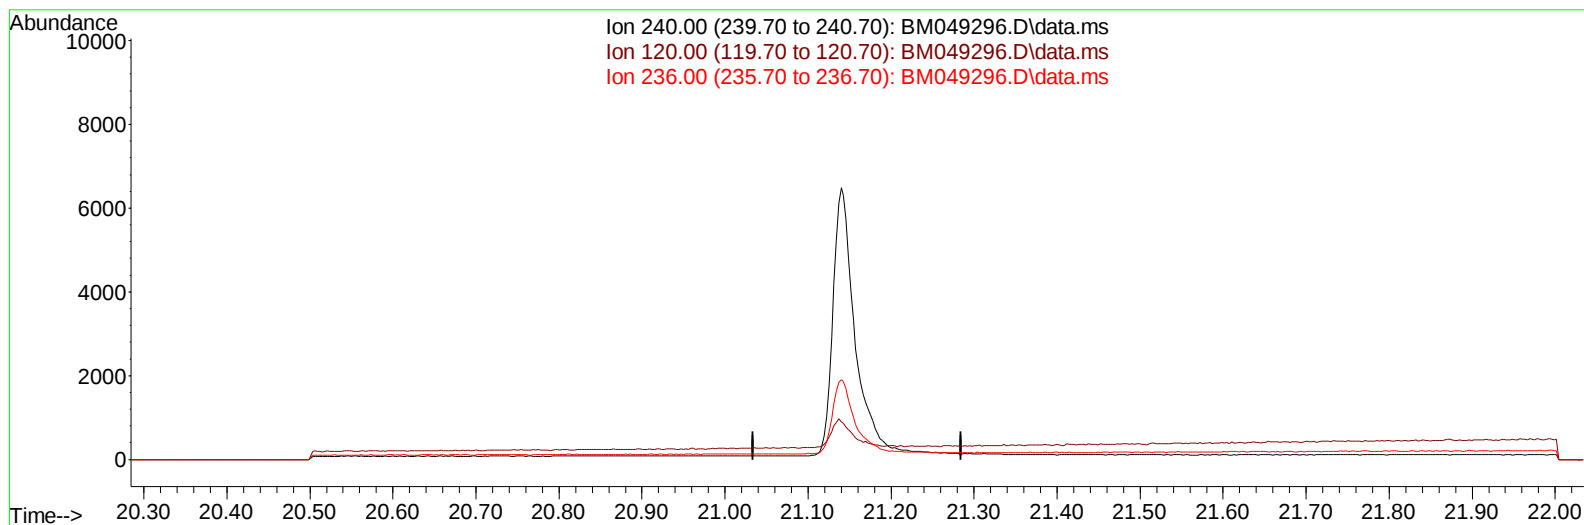

TIC: BM049296.D\data.ms

(17) Chrysene-d12




21.134min (-21.134) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	14.50	0.00#
236.00	29.80	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM123024\
Data File : BM049296.D
Acq On : 30 Dec 2024 10:58
Operator : RC/JU
Sample : PB165848BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Dec 30 11:32:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 26 11:35:38 2024
Response via : Initial Calibration

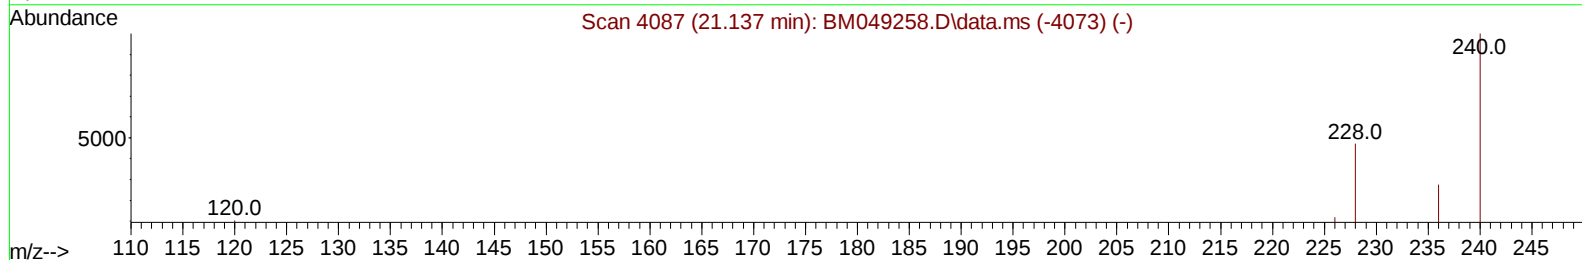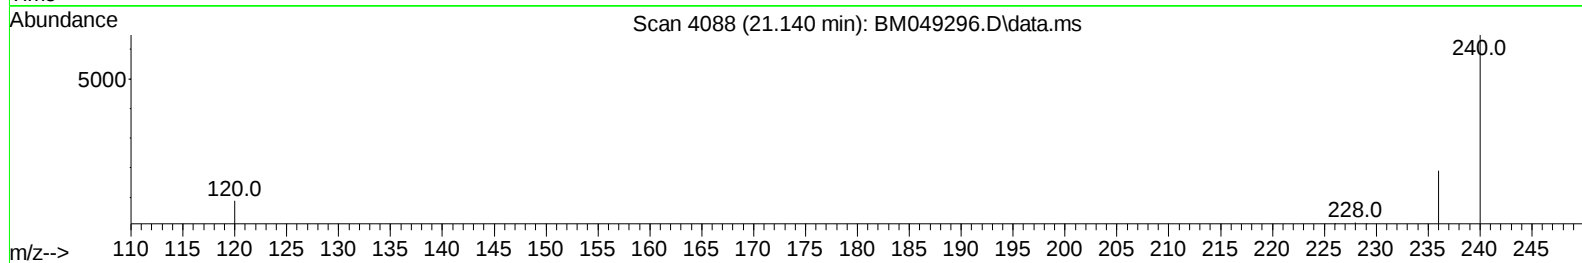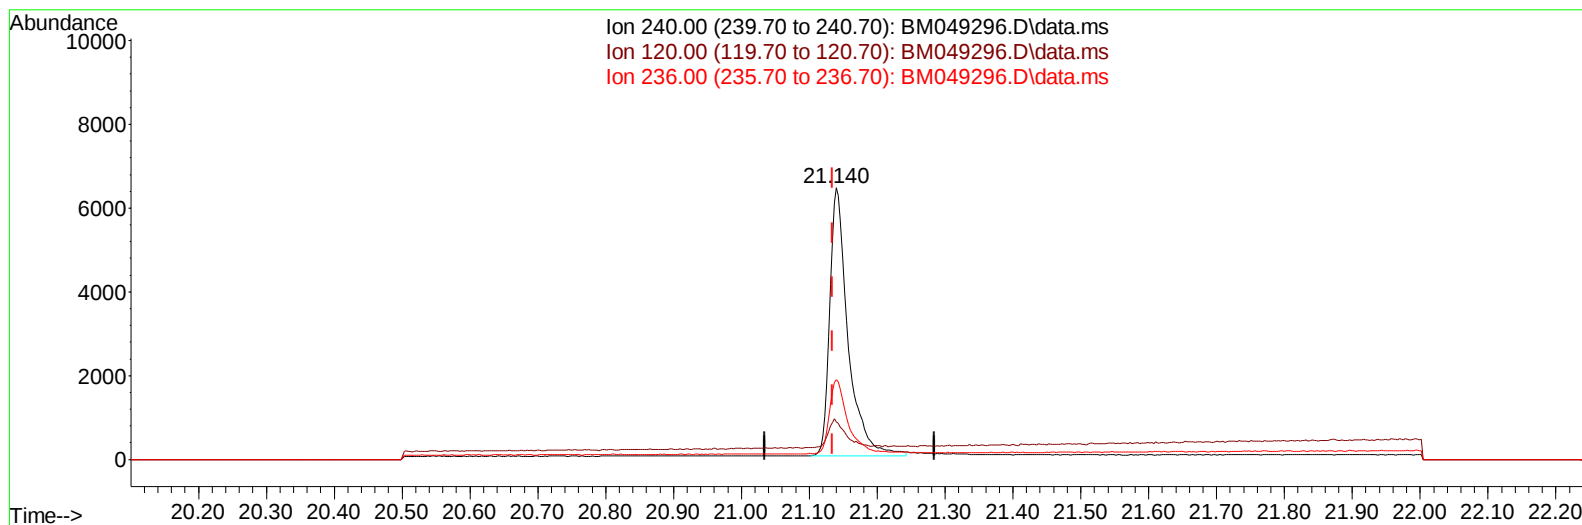

TIC: BM049296.D\data.ms

(17) Chrysene-d12




21.140min (+ 0.006) 0.40 ng/ul m

response 12019

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	14.50	13.70
236.00	29.80	29.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM123024\
Data File : BM049296.D
Acq On : 30 Dec 2024 10:58
Operator : RC/JU
Sample : PB165848BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Dec 30 11:32:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 26 11:35:38 2024
Response via : Initial Calibration

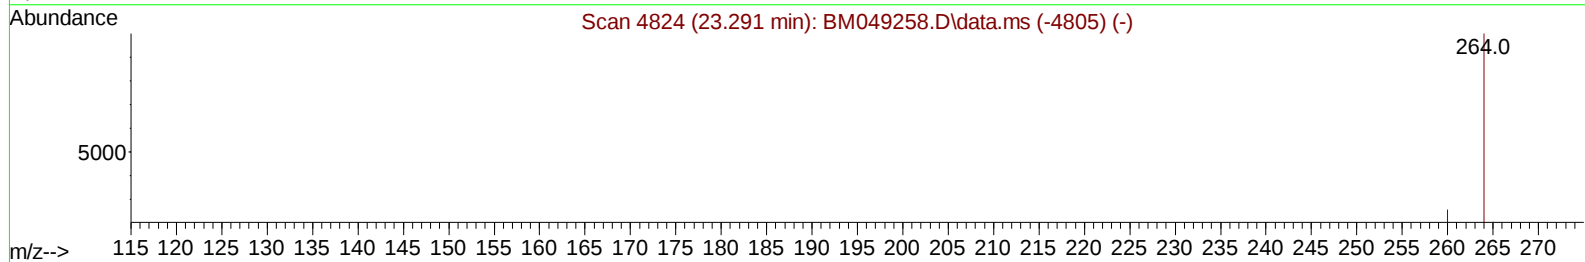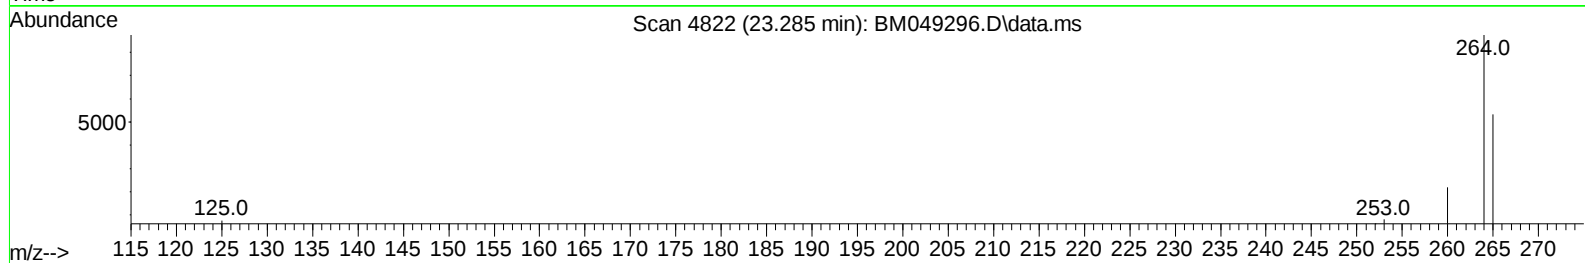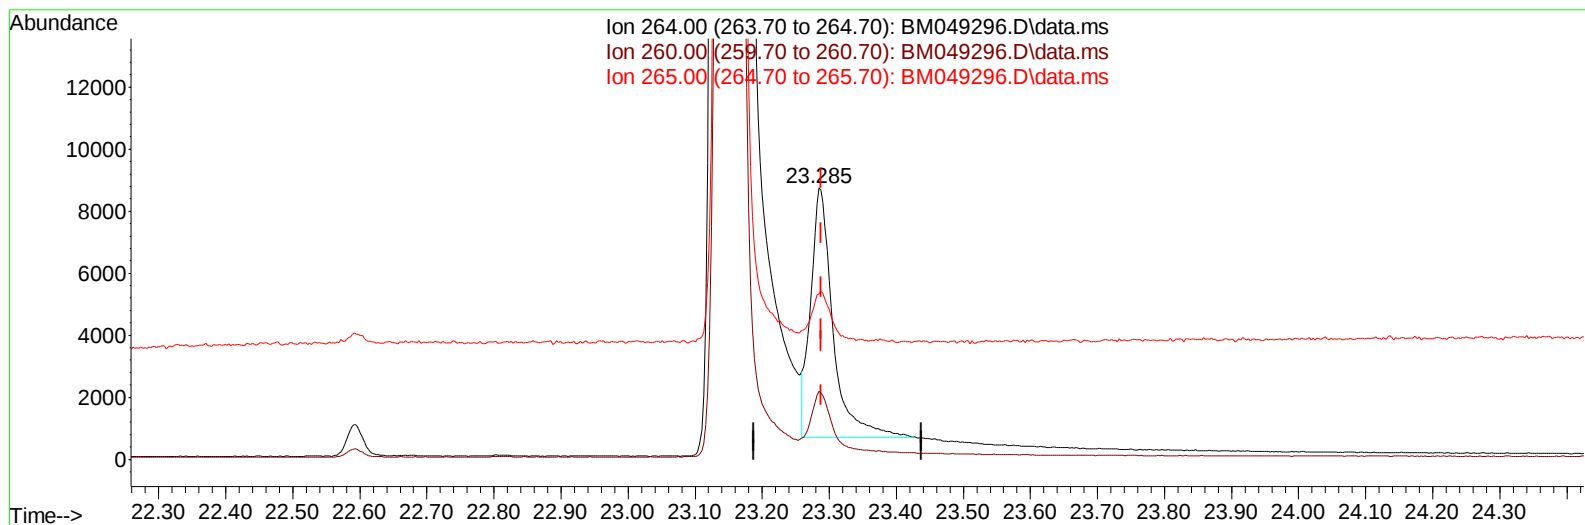

TIC: BM049296.D\data.ms

(23) Perylene-d12 (I)




23.285min (-0.003) 0.40 ng/u1

response 18617

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.80	25.11
265.00	78.30	61.05#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM123024\
Data File : BM049296.D
Acq On : 30 Dec 2024 10:58
Operator : RC/JU
Sample : PB165848BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Dec 30 11:32:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 26 11:35:38 2024
Response via : Initial Calibration

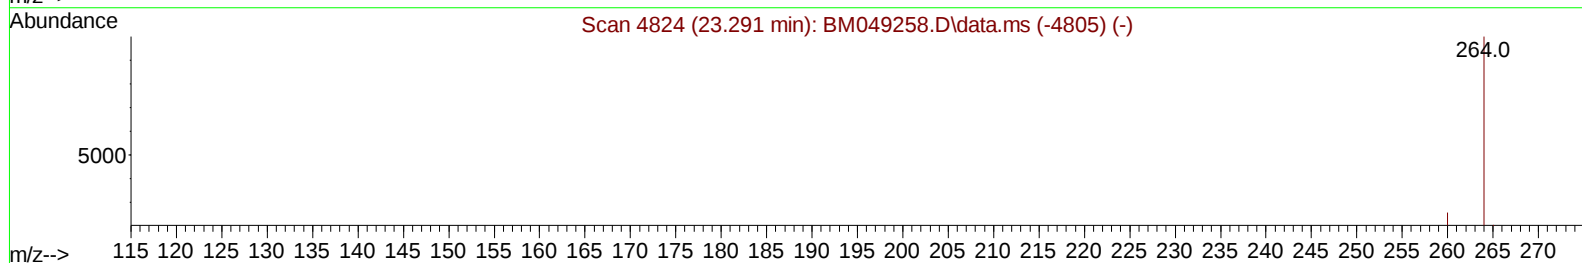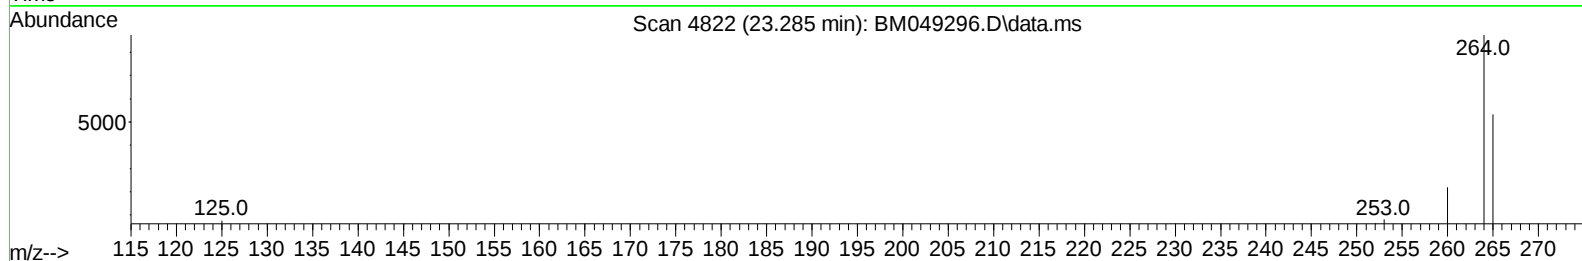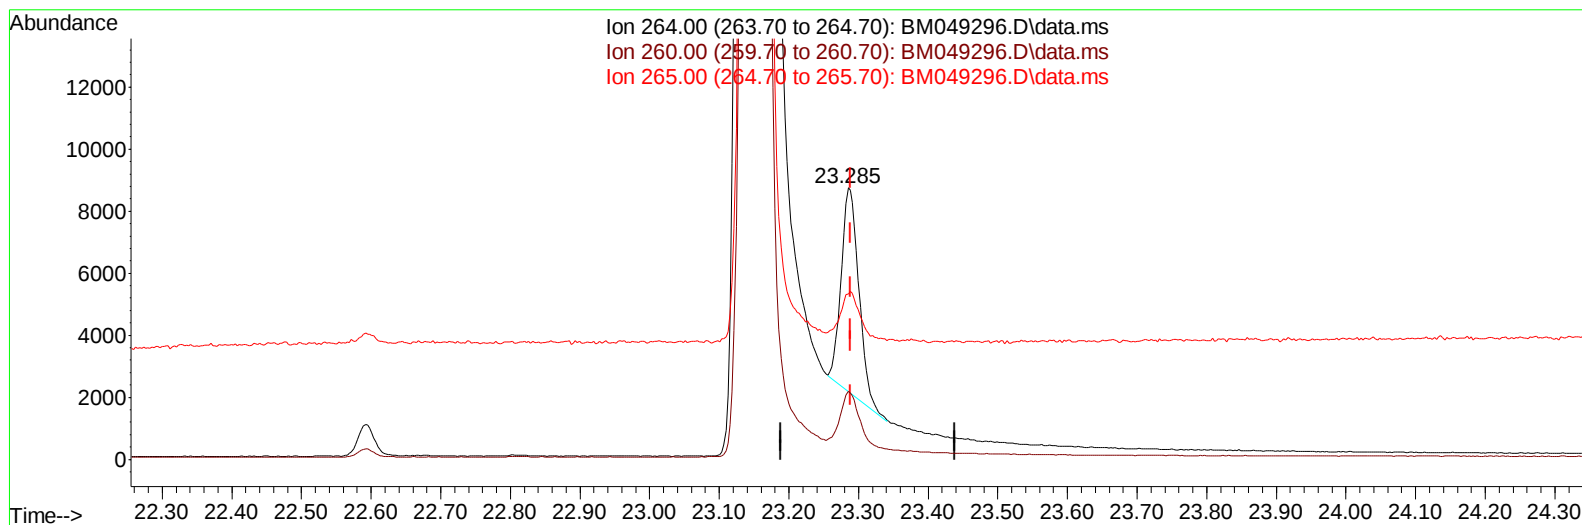

TIC: BM049296.D\data.ms

(23) Perylene-d12 (I)

23.285min (-0.003) 0.40 ng/ul m

response 11579

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.80	25.11
265.00	78.30	61.05#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM123024\
 Data File : BM049296.D
 Acq On : 30 Dec 2024 10:58
 Operator : RC/JU
 Sample : PB165848BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Quant Time: Dec 30 11:32:47 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 26 11:35:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.539	152	4063	0.400	ng/ul	0.00
4) Naphthalene-d8	10.299	136	12064	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.178	164	6670	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.926	188	15577m	0.400	ng/ul	0.00
17) Chrysene-d12	21.140	240	12019m	0.400	ng/ul	0.00
23) Perylene-d12	23.285	264	11579m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.134	96	26028	5.555	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.915	152	4835	0.298	ng/ul	0.00
18) Fluoranthene-d10	18.965	212	10674	0.313	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM123024\
Data File : BM049296.D
Acq On : 30 Dec 2024 10:58
Operator : RC/JU
Sample : PB165848BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Dec 30 11:32:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 26 11:35:38 2024
Response via : Initial Calibration

