


Data Path : Z:\HPCHEM1\BNA_M\Data\BM123114\
 Data File : BM000090.D
 Acq On : 31 Dec 2014 13:38
 Operator : TP
 Sample : DFTPP02
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP02

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM122914.M
 Title : SVOA CALIBRATION
 Last Update : Wed Dec 31 02:57:11 2014

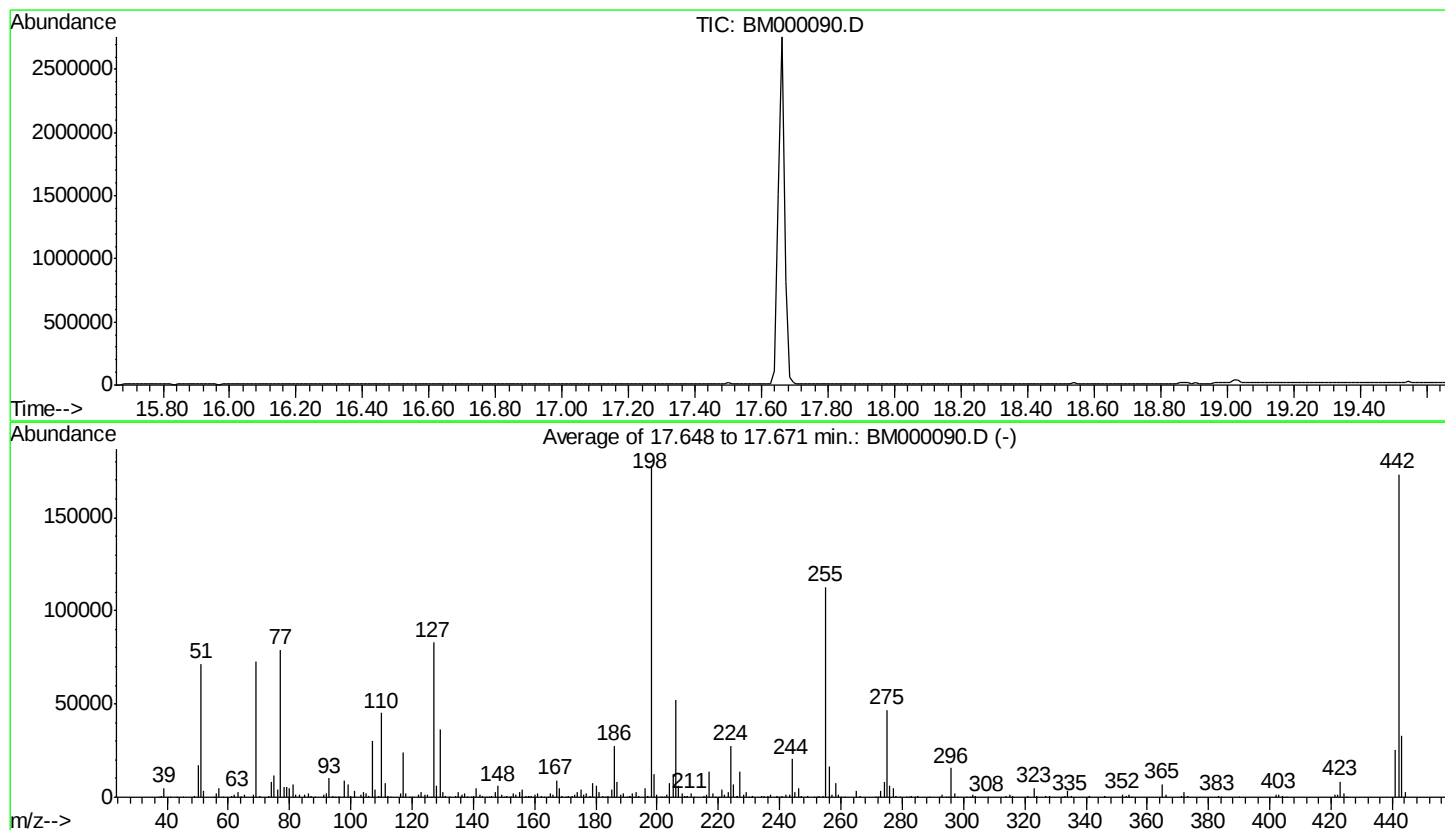

AutoFind: Scans 1309, 1310, 1311; Background Corrected with Scan 1306

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.2	71507	PASS
68	69	0.00	2	1.6	1139	PASS
69	198	0.00	100	41.1	73056	PASS
70	69	0.00	2	0.6	423	PASS
127	198	10	80	46.6	82938	PASS
197	198	0.00	2	0.4	725	PASS
198	198	100	100	100.0	177818	PASS
199	198	5	9	6.9	12303	PASS
275	198	10	60	26.3	46717	PASS
365	198	1	100	3.9	6971	PASS
441	443	0.01	100	78.0	25737	PASS
442	198	50	100	97.3	173082	PASS
443	442	15	24	19.1	32991	PASS