

Data Path : Z:\HPCHEM1\BNA M\DATA\BM123115\
 Data File : BM003868.D
 Acq On : 30 Dec 2015 03:33
 Operator : SJ/UM
 Sample : G4848-19DL 5X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9N65DL

Quant Time: Dec 30 06:00:28 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-SIM-BM121515.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 30 05:57:00 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	4687	0.40	ng/ul	0.00
4) Naphthalene-d8	10.46	136	19991	0.40	ng/ul	0.00
8) Acenaphthene-d10	14.33	164	11537	0.40	ng/ul	0.00
12) Phenanthrene-d10	17.07	188	25851	0.40	ng/ul	0.00
18) Chrysene-d12	21.28	240	18530	0.40	ng/ul	0.00
22) Perylene-d12	23.51	264	16115	0.40	ng/ul	0.00
System Monitoring Compounds						
2) 1,4-Dioxane-d8	3.14	96	6156	3.07	ng/uL	0.00
6) 2-Methylnaphthalene-d10	12.07	152	2120	0.09	ng/ul	0.01
16) Fluoranthene-d10	19.12	212	4869	0.09	ng/ul	0.00
Target Compounds				Ovalue		
5) Naphthalene	10.51	128	46124	1.02	ng/ul	98
7) 2-Methylnaphthalene	12.13	142	5100	0.17	ng/ul	99
9) Acenaphthylene	14.04	152	653	0.01	ng/ul#	79
10) Acenaphthene	14.38	153	3871	0.11	ng/ul#	83
11) Fluorene	15.38	166	4321	0.11	ng/ul#	79
13) Pentachlorophenol	16.75	266	142	0.04	ng/ul#	86
14) Phenanthrene	17.11	178	16914	0.25	ng/ul#	90
15) Anthracene	17.21	178	1379	0.02	ng/ul#	80
17) Fluoranthene	19.14	202	6236	0.09	ng/ul	97
19) Pyrene	19.51	202	4977	0.10	ng/ul#	95
20) Benzo(a)anthracene	21.26	228	654	0.01	ng/ul#	78
21) Chrysene	21.31	228	625	0.01	ng/ul#	78
23) Benzo(b)fluoranthene	22.85	252	584	0.01	ng/ul#	1
24) Benzo(k)fluoranthene	22.85	252	579	0.01	ng/ul#	1
25) Benzo(a)pyrene	23.37	252	1392	0.03	ng/ul#	1
26) Indeno(1,2,3-cd)pyrene	25.78	276	159	0.00	ng/ul#	74
27) Dibenzo(a,h)anthracene	25.79	278	128	0.00	ng/ul#	1
28) Benzo(a,h,i)perylene	26.46	276	154	0.00	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM123115\
Data File : BM003868.D
Acq On : 30 Dec 2015 03:33
Operator : SJ/UM
Sample : G4848-19DL 5X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9N65DL

Quant Time: Dec 30 06:00:28 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-SIM-BM121515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 30 05:57:00 2015
Response via : Initial Calibration

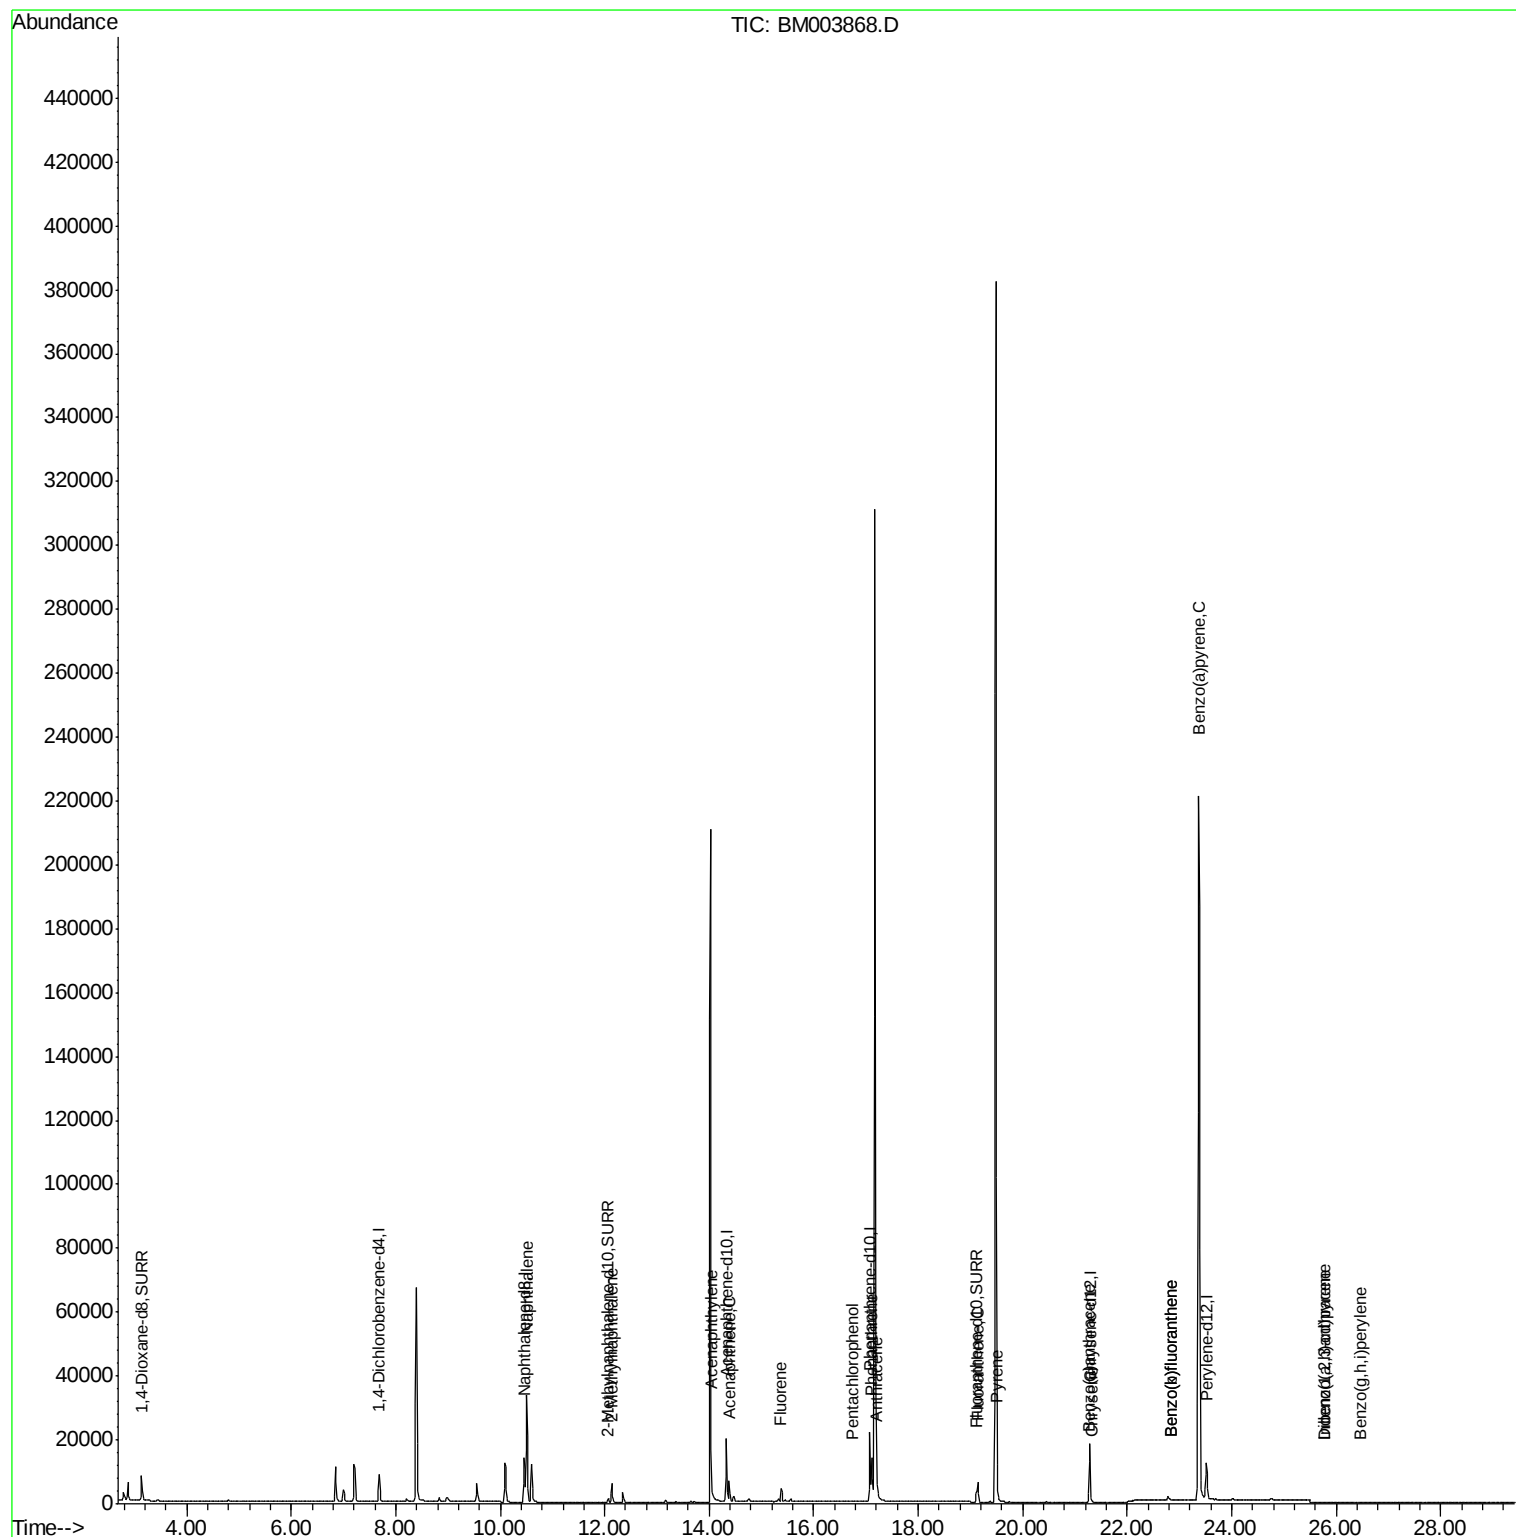

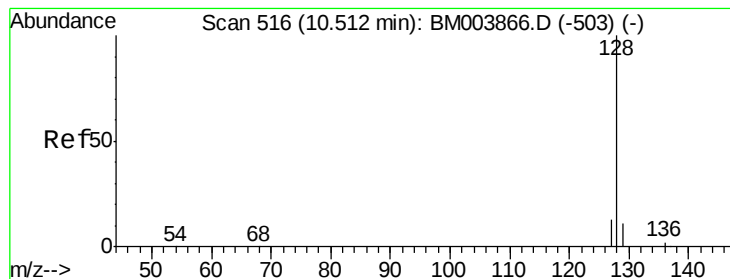

#5

Naphthalene

Concen: 1.02 ng/ul

RT: 10.51 min Scan# 516

Delta R.T. -0.00 min

Lab File: BM003868.D

Acq: 30 Dec 2015 03:33

Instrument :

BNA_M

ClientSampleId :

D9N65DL


Tot Ion:128 Resp: 46124

Ion Ratio Lower Upper

128 100

129 11.0 9.0 13.6




127 13.0 9.6 14.4

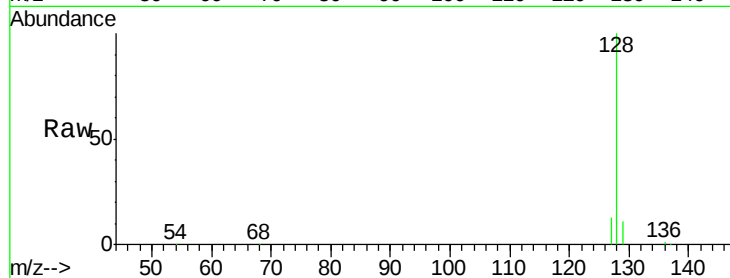

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

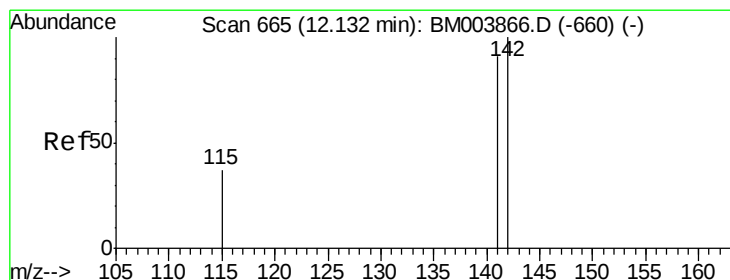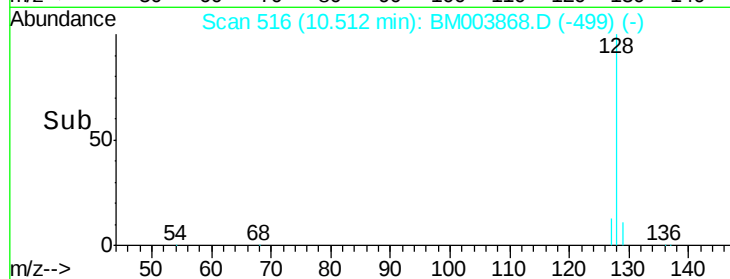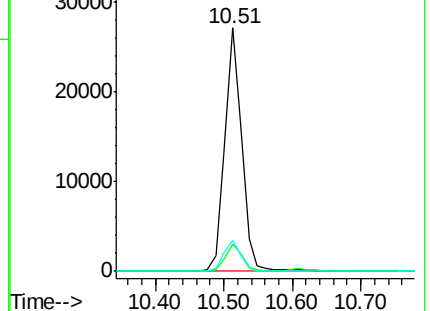

#7

2-Methylnaphthalene

Concen: 0.17 ng/ul

RT: 12.13 min Scan# 665

Delta R.T. -0.00 min

Lab File: BM003868.D


Acq: 30 Dec 2015 03:33

Tgt Ion:142 Resp: 5100

Ion Ratio Lower Upper



142 100


141 88.7 70.3 105.5

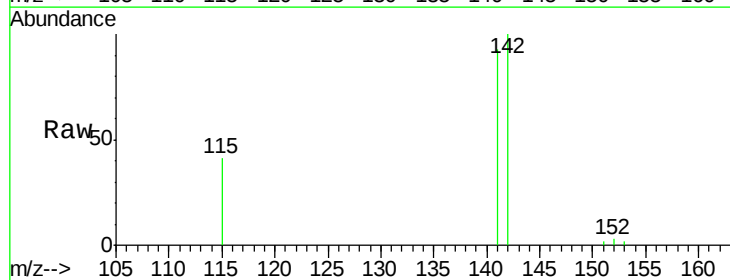

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

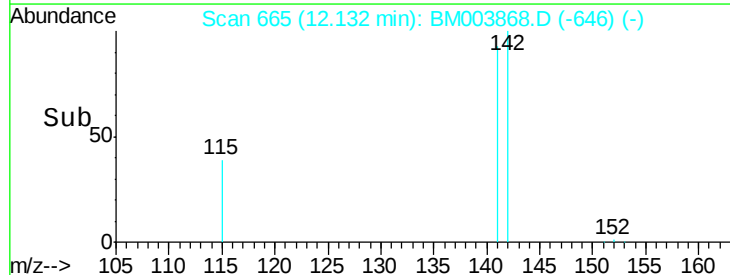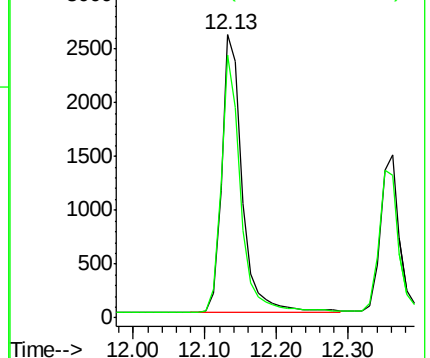



#9

Acenaphthylene

Concen: 0.01 ng/ul

RT: 14.04 min Scan# 847

Delta R.T. -0.00 min

Lab File: BM003868.D

Acq: 30 Dec 2015 03:33

Instrument :

BNA_M

ClientSampleId :

D9N65DL


Tot Ion:152 Resp: 653

Ion Ratio Lower Upper

152 100

151 28.9 17.6 26.4#




153 24.4 9.7 14.5#



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

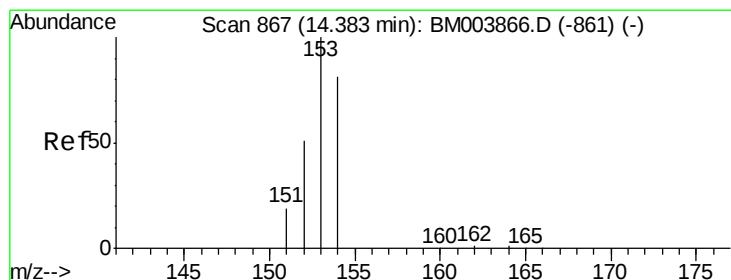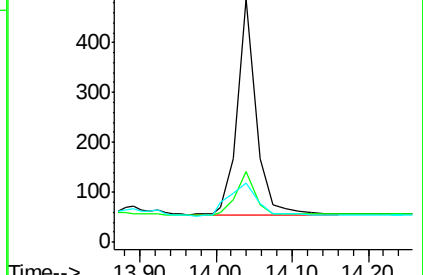

#10

Acenaphthene

Concen: 0.11 ng/ul

RT: 14.38 min Scan# 867

Delta R.T. -0.00 min

Lab File: BM003868.D

Acq: 30 Dec 2015 03:33


Tgt Ion:153 Resp: 3871

Ion Ratio Lower Upper

153 100

152 51.8 33.9 50.9#



154 83.3 80.6 121.0




Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

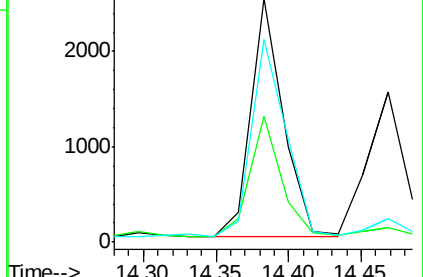

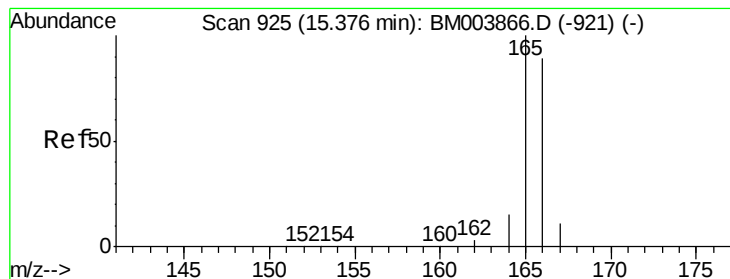

#11

Fluorene

Concen: 0.11 ng/ul

RT: 15.38 min Scan# 925

Delta R.T. -0.00 min

Lab File: BM003868.D

Acq: 30 Dec 2015 03:33

Instrument :

BNA_M

ClientSampleId :

D9N65DL


Tot Ion:166 Resp: 4321

Ion Ratio Lower Upper

166 100

165 109.5 69.6 104.4#




167 16.3 11.9 17.9

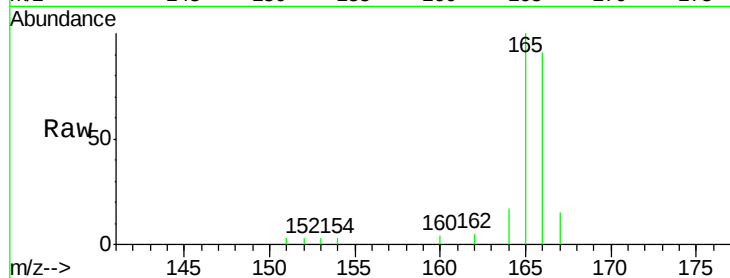

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

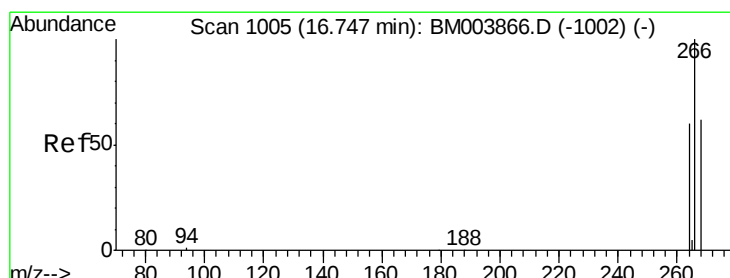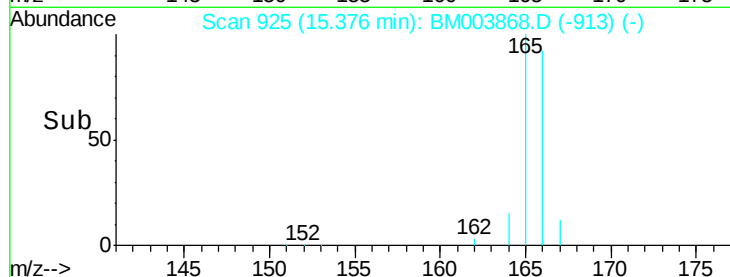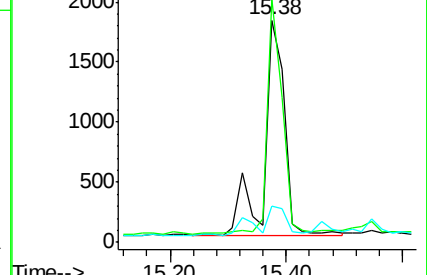

#13

Pentachlorophenol

Concen: 0.04 ng/ul

RT: 16.75 min Scan# 1005

Delta R.T. -0.00 min

Lab File: BM003868.D

Acq: 30 Dec 2015 03:33


Tgt Ion:266 Resp: 142

Ion Ratio Lower Upper

266 100

264 60.6 51.8 77.8



268 76.1 46.8 70.2#

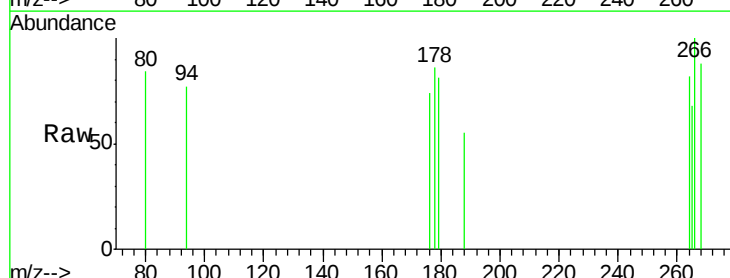


Abundance Ion 266.00 (265.70 to 266.70): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

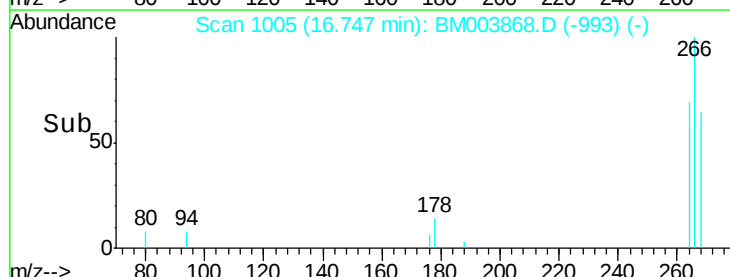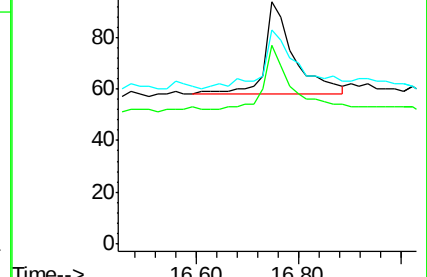

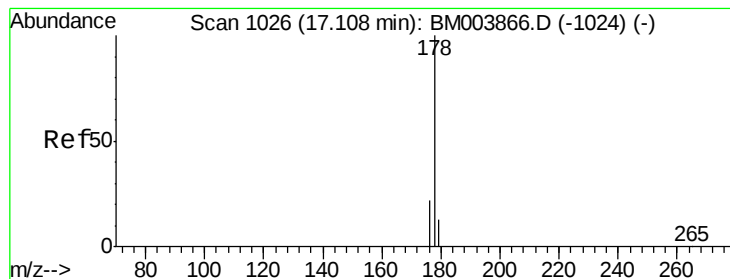

#14

Phenanthrene

Concen: 0.25 ng/ul

RT: 17.11 min Scan# 1026

Delta R.T. -0.00 min

Lab File: BM003868.D

Acq: 30 Dec 2015 03:33

Instrument :

BNA_M

ClientSampleId :

D9N65DL


Tot Ion:178 Resp: 16914

Ion Ratio Lower Upper

178 100

176 21.6 13.0 19.4#




179 14.4 14.2 21.2

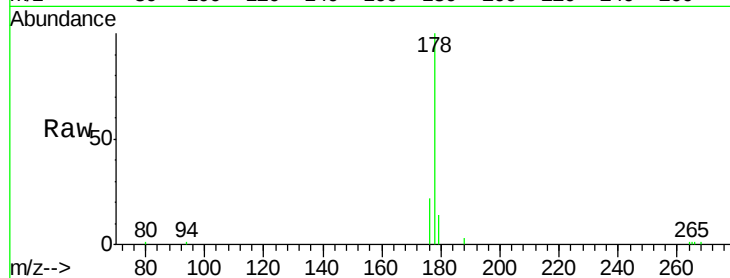

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

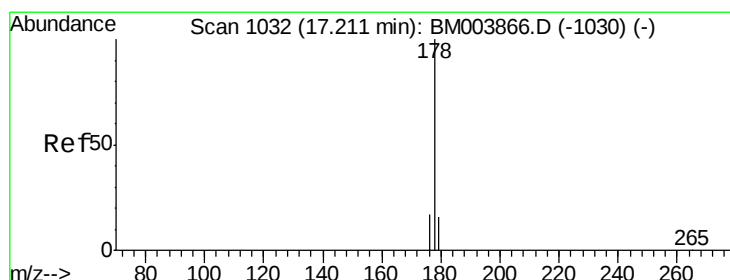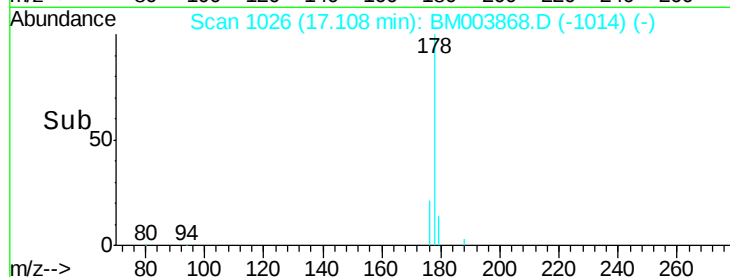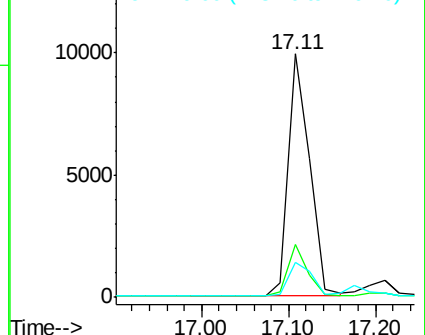

#15

Anthracene

Concen: 0.02 ng/ul

RT: 17.21 min Scan# 1032

Delta R.T. -0.00 min

Lab File: BM003868.D

Acq: 30 Dec 2015 03:33


Tgt Ion:178 Resp: 1379

Ion Ratio Lower Upper

178 100

176 23.9 14.0 21.0#



179 27.4 12.9 19.3#

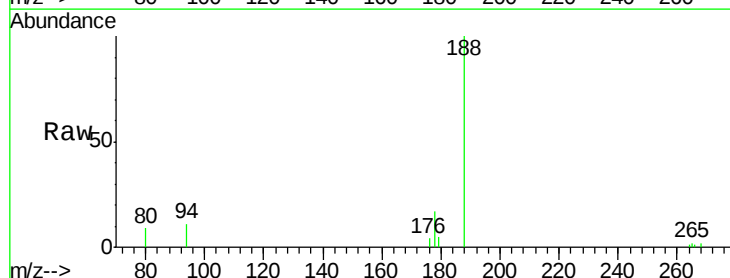


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

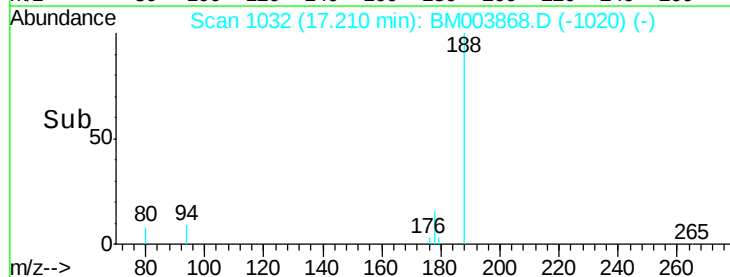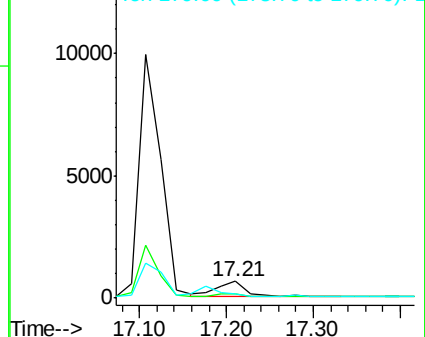


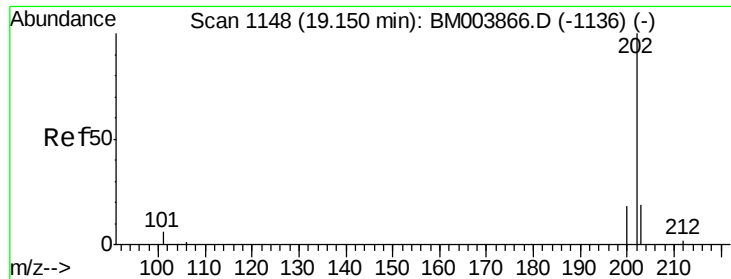




#17
Fluoranthene
Concen: 0.09 ng/ul
RT: 19.14 min Scan# 1148
Delta R.T. -0.01 min
Lab File: BM003868.D
Acq: 30 Dec 2015 03:33

Instrument :
BNA_M
ClientSampleId :
D9N65DL

Tot Ion:202 Resp: 6236
Ion Ratio Lower Upper
202 100
101 9.9 0.0 29.6
203 18.4 0.0 36.3

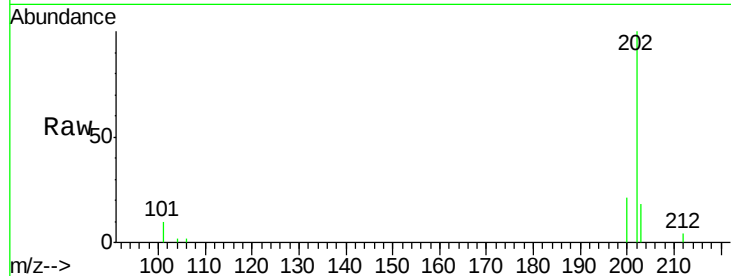


Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 203.00 (202.70 to 203.70): E

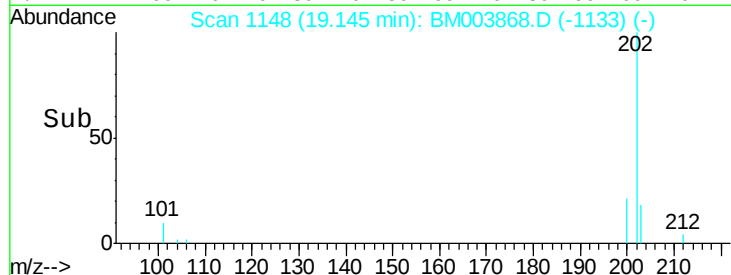
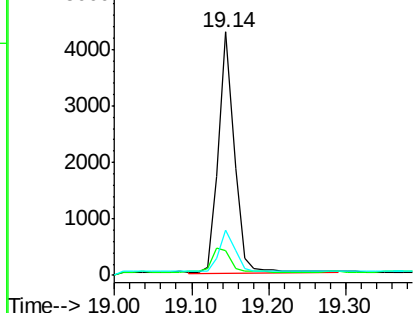



#19
Pyrene
Concen: 0.10 ng/ul
RT: 19.51 min Scan# 1178
Delta R.T. -0.01 min
Lab File: BM003868.D
Acq: 30 Dec 2015 03:33

Tgt Ion:202 Resp: 4977
Ion Ratio Lower Upper
202 100
200 21.4 17.8 26.8
203 20.1 12.8 19.2#



Abundance Ion 202.00 (201.70 to 202.70): E
Ion 200.00 (199.70 to 200.70): E
Ion 203.00 (202.70 to 203.70): E

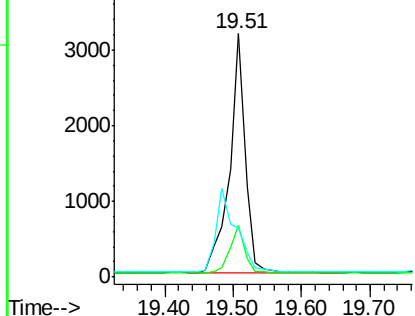

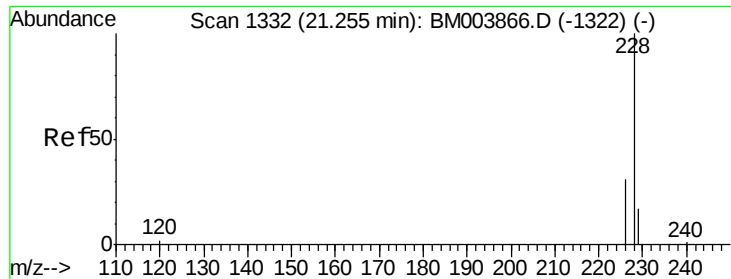

#20

Benzo(a)anthracene

Concen: 0.01 ng/ul

RT: 21.26 min Scan# 1333

Delta R.T. 0.01 min

Lab File: BM003868.D

Acq: 30 Dec 2015 03:33

Instrument :

BNA_M

ClientSampleId :

D9N65DL


Tot Ion:228 Resp: 654

Ion Ratio Lower Upper




228 100

226 36.4 18.8 28.2#

229 30.0 17.1 25.7#



Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

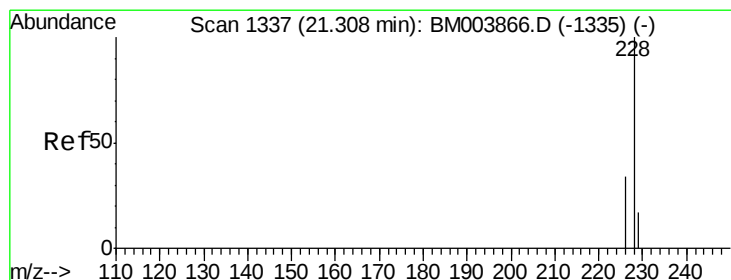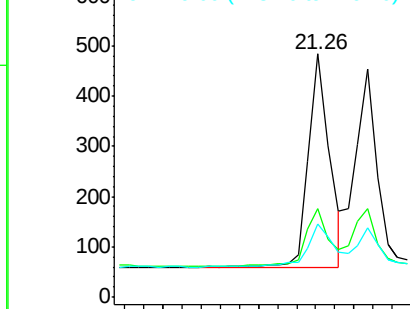

#21

Chrysene

Concen: 0.01 ng/ul

RT: 21.31 min Scan# 1338

Delta R.T. 0.01 min

Lab File: BM003868.D

Acq: 30 Dec 2015 03:33


Tgt Ion:228 Resp: 625

Ion Ratio Lower Upper



228 100


226 38.9 21.2 31.8#

229 30.5 17.0 25.6#



Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

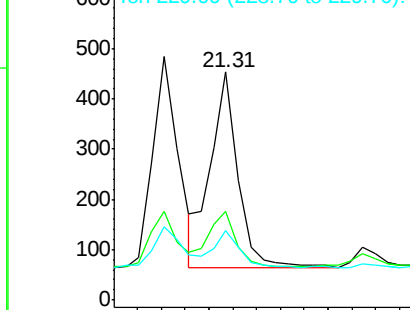

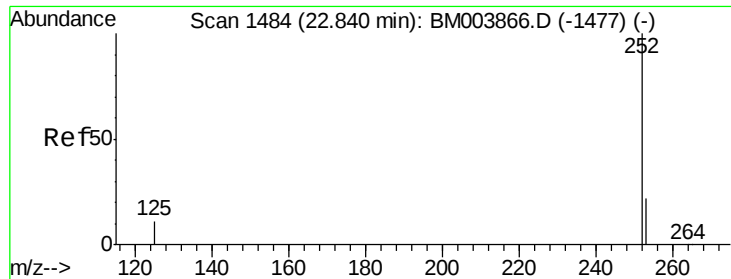

#23

Benzo(b)fluoranthene

Concen: 0.01 ng/ul

RT: 22.85 min Scan# 1485

Delta R.T. 0.01 min

Lab File: BM003868.D

Acq: 30 Dec 2015 03:33

Instrument :

BNA_M

ClientSampleId :

D9N65DL


Tot Ion:252 Resp: 584

Ion Ratio Lower Upper

252 100

253 99.3 0.0 45.4#



125 66.0 0.0 28.8#



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

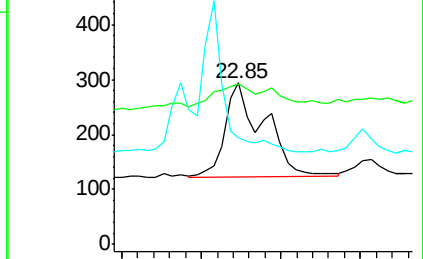

#24

Benzo(k)fluoranthene

Concen: 0.01 ng/ul

RT: 22.85 min Scan# 1485

Delta R.T. -0.03 min

Lab File: BM003868.D

Acq: 30 Dec 2015 03:33



Tgt Ion:252 Resp: 579

Ion Ratio Lower Upper

252 100

253 99.3 19.8 29.8#



125 66.0 10.4 15.6#




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

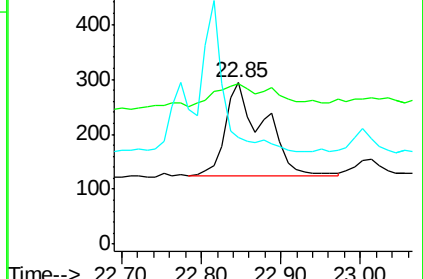

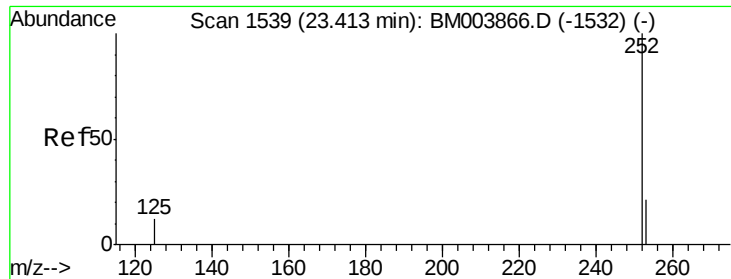

#25

Benzo(a)pyrene

Concen: 0.03 ng/ul

RT: 23.37 min Scan# 1535

Delta R.T. -0.05 min

Lab File: BM003868.D

Acq: 30 Dec 2015 03:33

Instrument :

BNA_M

ClientSampleId :

D9N65DL


Tot Ion:252 Resp: 1392

Ion Ratio Lower Upper

252 100

253 61.6 19.4 29.2#




125 83.7 12.7 19.1#

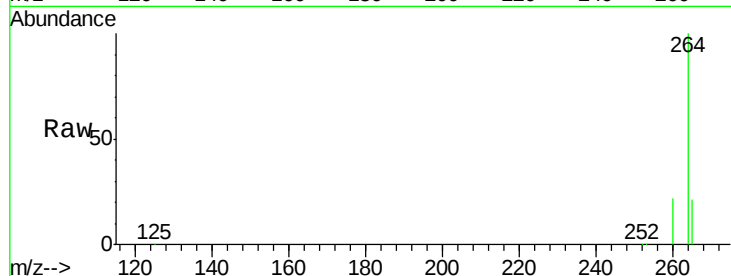

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

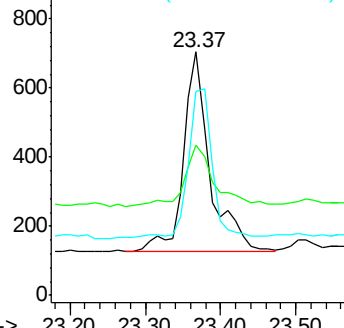

#26

Indeno(1,2,3-cd)pyrene

Concen: 0.00 ng/ul

RT: 25.78 min Scan# 1766

Delta R.T. 0.01 min

Lab File: BM003868.D

Acq: 30 Dec 2015 03:33


Tgt Ion:276 Resp: 159

Ion Ratio Lower Upper

276 100

138 38.4 16.3 24.5#



277 32.7 19.8 29.8#




Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

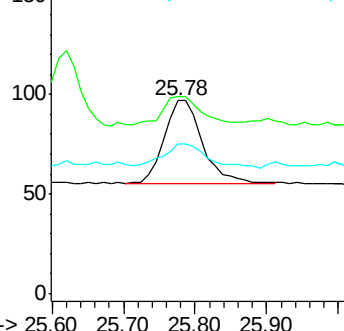


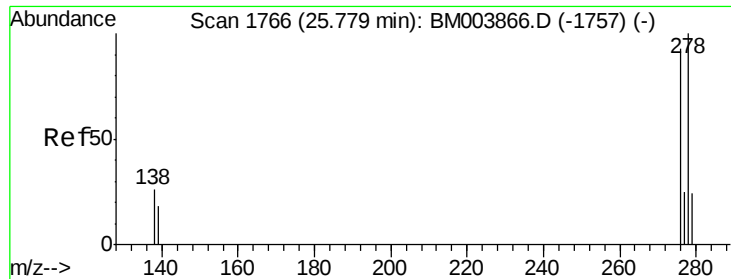




#27
Dibenzo(a,h)anthracene
Concen: 0.00 ng/ul
RT: 25.79 min Scan# 1767
Delta R.T. 0.01 min
Lab File: BM003868.D
Acq: 30 Dec 2015 03:33

Instrument :
BNA_M
ClientSampleId :
D9N65DL

Tot Ion:278 Resp: 128
Ion Ratio Lower Upper
278 100
139 108.8 16.4 24.6#
279 136.3 20.2 30.2#

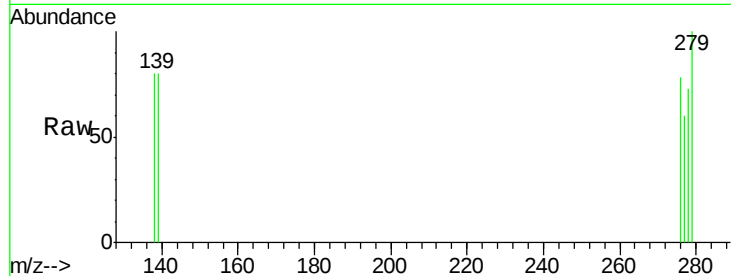


Abundance Ion 278.00 (277.70 to 278.70): E
Ion 139.00 (138.70 to 139.70): E
Ion 279.00 (278.70 to 279.70): E

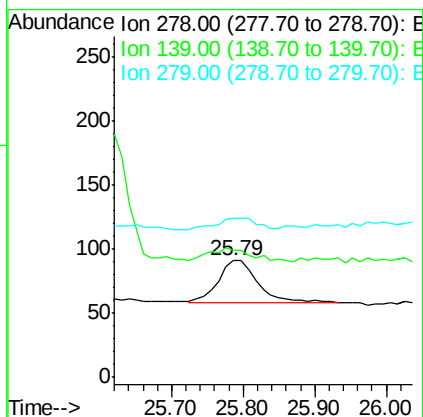

#28
Benzo(g,h,i)perylene
Concen: 0.00 ng/ul
RT: 26.46 min Scan# 1832
Delta R.T. 0.01 min
Lab File: BM003868.D
Acq: 30 Dec 2015 03:33

Tgt Ion:276 Resp: 154
Ion Ratio Lower Upper
276 100
277 81.3 18.9 28.3#
138 106.6 22.5 33.7#



Abundance Ion 276.00 (275.70 to 276.70): E
Ion 277.00 (276.70 to 277.70): E
Ion 138.00 (137.70 to 138.70): E

