
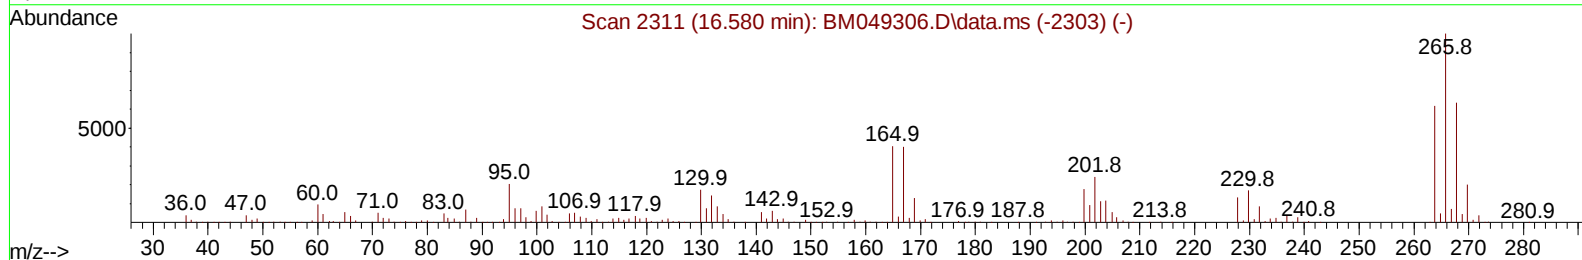
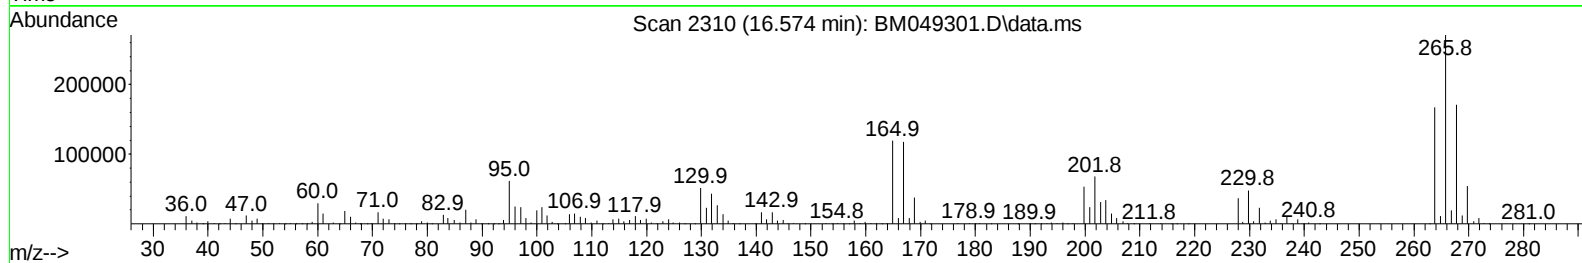


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM123124\  
Data File : BM049301.D  
Acq On : 31 Dec 2024 12:35  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 31 23:13:29 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM123124.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Dec 31 23:06:33 2024  
Response via : Initial Calibration

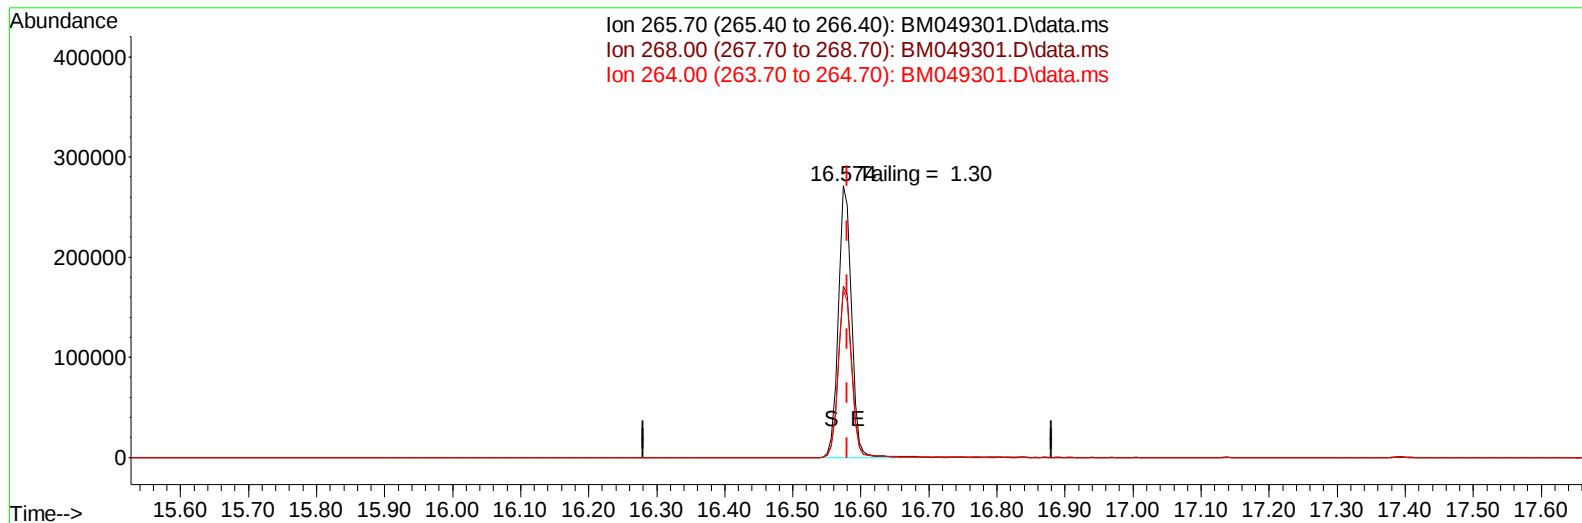

TIC: BM049301.D\data.ms

**(70) Pentachlorophenol (C)**




**16.574min (-0.006) 48731.47 ng**

**response 364867**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.50  | 63.08  |
| 264.00 | 61.60  | 61.69  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM123124\  
Data File : BM049301.D  
Acq On : 31 Dec 2024 12:35  
Operator : RC/JU  
Sample : DFTTP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 31 23:13:29 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM123124.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Dec 31 23:06:33 2024  
Response via : Initial Calibration

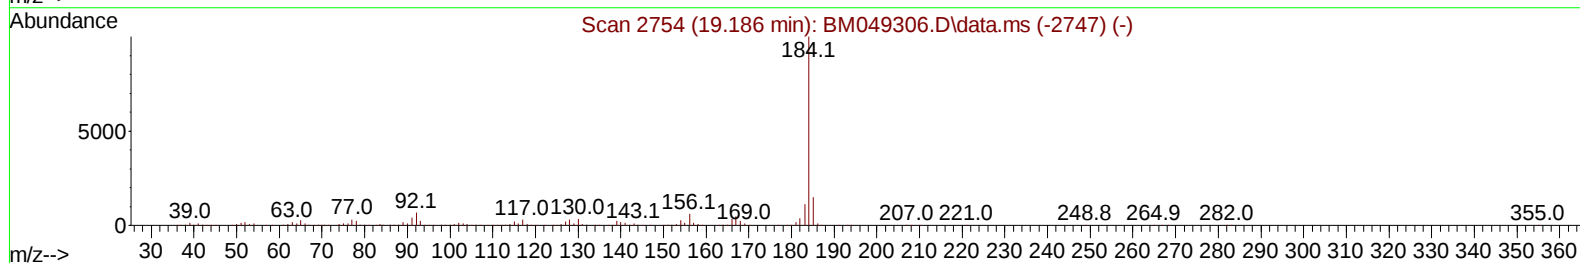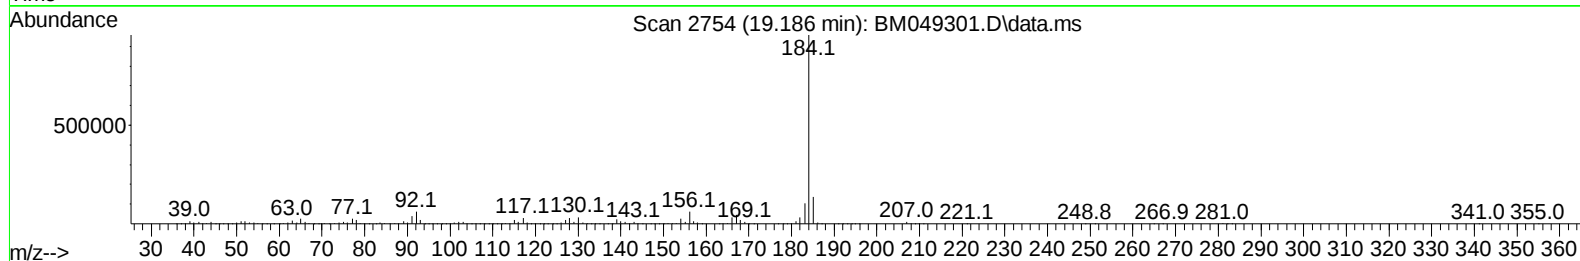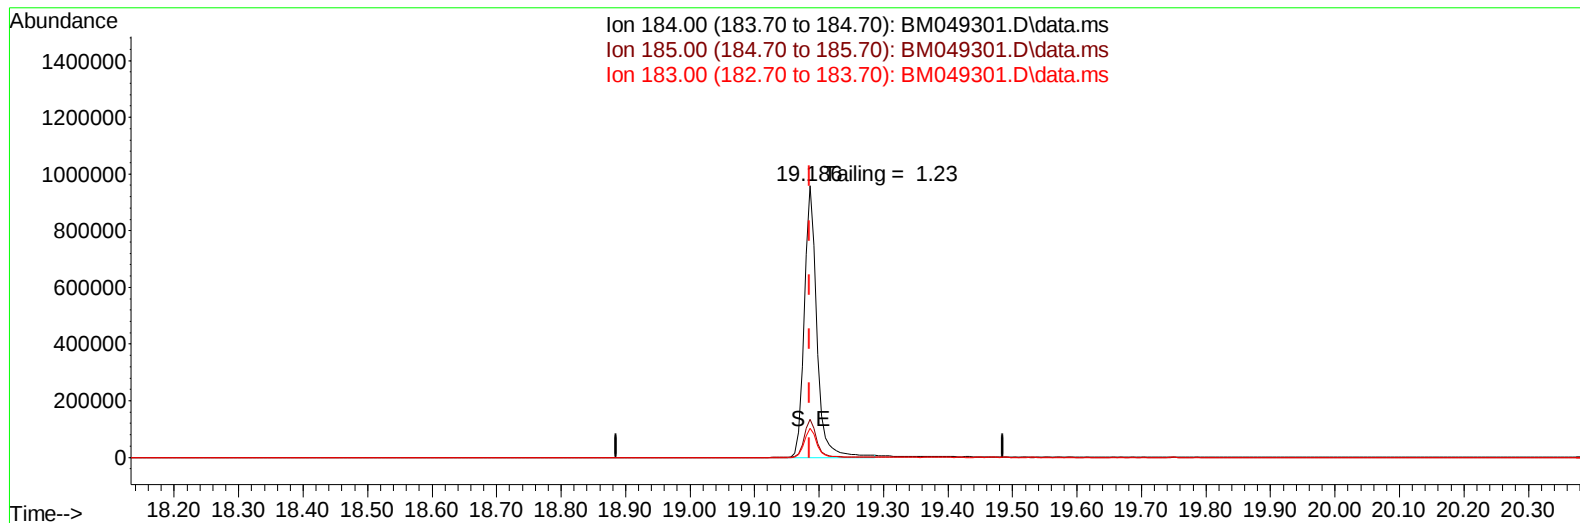

TIC: BM049301.D\data.ms

**(77) Benzidine****19.186min (+ 0.000) 103944.99 ng****response 1307681**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.00  | 14.13  |
| 183.00 | 11.10  | 10.86  |
| 0.00   | 0.00   | 0.00   |