
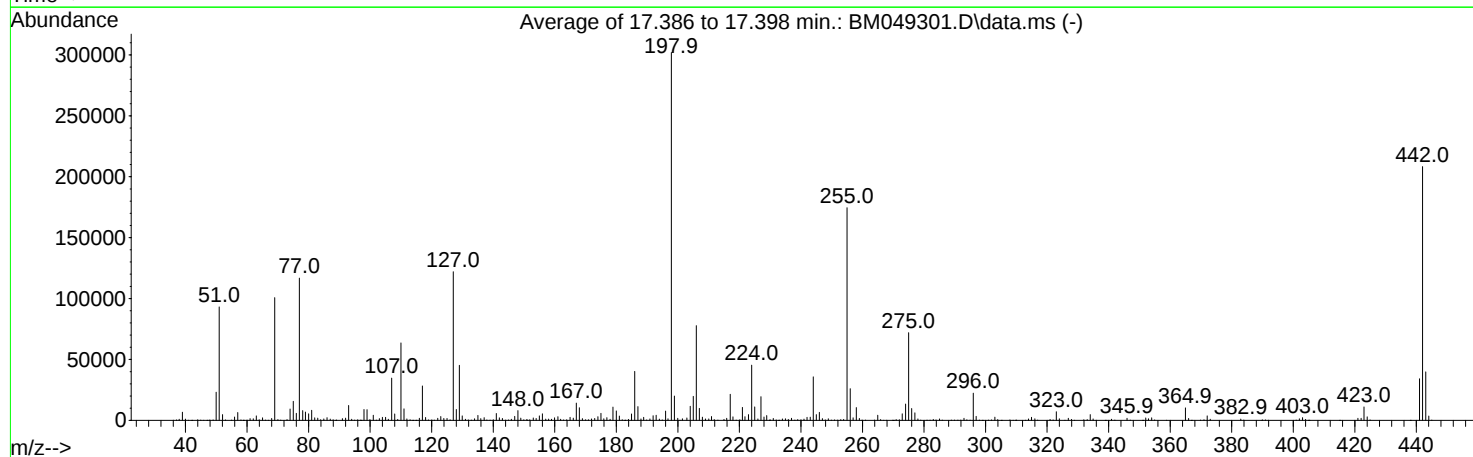


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM123124\
Data File : BM049301.D
Acq On : 31 Dec 2024 12:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM123124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Dec 31 23:06:33 2024

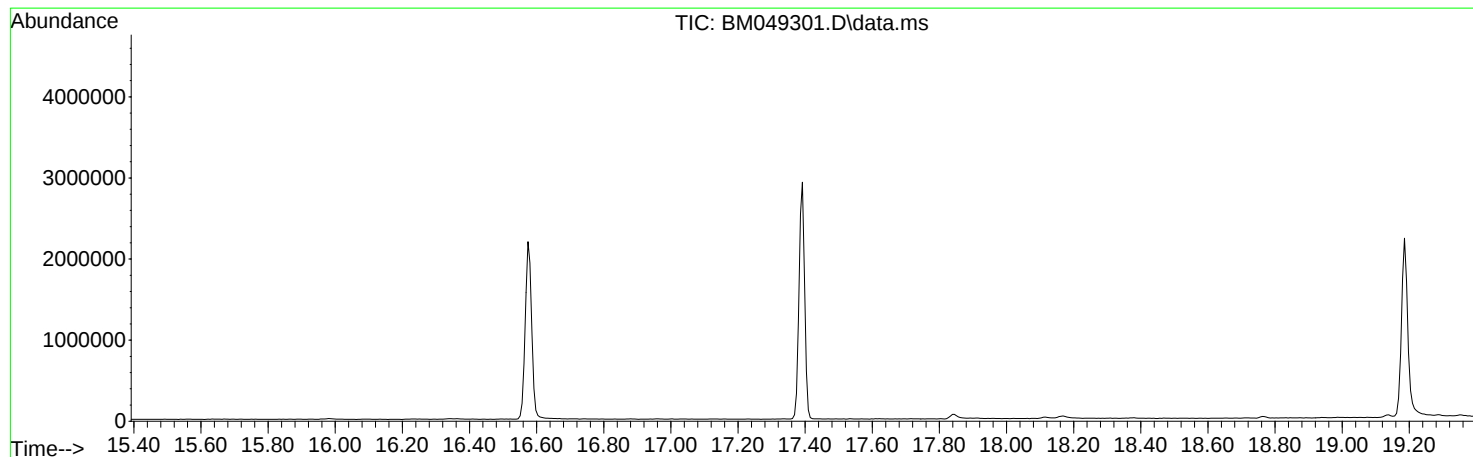

AutoFind: Scans 2448, 2449, 2450; Background Corrected with Scan 2441

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.9	93192	PASS
68	69	0.00	2	1.6	1617	PASS
69	198	0.00	100	33.4	100806	PASS
70	69	0.00	2	0.7	684	PASS
127	198	10	80	40.4	122051	PASS
197	198	0.00	2	0.4	1313	PASS
198	198	100	100	100.0	301995	PASS
199	198	5	9	6.6	20002	PASS
275	198	10	60	23.8	72016	PASS
365	198	1	100	3.4	10257	PASS
441	198	0.01	100	11.3	34165	PASS
442	442	50	100	100.0	208363	PASS
443	442	15	24	19.1	39843	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/31/2024	BNA_M	<u>BM049301.D</u>
Compound Name	Response	Retention Time
DDT	1002677	20.433
DDD	11779	20.039
DDE	299	19.474
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12078	1014755	1.19

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM123124\
Data File : BM049301.D
Acq On : 31 Dec 2024 12:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Dec 31 23:13:29 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM123124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 31 23:06:33 2024
Response via : Initial Calibration

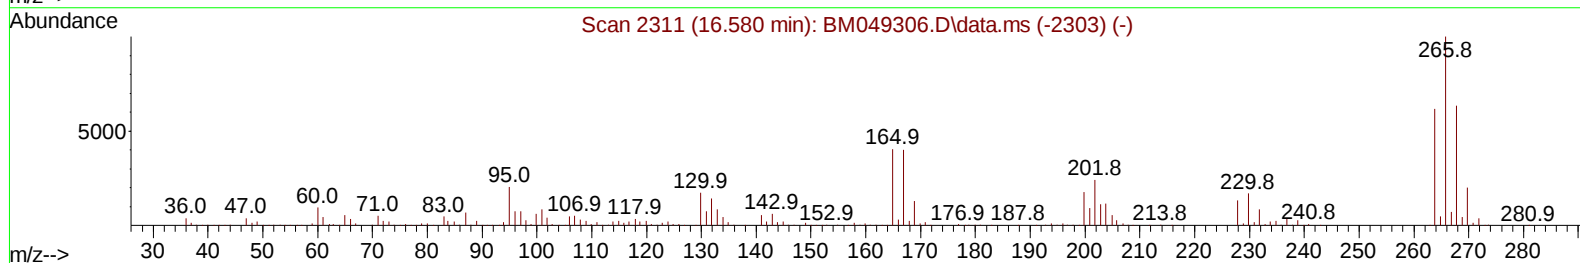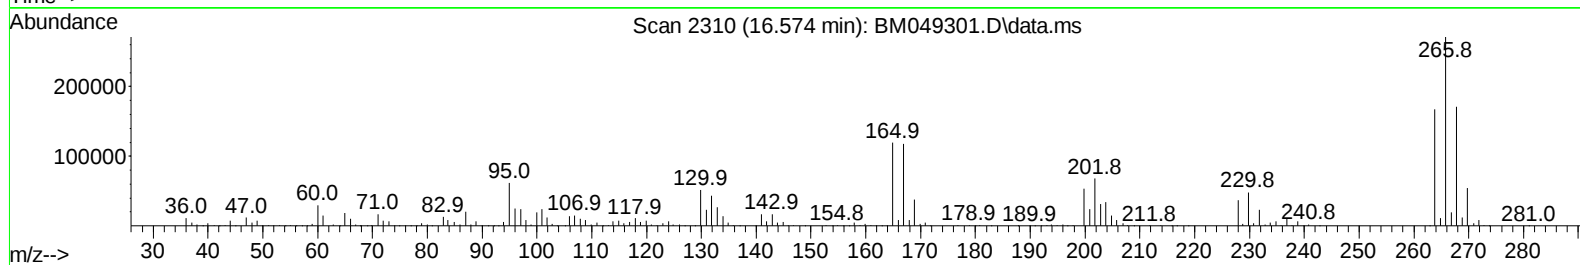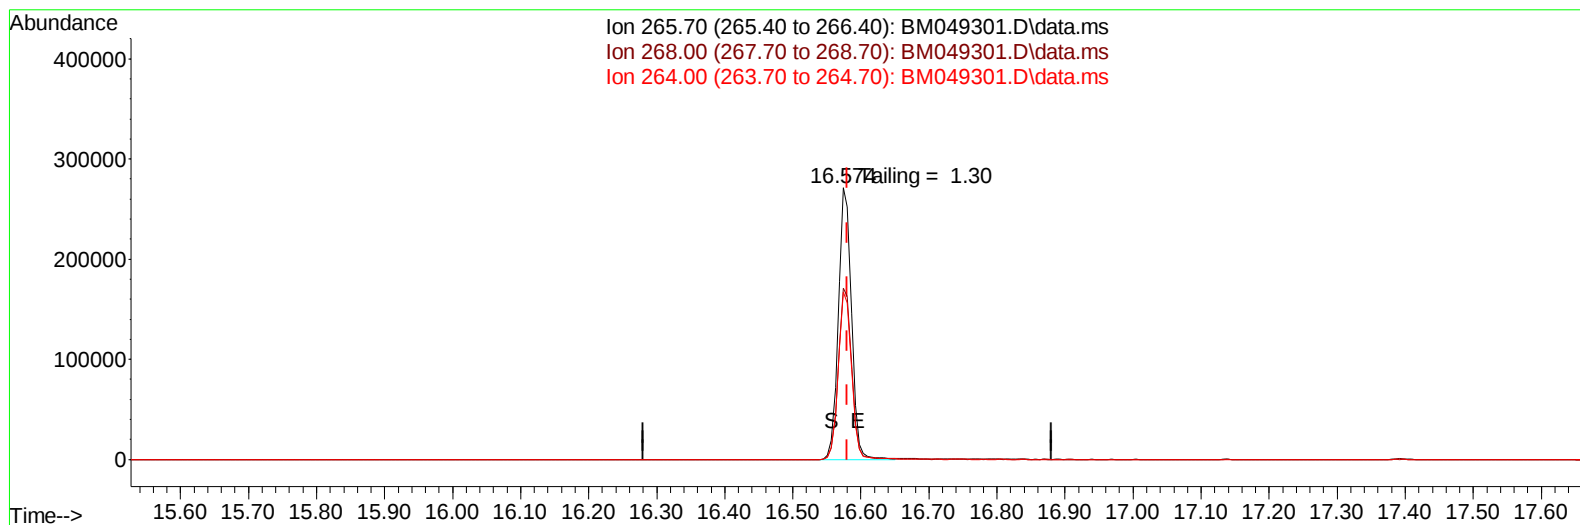

TIC: BM049301.D\data.ms

(70) Pentachlorophenol (C)

16.574min (-0.006) 48731.47 ng




response 364867

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.50	63.08
264.00	61.60	61.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM123124\
Data File : BM049301.D
Acq On : 31 Dec 2024 12:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Dec 31 23:13:29 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM123124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 31 23:06:33 2024
Response via : Initial Calibration

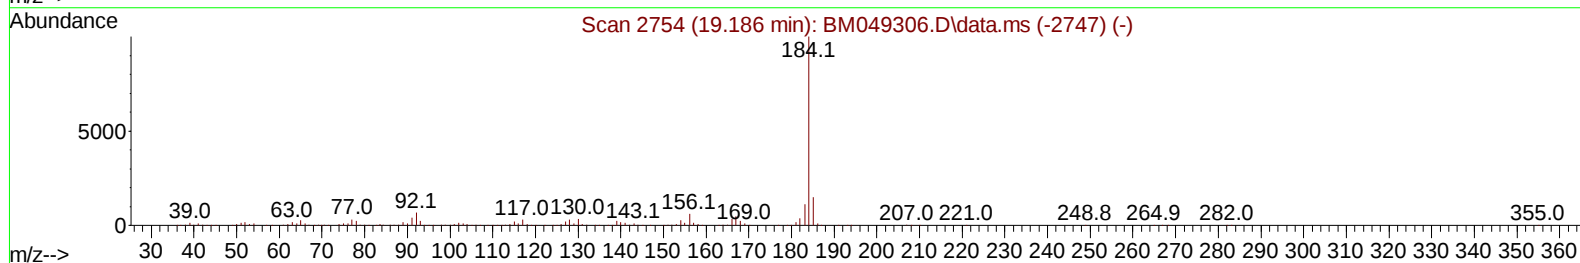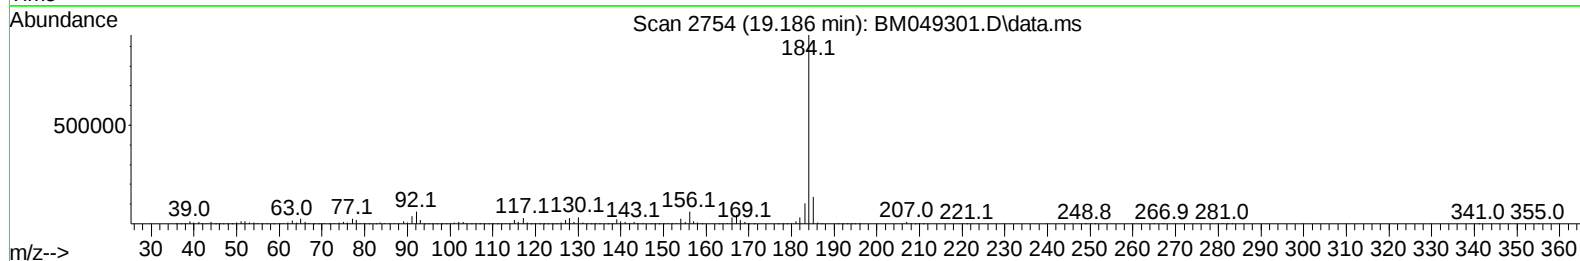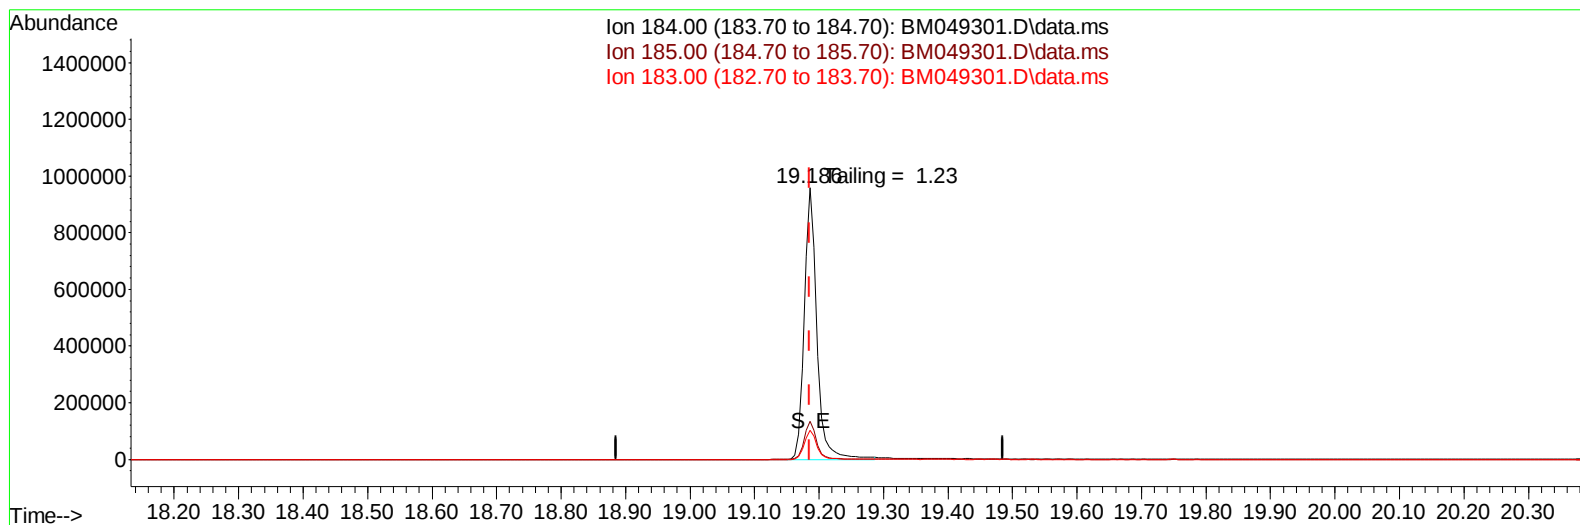

TIC: BM049301.D\data.ms

(77) Benzidine

19.186min (+ 0.000) 103944.99 ng

response 1307681

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.13
183.00	11.10	10.86
0.00	0.00	0.00