



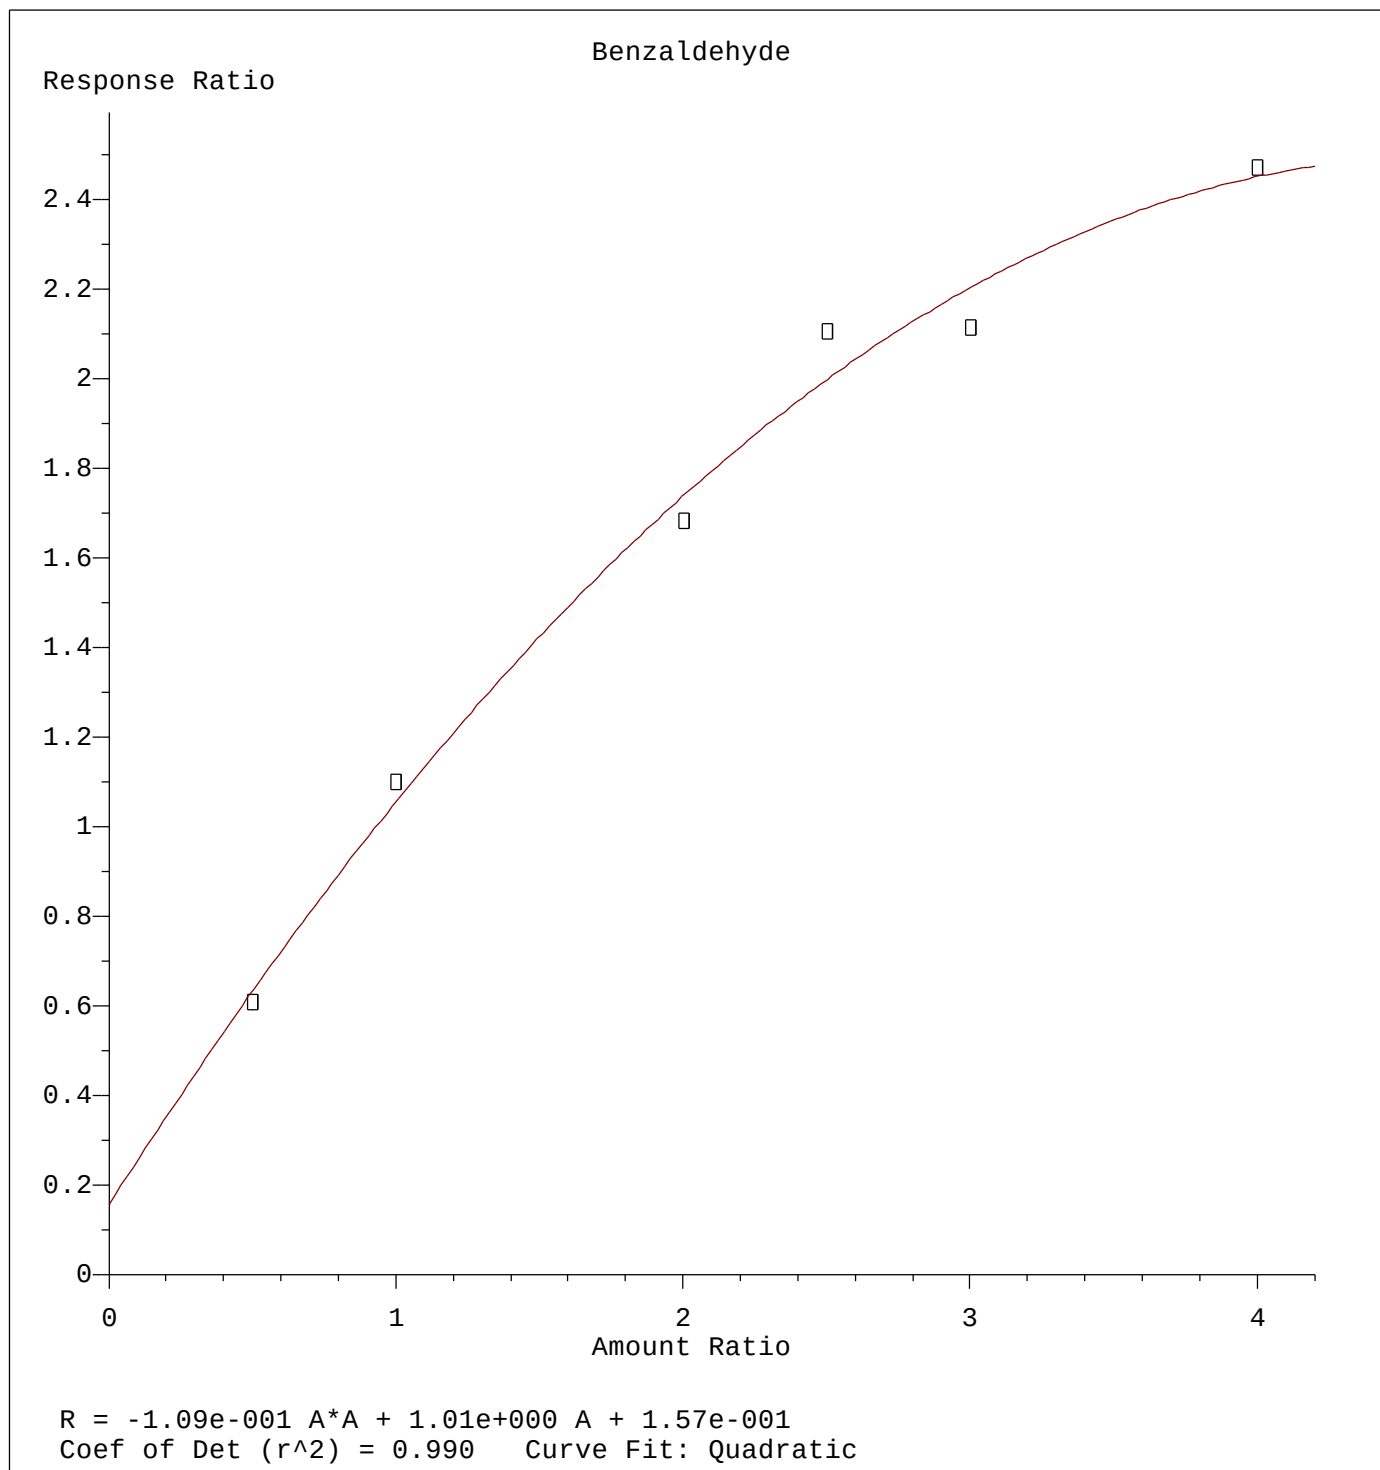


Method Name: Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP010320.M
Calibration Table Last Updated: Fri Jan 03 15:57:46 2020

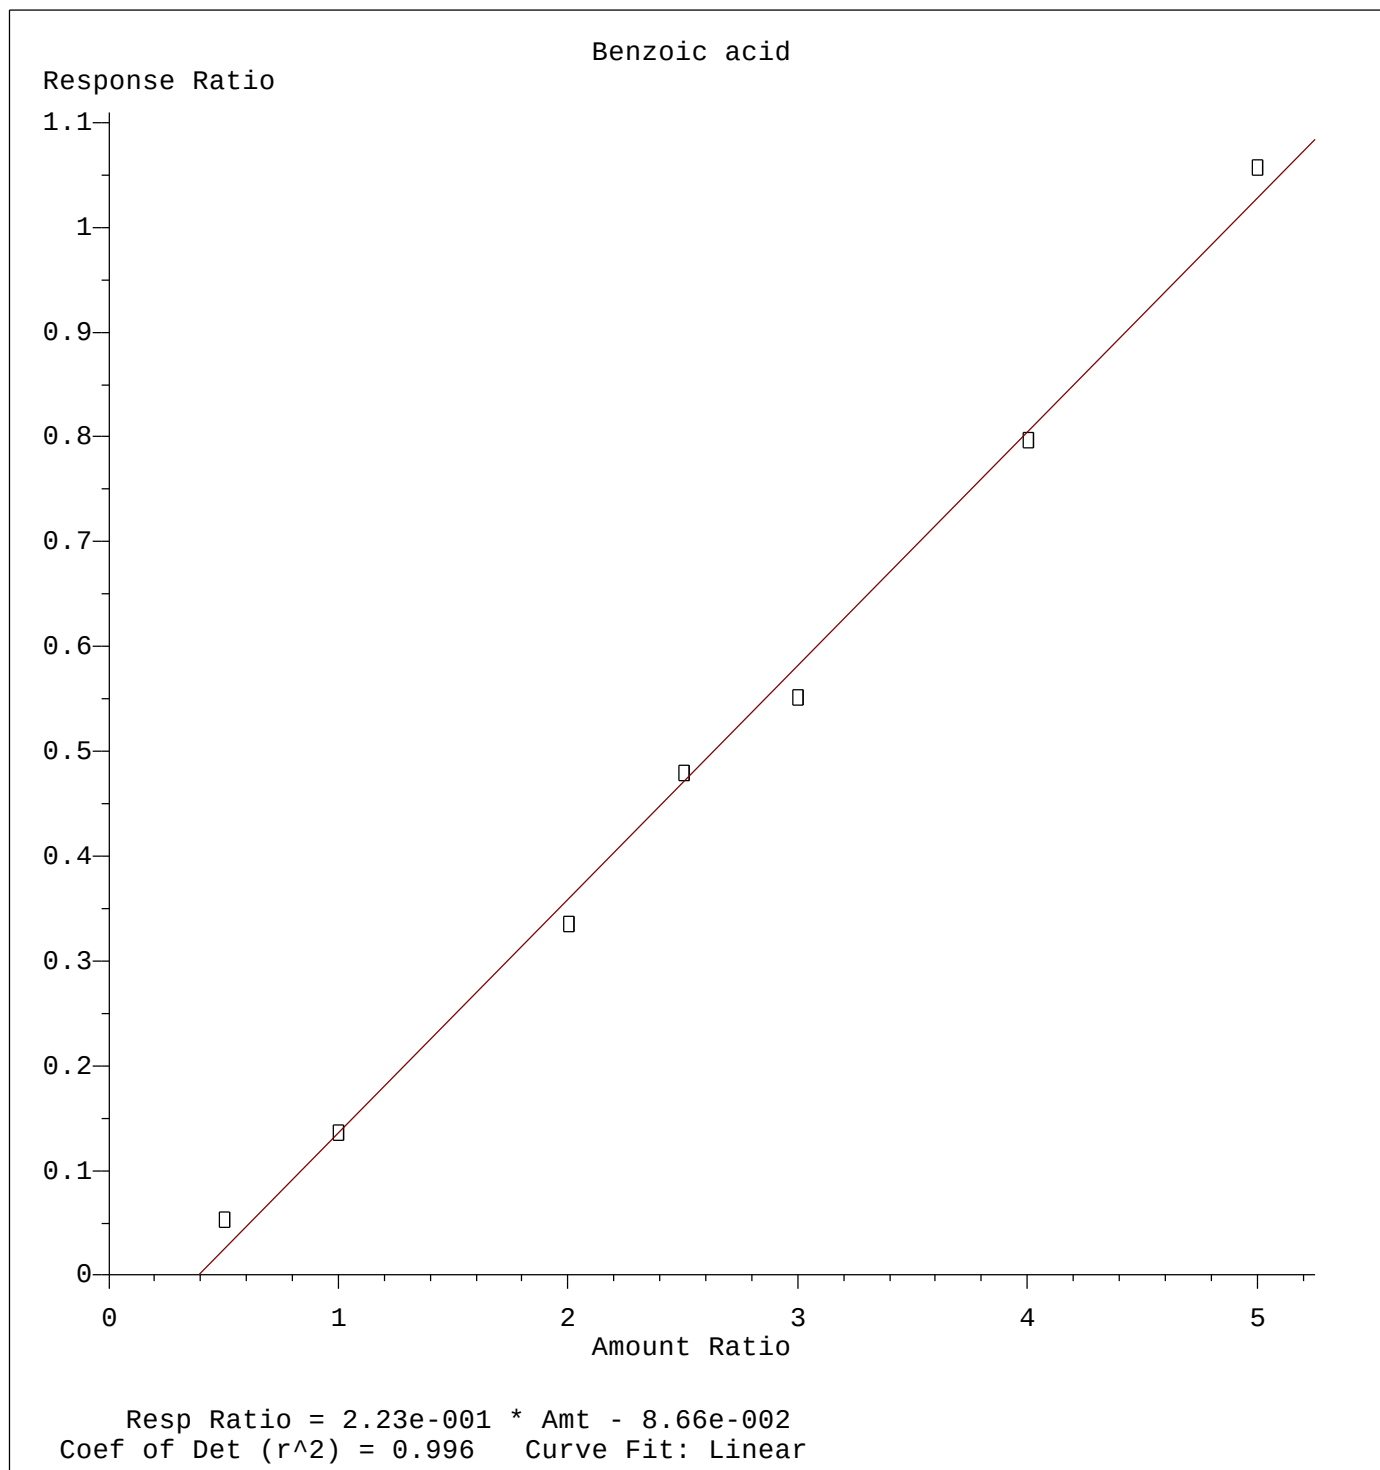

Method Name: Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP010320.M
Calibration Table Last Updated: Fri Jan 03 15:57:46 2020

2,4-Dinitrophenol


Response Ratio

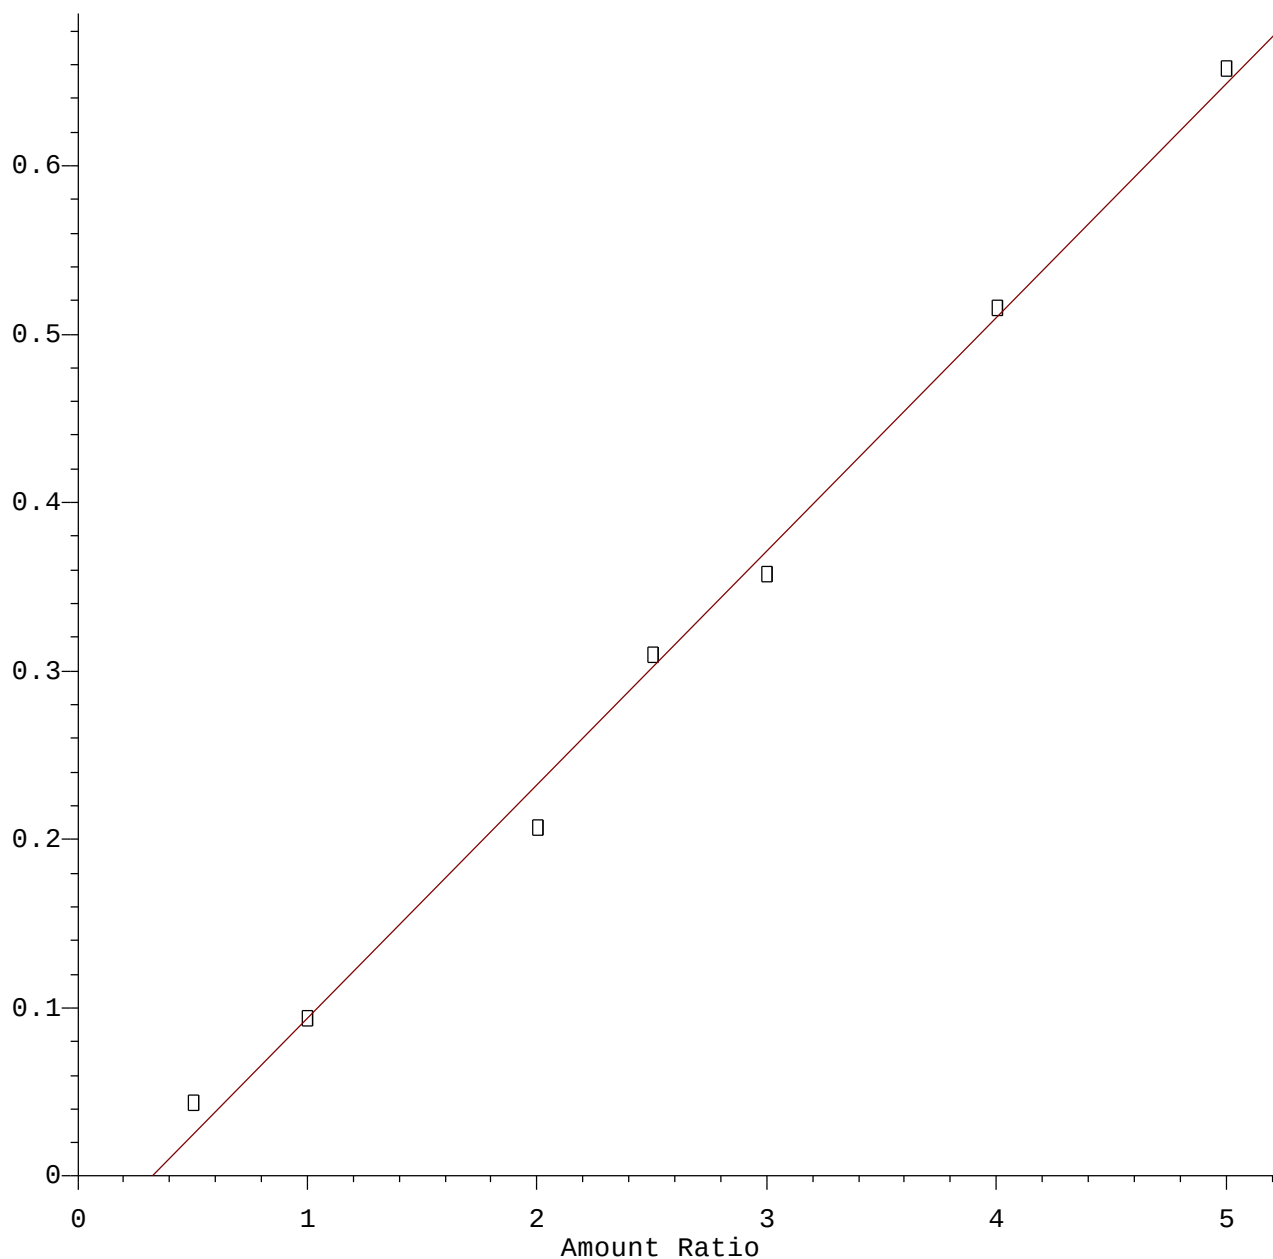

Resp Ratio = $1.39 \times 10^{-1} \times \text{Amt} - 4.47 \times 10^{-2}$
Coef of Det (r^2) = 0.995 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP010320.M
Calibration Table Last Updated: Fri Jan 03 15:57:46 2020

4,6-Dinitro-2-methylphenol

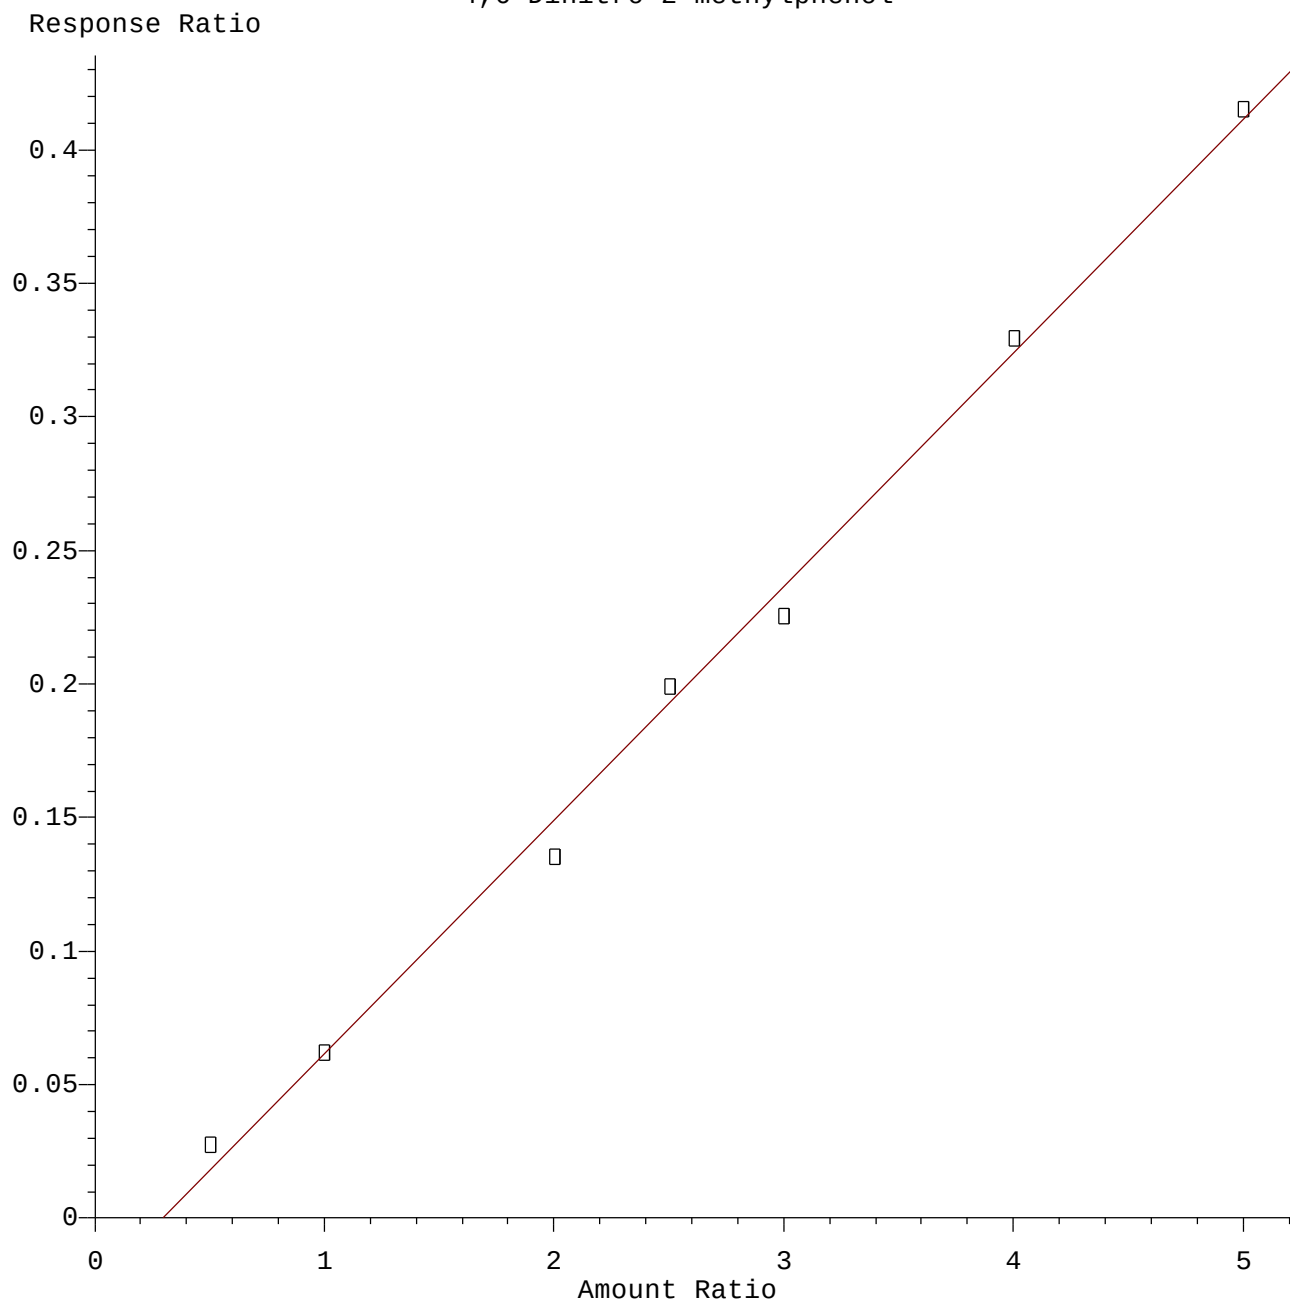

Resp Ratio = $8.73 \times 10^{-2} \times \text{Amt} - 2.56 \times 10^{-2}$
Coef of Det (r^2) = 0.996 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP010320.M
Calibration Table Last Updated: Fri Jan 03 15:57:46 2020