
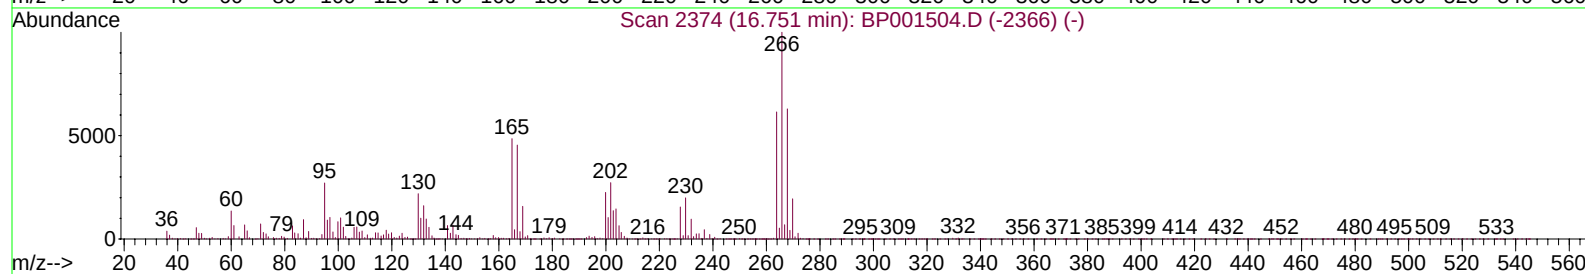
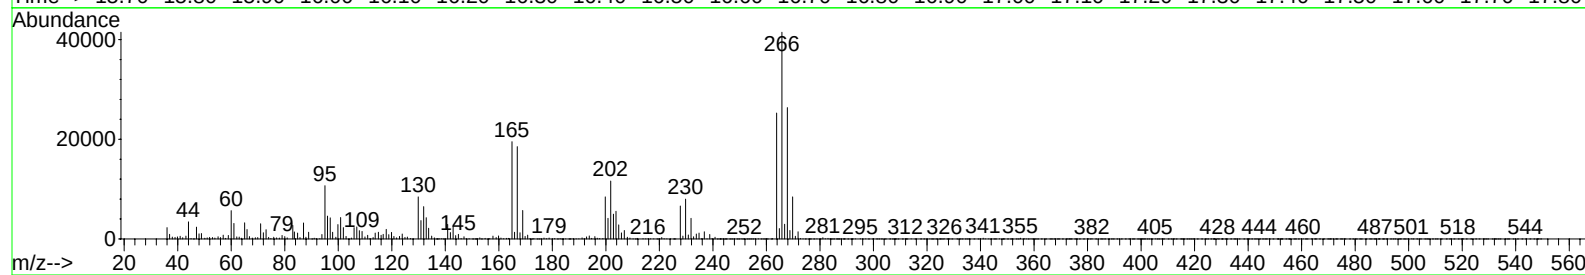


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP010320\
 Data File : BP001501.D
 Acq On : 03 Jan 2020 11:02
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 03 17:13:18 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP010320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 03 15:57:46 2020
 Response via : Initial Calibration

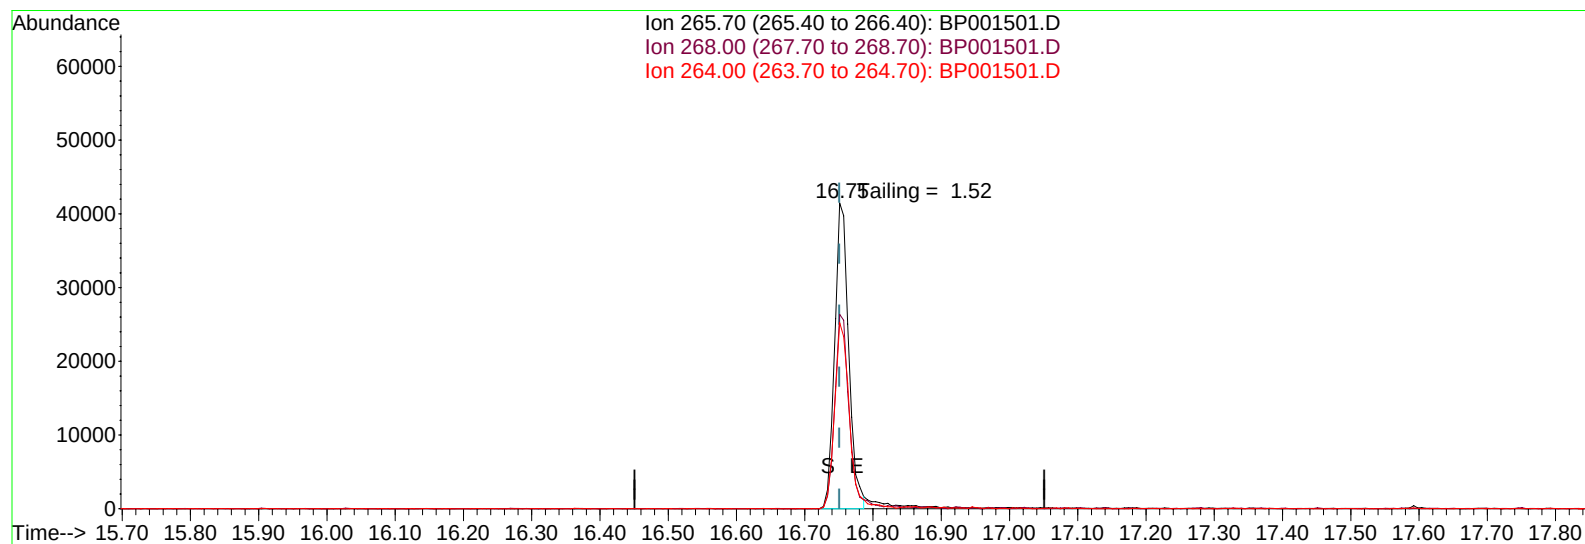

TIC: BP001501.D

(70) Pentachlorophenol (C)




16.751min (+0.000) 481322.15ng

response 61705

Ion	Exp%	Act%
265.70	100	100
268.00	62.90	63.56
264.00	61.50	60.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP010320\
 Data File : BP001501.D
 Acq On : 03 Jan 2020 11:02
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 03 17:13:18 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP010320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 03 15:57:46 2020
 Response via : Initial Calibration

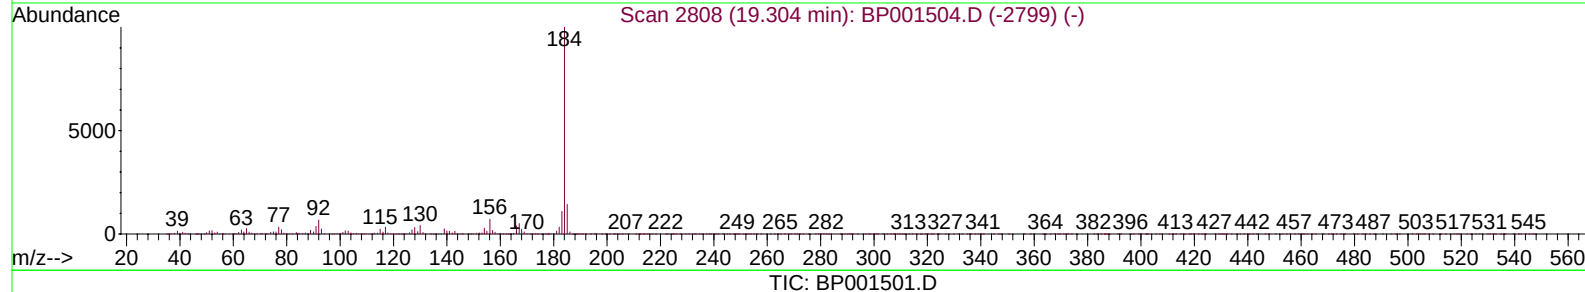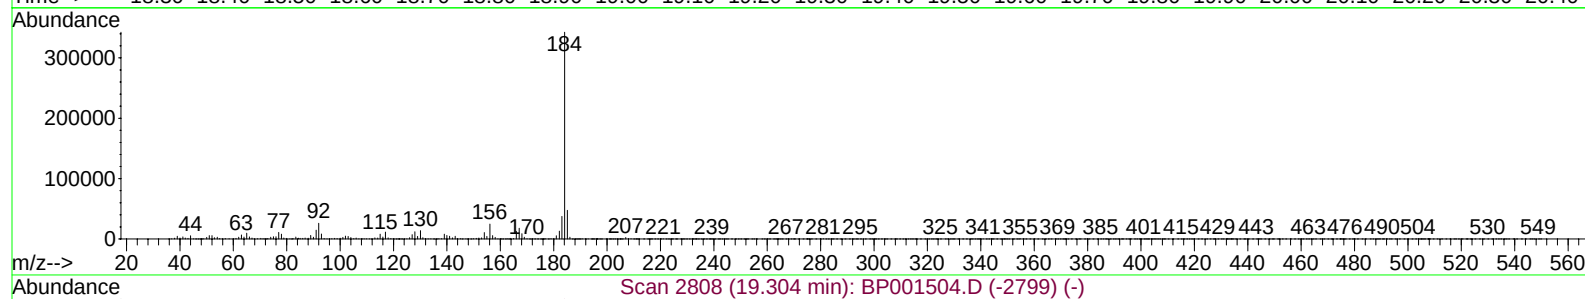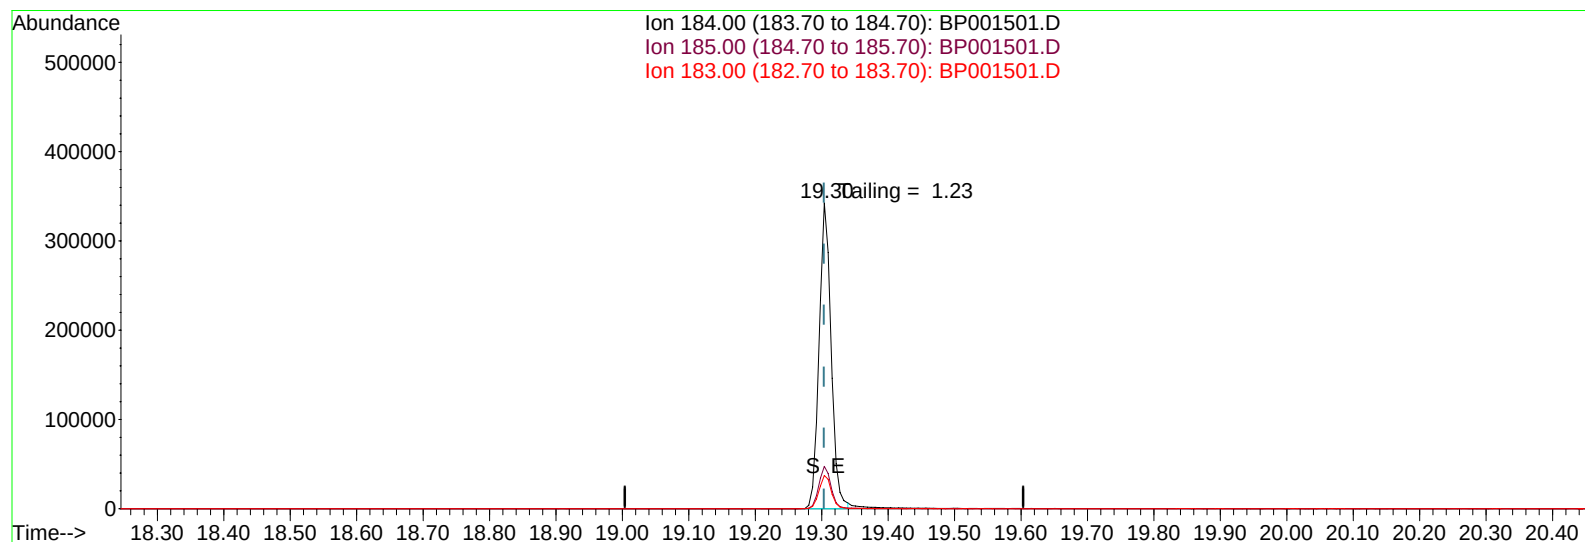

(77) Benzidine

19.304min (+0.000) 2404437.11ng

response 439830

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	13.85
183.00	10.90	10.89
0.00	0.00	0.00