
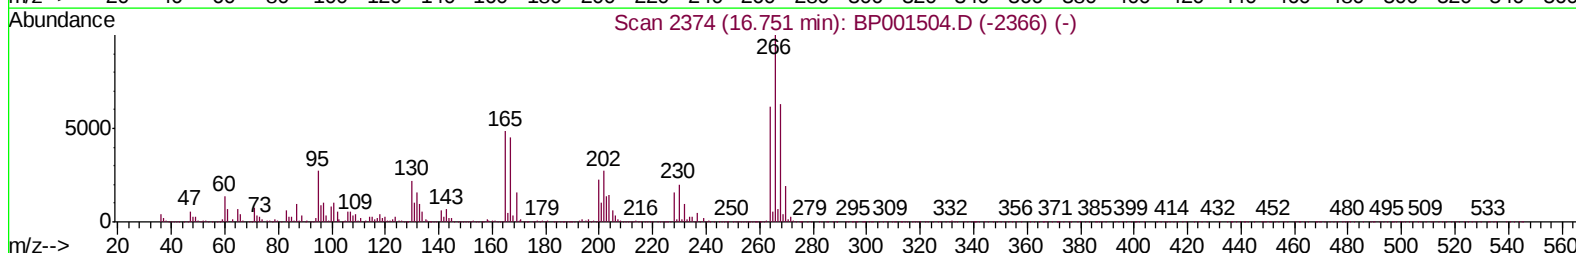
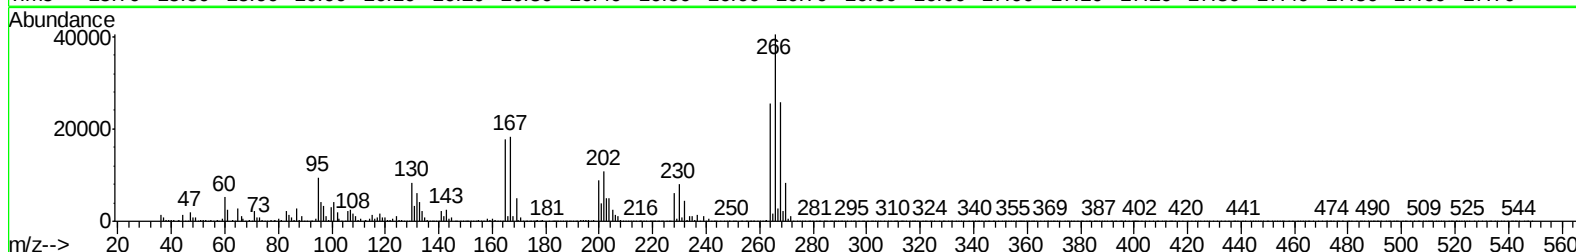


Data File : BP001510.D
Acq On : 03 Jan 2020 16:30
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 04 04:15:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP010320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 03 15:57:46 2020
Response via : Initial Calibration

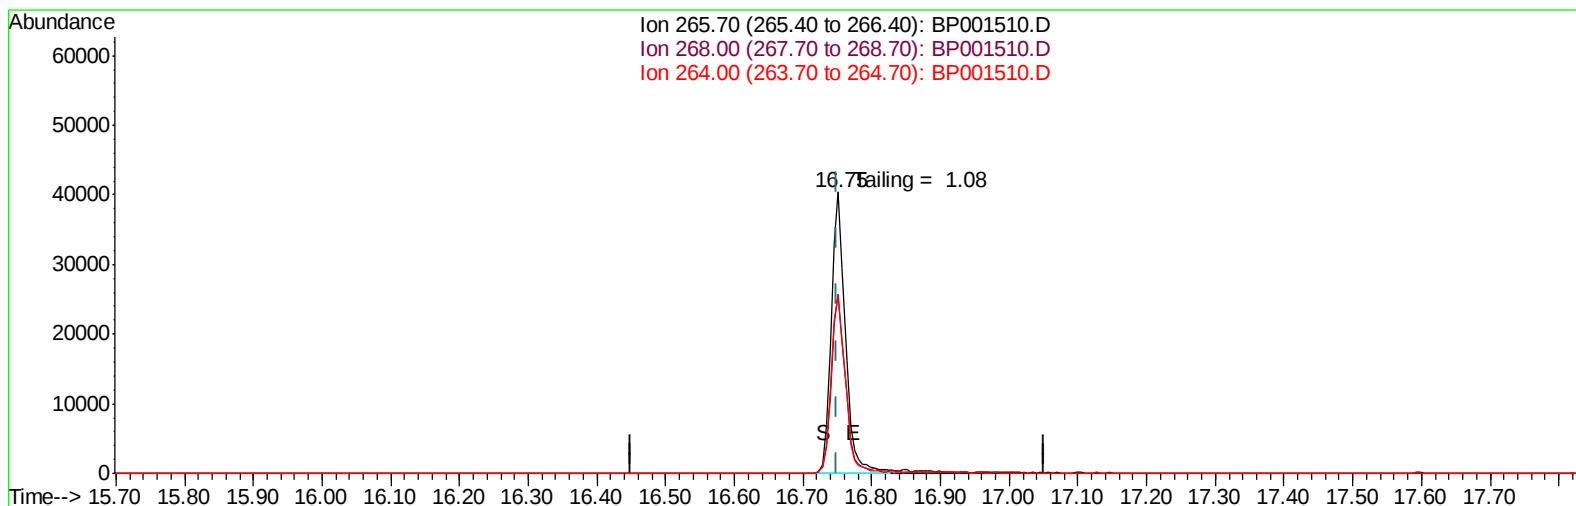

TIC: BP001510.D

(70) Pentachlorophenol (C)




16.751min (+0.000) 695073.43ng

response 57920

Ion	Exp%	Act%
265.70	100	100
268.00	62.90	63.64
264.00	61.50	63.26
0.00	0.00	0.00

Data File : BP001510.D
Acq On : 03 Jan 2020 16:30
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 04 04:15:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP010320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 03 15:57:46 2020
Response via : Initial Calibration

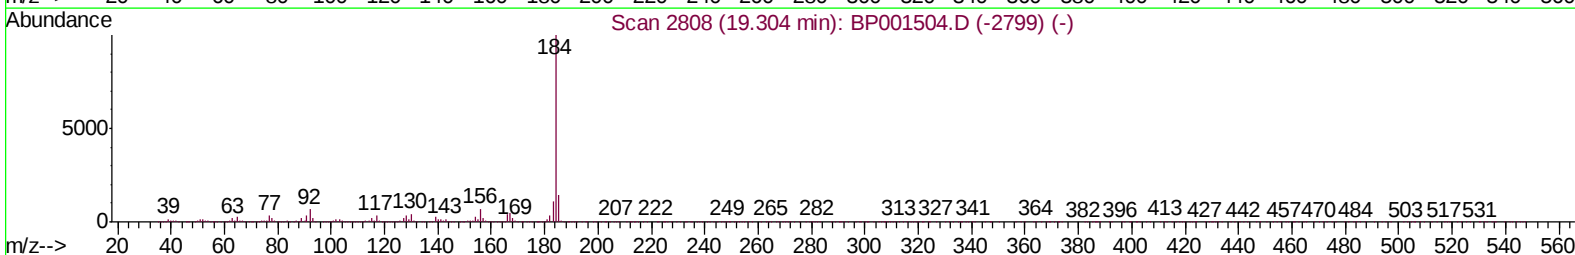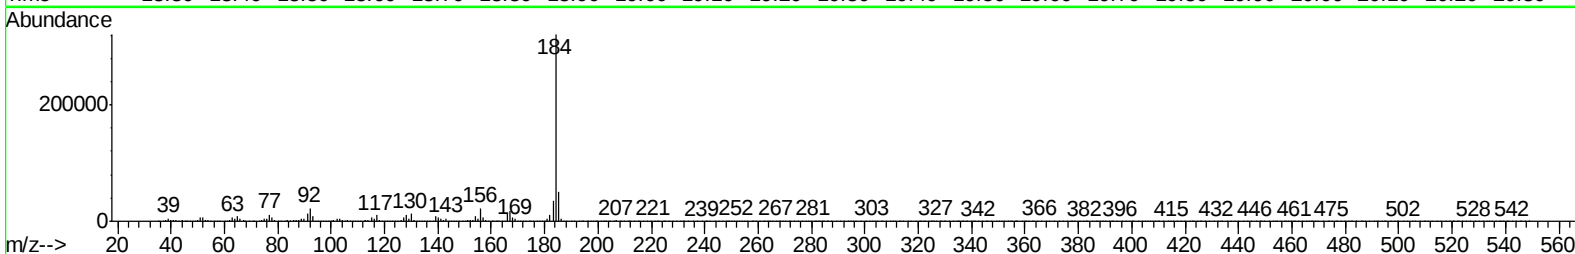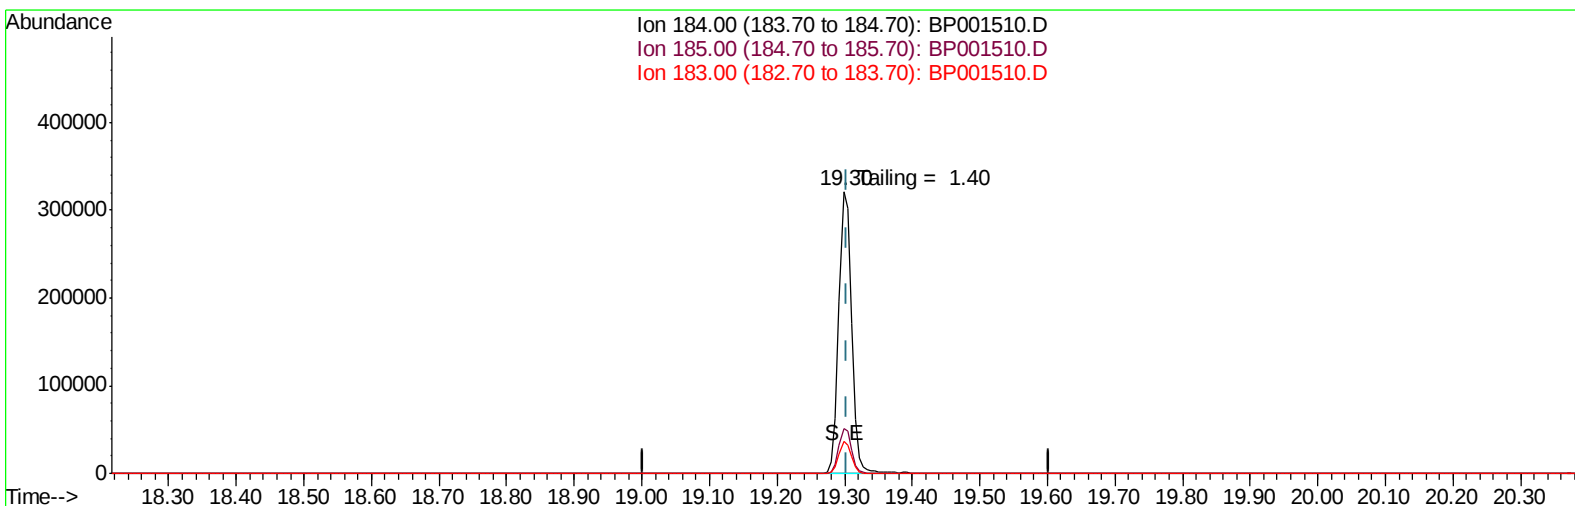

TIC: BP001510.D

(77) Benzidine

19.298min (-0.005) 1387856.08ng

response 412543

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	16.08
183.00	10.90	11.26
0.00	0.00	0.00