


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP010320\
 Data File : BP001501.D
 Acq On : 03 Jan 2020 11:02
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP010320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 03 15:57:46 2020

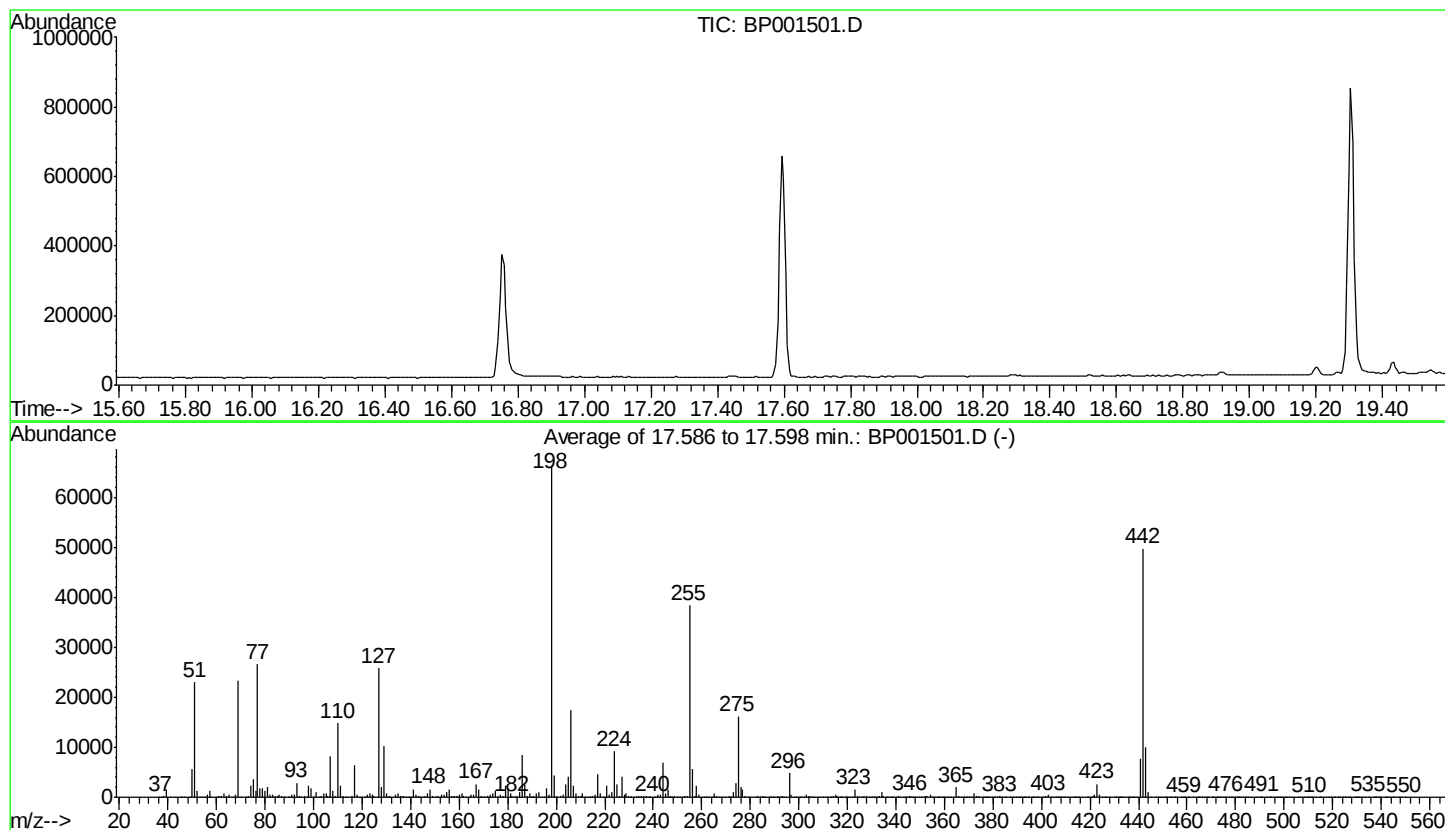

AutoFind: Scans 2516, 2517, 2518; Background Corrected with Scan 2507

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.6	22949	PASS
68	69	0.00	2	1.7	397	PASS
69	198	0.00	100	35.2	23375	PASS
70	69	0.00	2	0.4	88	PASS
127	198	10	80	38.9	25819	PASS
197	198	0.00	2	0.6	396	PASS
198	198	100	100	100.0	66322	PASS
199	198	5	9	6.7	4412	PASS
275	198	10	60	24.2	16031	PASS
365	198	1	100	3.0	1965	PASS
441	198	0.01	100	11.6	7714	PASS
442	198	50	100	75.0	49760	PASS
443	442	15	24	20.3	10080	PASS