

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010323\
 Data File : BP013376.D
 Acq On : 03 Jan 2023 12:20
 Operator : CG/JU
 Sample : PB149944BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK944

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013376.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.323	19	23	29	rVB	117713	159678	1.18%	0.121%
2	3.746	92	95	124	rBV	1601546	2575014	19.07%	1.946%
3	4.075	147	151	156	rVB	30294	43418	0.32%	0.033%
4	7.093	657	664	676	rBV	1831641	2883592	21.36%	2.179%
5	7.258	684	692	701	rBV	1599116	2385258	17.67%	1.802%
6	7.458	719	726	735	rBV	1921720	2940726	21.78%	2.222%
7	7.928	799	806	814	rBV	1756852	2690475	19.93%	2.033%
8	8.640	919	927	942	rBV	2242954	3627205	26.87%	2.740%
9	9.099	998	1005	1021	rBV	1893821	2951718	21.86%	2.230%
10	9.822	1120	1128	1140	rBV	1491826	2448228	18.13%	1.850%
11	10.363	1212	1220	1230	rBV	2197517	3760827	27.86%	2.841%
12	10.746	1276	1285	1300	rBV	2464264	4104658	30.40%	3.101%
13	10.881	1300	1308	1321	rBV	2291368	3993839	29.58%	3.018%
14	12.328	1547	1554	1561	rBV	42022	74497	0.55%	0.056%
15	12.404	1563	1567	1572	rVB6	8338	14611	0.11%	0.011%
16	13.381	1727	1733	1736	rBV7	8903	16932	0.13%	0.013%
17	13.457	1743	1746	1754	rVB8	9928	17163	0.13%	0.013%
18	13.981	1827	1835	1850	rBV	4464054	6284293	46.55%	4.748%
19	14.269	1877	1884	1899	rBV	5053487	7222709	53.50%	5.457%
20	14.575	1928	1936	1944	rBV	4275025	6051199	44.82%	4.572%
21	14.640	1944	1947	1950	rVB3	12641	17844	0.13%	0.013%
22	14.775	1963	1970	1984	rBV	1845203	2849893	21.11%	2.153%
23	14.975	2001	2004	2010	rVB4	17068	30558	0.23%	0.023%
24	15.204	2035	2043	2048	rBV4	11310	22403	0.17%	0.017%
25	15.393	2071	2075	2081	rVB3	12109	15310	0.11%	0.012%
26	15.569	2096	2105	2112	rBV	6738837	9549780	70.73%	7.215%
27	15.693	2119	2126	2141	rBV	2172445	2867878	21.24%	2.167%
28	15.816	2141	2147	2156	rVB4	30030	67853	0.50%	0.051%
29	16.351	2234	2238	2244	rBV7	9679	16281	0.12%	0.012%
30	16.516	2263	2266	2271	rVB6	12014	13990	0.10%	0.011%
31	16.628	2280	2285	2290	rBV9	14591	23477	0.17%	0.018%
32	16.792	2308	2313	2321	rBV9	13402	25606	0.19%	0.019%
33	17.122	2366	2369	2375	rVB5	11547	16549	0.12%	0.013%
34	17.334	2398	2405	2415	rBV	5775229	7909247	58.58%	5.976%
35	17.434	2415	2422	2437	rVV	7748483	10725090	79.44%	8.103%
36	18.281	2563	2566	2570	rBV2	15767	24259	0.18%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010323\
Data File : BP013376.D
Acq On : 03 Jan 2023 12:20
Operator : CG/JU
Sample : PB149944BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK944

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Title : SVOA CALIBRATION

37	19.245	2725	2730	2735	rBV	99426	147976	1.10%	0.112%
38	19.310	2737	2741	2745	rBV	96128	133332	0.99%	0.101%
39	19.669	2796	2802	2813	rBV	10436722	13500869	100.00%	10.200%
40	21.422	3095	3100	3112	rBV	7227651	9084349	67.29%	6.864%
41	23.733	3485	3493	3507	rBV	6133683	12486472	92.49%	9.434%
42	23.892	3513	3520	3534	rVB2	4093887	8580542	63.56%	6.483%




Sum of corrected areas: 132355598

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010323\
Data File : BP013376.D
Acq On : 03 Jan 2023 12:20
Operator : CG/JU
Sample : PB149944BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK944

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

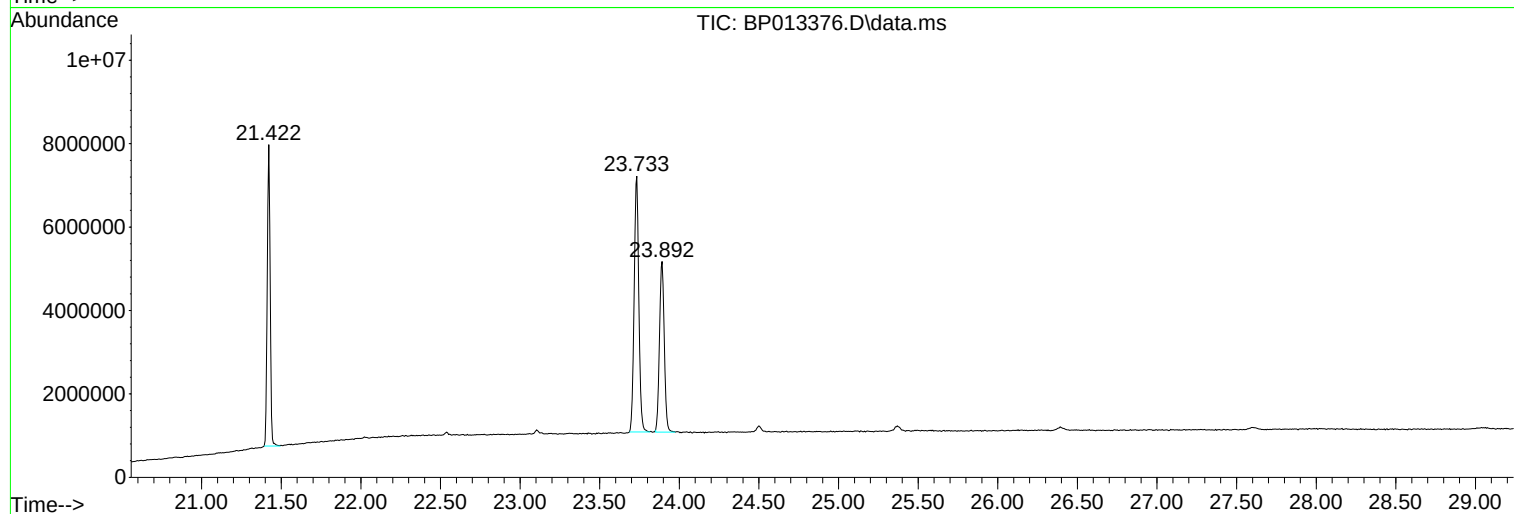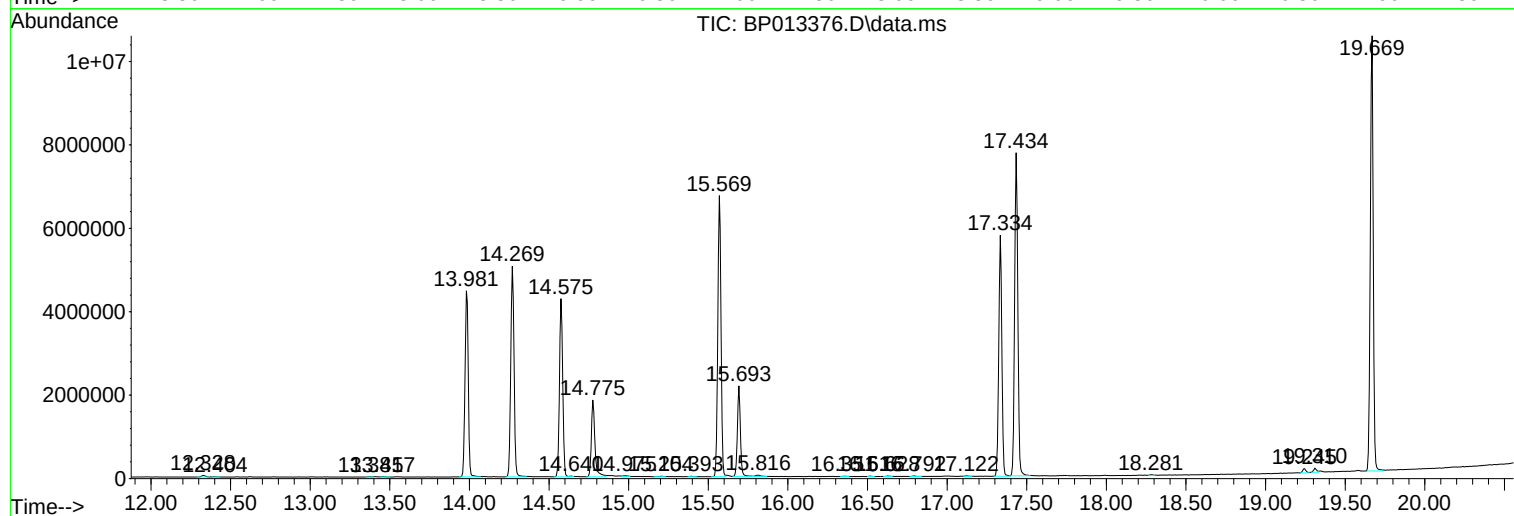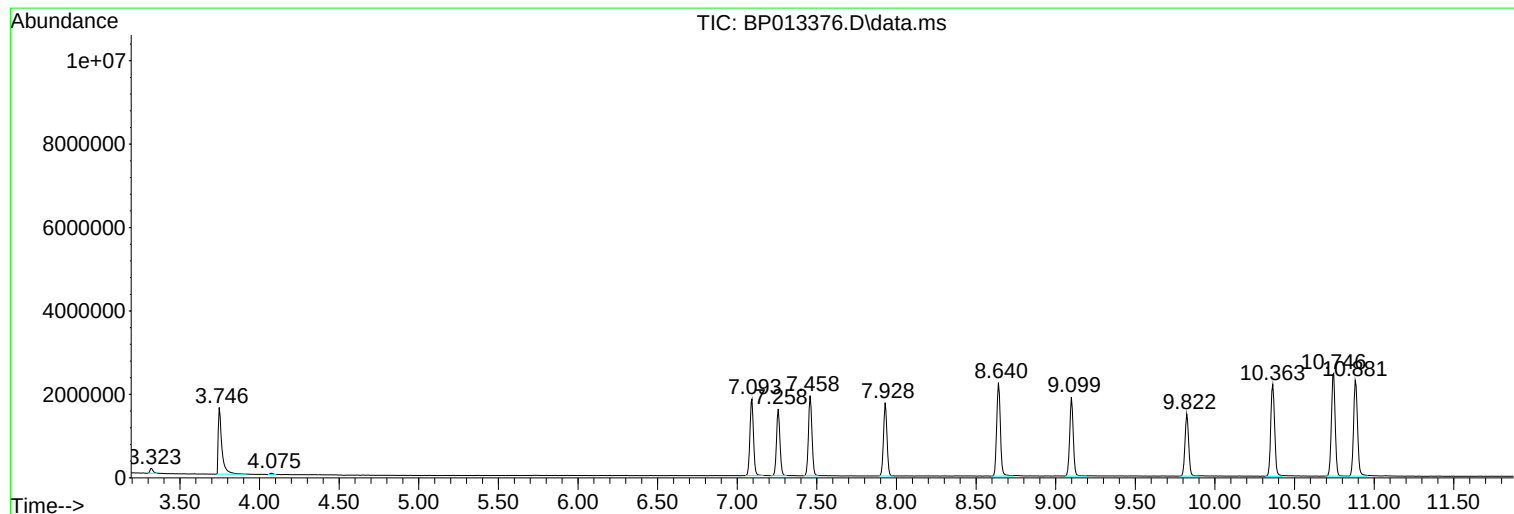

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010323\
Data File : BP013376.D
Acq On : 03 Jan 2023 12:20
Operator : CG/JU
Sample : PB149944BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK944

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010323\
Data File : BP013376.D
Acq On : 03 Jan 2023 12:20
Operator : CG/JU
Sample : PB149944BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK944

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc