

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010323\
 Data File : BP013378.D
 Acq On : 03 Jan 2023 15:14
 Operator : CG/JU
 Sample : PB149946BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK946

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013378.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.322	19	23	31	rVB	131525	187919	1.40%	0.139%
2	3.746	92	95	120	rBV	1752389	2788907	20.74%	2.063%
3	4.075	147	151	159	rVB	35463	56479	0.42%	0.042%
4	7.093	656	664	674	rBV	1983540	3103080	23.07%	2.295%
5	7.258	685	692	703	rVB	1698739	2610252	19.41%	1.931%
6	7.458	718	726	736	rBV	2067416	3180688	23.65%	2.352%
7	7.928	799	806	816	rBV	1816899	2910935	21.64%	2.153%
8	8.640	919	927	941	rBV	2451667	3901905	29.01%	2.886%
9	9.099	996	1005	1020	rBV	1987778	3232950	24.04%	2.391%
10	9.822	1120	1128	1141	rBV	1641801	2688340	19.99%	1.988%
11	10.363	1212	1220	1231	rBV	2502964	4124054	30.66%	3.050%
12	10.746	1277	1285	1295	rBV	2749803	4537602	33.74%	3.356%
13	10.881	1300	1308	1322	rBV	2468227	4400467	32.72%	3.255%
14	12.334	1549	1555	1561	rVB	45411	76530	0.57%	0.057%
15	12.545	1583	1591	1597	rVB	5790	14480	0.11%	0.011%
16	13.540	1753	1760	1766	rBV10	7332	14726	0.11%	0.011%
17	13.987	1825	1836	1850	rBV	5063984	7138582	53.07%	5.280%
18	14.269	1877	1884	1903	rBV	5603088	8104276	60.25%	5.994%
19	14.575	1927	1936	1944	rBV	4680757	6890101	51.23%	5.096%
20	14.775	1963	1970	1989	rBV	1873335	3020467	22.46%	2.234%
21	14.939	1994	1998	2001	rVB6	7536	14656	0.11%	0.011%
22	15.204	2039	2043	2050	rBV8	6735	13700	0.10%	0.010%
23	15.575	2098	2106	2120	rBV	7312008	10705486	79.59%	7.918%
24	15.692	2120	2126	2142	rVV	2310459	3149504	23.42%	2.329%
25	15.810	2142	2146	2156	rVB4	36837	67013	0.50%	0.050%
26	16.363	2234	2240	2245	rVB8	8706	14299	0.11%	0.011%
27	17.010	2344	2350	2355	rVB10	13148	26944	0.20%	0.020%
28	17.116	2366	2368	2373	rVB3	11247	17269	0.13%	0.013%
29	17.333	2398	2405	2415	rBV	6144080	8681378	64.54%	6.421%
30	17.433	2415	2422	2447	rVV	8158326	11612139	86.33%	8.588%
31	17.992	2514	2517	2522	rBV7	9434	14121	0.10%	0.010%
32	18.280	2563	2566	2568	rBV4	13490	17787	0.13%	0.013%
33	19.245	2726	2730	2736	rBV2	99801	136558	1.02%	0.101%
34	19.310	2738	2741	2747	rBV	84000	118620	0.88%	0.088%
35	19.669	2796	2802	2815	rBV	10295558	13450181	100.00%	9.948%
36	21.421	3095	3100	3111	rBV	6307299	8087231	60.13%	5.981%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010323\
Data File : BP013378.D
Acq On : 03 Jan 2023 15:14
Operator : CG/JU
Sample : PB149946BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK946

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Title : SVOA CALIBRATION

37	23.733	3486	3493	3506	rVB2	4652605	9408816	69.95%	6.959%
38	23.892	3513	3520	3533	rVB2	3305076	6691327	49.75%	4.949%




Sum of corrected areas: 135209769

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010323\
Data File : BP013378.D
Acq On : 03 Jan 2023 15:14
Operator : CG/JU
Sample : PB149946BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK946

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

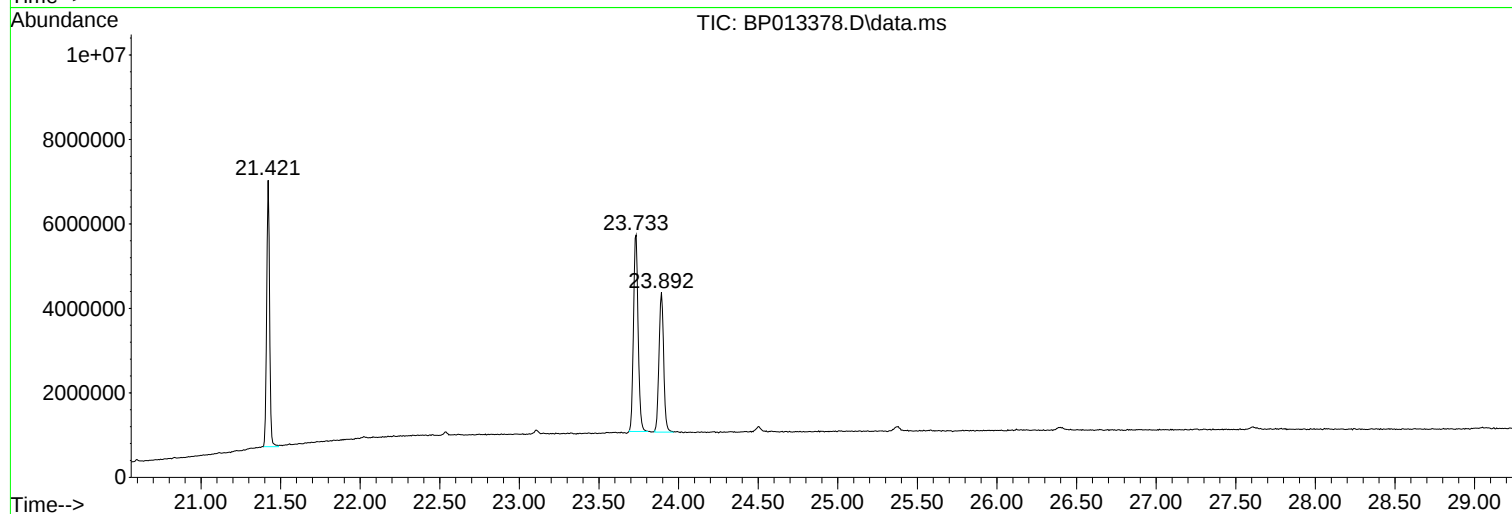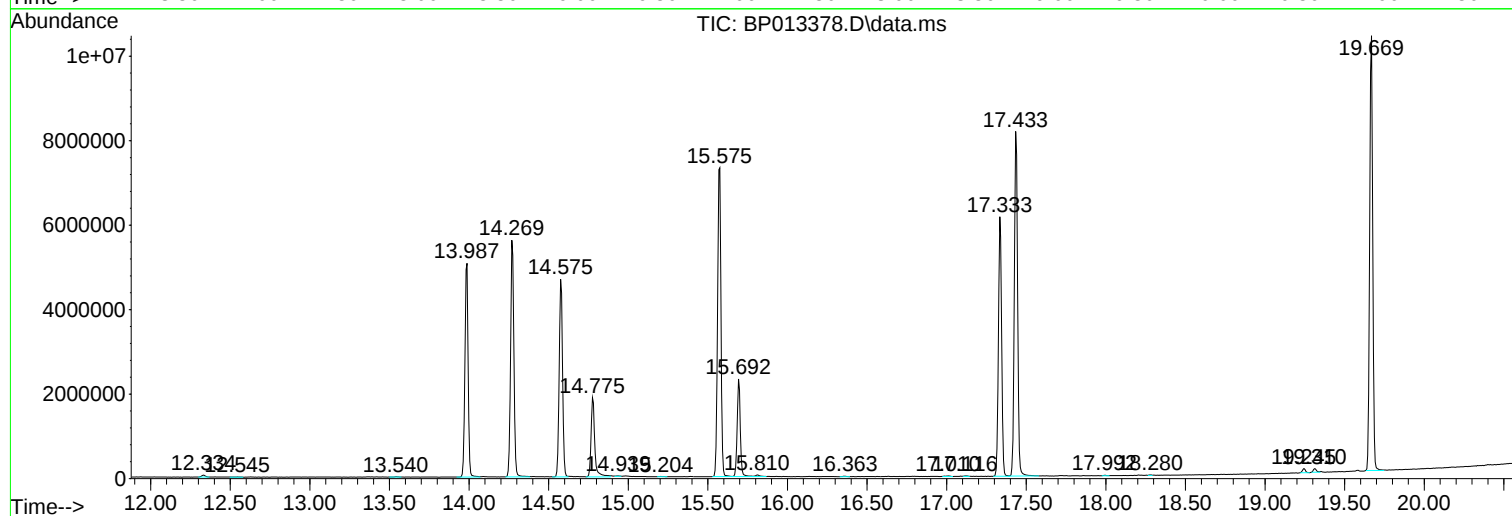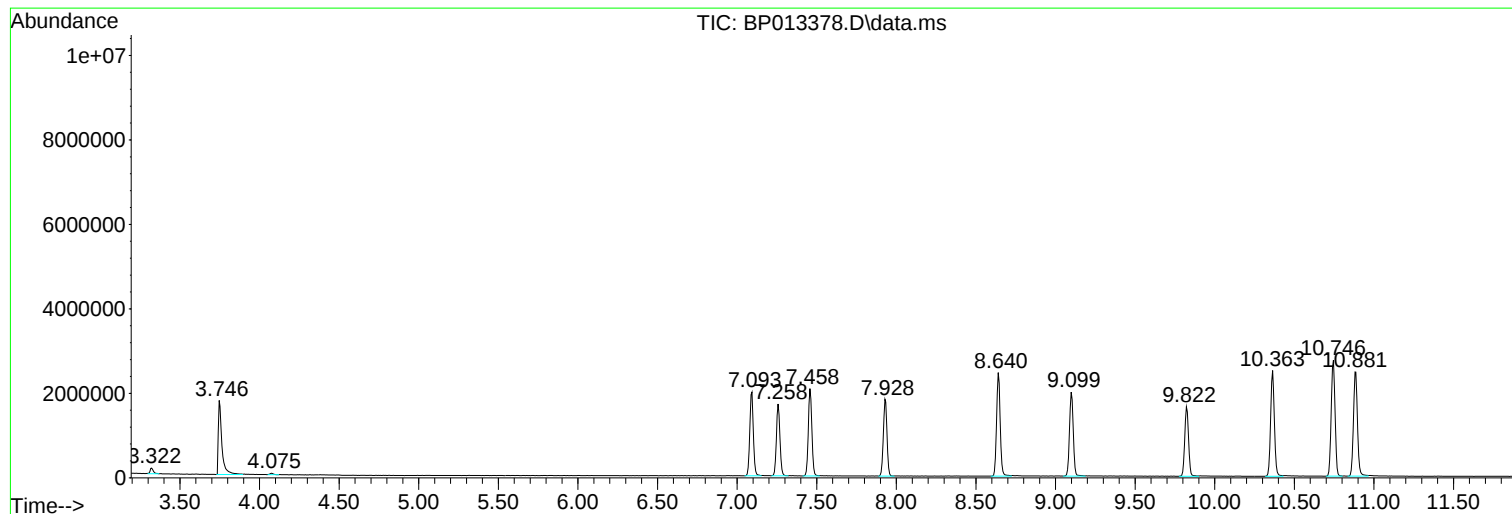

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010323\
Data File : BP013378.D
Acq On : 03 Jan 2023 15:14
Operator : CG/JU
Sample : PB149946BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK946

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010323\
Data File : BP013378.D
Acq On : 03 Jan 2023 15:14
Operator : CG/JU
Sample : PB149946BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK946

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc