

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010323\
 Data File : BP013381.D
 Acq On : 03 Jan 2023 16:57
 Operator : CG/JU
 Sample : PB149947BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK947

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013381.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.323	19	23	30	rVB	164046	209188	1.80%	0.152%
2	3.746	92	95	116	rBV	2133823	3214510	27.72%	2.329%
3	4.075	147	151	157	rVB	40024	55117	0.48%	0.040%
4	7.087	656	663	674	rBV	2414299	3685973	31.79%	2.670%
5	7.252	683	691	699	rBV	1951997	3039064	26.21%	2.202%
6	7.458	717	726	738	rBV	2360926	3761723	32.44%	2.725%
7	7.928	798	806	817	rBV	2176529	3456214	29.81%	2.504%
8	8.634	918	926	944	rBV	2797712	4524217	39.02%	3.277%
9	9.093	996	1004	1017	rBV	2281337	3715458	32.04%	2.692%
10	9.816	1118	1127	1139	rBV	1879490	3082859	26.59%	2.233%
11	10.358	1210	1219	1233	rBV	2819427	4692235	40.47%	3.399%
12	10.740	1275	1284	1296	rBV	3079463	5143872	44.36%	3.726%
13	10.875	1299	1307	1322	rBV	2806862	4863962	41.95%	3.524%
14	12.322	1545	1553	1561	rBV2	51526	94654	0.82%	0.069%
15	13.534	1752	1759	1765	rVB8	10315	22531	0.19%	0.016%
16	13.975	1828	1834	1845	rBV	5383114	7313818	63.08%	5.298%
17	14.263	1875	1883	1899	rBV	6020594	8683046	74.88%	6.290%
18	14.569	1926	1935	1949	rBV	5118749	7321190	63.14%	5.304%
19	14.769	1963	1969	1992	rBV	1969367	3036021	26.18%	2.199%
20	14.975	2001	2004	2009	rVB7	13802	23226	0.20%	0.017%
21	15.563	2097	2104	2119	rBV	7983357	11063105	95.41%	8.014%
22	15.687	2119	2125	2139	rVV	2362932	3151637	27.18%	2.283%
23	15.804	2141	2145	2154	rVB	35120	69048	0.60%	0.050%
24	16.345	2233	2237	2242	rBV7	10600	19728	0.17%	0.014%
25	17.004	2346	2349	2353	rVB4	11478	15304	0.13%	0.011%
26	17.110	2365	2367	2375	rVB4	11999	21441	0.18%	0.016%
27	17.328	2397	2404	2414	rBV	6101206	8408673	72.52%	6.091%
28	17.428	2414	2421	2443	rVV	8244656	11265231	97.15%	8.161%
29	17.710	2465	2469	2470	rBV4	9815	13211	0.11%	0.010%
30	17.981	2513	2515	2520	rVB6	14680	17696	0.15%	0.013%
31	19.234	2724	2728	2734	rBV3	86718	136680	1.18%	0.099%
32	19.304	2736	2740	2744	rBV	76660	108123	0.93%	0.078%
33	19.657	2794	2800	2813	rBV	8650495	11595252	100.00%	8.400%
34	21.410	3093	3098	3109	rBV	4727364	6346747	54.74%	4.598%
35	23.716	3483	3490	3505	rVB	4414025	9361249	80.73%	6.781%
36	23.874	3511	3517	3531	rVB2	3116944	6510436	56.15%	4.716%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010323\
Data File : BP013381.D
Acq On : 03 Jan 2023 16:57
Operator : CG/JU
Sample : PB149947BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK947

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Title : SVOA CALIBRATION




Sum of corrected areas: 138042439

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010323\
Data File : BP013381.D
Acq On : 03 Jan 2023 16:57
Operator : CG/JU
Sample : PB149947BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK947

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

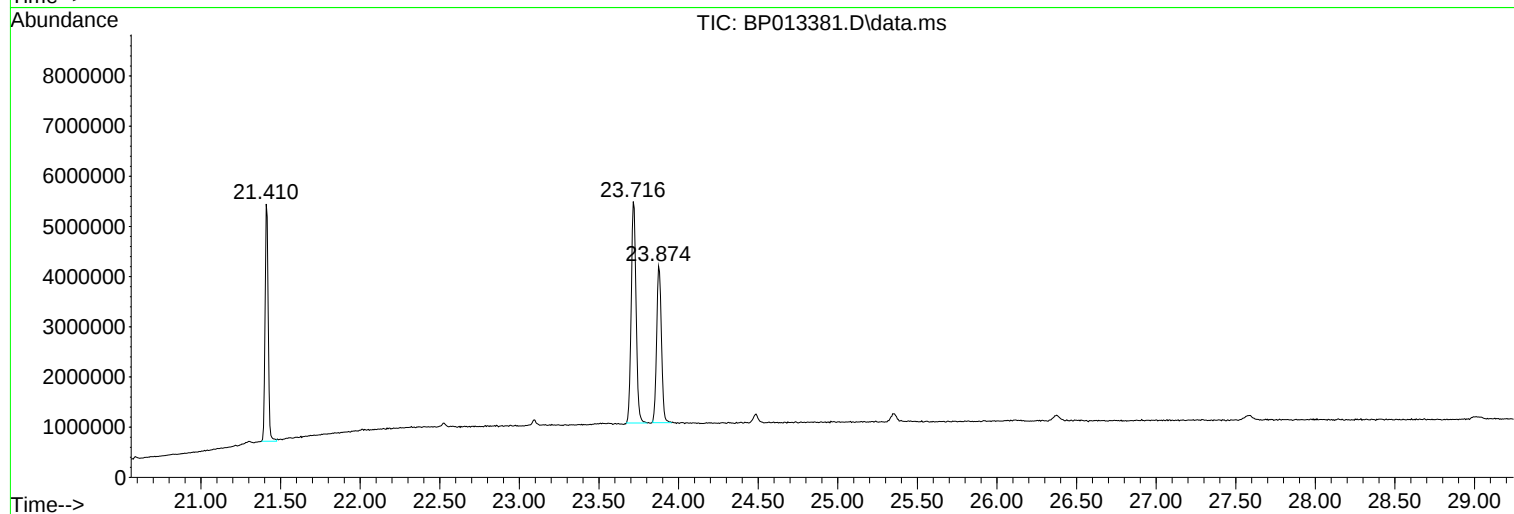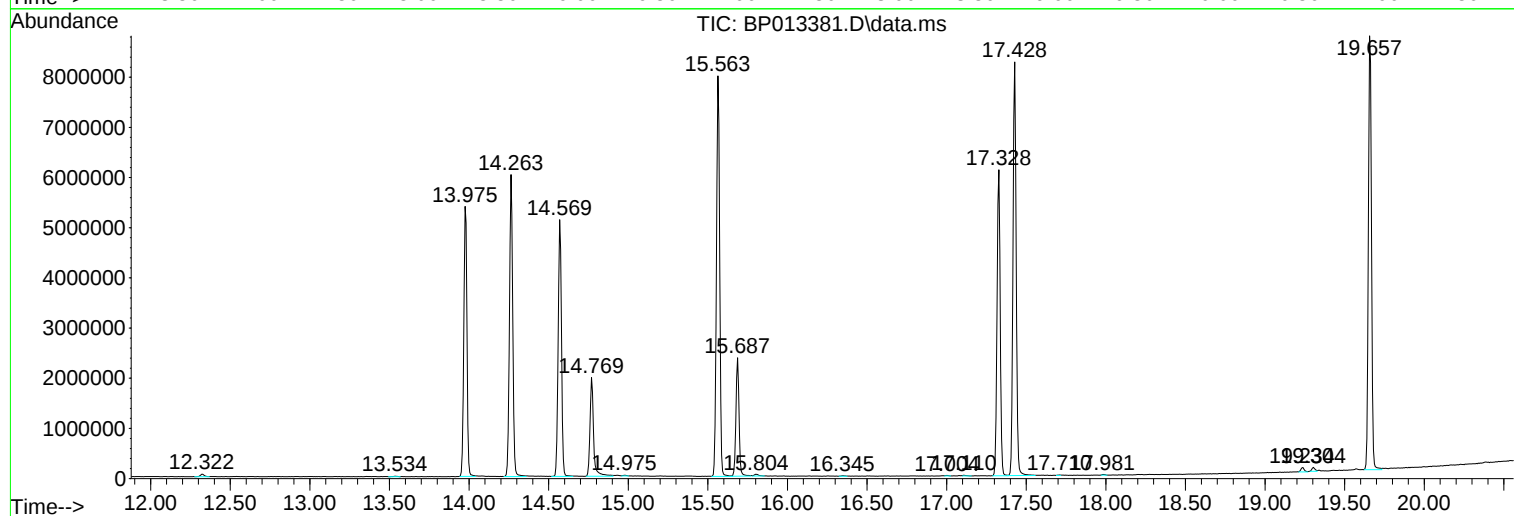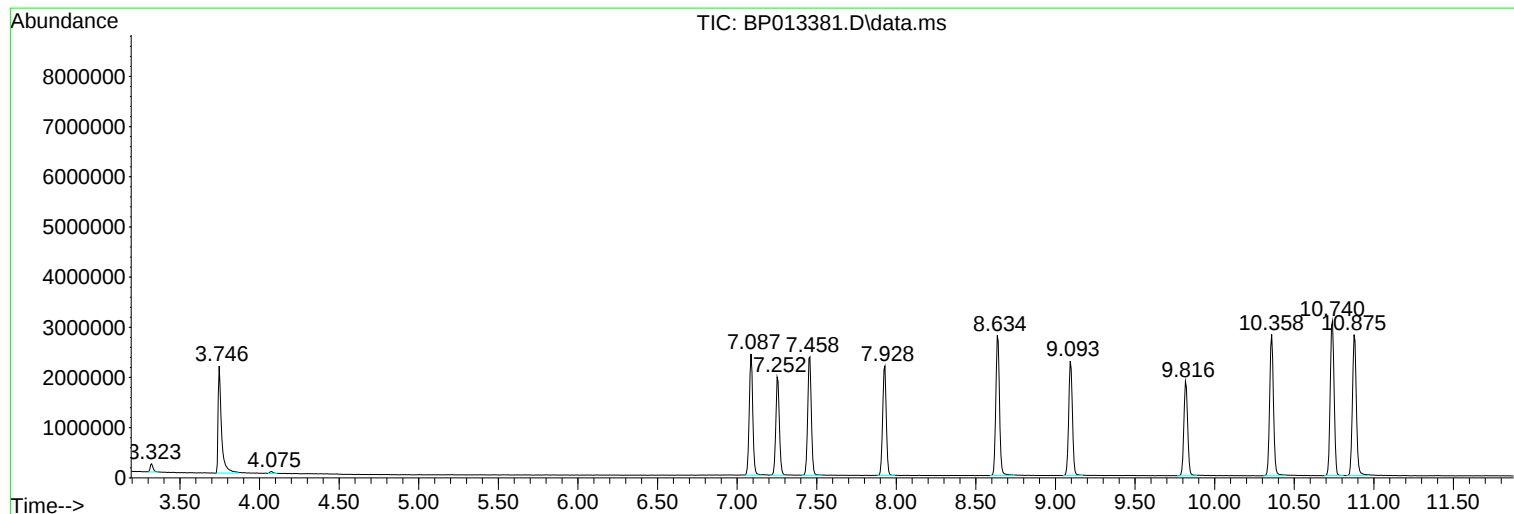

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010323\
Data File : BP013381.D
Acq On : 03 Jan 2023 16:57
Operator : CG/JU
Sample : PB149947BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK947

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010323\
Data File : BP013381.D
Acq On : 03 Jan 2023 16:57
Operator : CG/JU
Sample : PB149947BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK947

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc