

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010423\
 Data File : BP013385.D
 Acq On : 04 Jan 2023 11:02
 Operator : CG/JU
 Sample : PB 149983BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK983

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013385.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.322	19	23	29	rVB	157846	204426	1.42%	0.132%
2	3.746	92	95	114	rBV	2027991	3103738	21.63%	2.008%
3	4.075	147	151	155	rVB	49842	63218	0.44%	0.041%
4	7.087	656	663	674	rBV	2316047	3542552	24.69%	2.292%
5	7.251	685	691	702	rBV	1860182	2896832	20.19%	1.874%
6	7.457	719	726	741	rVB	2242894	3593341	25.05%	2.325%
7	7.928	799	806	815	rBV	2817375	4384292	30.56%	2.836%
8	8.634	917	926	942	rBV	2675977	4344219	30.28%	2.810%
9	9.092	997	1004	1018	rBV	2140940	3509750	24.46%	2.271%
10	9.816	1120	1127	1139	rBV	1755840	2899071	20.21%	1.875%
11	10.357	1210	1219	1231	rBV	2745980	4435589	30.92%	2.869%
12	10.739	1276	1284	1296	rBV	3946281	6425017	44.78%	4.156%
13	10.875	1299	1307	1324	rBV	2613599	4598038	32.05%	2.975%
14	12.328	1548	1554	1559	rBV	42861	73972	0.52%	0.048%
15	13.539	1757	1760	1769	rVB10	9524	19155	0.13%	0.012%
16	13.975	1824	1834	1850	rBV	5099885	7028366	48.99%	4.547%
17	14.263	1876	1883	1906	rBV	5575547	8026539	55.95%	5.193%
18	14.569	1927	1935	1943	rBV	6245546	8863427	61.78%	5.734%
19	14.769	1962	1969	1986	rBV	2111685	3178820	22.16%	2.056%
20	15.563	2097	2104	2118	rBV	7462569	10466670	72.96%	6.771%
21	15.686	2118	2125	2139	rVV	2519588	3397296	23.68%	2.198%
22	15.804	2140	2145	2152	rVB3	30941	61847	0.43%	0.040%
23	16.998	2344	2348	2352	rVB6	9278	14772	0.10%	0.010%
24	17.110	2363	2367	2372	rVB2	15279	20847	0.15%	0.013%
25	17.327	2397	2404	2414	rBV	7872443	10966107	76.44%	7.094%
26	17.427	2414	2421	2443	rVB	8233266	11898804	82.94%	7.698%
27	19.233	2724	2728	2734	rBV2	102876	128636	0.90%	0.083%
28	19.304	2736	2740	2743	rBV	93820	125083	0.87%	0.081%
29	19.568	2783	2785	2789	rBV4	25308	24866	0.17%	0.016%
30	19.657	2794	2800	2813	rBV	10956499	14346445	100.00%	9.281%
31	21.409	3093	3098	3109	rBV	8454355	11090494	77.30%	7.175%
32	23.715	3483	3490	3503	rVB2	5625127	11235891	78.32%	7.269%
33	23.874	3510	3517	3534	rVB2	4706098	9610051	66.99%	6.217%




Sum of corrected areas: 154578171

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010423\
Data File : BP013385.D
Acq On : 04 Jan 2023 11:02
Operator : CG/JU
Sample : PB 149983BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK983

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

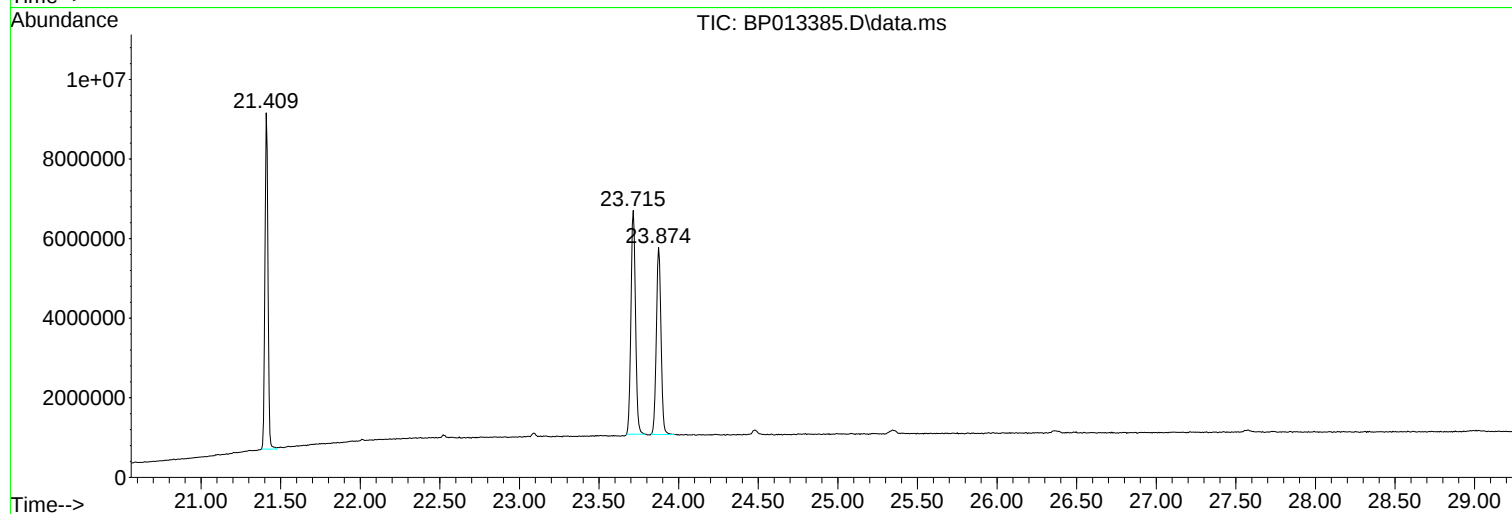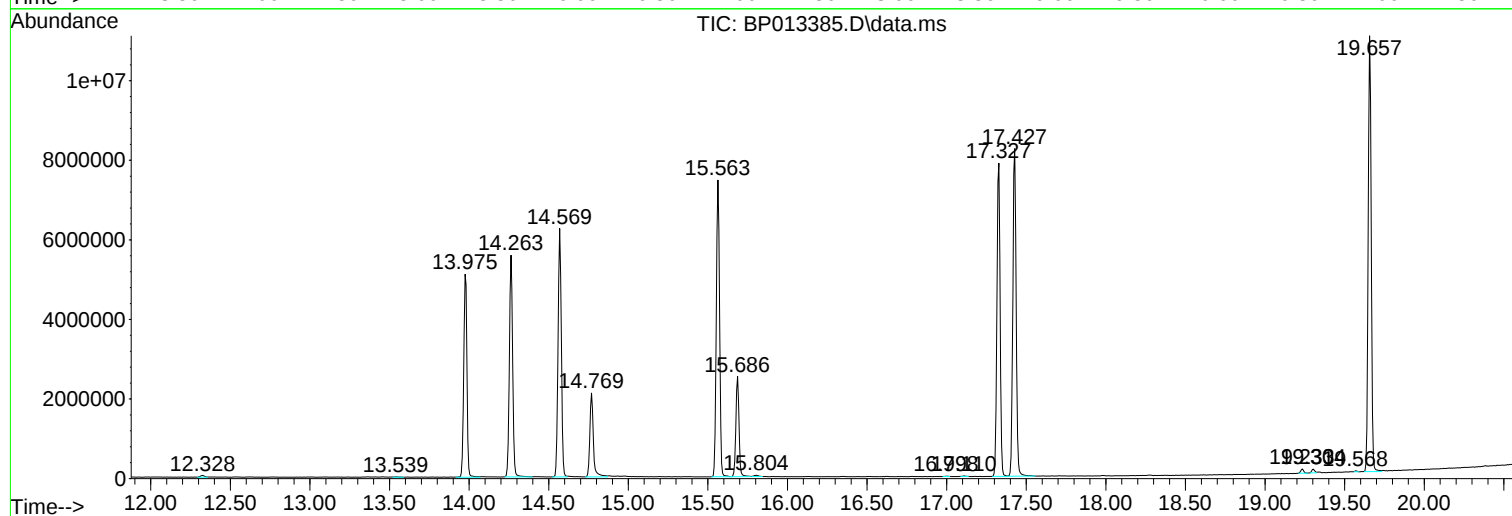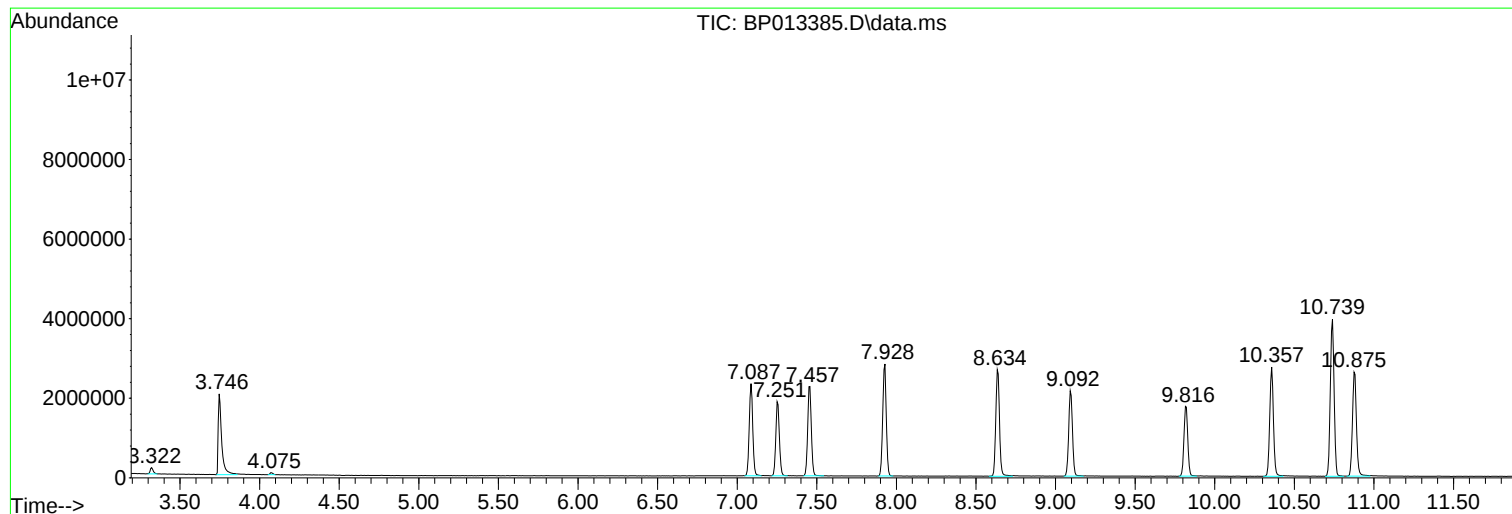

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010423\
Data File : BP013385.D
Acq On : 04 Jan 2023 11:02
Operator : CG/JU
Sample : PB 149983BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK983

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010423\
Data File : BP013385.D
Acq On : 04 Jan 2023 11:02
Operator : CG/JU
Sample : PB 149983BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK983

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------