

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010423\
 Data File : BP013389.D
 Acq On : 04 Jan 2023 14:15
 Operator : CG/JU
 Sample : PB149980BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK980

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013389.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.322	19	23	32	rVB	197270	253354	2.03%	0.177%
2	3.746	92	95	113	rBV	2402220	3547715	28.41%	2.476%
3	4.075	147	151	156	rVB	45502	64032	0.51%	0.045%
4	7.087	656	663	674	rBV	2711968	4114496	32.95%	2.872%
5	7.252	685	691	702	rBV	2157950	3360363	26.91%	2.345%
6	7.452	718	725	736	rBV	2650974	4223643	33.82%	2.948%
7	7.928	798	806	813	rBV	2453015	3803427	30.46%	2.654%
8	8.634	918	926	943	rBV	3050032	4987726	39.94%	3.481%
9	9.093	997	1004	1021	rBV	2488125	4028897	32.26%	2.812%
10	9.816	1118	1127	1139	rBV	2029112	3354141	26.86%	2.341%
11	9.904	1140	1142	1147	rVB6	9221	13455	0.11%	0.009%
12	10.357	1208	1219	1235	rBV	3104132	5119595	41.00%	3.573%
13	10.740	1274	1284	1297	rBV	3283563	5490366	43.97%	3.832%
14	10.875	1300	1307	1327	rBV	2932743	5186298	41.53%	3.620%
15	12.322	1544	1553	1561	rBV2	52165	96120	0.77%	0.067%
16	13.451	1742	1745	1750	rVB7	8805	14226	0.11%	0.010%
17	13.539	1757	1760	1765	rVB6	8963	13931	0.11%	0.010%
18	13.975	1824	1834	1845	rBV	5485597	7401547	59.27%	5.166%
19	14.081	1850	1852	1859	rVB8	8284	13712	0.11%	0.010%
20	14.263	1876	1883	1905	rBV	6332279	8887452	71.17%	6.203%
21	14.569	1928	1935	1943	rBV	5080903	7307918	58.52%	5.100%
22	14.769	1963	1969	1987	rBV	2023505	3115324	24.95%	2.174%
23	14.975	2001	2004	2013	rVB5	20041	40179	0.32%	0.028%
24	15.563	2094	2104	2118	rBV	7967218	11224111	89.89%	7.833%
25	15.686	2119	2125	2141	rVV	2535841	3343663	26.78%	2.334%
26	15.804	2141	2145	2154	rVB5	37178	76476	0.61%	0.053%
27	16.351	2233	2238	2244	rBV9	10178	20229	0.16%	0.014%
28	16.510	2260	2265	2271	rBV9	10234	15788	0.13%	0.011%
29	17.116	2364	2368	2371	rVB3	13549	18909	0.15%	0.013%
30	17.328	2397	2404	2414	rBV	6081457	8511186	68.16%	5.940%
31	17.428	2414	2421	2438	rVV	8221600	11417676	91.44%	7.968%
32	17.980	2513	2515	2519	rVB5	10227	12626	0.10%	0.009%
33	18.275	2562	2565	2568	rVB	16099	16375	0.13%	0.011%
34	19.233	2724	2728	2733	rBV3	87729	120316	0.96%	0.084%
35	19.304	2736	2740	2744	rBV	82633	112852	0.90%	0.079%
36	19.657	2794	2800	2813	rBV	9311775	12486953	100.00%	8.715%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010423\
Data File : BP013389.D
Acq On : 04 Jan 2023 14:15
Operator : CG/JU
Sample : PB149980BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK980

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Title : SVOA CALIBRATION

37	21.410	3093	3098	3108	rBV	5031150	6831611	54.71%	4.768%
38	23.715	3484	3490	3507	rVB2	4271185	8718235	69.82%	6.085%
39	23.874	3511	3517	3530	rVB2	2800785	5921034	47.42%	4.132%




Sum of corrected areas: 143285957

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010423\
Data File : BP013389.D
Acq On : 04 Jan 2023 14:15
Operator : CG/JU
Sample : PB149980BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK980

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

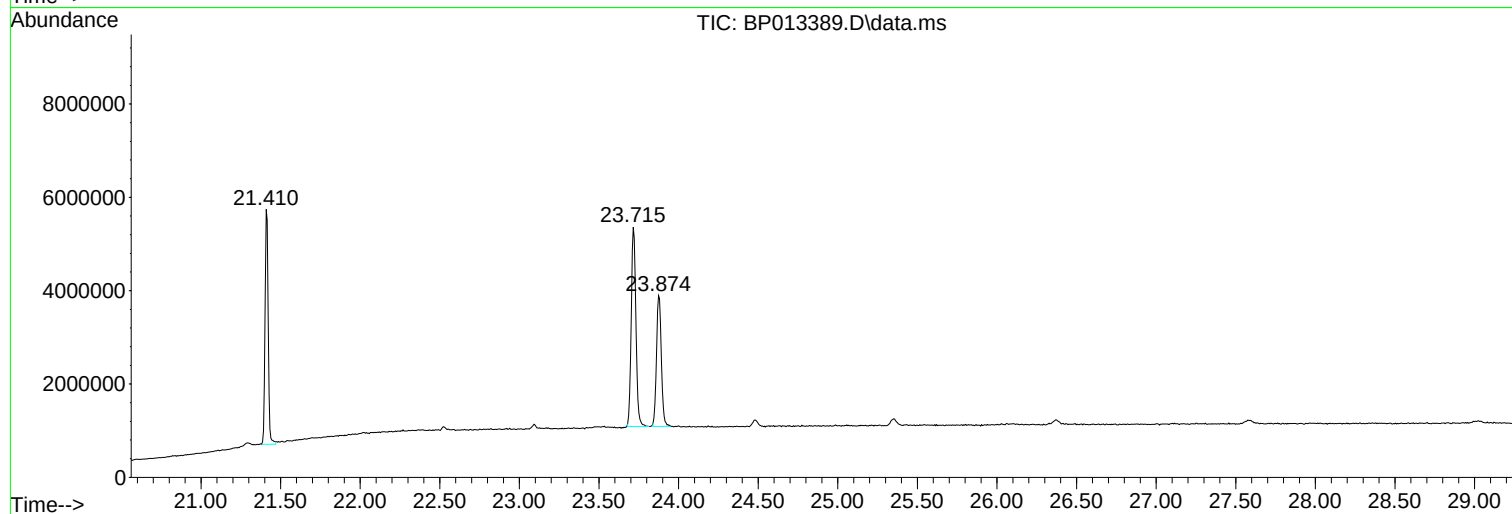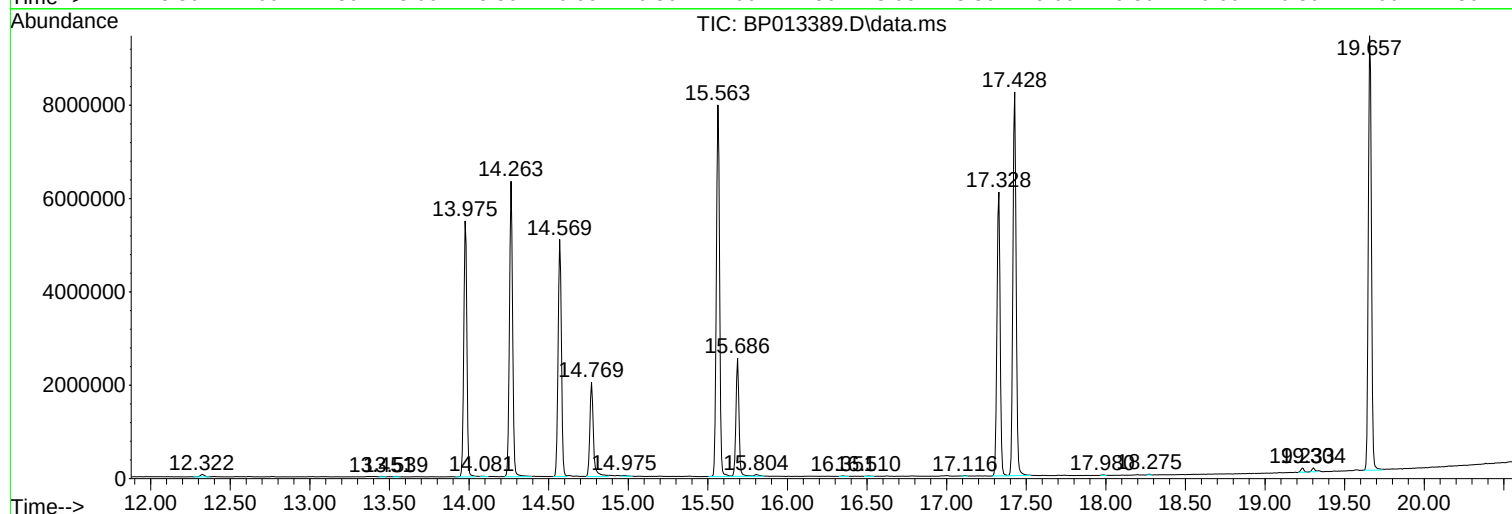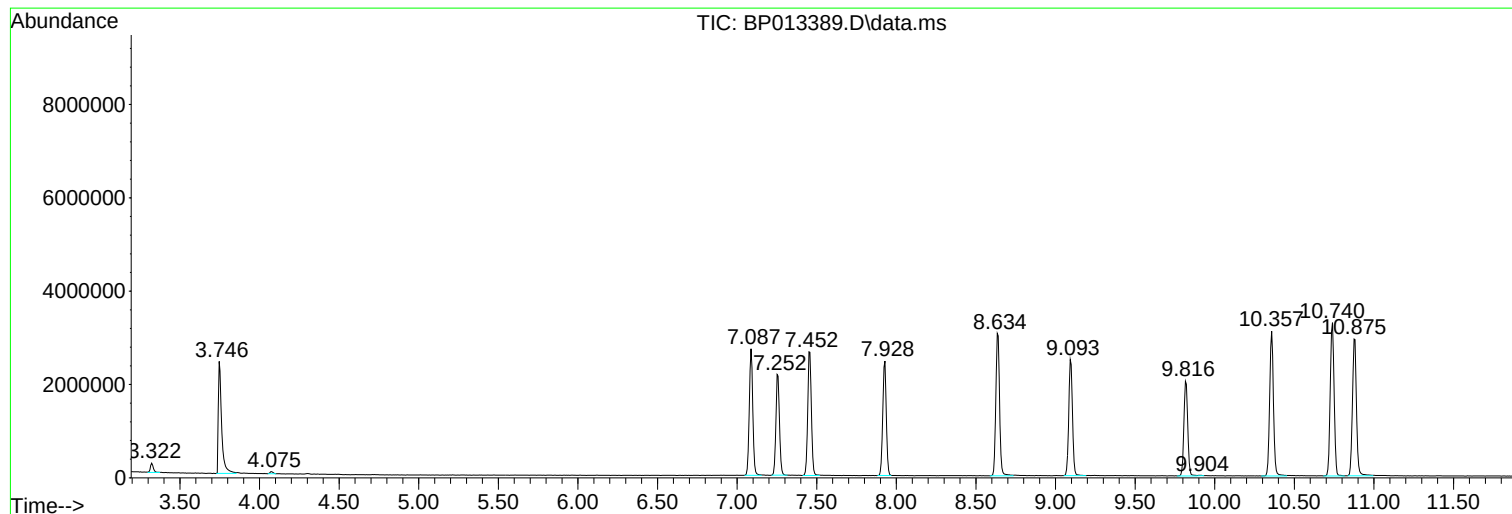

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010423\
Data File : BP013389.D
Acq On : 04 Jan 2023 14:15
Operator : CG/JU
Sample : PB149980BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK980

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010423\
Data File : BP013389.D
Acq On : 04 Jan 2023 14:15
Operator : CG/JU
Sample : PB149980BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK980

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc