

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010423\
 Data File : BP013390.D
 Acq On : 04 Jan 2023 14:49
 Operator : CG/JU
 Sample : PB149982BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK982

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013390.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.322	19	23	31	rVB	175386	231434	1.68%	0.160%
2	3.746	92	95	117	rBV	2196993	3317342	24.11%	2.296%
3	4.075	147	151	156	rVB	39723	55991	0.41%	0.039%
4	7.087	656	663	678	rBV	2472187	3772723	27.42%	2.611%
5	7.252	685	691	701	rBV	1973281	3071085	22.32%	2.125%
6	7.457	718	726	734	rBV	2399247	3815485	27.73%	2.640%
7	7.928	798	806	816	rBV	2192938	3504417	25.47%	2.425%
8	8.634	919	926	941	rBV	2877484	4588662	33.35%	3.175%
9	9.093	997	1004	1021	rBV	2335710	3749941	27.26%	2.595%
10	9.816	1119	1127	1137	rBV	1910303	3097150	22.51%	2.143%
11	10.357	1210	1219	1235	rBV	2870243	4693632	34.12%	3.248%
12	10.740	1276	1284	1294	rBV	3075963	5127613	37.27%	3.548%
13	10.875	1300	1307	1329	rBV	2763225	4857000	35.31%	3.361%
14	12.328	1548	1554	1560	rBV	44840	81993	0.60%	0.057%
15	13.539	1756	1760	1766	rVB5	8349	16325	0.12%	0.011%
16	13.975	1823	1834	1846	rBV	5139775	7125594	51.80%	4.931%
17	14.263	1876	1883	1895	rBV	5864668	8414846	61.17%	5.823%
18	14.569	1928	1935	1949	rBV	4968540	7099568	51.61%	4.913%
19	14.769	1962	1969	1994	rBV	2062748	3213057	23.36%	2.224%
20	14.975	2001	2004	2010	rVB8	13375	22758	0.17%	0.016%
21	15.204	2034	2043	2045	rBV10	5952	15848	0.12%	0.011%
22	15.563	2094	2104	2118	rBV	7880307	10908783	79.29%	7.549%
23	15.686	2118	2125	2135	rBV	2470256	3267404	23.75%	2.261%
24	15.804	2141	2145	2153	rVB2	36644	59500	0.43%	0.041%
25	16.998	2345	2348	2354	rVB8	13303	19762	0.14%	0.014%
26	17.116	2365	2368	2376	rVB3	12682	21121	0.15%	0.015%
27	17.327	2397	2404	2414	rBV	6218161	8709716	63.31%	6.027%
28	17.427	2414	2421	2438	rVV	8161679	11652363	84.70%	8.064%
29	17.986	2512	2516	2519	rBV5	12623	17907	0.13%	0.012%
30	19.233	2724	2728	2734	rBV	107287	141647	1.03%	0.098%
31	19.304	2736	2740	2744	rBV	92698	119824	0.87%	0.083%
32	19.657	2794	2800	2813	rBV	10351049	13757216	100.00%	9.520%
33	21.410	3093	3098	3110	rBV	6104077	8490654	61.72%	5.876%
34	23.721	3484	3491	3507	rVB	5182443	10497071	76.30%	7.264%
35	23.880	3511	3518	3530	rVB2	3418009	6967704	50.65%	4.822%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010423\
Data File : BP013390.D
Acq On : 04 Jan 2023 14:49
Operator : CG/JU
Sample : PB149982BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK982

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Title : SVOA CALIBRATION




Sum of corrected areas: 144503136

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010423\
Data File : BP013390.D
Acq On : 04 Jan 2023 14:49
Operator : CG/JU
Sample : PB149982BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK982

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

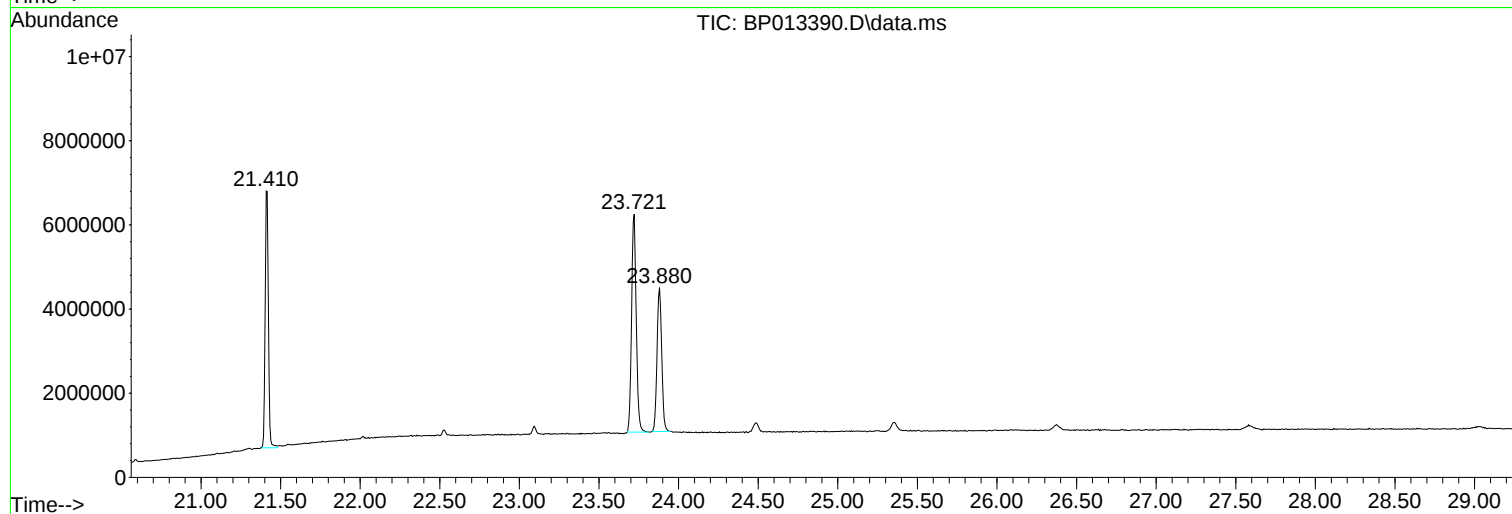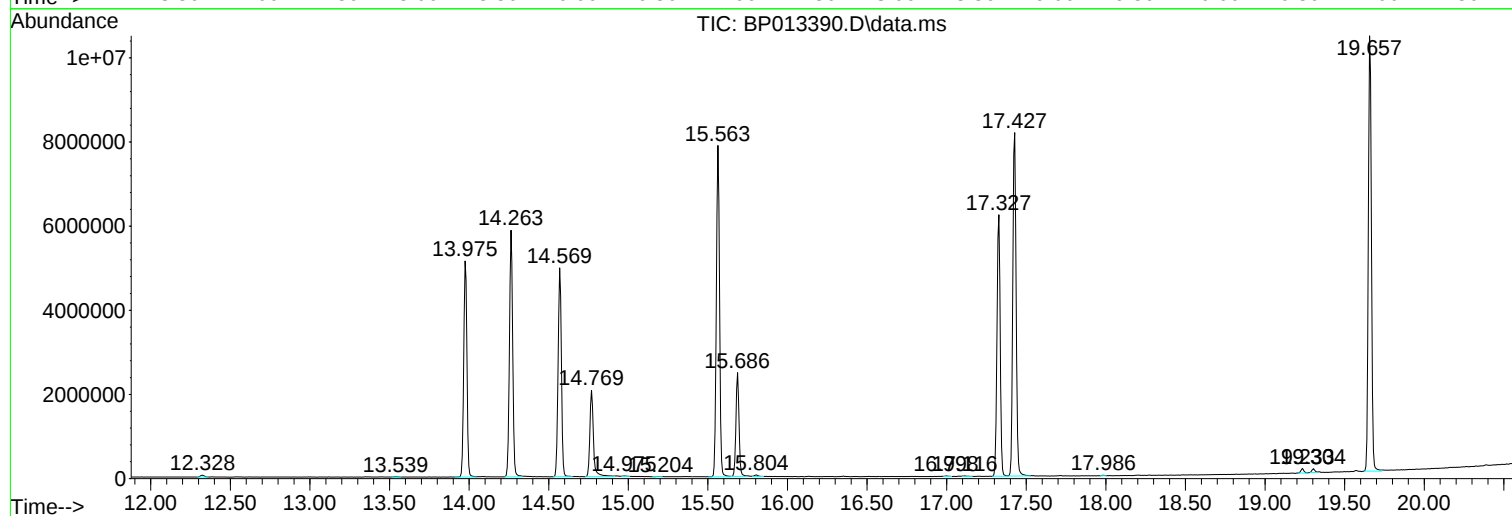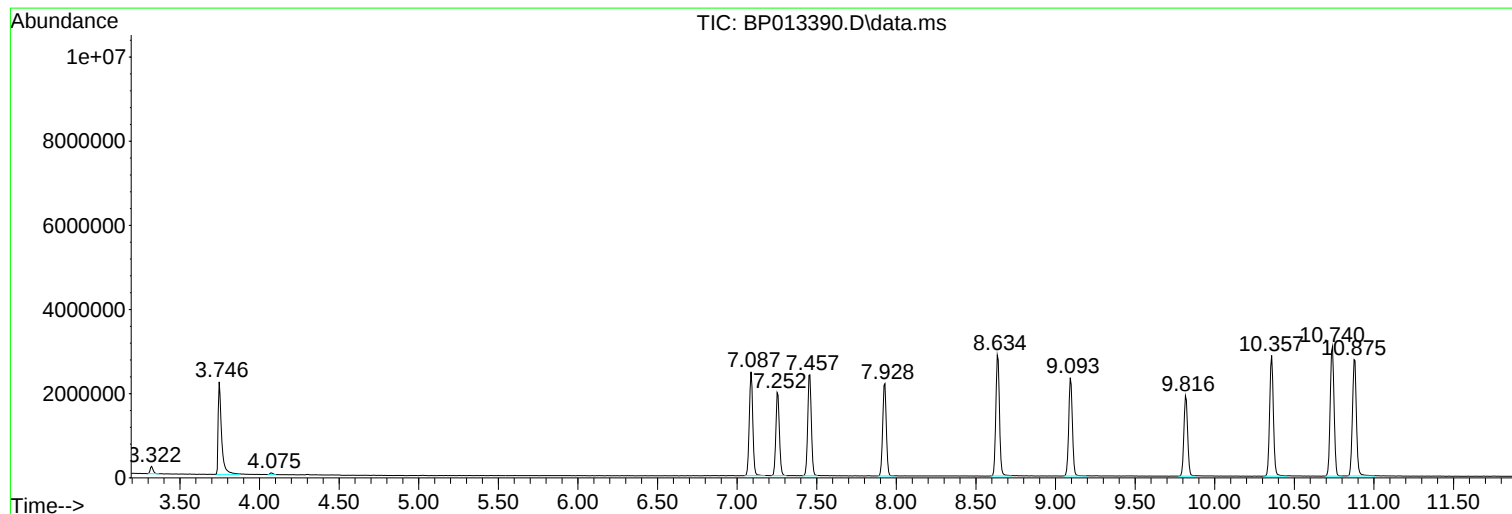

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010423\
Data File : BP013390.D
Acq On : 04 Jan 2023 14:49
Operator : CG/JU
Sample : PB149982BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK982

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010423\
Data File : BP013390.D
Acq On : 04 Jan 2023 14:49
Operator : CG/JU
Sample : PB149982BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK982

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc