

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010524\
 Data File : BP019292.D
 Acq On : 05 Jan 2024 21:36
 Operator : MA/JU
 Sample : 05953-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCFA5

Quant Time: Jan 05 23:23:17 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 29 03:48:11 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.793	152	98173	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.587	136	344414	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.440	164	220960	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.192	188	529102	20.000	ng/ul	-0.01
79) Chrysene-d12	21.298	240	627981	20.000	ng/ul	-0.01
88) Perylene-d12	23.663	264	750629	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.228	96	12056	4.194	ng/uL	0.00
4) Pyridine-d5	3.646	84	203832	28.252	ng/ul	0.00
7) Phenol-d5	6.981	99	298621	33.919	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.134	67	165681	32.530	ng/ul	0.00
11) 2-Chlorophenol-d4	7.328	132	219023	30.859	ng/ul	0.00
15) 4-Methylphenol-d8	8.522	113	247900	36.167	ng/ul	0.00
21) Nitrobenzene-d5	8.957	128	113894	38.255	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.681	143	139514	43.359	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.222	165	265322	40.835	ng/ul	0.00
31) 4-Chloroaniline-d4	10.740	131	289599	36.236	ng/ul	0.00
46) Dimethylphthalate-d6	13.857	166	890693	45.637	ng/ul	-0.01
49) Acenaphthylene-d8	14.134	160	1004925	47.454	ng/ul	0.00
54) 4-Nitrophenol-d4	14.687	143	156403	47.457	ng/ul	0.02
60) Fluorene-d10	15.434	176	798646	47.367	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.575	200	153347	44.210	ng/ul	0.00
73) Anthracene-d10	17.292	188	1302975	47.156	ng/ul	-0.01
81) Pyrene-d10	19.539	212	1773124	46.330	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.510	264	2062276	47.798	ng/ul	0.00
Target Compounds						
					Qvalue	
71) Pentachlorophenol	16.851	266	110718	23.465	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010524\
Data File : BP019292.D
Acq On : 05 Jan 2024 21:36
Operator : MA/JU
Sample : 05953-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCFA5

Quant Time: Jan 05 23:23:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 03:48:11 2023
Response via : Initial Calibration

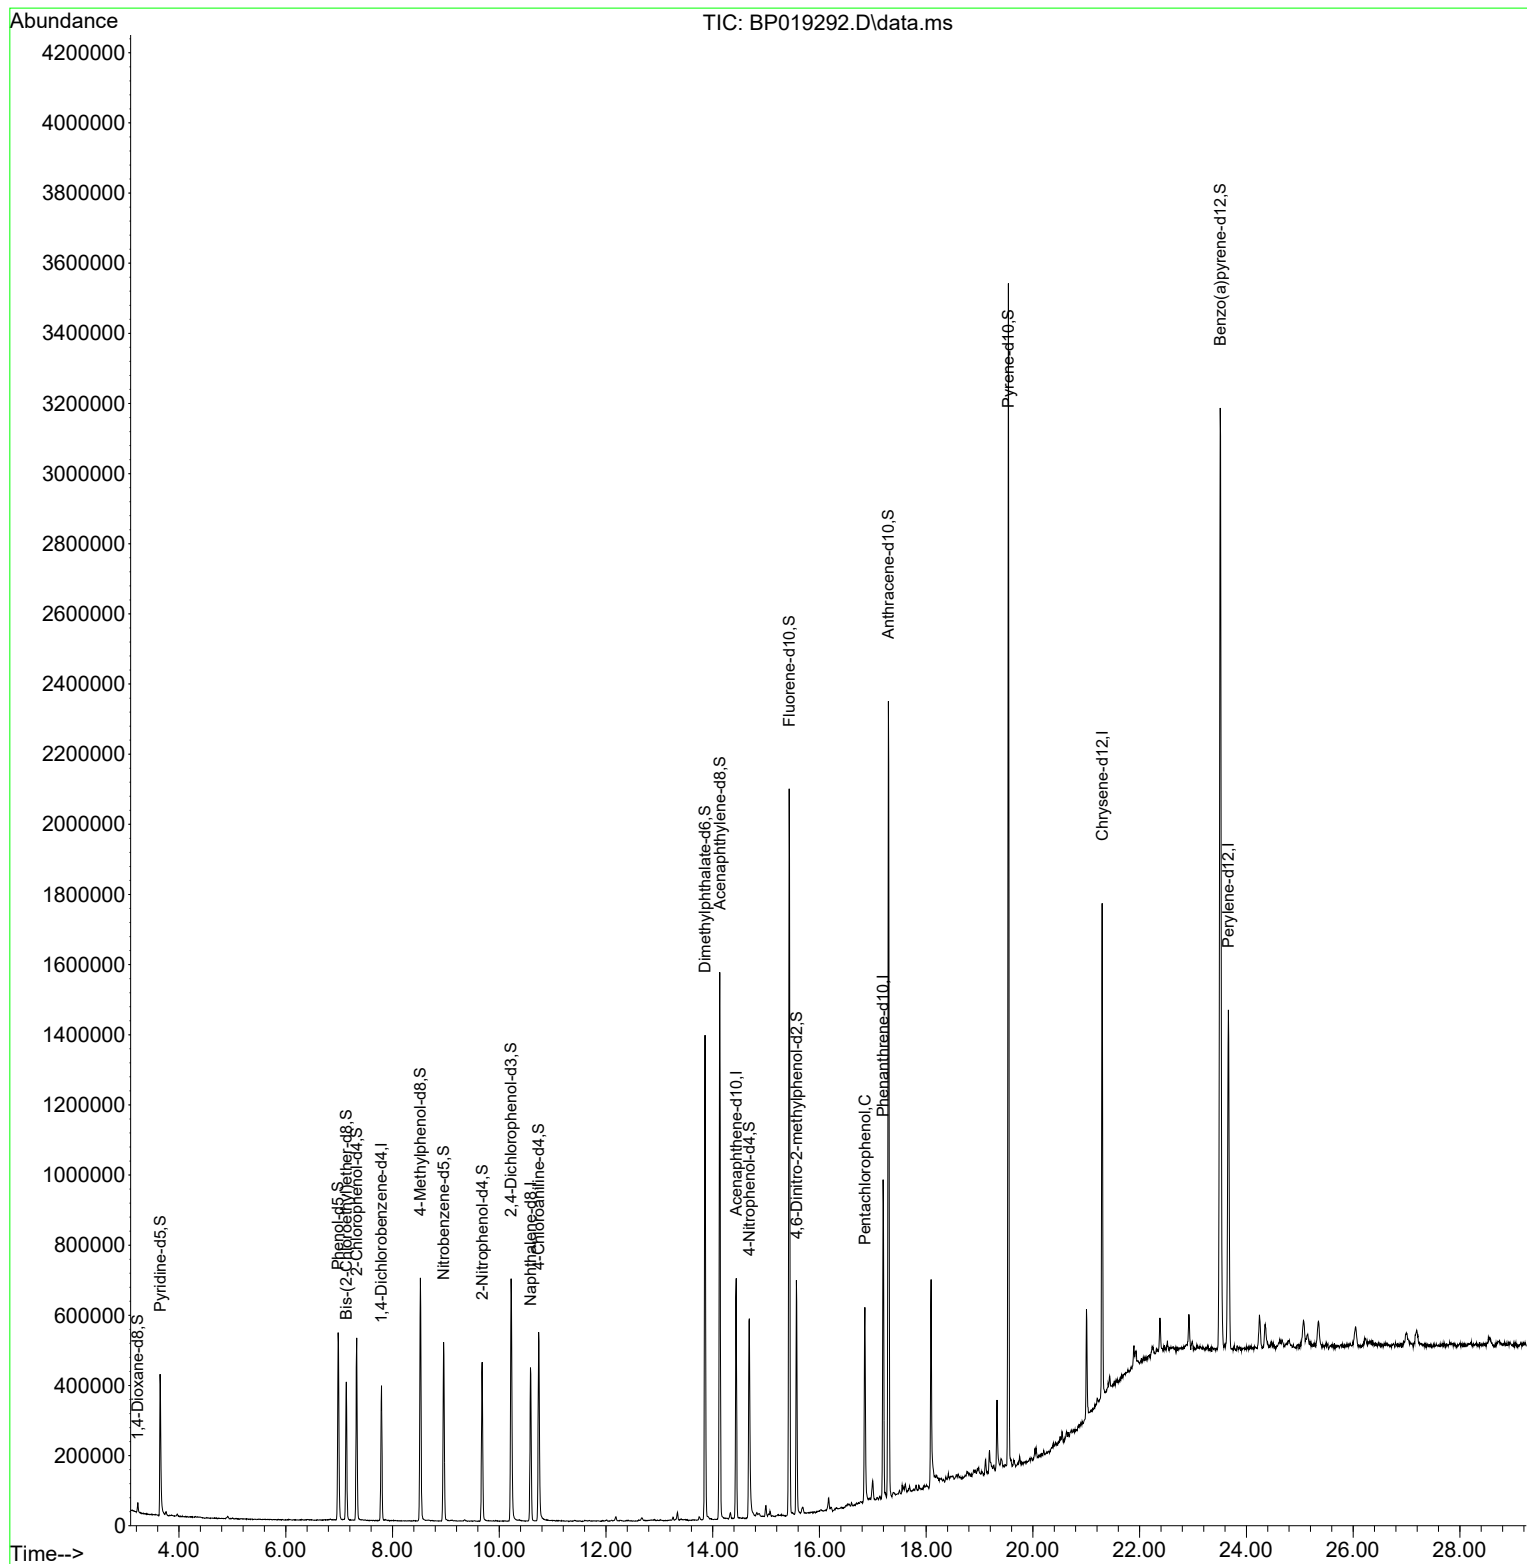

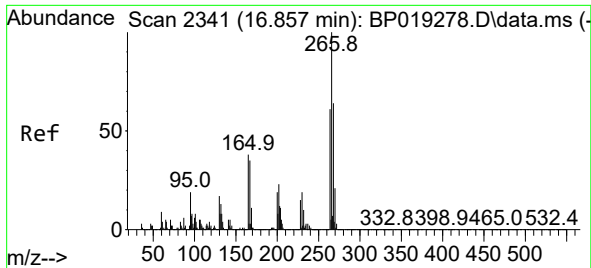

#71
 Pentachlorophenol
 Concen: 23.465 ng/ul
 RT: 16.851 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BP019292.D
 Acq: 05 Jan 2024 21:36

Instrument :
 BNA_P
 ClientSampleId :
 GCFA5

Tgt Ion:266 Resp: 110718
 Ion Ratio Lower Upper
 266 100
 264 64.3 50.0 75.0
 268 64.2 52.8 79.2

