

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010524\
 Data File : BP019293.D
 Acq On : 05 Jan 2024 22:10
 Operator : MA/JU
 Sample : 05953-09
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCFB1

Quant Time: Jan 05 23:23:28 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 29 03:48:11 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.793	152	99224	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.587	136	354531	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.440	164	234736	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.192	188	564084	20.000	ng/ul	-0.01
79) Chrysene-d12	21.298	240	628323	20.000	ng/ul	#-0.01
88) Perylene-d12	23.663	264	745950	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.228	96	9896	3.406	ng/uL	0.00
4) Pyridine-d5	3.652	84	85756	11.760	ng/ul	0.00
7) Phenol-d5	6.981	99	200786	22.565	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.134	67	115272	22.393	ng/ul	0.00
11) 2-Chlorophenol-d4	7.328	132	157459	21.950	ng/ul	0.00
15) 4-Methylphenol-d8	8.522	113	141719	20.457	ng/ul	0.00
21) Nitrobenzene-d5	8.958	128	72487	23.652	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.681	143	84644	25.555	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.228	165	159972	23.918	ng/ul	0.00
31) 4-Chloroaniline-d4	10.746	131	111094	13.504	ng/ul	0.00
46) Dimethylphthalate-d6	13.857	166	485210	23.402	ng/ul	-0.01
49) Acenaphthylene-d8	14.128	160	554584	24.651	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.687	143	74559	21.295	ng/ul	0.02
60) Fluorene-d10	15.434	176	443212	24.744	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.569	200	72273	19.544	ng/ul	0.00
73) Anthracene-d10	17.292	188	699635	23.750	ng/ul	-0.01
81) Pyrene-d10	19.539	212	930742	24.306	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.510	264	1016304	23.703	ng/ul	0.00
Target Compounds						
71) Pentachlorophenol	16.851	266	65536	13.028	ng/ul	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010524\
Data File : BP019293.D
Acq On : 05 Jan 2024 22:10
Operator : MA/JU
Sample : 05953-09
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCFB1

Quant Time: Jan 05 23:23:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 03:48:11 2023
Response via : Initial Calibration

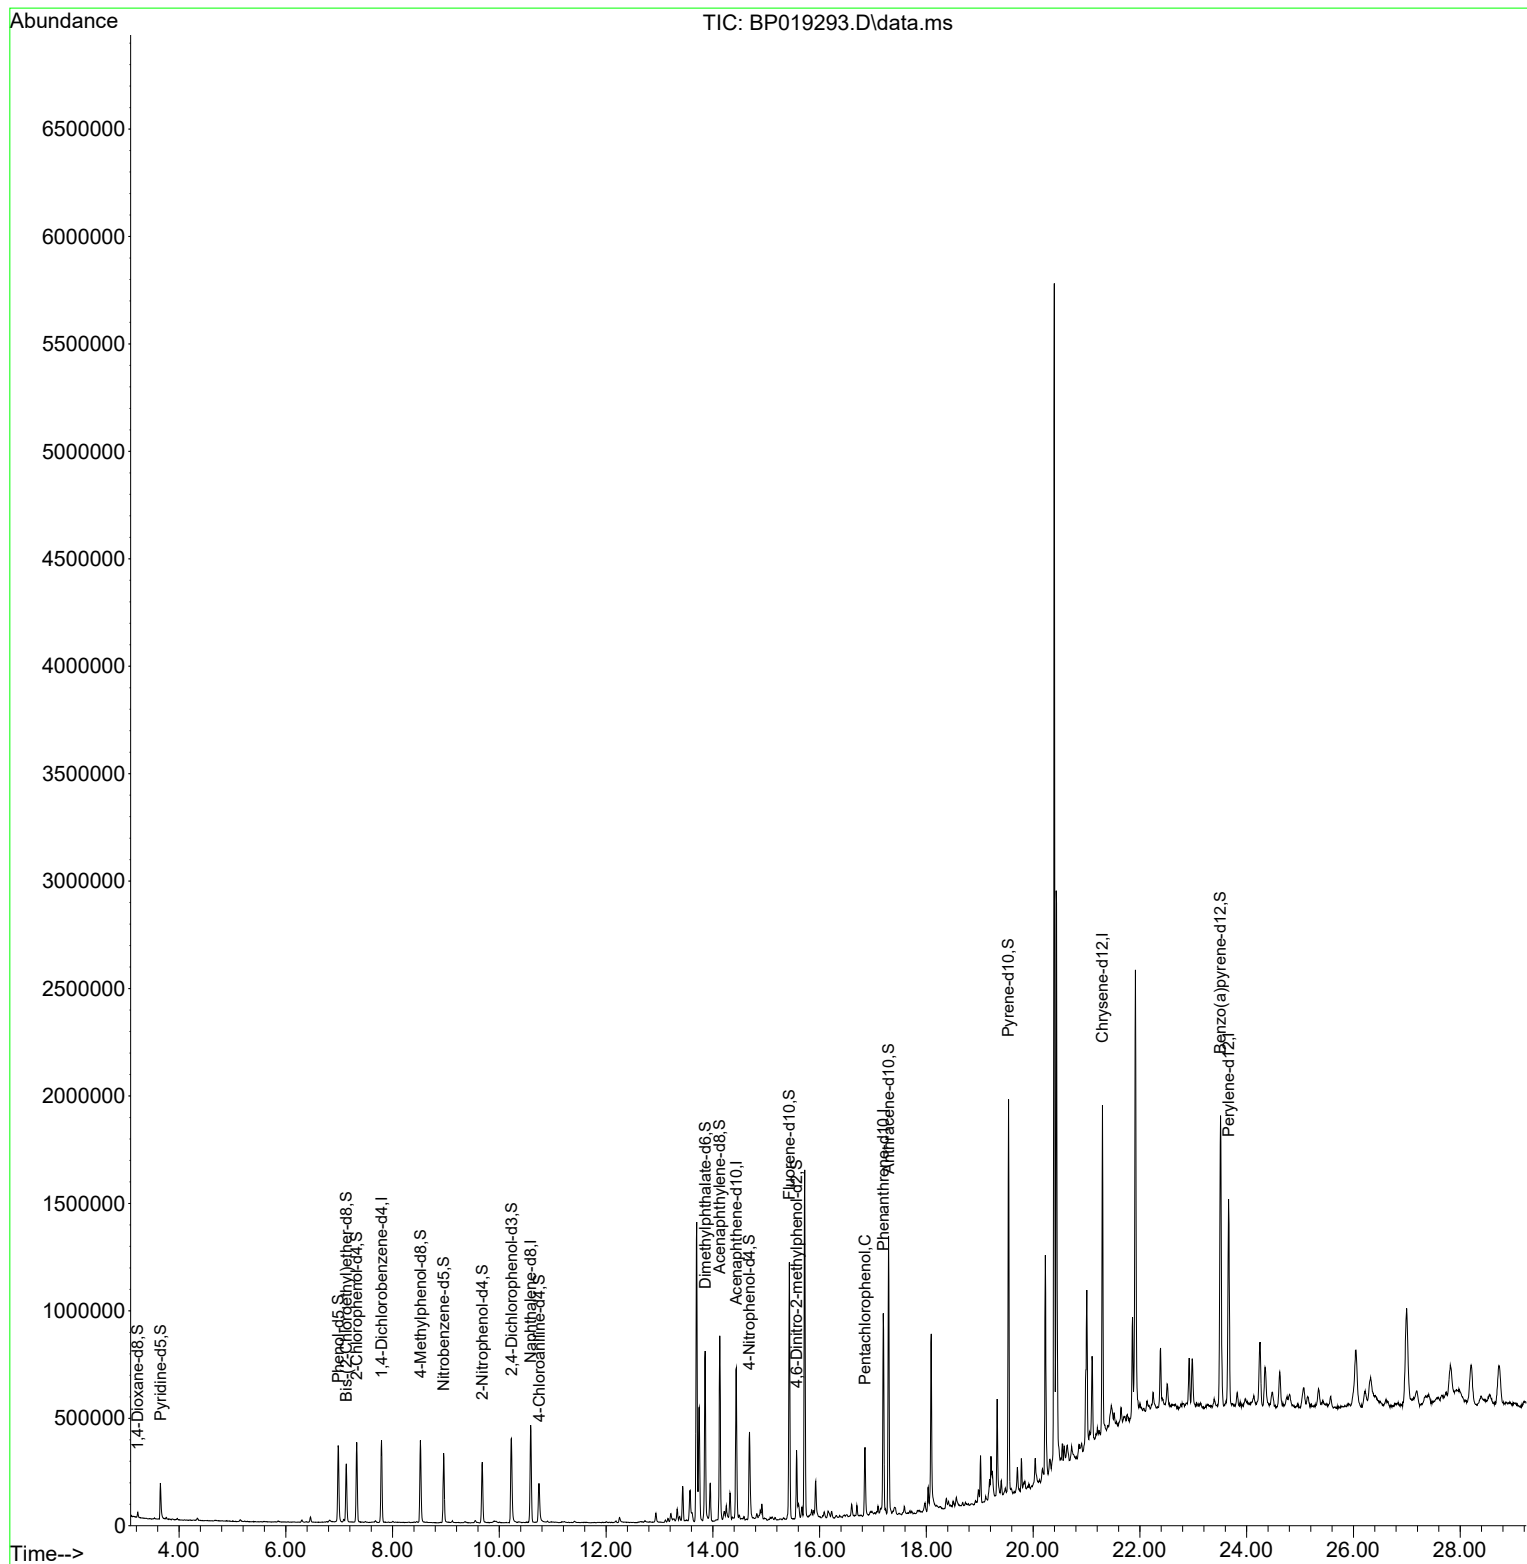

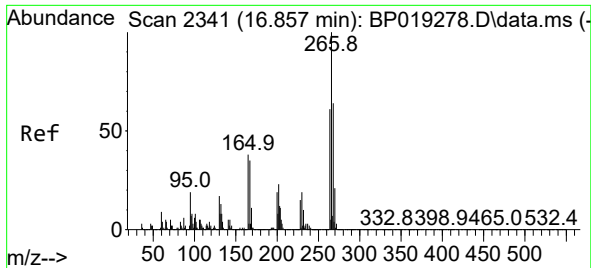

#71
 Pentachlorophenol
 Concen: 13.028 ng/ul
 RT: 16.851 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BP019293.D
 Acq: 05 Jan 2024 22:10

Instrument :
 BNA_P
 ClientSampleId :
 GCFB1

Tgt Ion:266 Resp: 65536
 Ion Ratio Lower Upper
 266 100
 264 65.4 50.0 75.0
 268 69.2 52.8 79.2

