

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010524\
 Data File : BP019281.D
 Acq On : 05 Jan 2024 14:49
 Operator : MA/JU
 Sample : 05953-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCFA6

Quant Time: Jan 05 15:23:08 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 29 03:48:11 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.787	152	143466	20.000	ng/ul	-0.02
20) Naphthalene-d8	10.587	136	585454	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.440	164	402953	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.204	188	973145	20.000	ng/ul	0.00
79) Chrysene-d12	21.310	240	1002220	20.000	ng/ul	0.00
88) Perylene-d12	23.686	264	1151901	20.000	ng/ul	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.228	96	15480	3.685	ng/uL	0.00
4) Pyridine-d5	3.646	84	218089	20.685	ng/ul	0.00
7) Phenol-d5	6.981	99	348530	27.090	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.128	67	193970	26.061	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.322	132	261489	25.211	ng/ul	-0.01
15) 4-Methylphenol-d8	8.522	113	269860	26.942	ng/ul	0.00
21) Nitrobenzene-d5	8.957	128	129472	25.583	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.675	143	157579	28.810	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.222	165	306296	27.732	ng/ul	0.00
31) 4-Chloroaniline-d4	10.746	131	78052	5.745	ng/ul	0.00
46) Dimethylphthalate-d6	13.863	166	1007857	28.317	ng/ul	0.00
49) Acenaphthylene-d8	14.134	160	1119930	28.999	ng/ul	0.00
54) 4-Nitrophenol-d4	14.692	143	164354	27.346	ng/ul	0.03
60) Fluorene-d10	15.440	176	901433	29.316	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.581	200	148200	23.230	ng/ul	0.00
73) Anthracene-d10	17.304	188	1441391	28.362	ng/ul	0.00
81) Pyrene-d10	19.551	212	1835542	30.052	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.533	264	1866962	28.197	ng/ul	0.02
Target Compounds						
71) Pentachlorophenol	16.857	266	91807	10.579	ng/ul	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010524\
Data File : BP019281.D
Acq On : 05 Jan 2024 14:49
Operator : MA/JU
Sample : 05953-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCFA6

Quant Time: Jan 05 15:23:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 03:48:11 2023
Response via : Initial Calibration

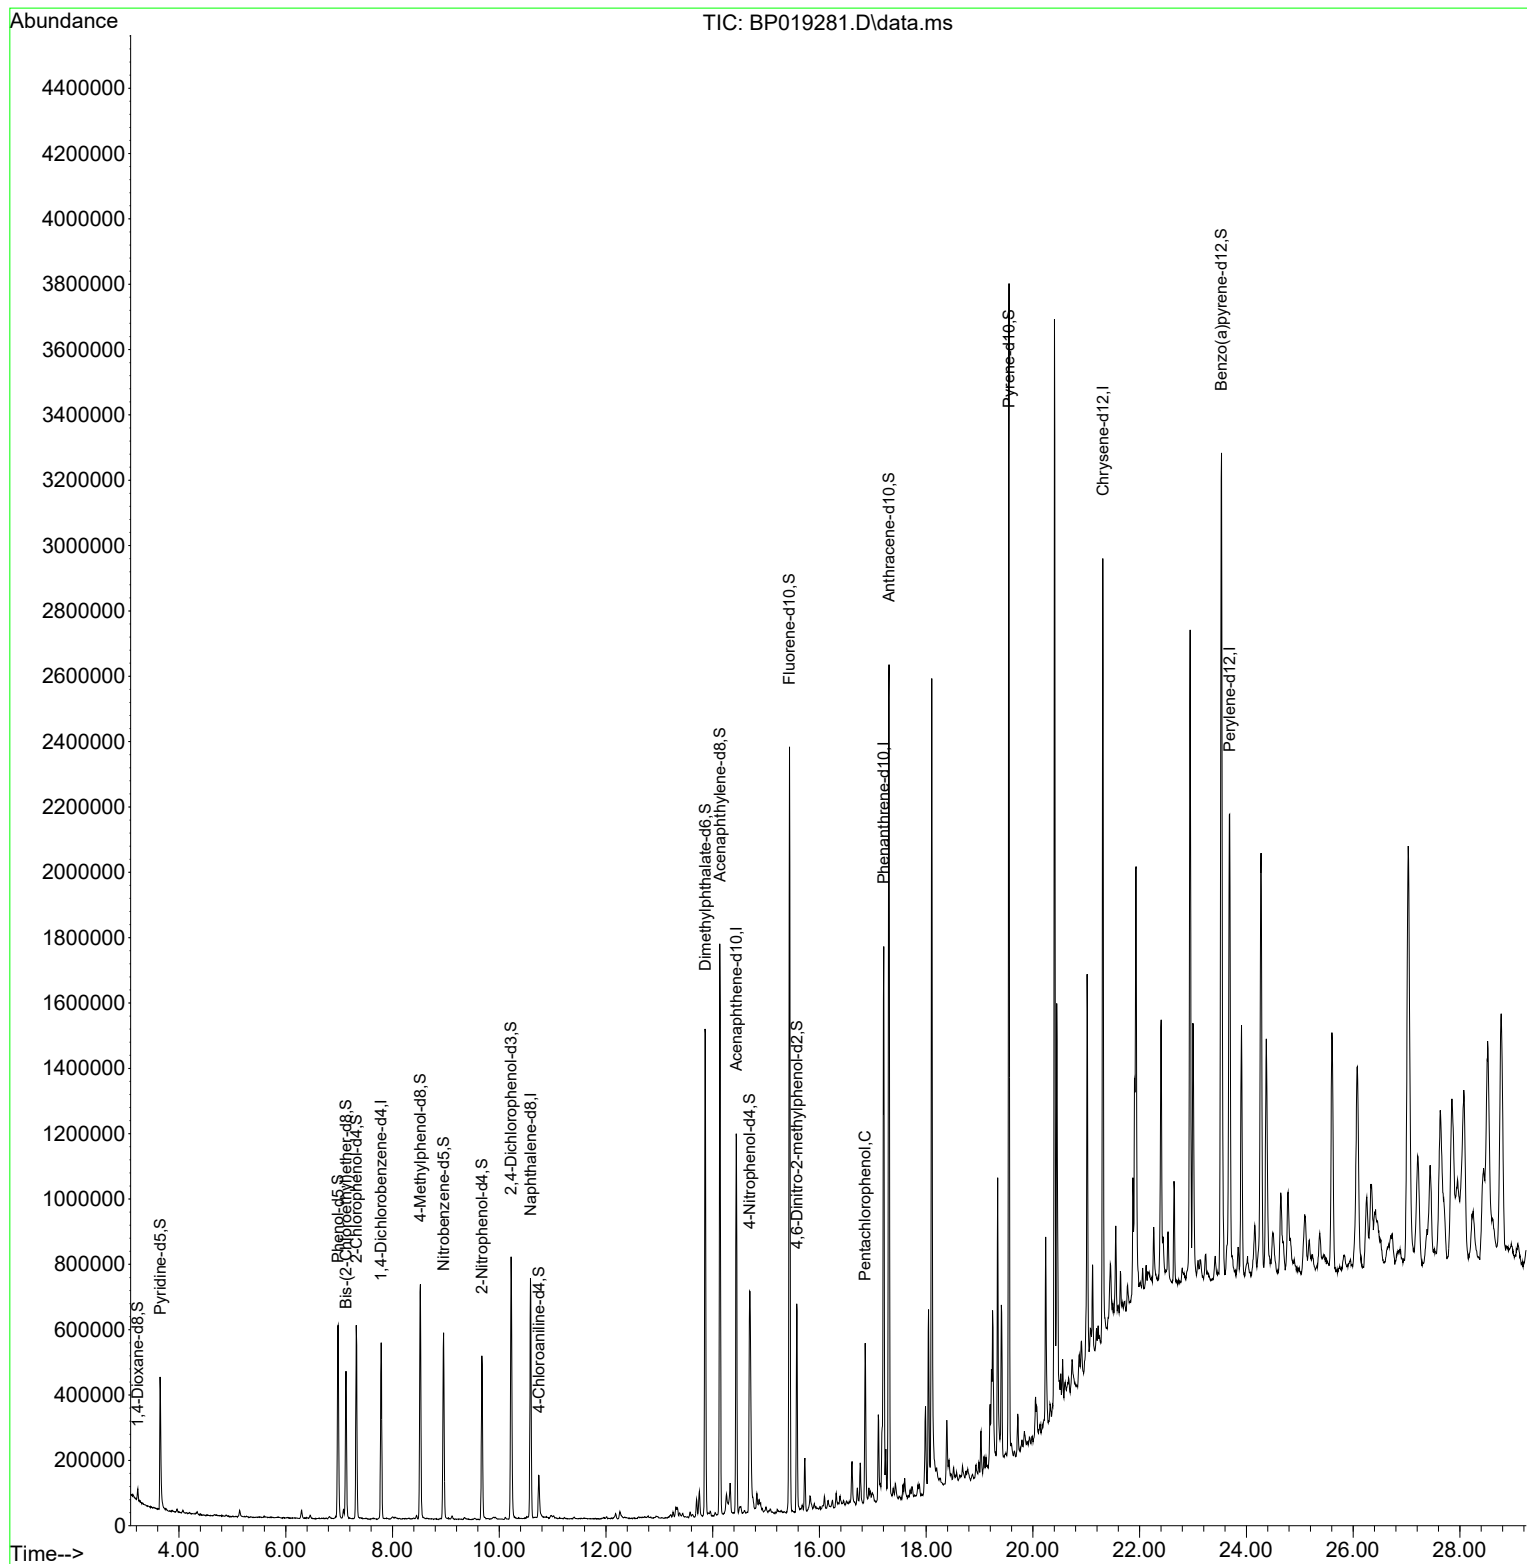

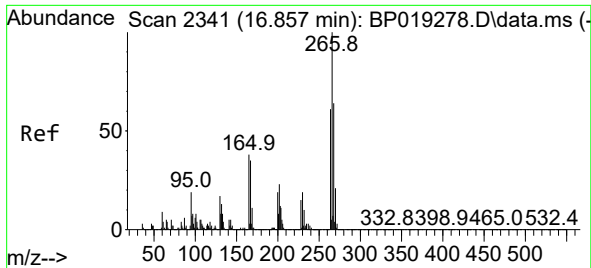

#71
 Pentachlorophenol
 Concen: 10.579 ng/ul
 RT: 16.857 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: BP019281.D
 Acq: 05 Jan 2024 14:49

Instrument :
 BNA_P
 ClientSampleId :
 GCFA6

Tgt Ion	Ratio	Lower	Upper
266	100		
264	61.3	50.0	75.0
268	64.7	52.8	79.2

