

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP019288\
 Data File : BP019288.D
 Acq On : 05 Jan 2024 19:20
 Operator : MA/JU
 Sample : PB158246BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK246

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019288.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	21	24	31	rVB	34388	40700	1.21%	0.144%
2	3.652	92	96	114	rVB	398659	595022	17.73%	2.101%
3	3.970	147	150	156	rVB	9671	13687	0.41%	0.048%
4	6.593	594	596	602	rBV7	1949	3734	0.11%	0.013%
5	6.987	656	663	672	rBV	435861	708704	21.12%	2.502%
6	7.134	682	688	697	rVB	345886	523016	15.58%	1.847%
7	7.328	714	721	732	rBV	458392	719638	21.44%	2.541%
8	7.793	790	800	809	rBV	385316	603076	17.97%	2.129%
9	8.522	916	924	938	rBV	491788	827351	24.65%	2.921%
10	8.963	990	999	1010	rBV	378723	634099	18.89%	2.239%
11	9.681	1111	1121	1130	rBV	341276	569760	16.98%	2.012%
12	10.228	1206	1214	1226	rBV	476782	862476	25.70%	3.045%
13	10.593	1268	1276	1284	rBV	477150	801657	23.89%	2.831%
14	10.746	1292	1302	1316	rBV	446410	808694	24.10%	2.855%
15	12.187	1540	1547	1555	rBV3	7364	14506	0.43%	0.051%
16	13.340	1736	1743	1747	rBV5	7892	14966	0.45%	0.053%
17	13.857	1824	1831	1841	rBV	840474	1186540	35.36%	4.190%
18	13.934	1843	1844	1852	rVB8	3549	5905	0.18%	0.021%
19	14.134	1870	1878	1894	rBV	989852	1481337	44.14%	5.230%
20	14.322	1905	1910	1916	rBV10	3952	8135	0.24%	0.029%
21	14.440	1923	1930	1939	rBV	721482	1084208	32.31%	3.828%
22	14.693	1966	1973	1991	rBV	299692	643681	19.18%	2.273%
23	15.434	2093	2099	2113	rBV	1292884	1863158	55.52%	6.579%
24	15.575	2116	2123	2134	rVV	332395	515144	15.35%	1.819%
25	15.675	2136	2140	2145	rVB8	6221	11253	0.34%	0.040%
26	16.245	2228	2237	2240	rBV10	14430	27427	0.82%	0.097%
27	16.863	2339	2342	2343	rBV3	5166	5547	0.17%	0.020%
28	16.987	2359	2363	2365	rBV5	3080	3887	0.12%	0.014%
29	17.198	2391	2399	2408	rBV	980524	1424526	42.45%	5.030%
30	17.292	2409	2415	2428	rVV	1468400	2164066	64.48%	7.641%
31	17.498	2445	2450	2454	rBV8	6564	14613	0.44%	0.052%
32	18.086	2546	2550	2558	rBV	36854	61974	1.85%	0.219%
33	19.116	2722	2725	2729	rVB3	20858	26916	0.80%	0.095%
34	19.186	2734	2737	2746	rBV	20781	37924	1.13%	0.134%
35	19.328	2759	2761	2770	rVB8	18666	25940	0.77%	0.092%
36	19.539	2792	2797	2806	rBV	2068284	2767620	82.47%	9.772%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010524\
Data File : BP019288.D
Acq On : 05 Jan 2024 19:20
Operator : MA/JU
Sample : PB158246BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK246

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Title : SVOA CALIBRATION

37	21.298	3092	3096	3102	rBV	1447581	1823882	54.35%	6.440%
38	23.516	3466	3473	3487	rVB	1618197	3356034	100.00%	11.850%
39	23.669	3493	3499	3507	rVB	1051766	2040940	60.81%	7.206%




Sum of corrected areas: 28321743

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010524\
Data File : BP019288.D
Acq On : 05 Jan 2024 19:20
Operator : MA/JU
Sample : PB158246BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK246

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

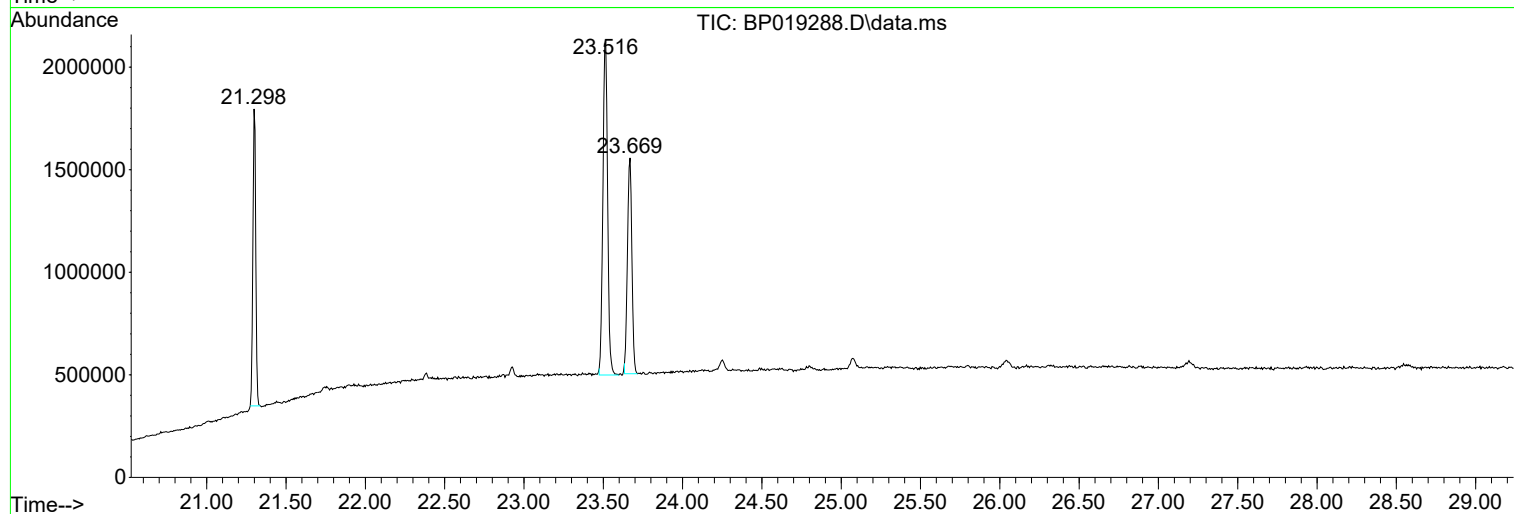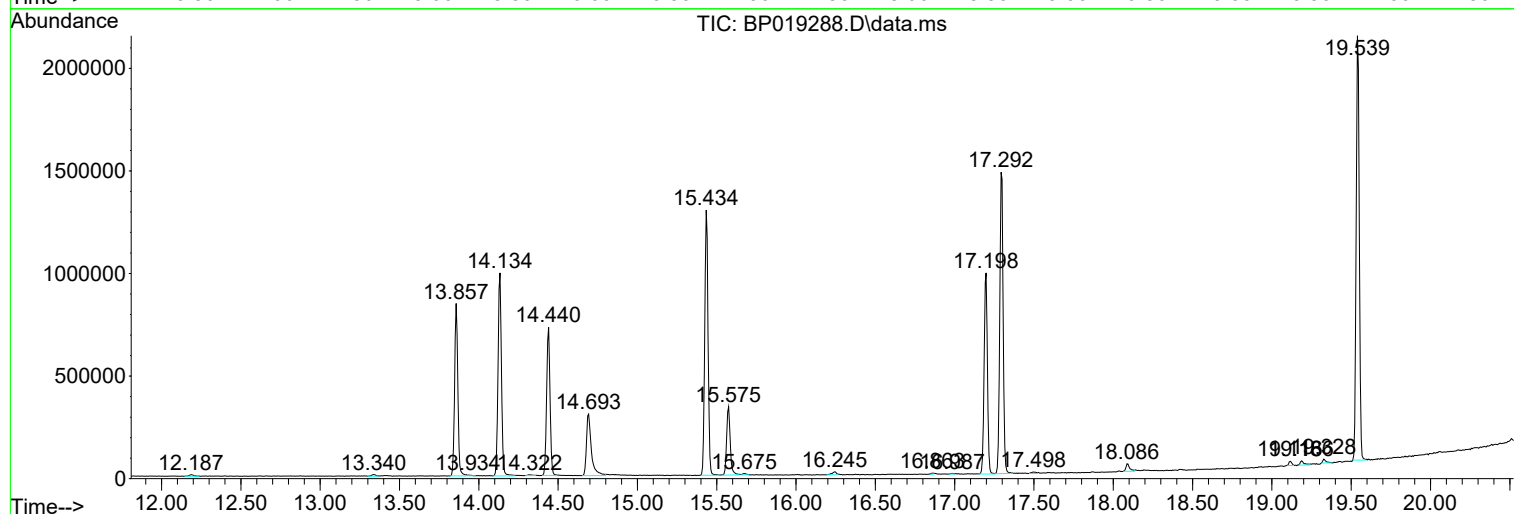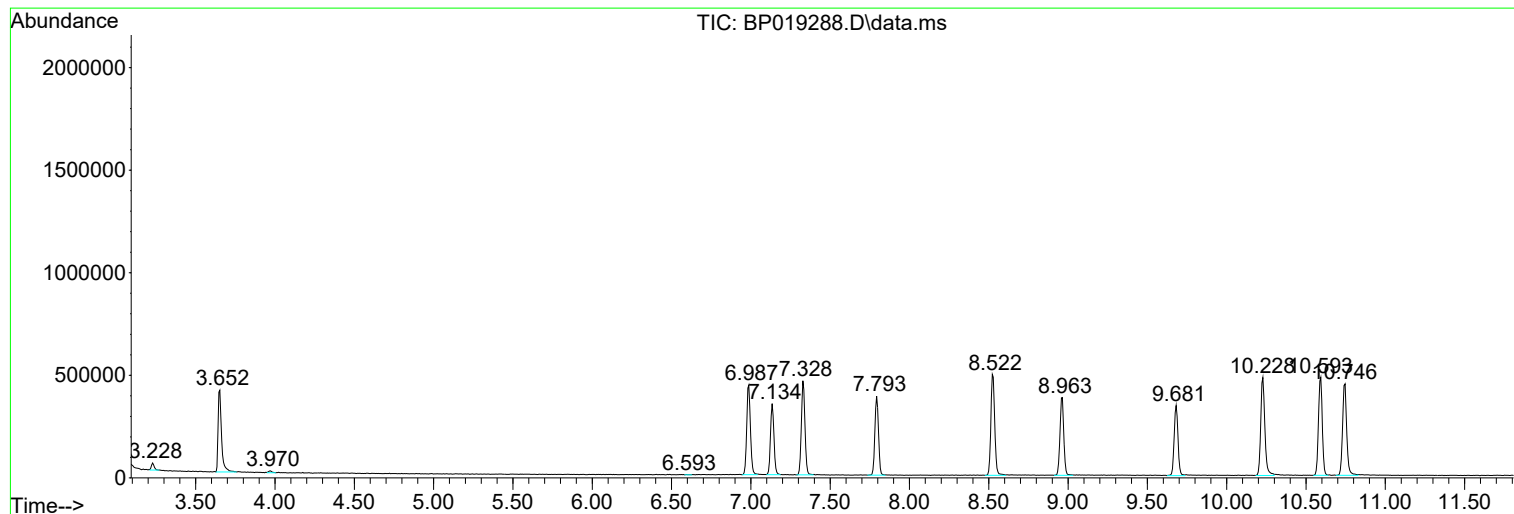

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010524\
Data File : BP019288.D
Acq On : 05 Jan 2024 19:20
Operator : MA/JU
Sample : PB158246BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK246

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010524\
Data File : BP019288.D
Acq On : 05 Jan 2024 19:20
Operator : MA/JU
Sample : PB158246BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK246

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------