
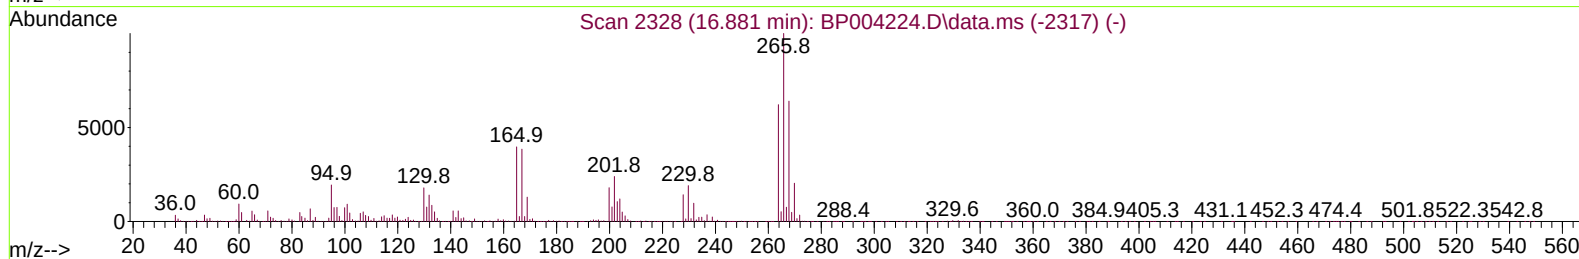
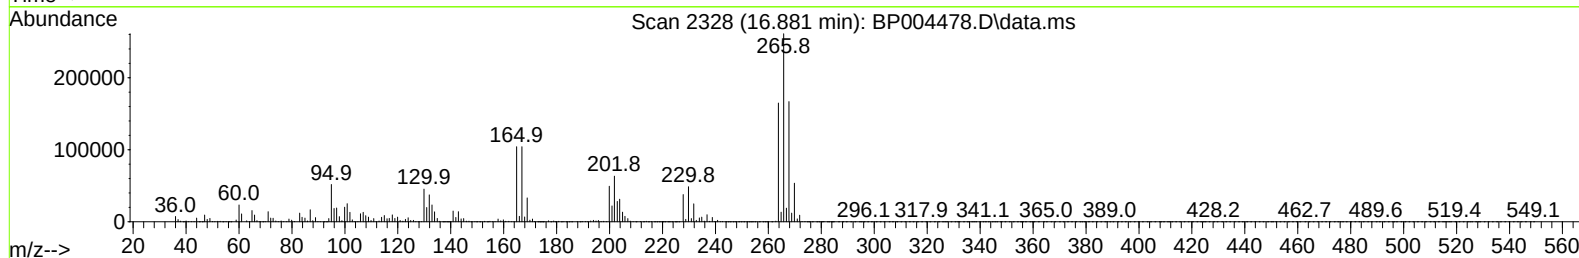


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010721\
 Data File : BP004478.D
 Acq On : 07 Jan 2021 13:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 08 03:25:15 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP121120.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 07 14:50:44 2021
 Response via : Initial Calibration

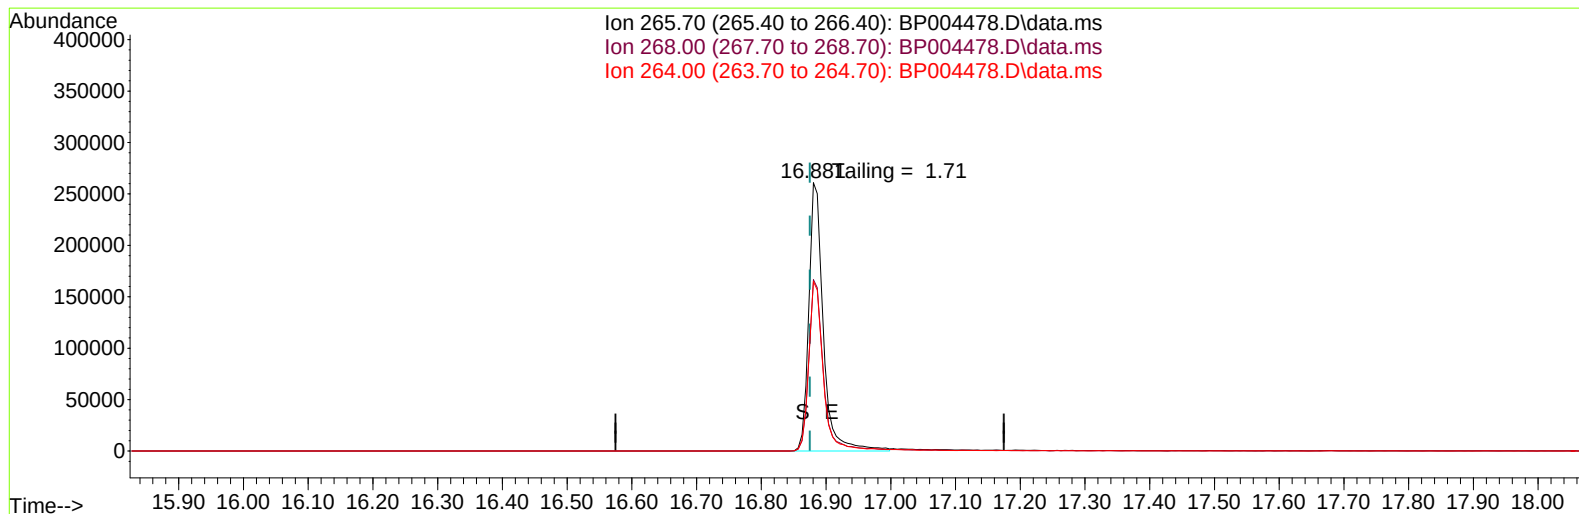

TIC: BP004478.D\data.ms

(70) Pentachlorophenol (C)




16.881min (+ 0.006) 101536.40 ng

response 414344

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	63.88
264.00	63.30	63.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010721\
 Data File : BP004478.D
 Acq On : 07 Jan 2021 13:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 08 03:25:15 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP121120.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 07 14:50:44 2021
 Response via : Initial Calibration

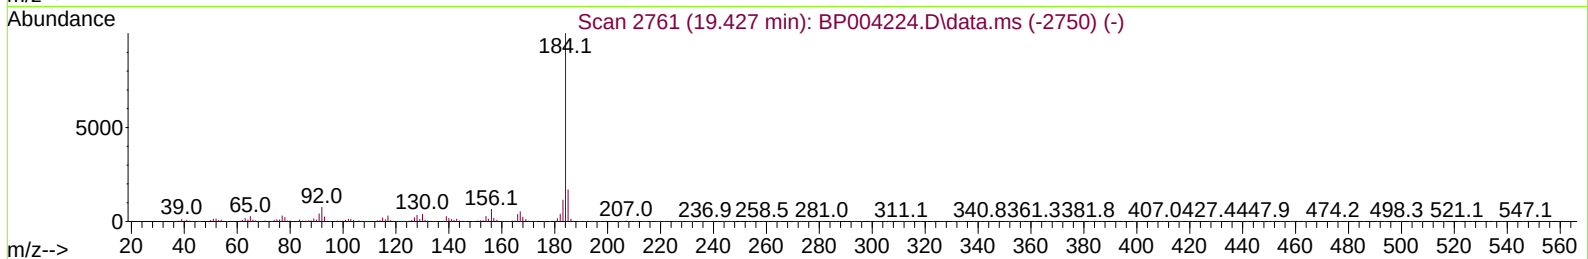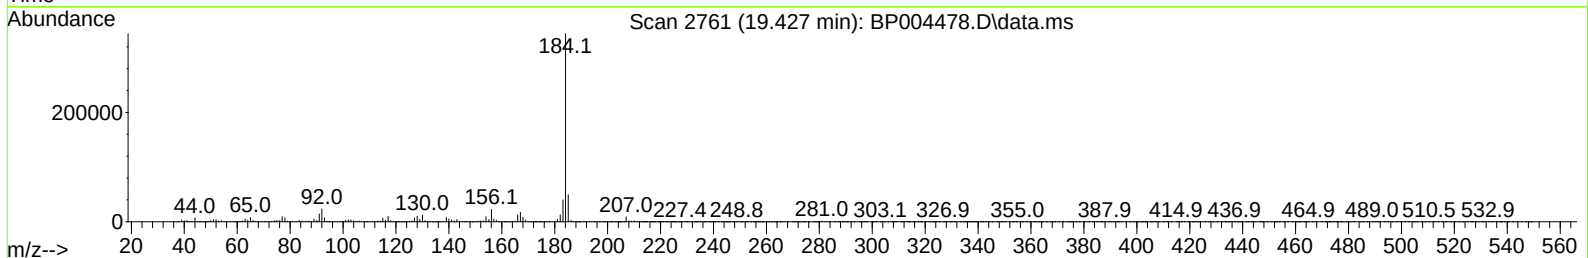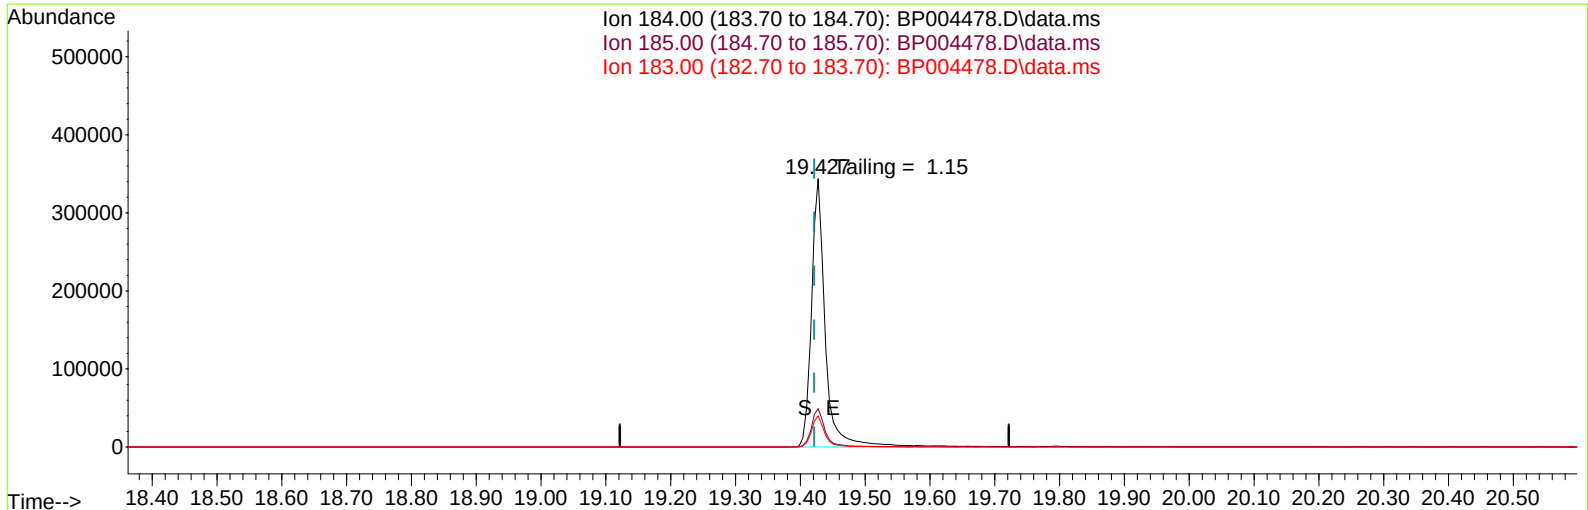

TIC: BP004478.D\data.ms

(77) Benzidine**19.427min (+ 0.006) 20775.46 ng****response 505807**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.35
183.00	12.00	11.66
0.00	0.00	0.00